

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052122\
 Data File : VY008948.D
 Acq On : 21 May 2022 14:40
 Operator : KP/MD
 Sample : N2919-13
 Misc : 5.21g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 P013-SS002-2430-01

Quant Time: May 21 21:29:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052022S.M
 Quant Title : SW846 8260
 QLast Update : Fri May 20 23:50:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	130583	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	236921	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	223209	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	99543	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	82158	61.132	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	122.260%
35) Dibromofluoromethane	7.710	113	76304	51.792	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	103.580%
50) Toluene-d8	10.179	98	294272	54.143	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	108.280%
62) 4-Bromofluorobenzene	12.483	95	89391	40.772	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	81.540%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052122\
Data File : VY008948.D
Acq On : 21 May 2022 14:40
Operator : KP/MD
Sample : N2919-13
Misc : 5.21g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
P013-SS002-2430-01

Quant Time: May 21 21:29:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052022S.M
Quant Title : SW846 8260
QLast Update : Fri May 20 23:50:52 2022
Response via : Initial Calibration




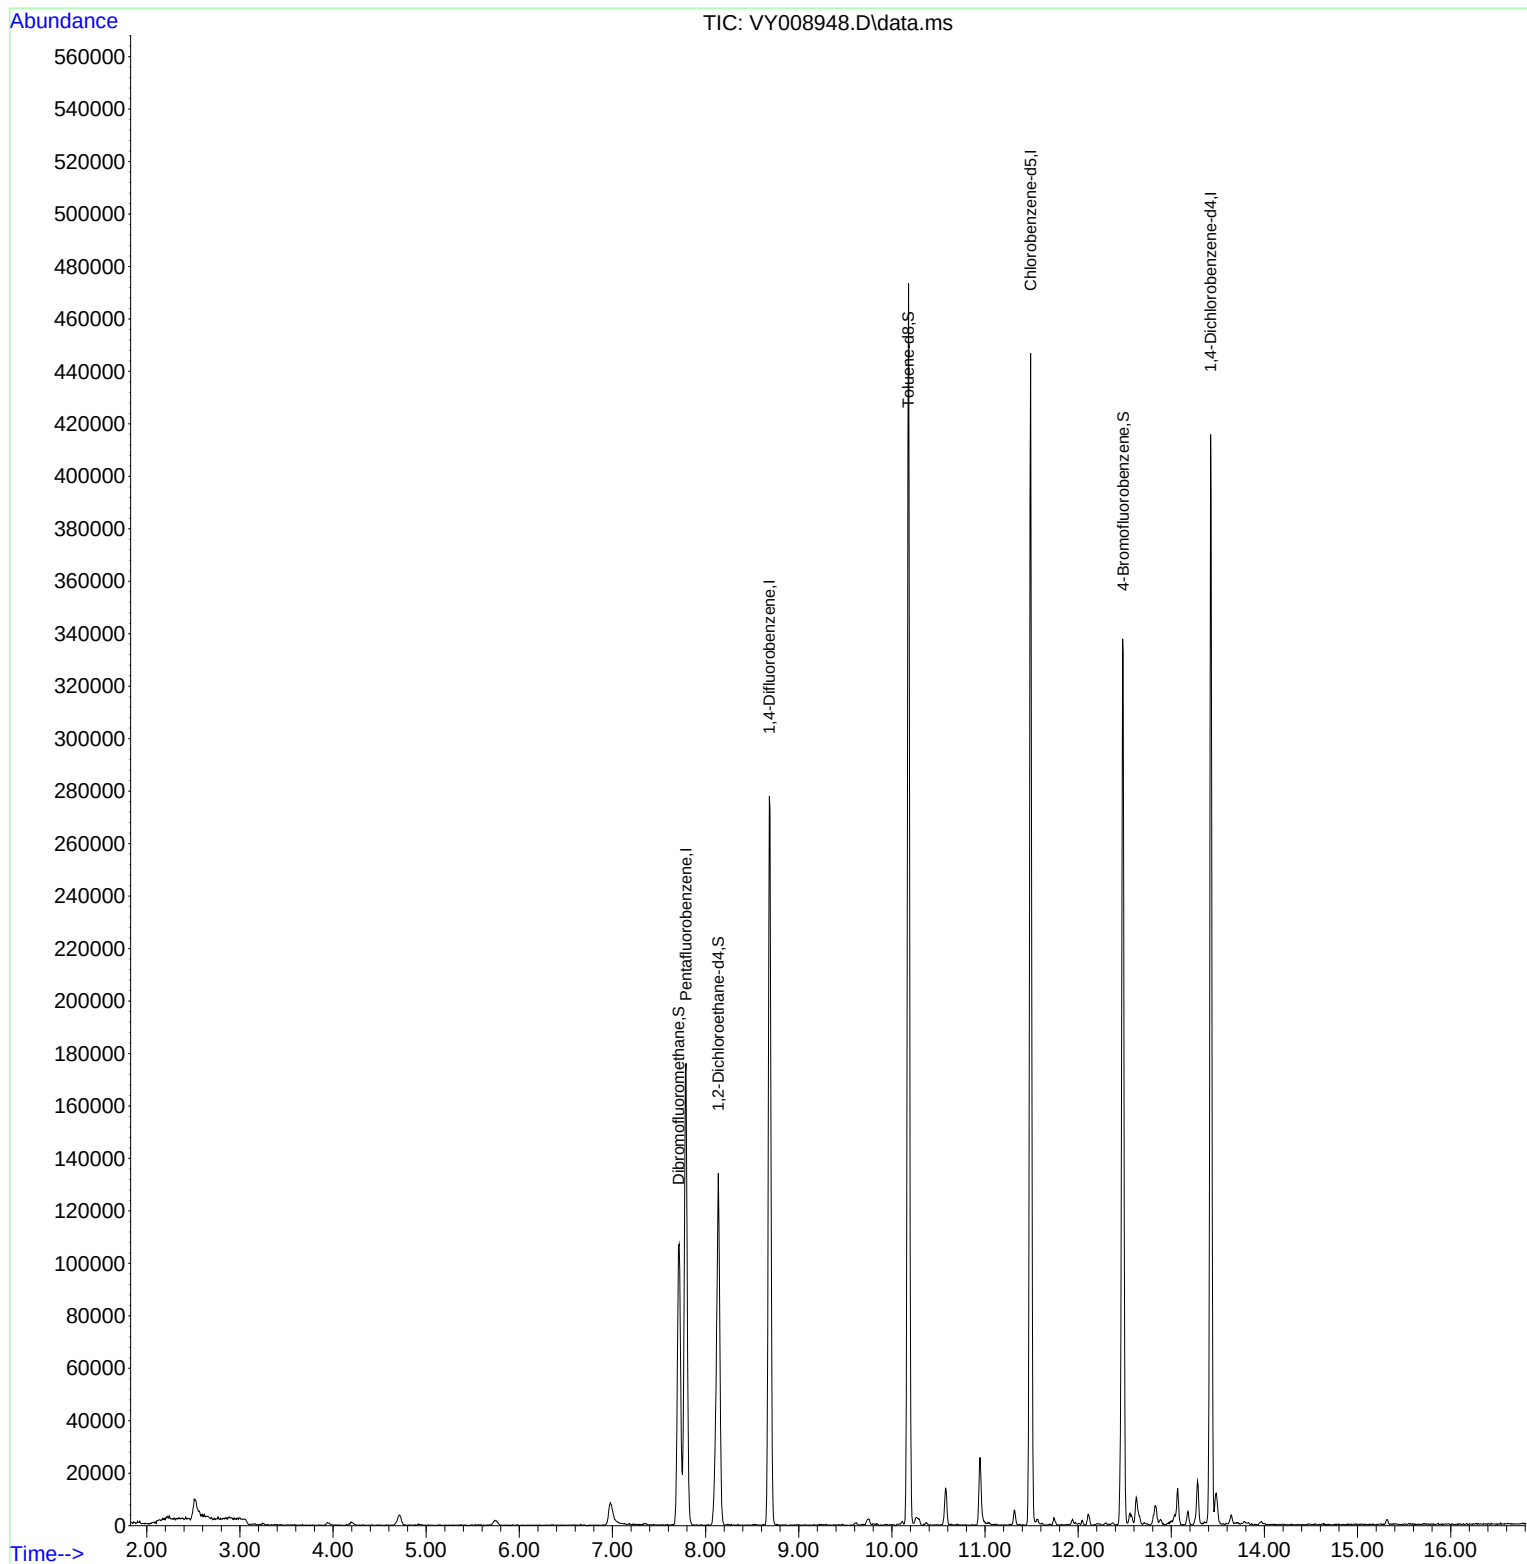


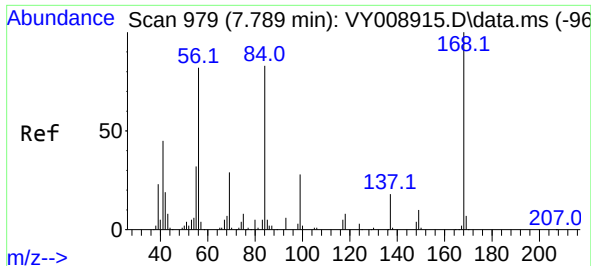

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY008948.D
Acq: 21 May 2022 14:40




Instrument :
MSVOA_Y
ClientSampleId :
P013-SS002-2430-01


Tgt Ion:168 Resp: 130583
Ion Ratio Lower Upper
168 100
99 53.5 46.9 70.3

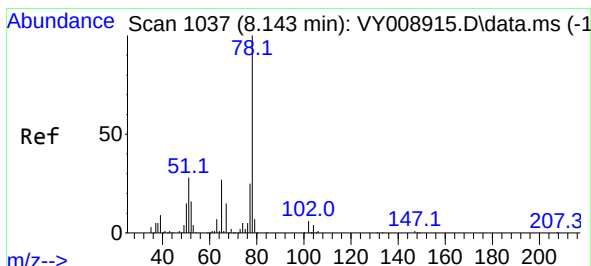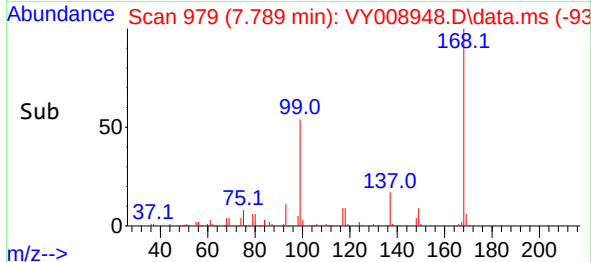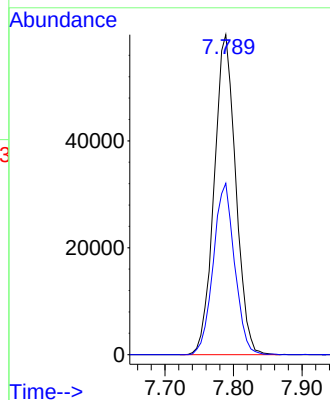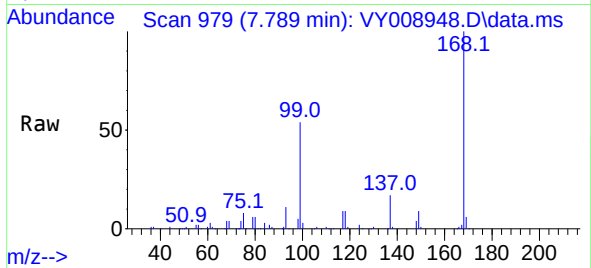

#33
1,2-Dichloroethane-d4
Concen: 61.132 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. -0.007 min
Lab File: VY008948.D
Acq: 21 May 2022 14:40

Tgt Ion: 65 Resp: 82158
Ion Ratio Lower Upper
65 100
67 53.5 0.0 99.4

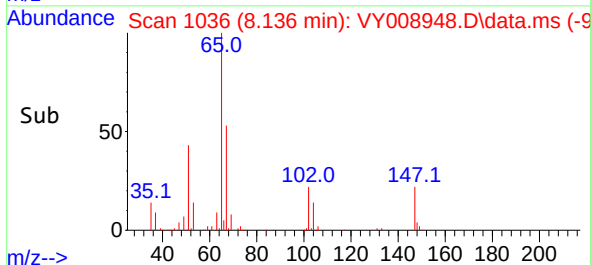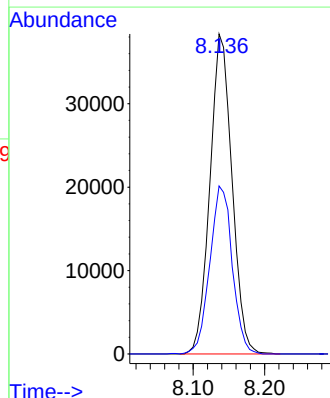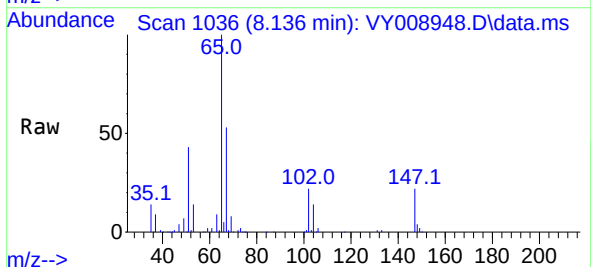

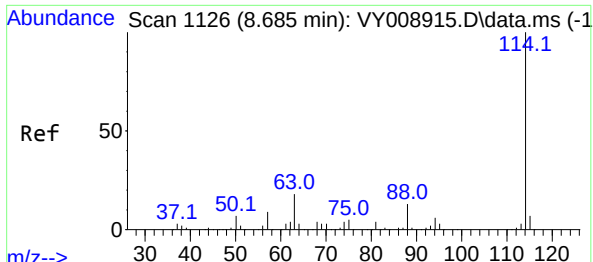

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. -0.000 min

Lab File: VY008948.D

Acq: 21 May 2022 14:40

Instrument :

MSVOA_Y

ClientSampleId :

P013-SS002-2430-01





Tgt Ion:114 Resp: 236921

Ion Ratio Lower Upper

114 100

63 18.6 0.0 43.2

88 13.5 0.0 31.8

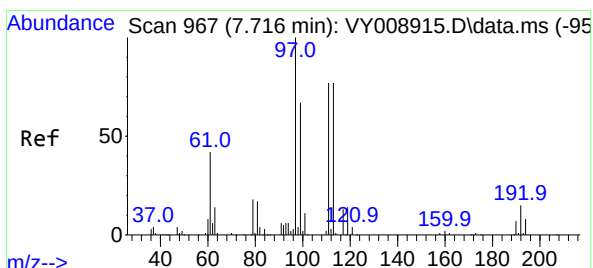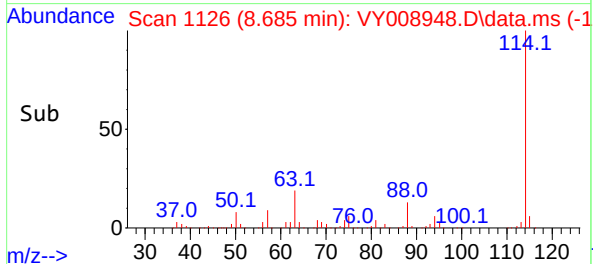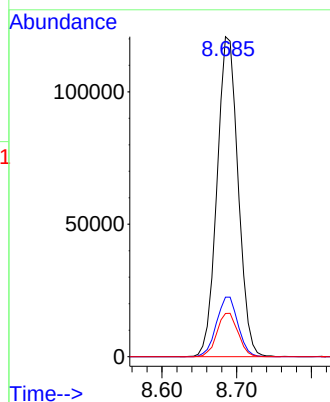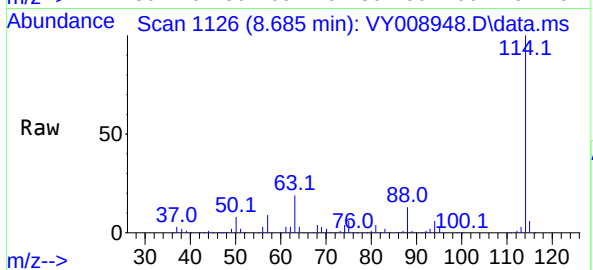

#35

Dibromofluoromethane

Concen: 51.792 ug/l

RT: 7.710 min Scan# 966

Delta R.T. -0.006 min

Lab File: VY008948.D

Acq: 21 May 2022 14:40




Tgt Ion:113 Resp: 76304


Ion Ratio Lower Upper

113 100

111 101.2 82.6 124.0

192 18.3 17.6 26.4


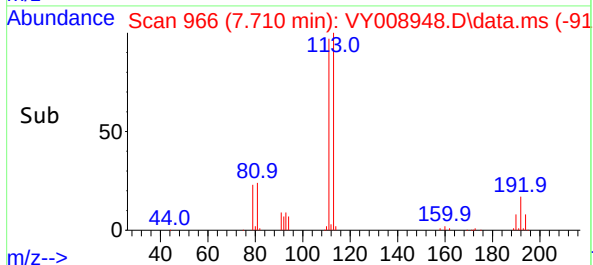
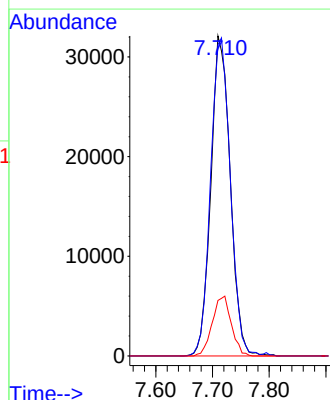
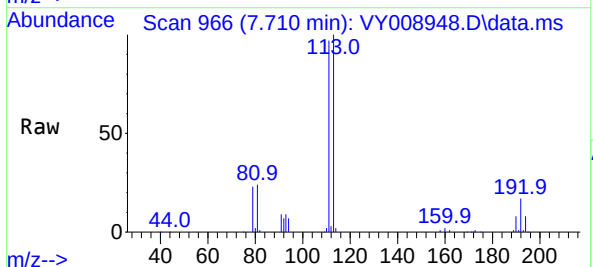


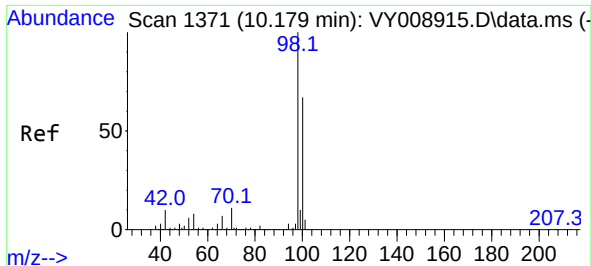

#50
Toluene-d8
Concen: 54.143 ug/l
RT: 10.179 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY008948.D
Acq: 21 May 2022 14:40




Instrument :
MSVOA_Y
ClientSampleId :
P013-SS002-2430-01


Tgt Ion: 98 Resp: 294272
Ion Ratio Lower Upper
98 100
100 65.1 50.2 75.2

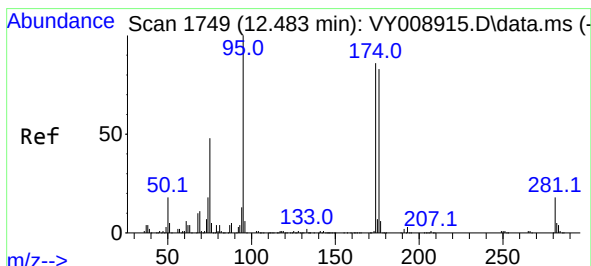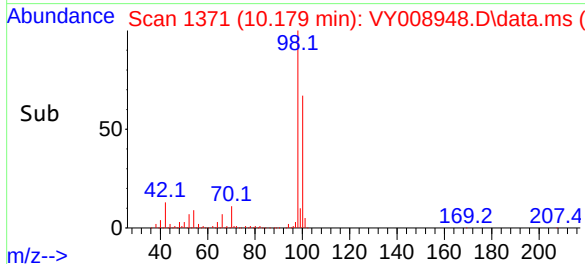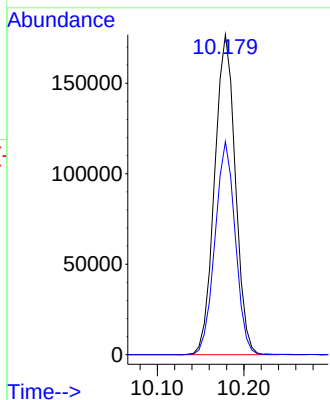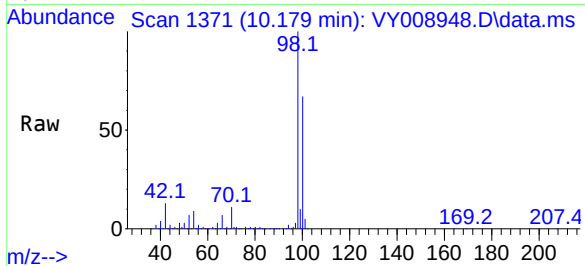

#62
4-Bromofluorobenzene
Concen: 40.772 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY008948.D
Acq: 21 May 2022 14:40

Tgt Ion: 95 Resp: 89391
Ion Ratio Lower Upper
95 100
174 89.7 0.0 177.0
176 87.4 0.0 175.8


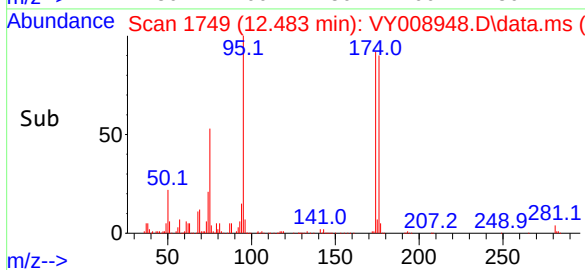
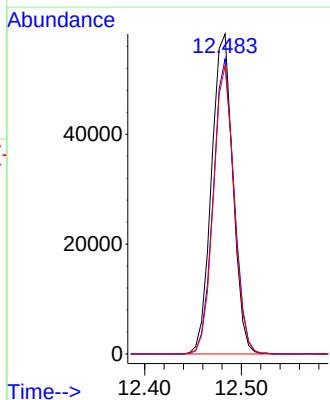
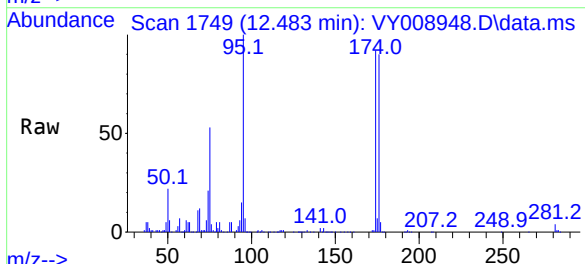


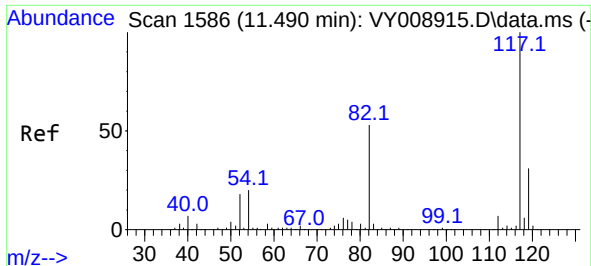

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 11
Delta R.T. -0.001 min
Lab File: VY008948.D
Acq: 21 May 2022 14:40

Instrument :
MSVOA_Y
ClientSampleId :
P013-SS002-2430-01

Tgt Ion:117 Resp: 223209
Ion Ratio Lower Upper
117 100
82 54.4 43.0 64.4
119 32.8 25.4 38.0

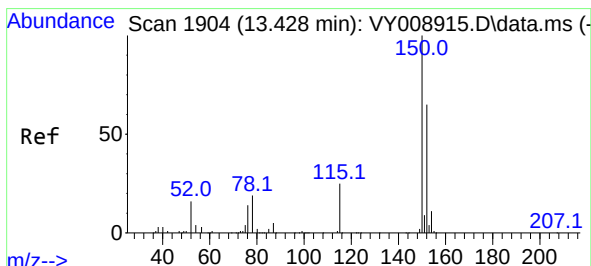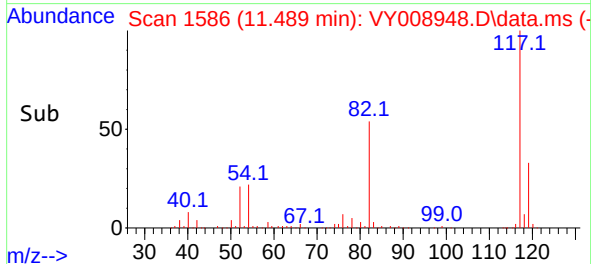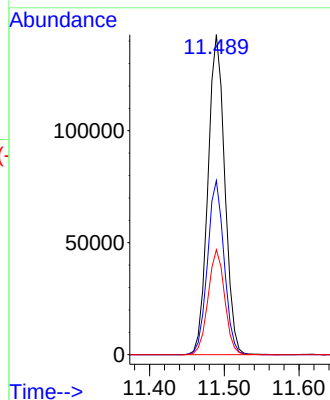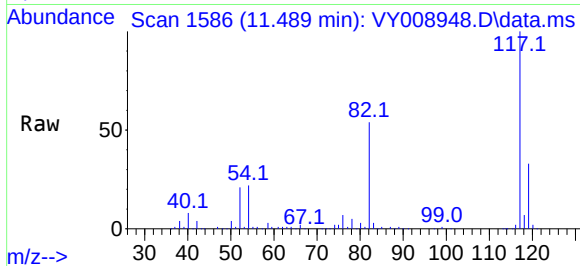

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. -0.006 min
Lab File: VY008948.D
Acq: 21 May 2022 14:40

Tgt Ion:152 Resp: 99543
Ion Ratio Lower Upper
152 100
115 56.0 28.2 84.7
150 157.7 0.0 347.6

