

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052122\
 Data File : VY008976.D
 Acq On : 22 May 2022 03:04
 Operator : KP/MD
 Sample : N2887-09
 Misc : 6.24g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 P038-SS001-1218-01

Quant Time: May 22 04:49:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052022S.M
 Quant Title : SW846 8260
 QLast Update : Fri May 20 23:50:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	116158	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	208418	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	200397	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	88515	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	78412	65.590	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	131.180%
35) Dibromofluoromethane	7.716	113	68626	52.951	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	105.900%
50) Toluene-d8	10.179	98	262357	54.872	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	109.740%
62) 4-Bromofluorobenzene	12.477	95	76768	39.803	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	79.600%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052122\
Data File : VY008976.D
Acq On : 22 May 2022 03:04
Operator : KP/MD
Sample : N2887-09
Misc : 6.24g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
P038-SS001-1218-01

Quant Time: May 22 04:49:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052022S.M
Quant Title : SW846 8260
QLast Update : Fri May 20 23:50:52 2022
Response via : Initial Calibration




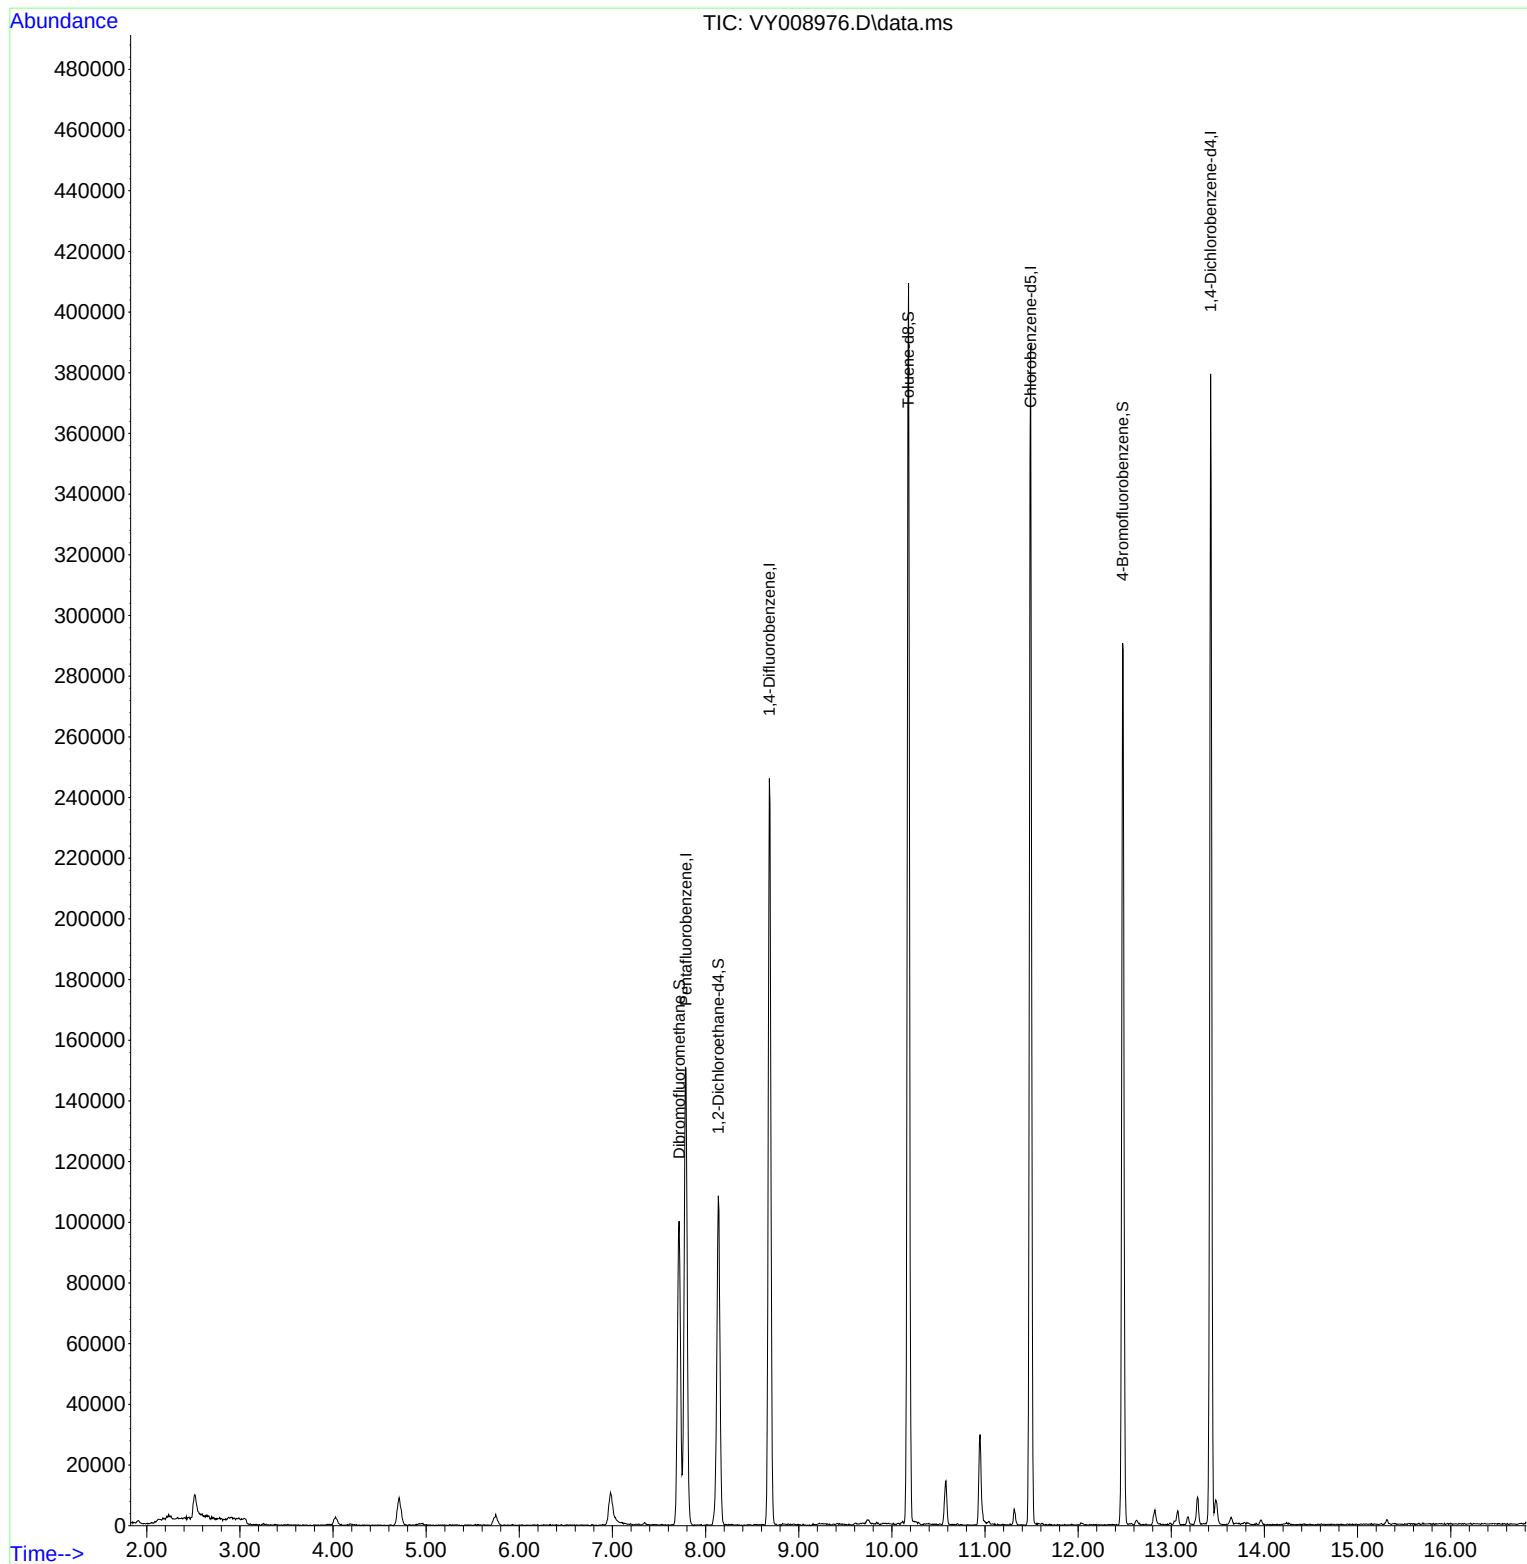


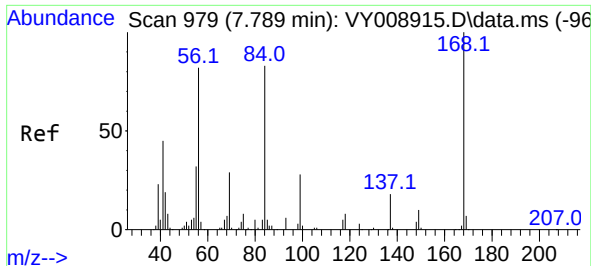

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY008976.D
Acq: 22 May 2022 03:04




Instrument :
MSVOA_Y
ClientSampleId :
P038-SS001-1218-01


Tgt Ion:168 Resp: 116158
Ion Ratio Lower Upper
168 100
99 51.8 46.9 70.3

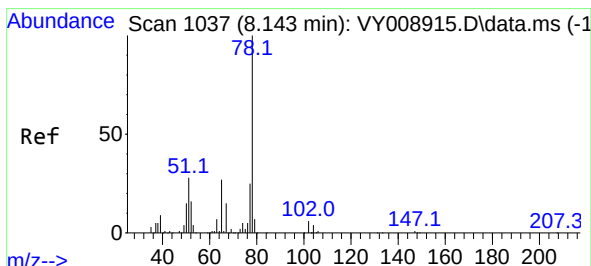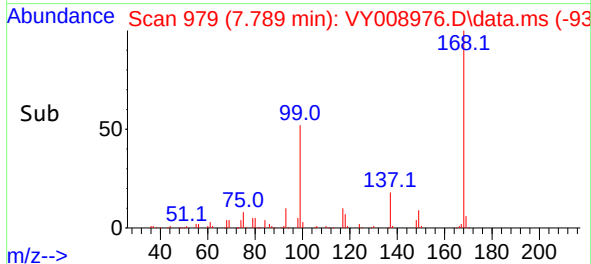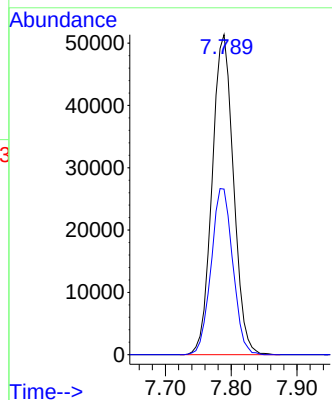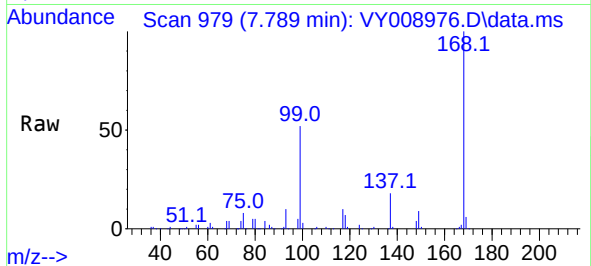

#33
1,2-Dichloroethane-d4
Concen: 65.590 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. -0.007 min
Lab File: VY008976.D
Acq: 22 May 2022 03:04

Tgt Ion: 65 Resp: 78412
Ion Ratio Lower Upper
65 100
67 51.8 0.0 99.4

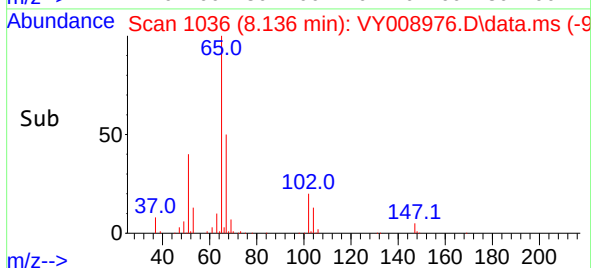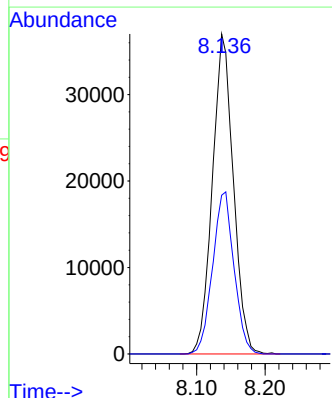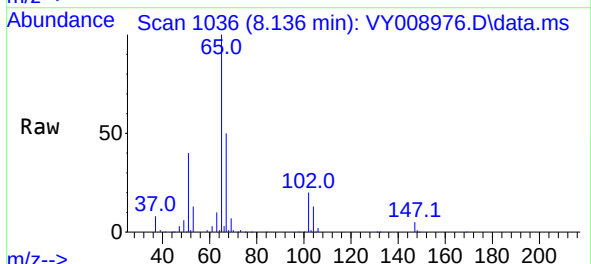

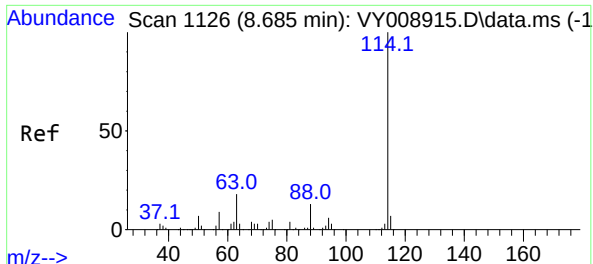

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. 0.000 min

Lab File: VY008976.D

Acq: 22 May 2022 03:04

Instrument :

MSVOA_Y

ClientSampleId :

P038-SS001-1218-01





Tgt Ion:114 Resp: 208418

Ion Ratio Lower Upper

114 100

63 18.9 0.0 43.2

88 14.2 0.0 31.8

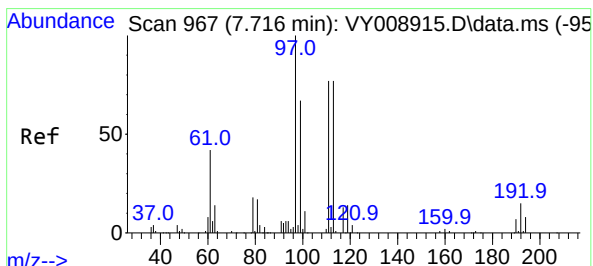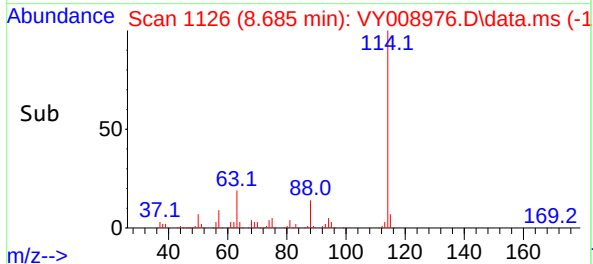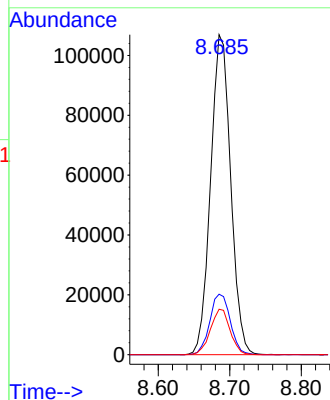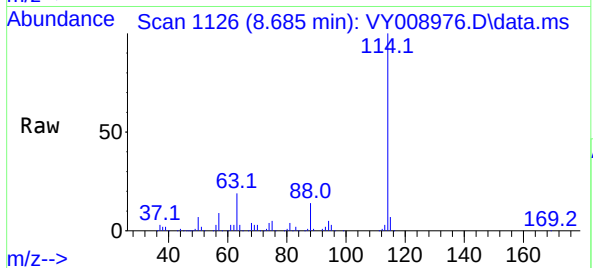

#35

Dibromofluoromethane

Concen: 52.951 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY008976.D

Acq: 22 May 2022 03:04




Tgt Ion:113 Resp: 68626


Ion Ratio Lower Upper

113 100

111 102.3 82.6 124.0

192 18.8 17.6 26.4


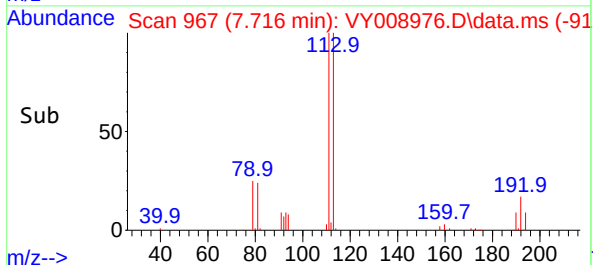
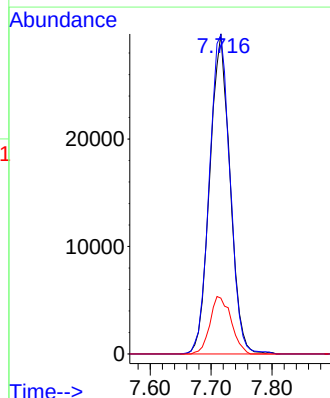
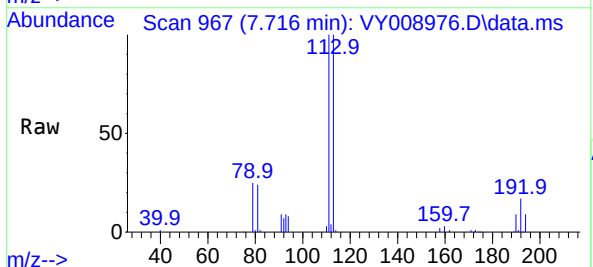


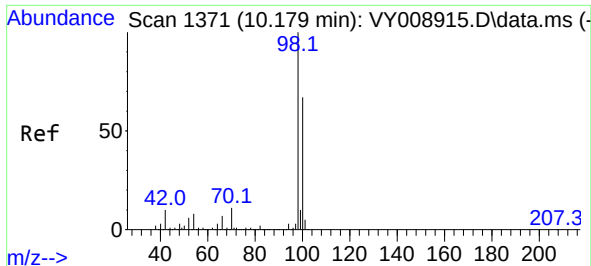

#50
Toluene-d8
Concen: 54.872 ug/l
RT: 10.179 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY008976.D
Acq: 22 May 2022 03:04




Instrument :
MSVOA_Y
ClientSampleId :
P038-SS001-1218-01


Tgt Ion: 98 Resp: 262357
Ion Ratio Lower Upper
98 100
100 63.8 50.2 75.2

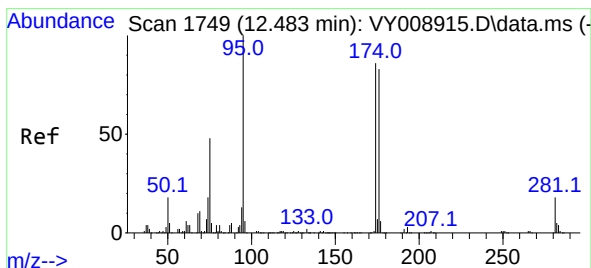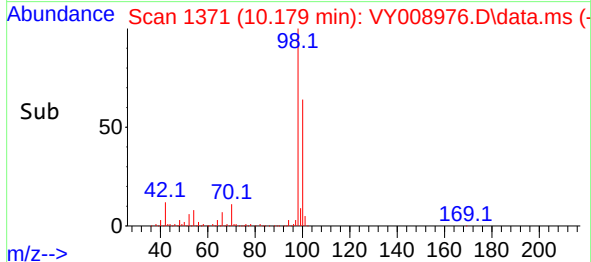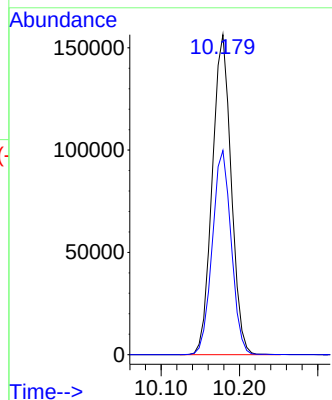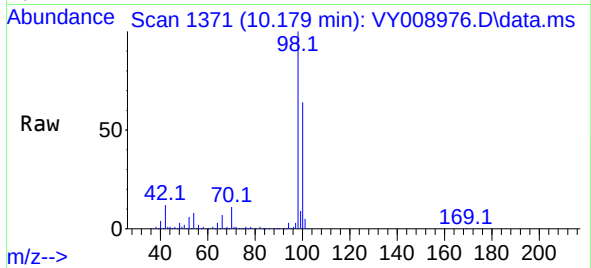

#62
4-Bromofluorobenzene
Concen: 39.803 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.006 min
Lab File: VY008976.D
Acq: 22 May 2022 03:04

Tgt Ion: 95 Resp: 76768
Ion Ratio Lower Upper
95 100
174 91.0 0.0 177.0
176 88.4 0.0 175.8


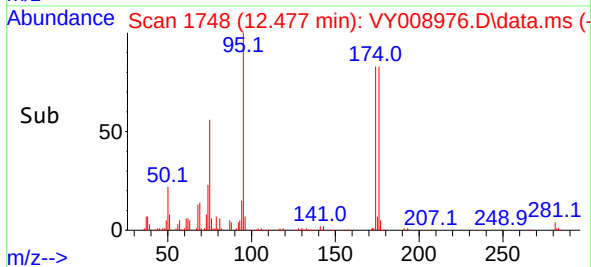
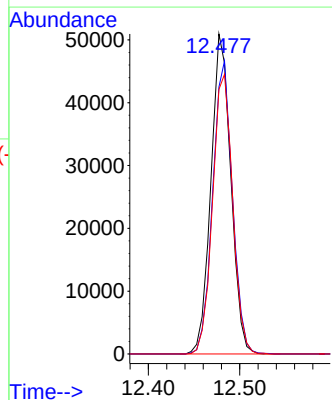
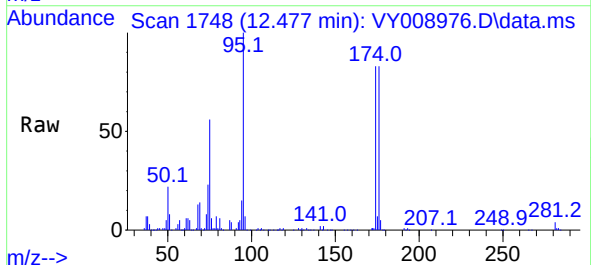


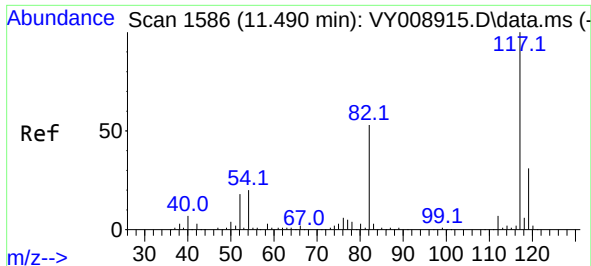

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY008976.D
Acq: 22 May 2022 03:04

Instrument :
MSVOA_Y
ClientSampleId :
P038-SS001-1218-01

Tgt Ion:117 Resp: 200397
Ion Ratio Lower Upper
117 100
82 52.7 43.0 64.4
119 31.6 25.4 38.0

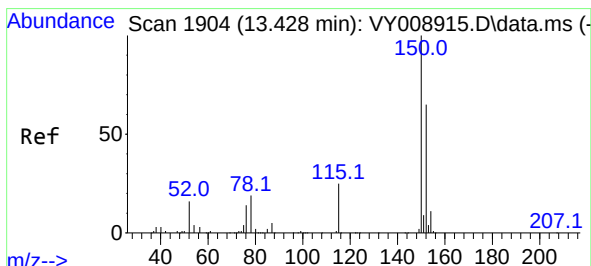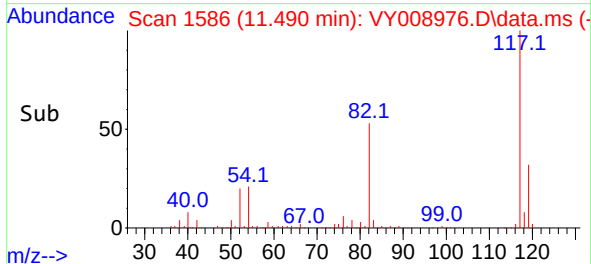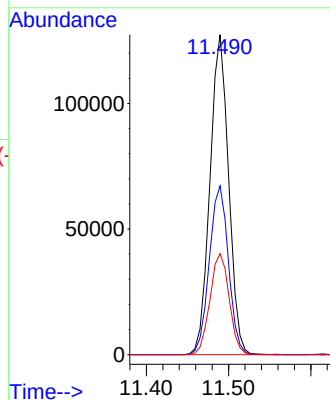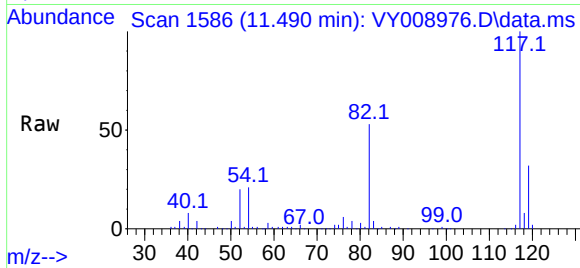

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. -0.006 min
Lab File: VY008976.D
Acq: 22 May 2022 03:04

Tgt Ion:152 Resp: 88515
Ion Ratio Lower Upper
152 100
115 56.9 28.2 84.7
150 158.7 0.0 347.6

