

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052122\
 Data File : VY008979.D
 Acq On : 22 May 2022 04:14
 Operator : KP/MD
 Sample : N2887-12
 Misc : 4.43g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 P039-SS001-0006-01

Quant Time: May 22 04:49:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052022S.M
 Quant Title : SW846 8260
 QLast Update : Fri May 20 23:50:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	116852	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	208521	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	193590	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	77549	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	77171	64.169	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	128.340%
35) Dibromofluoromethane	7.716	113	67890	52.357	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	104.720%
50) Toluene-d8	10.179	98	261090	54.580	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	109.160%
62) 4-Bromofluorobenzene	12.477	95	72234	37.434	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	74.860%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052122\
Data File : VY008979.D
Acq On : 22 May 2022 04:14
Operator : KP/MD
Sample : N2887-12
Misc : 4.43g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
P039-SS001-0006-01

Quant Time: May 22 04:49:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052022S.M
Quant Title : SW846 8260
QLast Update : Fri May 20 23:50:52 2022
Response via : Initial Calibration




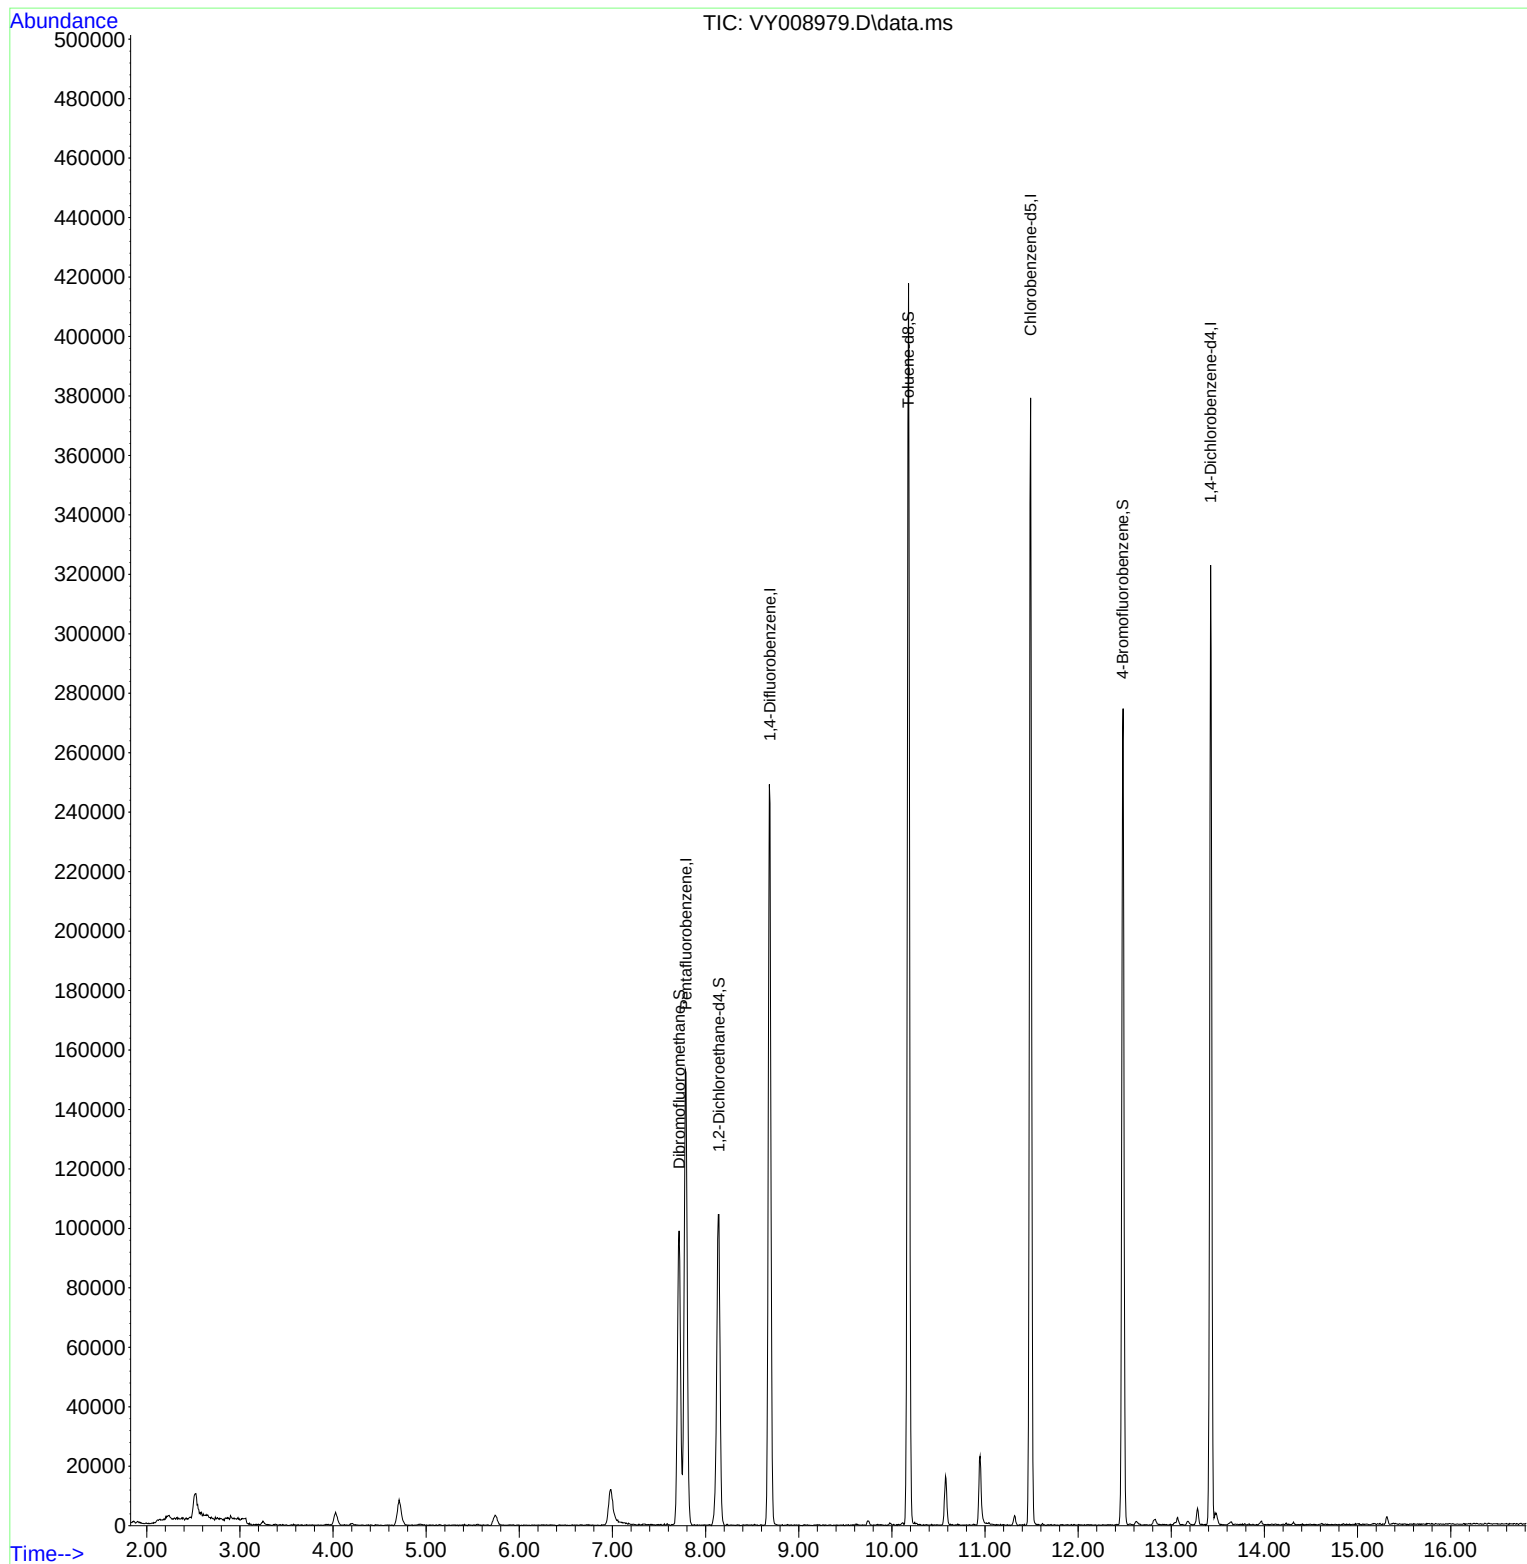


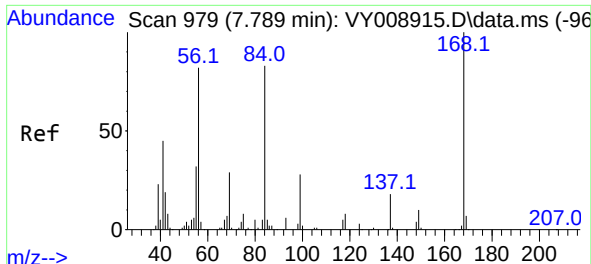

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY008979.D
Acq: 22 May 2022 04:14




Instrument :
MSVOA_Y
ClientSampleId :
P039-SS001-0006-01


Tgt Ion:168 Resp: 116852
Ion Ratio Lower Upper
168 100
99 53.0 46.9 70.3

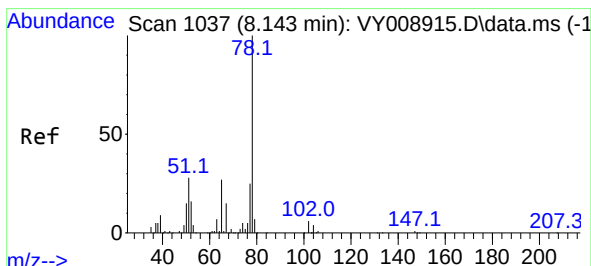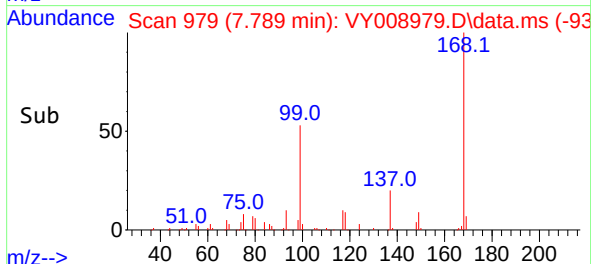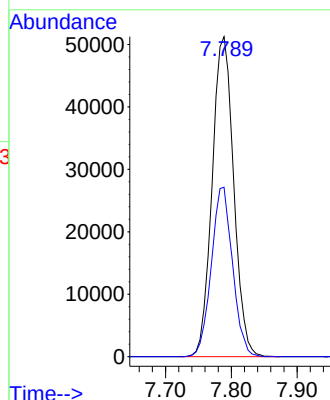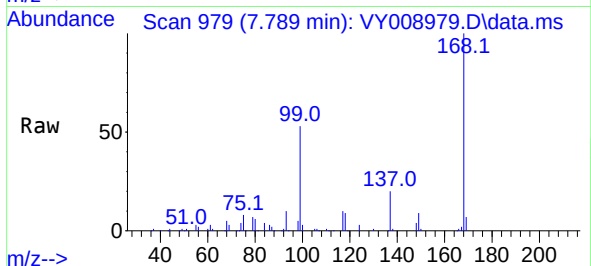

#33
1,2-Dichloroethane-d4
Concen: 64.169 ug/l
RT: 8.142 min Scan# 1037
Delta R.T. -0.001 min
Lab File: VY008979.D
Acq: 22 May 2022 04:14

Tgt Ion: 65 Resp: 77171
Ion Ratio Lower Upper
65 100
67 52.3 0.0 99.4

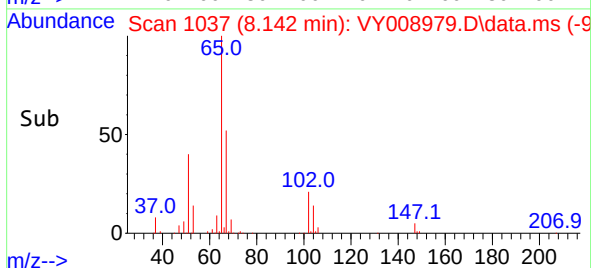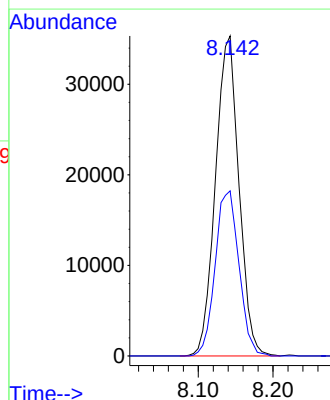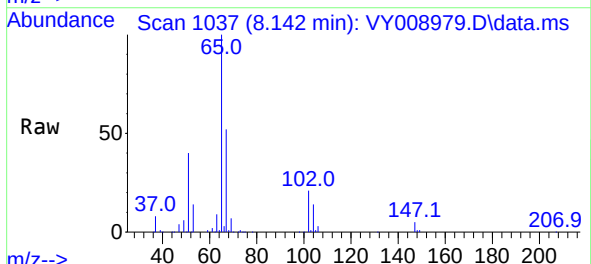

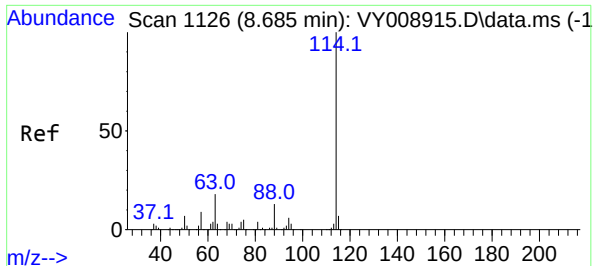

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 11

Delta R.T. 0.006 min

Lab File: VY008979.D

Acq: 22 May 2022 04:14

Instrument :

MSVOA_Y

ClientSampleId :

P039-SS001-0006-01





Tgt Ion:114 Resp: 208521

Ion Ratio Lower Upper

114 100

63 18.0 0.0 43.2

88 13.1 0.0 31.8

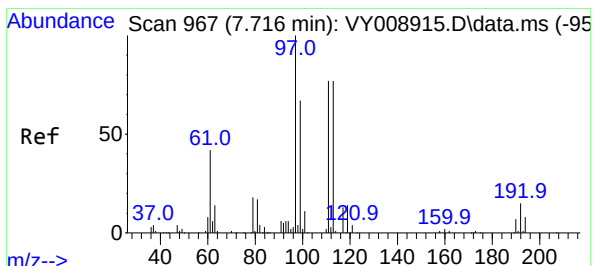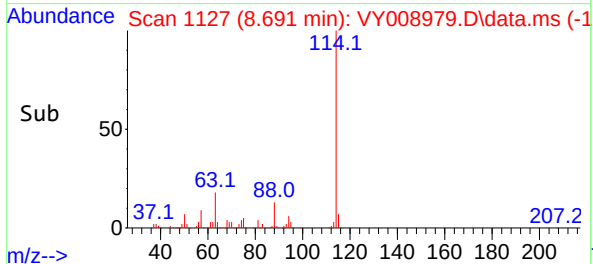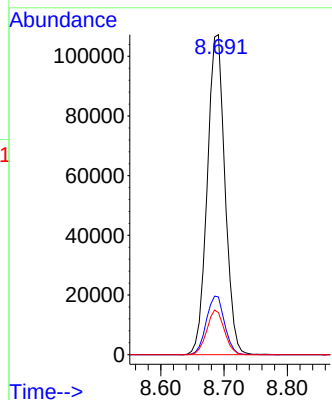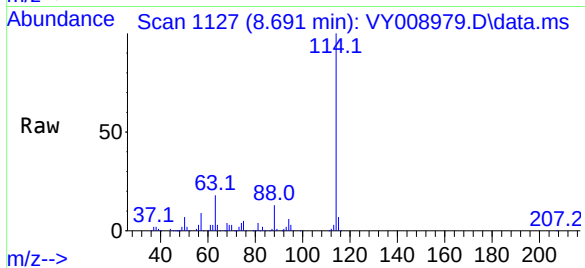

#35

Dibromofluoromethane

Concen: 52.357 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY008979.D

Acq: 22 May 2022 04:14




Tgt Ion:113 Resp: 67890


Ion Ratio Lower Upper

113 100

111 101.8 82.6 124.0

192 18.7 17.6 26.4


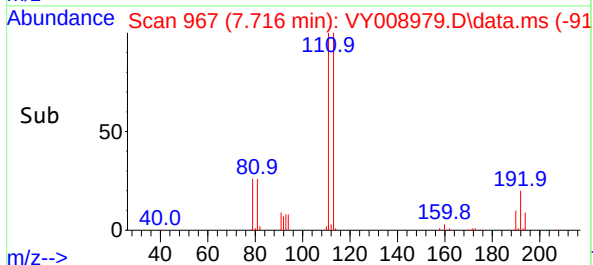
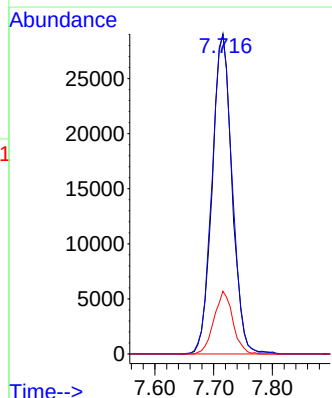
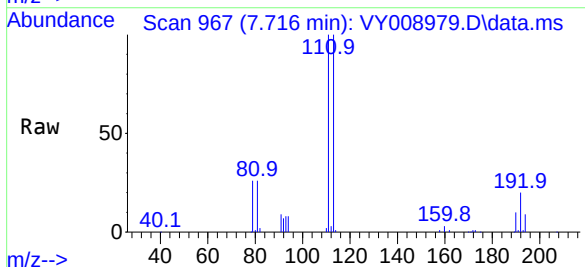


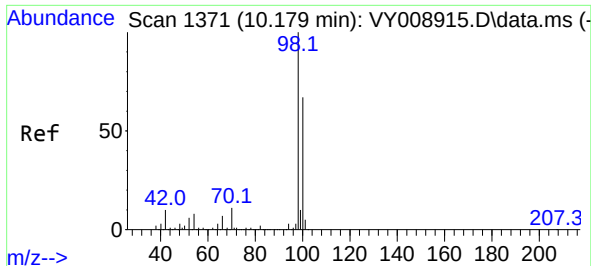

#50
Toluene-d8
Concen: 54.580 ug/l
RT: 10.179 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY008979.D
Acq: 22 May 2022 04:14




Instrument :
MSVOA_Y
ClientSampleId :
P039-SS001-0006-01


Tgt Ion: 98 Resp: 261090
Ion Ratio Lower Upper
98 100
100 64.3 50.2 75.2

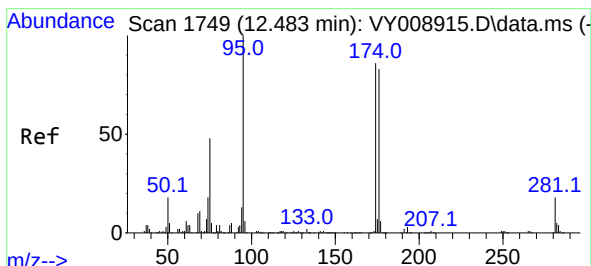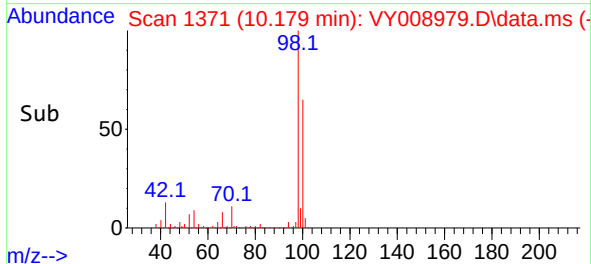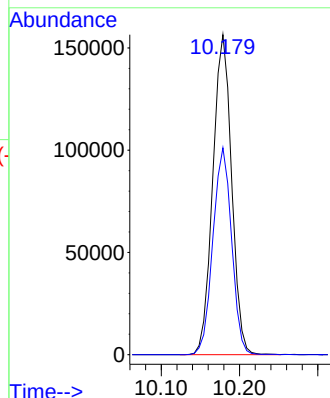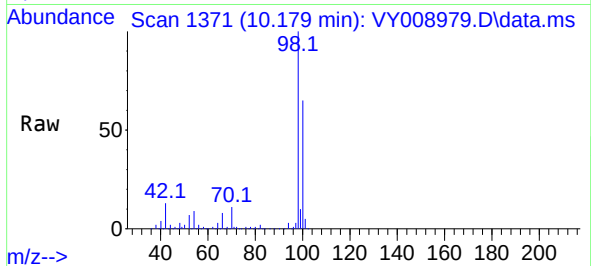

#62
4-Bromofluorobenzene
Concen: 37.434 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.006 min
Lab File: VY008979.D
Acq: 22 May 2022 04:14

Tgt Ion: 95 Resp: 72234
Ion Ratio Lower Upper
95 100
174 92.0 0.0 177.0
176 86.1 0.0 175.8


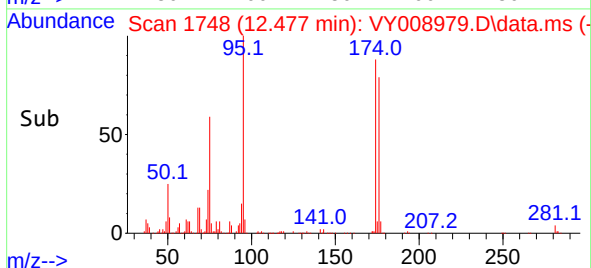
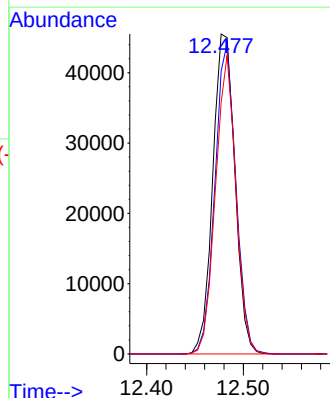
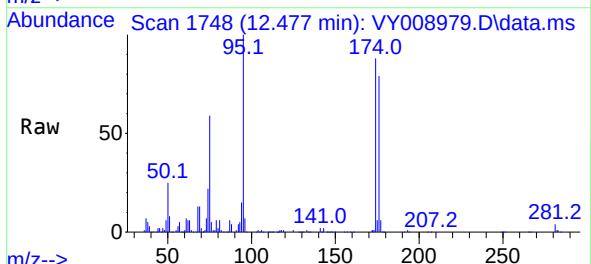


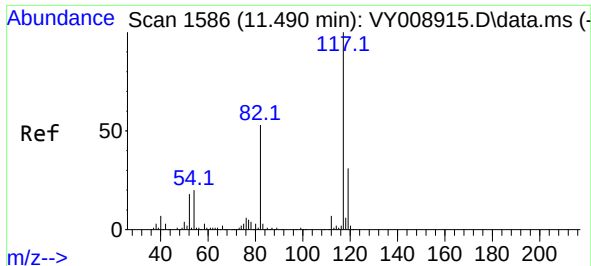

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 117
Delta R.T. -0.001 min
Lab File: VY008979.D
Acq: 22 May 2022 04:14

Instrument :
MSVOA_Y
ClientSampleId :
P039-SS001-0006-01

Tgt Ion:117 Resp: 193590
Ion Ratio Lower Upper
117 100
82 54.1 43.0 64.4
119 33.1 25.4 38.0

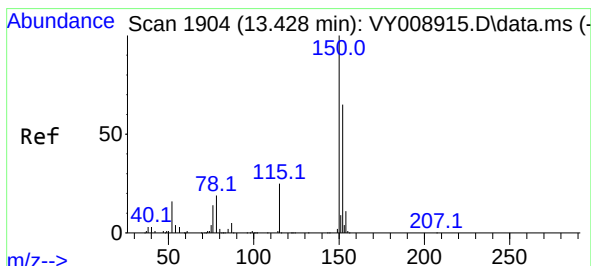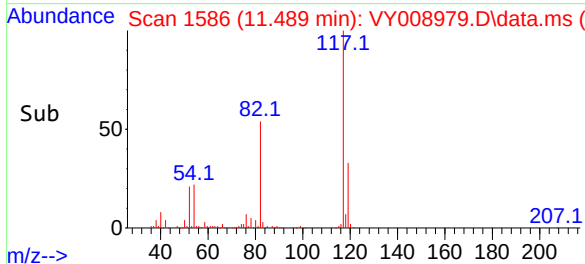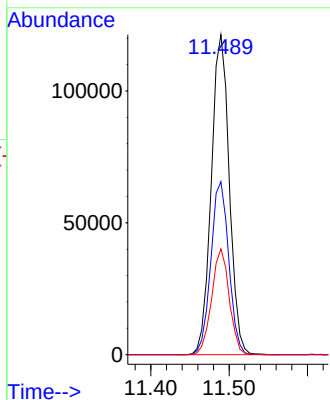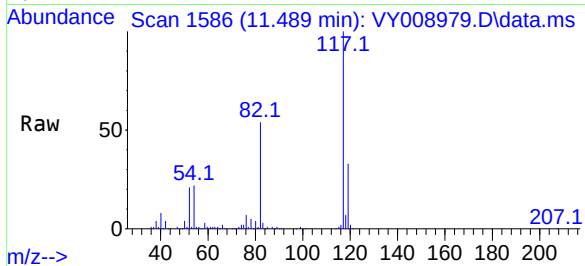

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. -0.006 min
Lab File: VY008979.D
Acq: 22 May 2022 04:14

Tgt Ion:152 Resp: 77549
Ion Ratio Lower Upper
152 100
115 55.0 28.2 84.7
150 157.1 0.0 347.6

