


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052122\
Data File : VY008936.D
Acq On : 21 May 2022 09:24
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052022S.M
Title : SW846 8260
Last Update : Fri May 20 23:50:52 2022

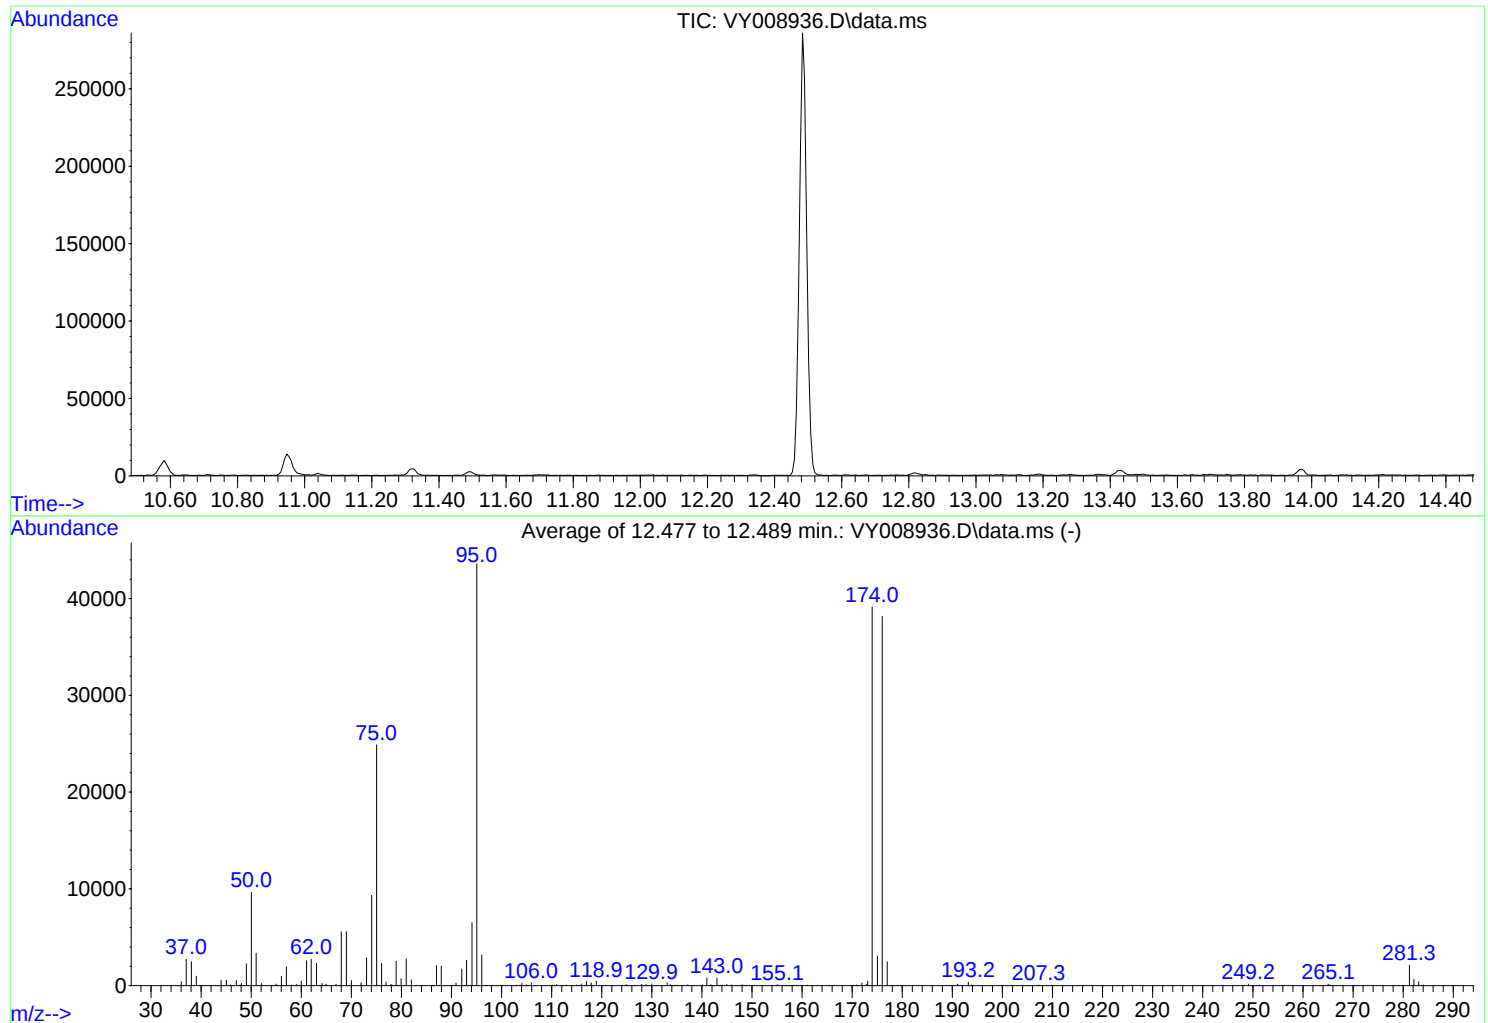

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	9647	PASS
75	95	30	60	57.1	24883	PASS
95	95	100	100	100.0	43589	PASS
96	95	5	9	7.3	3162	PASS
173	174	0.00	2	1.2	465	PASS
174	95	50	100	89.8	39125	PASS
175	174	5	9	7.8	3052	PASS
176	174	95	101	97.6	38187	PASS
177	176	5	9	6.5	2469	PASS