
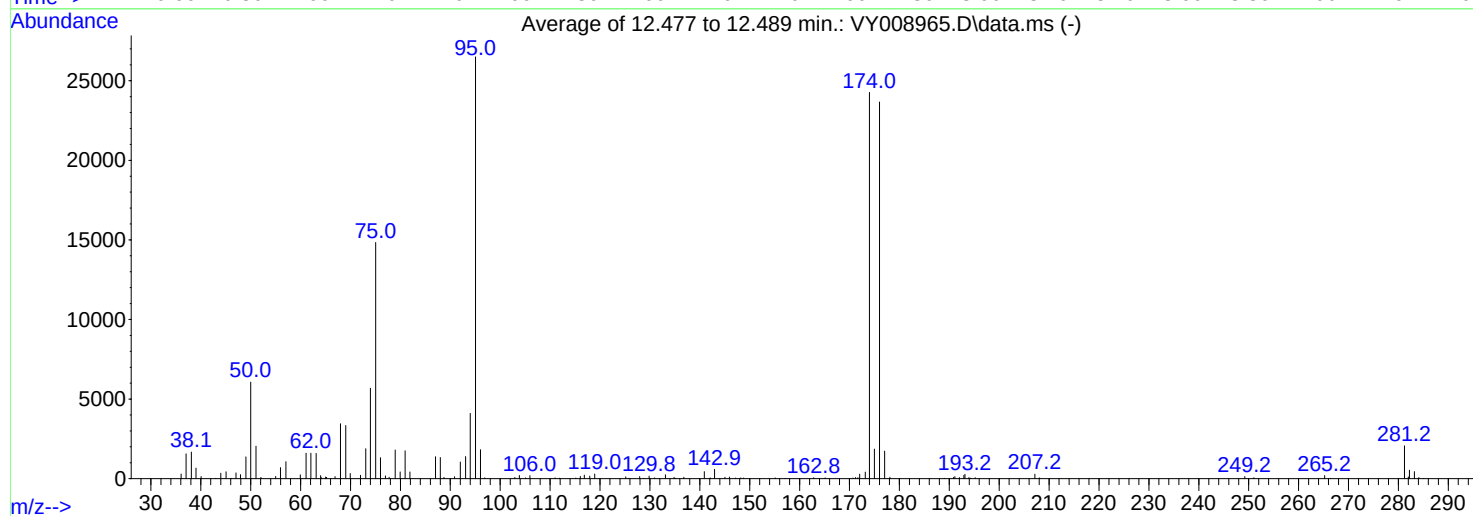


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052122\
 Data File : VY008965.D
 Acq On : 21 May 2022 22:15
 Operator : KP/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052022S.M
 Title : SW846 8260
 Last Update : Fri May 20 23:50:52 2022

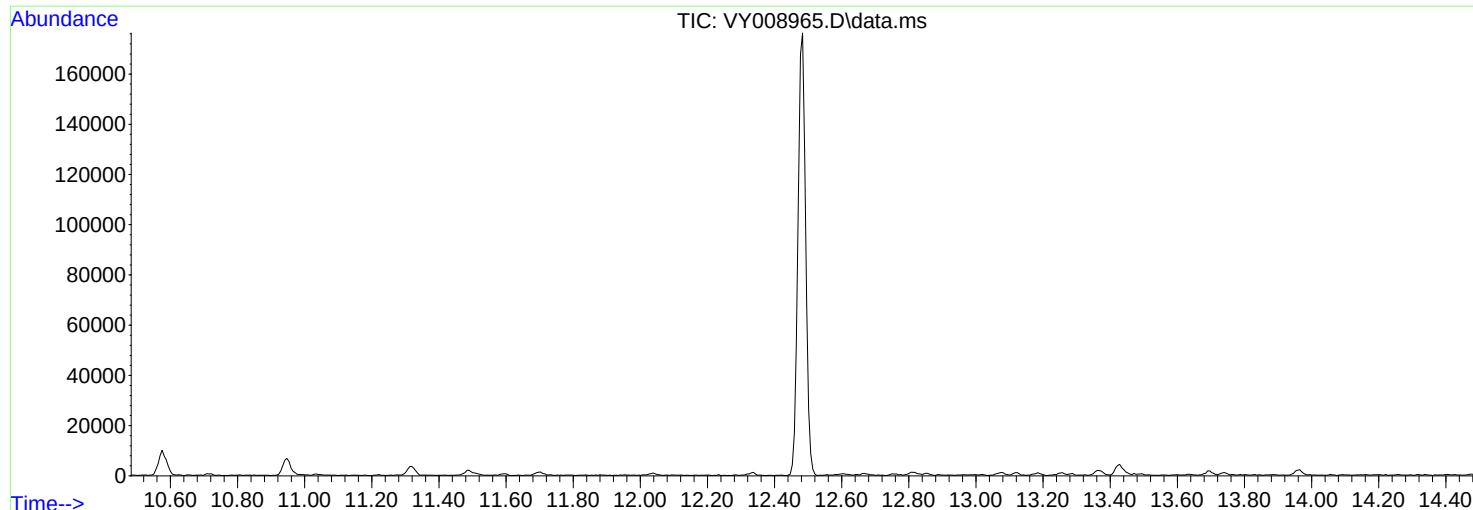

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	6066	PASS
75	95	30	60	56.0	14837	PASS
95	95	100	100	100.0	26501	PASS
96	95	5	9	6.9	1824	PASS
173	174	0.00	2	1.7	417	PASS
174	95	50	100	91.6	24267	PASS
175	174	5	9	7.7	1858	PASS
176	174	95	101	97.5	23661	PASS
177	176	5	9	7.3	1725	PASS