

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY052322\  
 Data File : VY009041.D  
 Acq On : 24 May 2022 05:31  
 Operator : KP/MD  
 Sample : N2948-27  
 Misc : 5.73g/5.0mL/MSVOA\_Y/SOIL  
 ALS Vial : 50 Sample Multiplier: 1

Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 P037-SS001-1218-02

Quant Time: May 24 07:49:08 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y052022S.M  
 Quant Title : SW846 8260  
 QLast Update : Fri May 20 23:50:52 2022  
 Response via : Initial Calibration

| Compound                   | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|----------------------------|--------|------|----------|--------|-------|----------|
| -----                      |        |      |          |        |       |          |
| Internal Standards         |        |      |          |        |       |          |
| 1) Pentafluorobenzene      | 7.789  | 168  | 110304   | 50.000 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 8.691  | 114  | 202870   | 50.000 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 11.490 | 117  | 190989   | 50.000 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 13.428 | 152  | 84986    | 50.000 | ug/l  | 0.00     |

|                             |        |       |          |          |      |          |
|-----------------------------|--------|-------|----------|----------|------|----------|
| System Monitoring Compounds |        |       |          |          |      |          |
| 33) 1,2-Dichloroethane-d4   | 8.143  | 65    | 71386    | 62.882   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 50 - 163 | Recovery | =    | 125.760% |
| 35) Dibromofluoromethane    | 7.716  | 113   | 64608    | 51.214   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 54 - 147 | Recovery | =    | 102.420% |
| 50) Toluene-d8              | 10.179 | 98    | 255384   | 54.874   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 49 - 140 | Recovery | =    | 109.740% |
| 62) 4-Bromofluorobenzene    | 12.477 | 95    | 73883    | 39.355   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 25 - 144 | Recovery | =    | 78.700%  |


| Target Compounds | Qvalue |
|------------------|--------|
| -----            |        |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY052322\  
Data File : VY009041.D  
Acq On : 24 May 2022 05:31  
Operator : KP/MD  
Sample : N2948-27  
Misc : 5.73g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 50 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
P037-SS001-1218-02

Quant Time: May 24 07:49:08 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y052022S.M  
Quant Title : SW846 8260  
QLast Update : Fri May 20 23:50:52 2022  
Response via : Initial Calibration



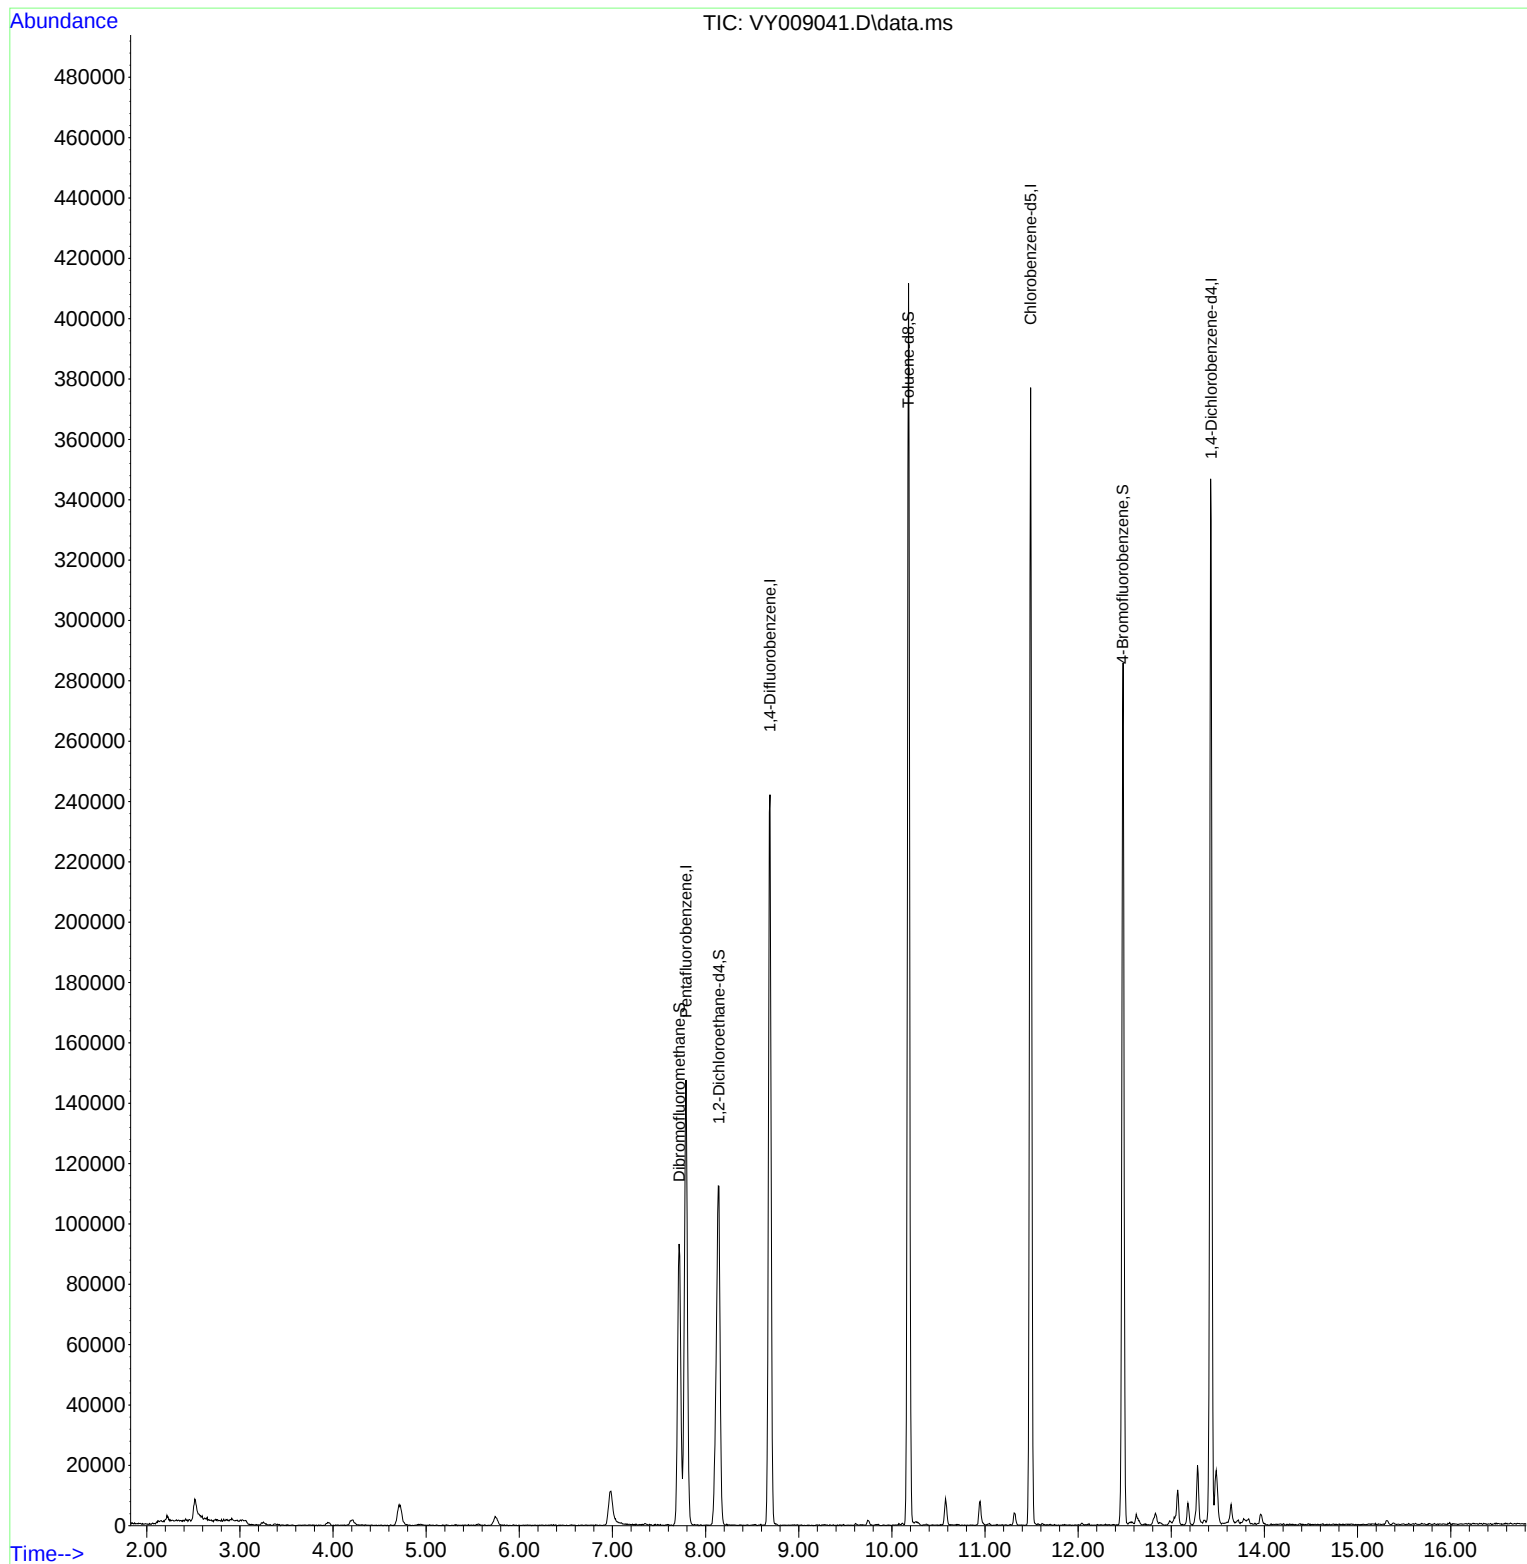


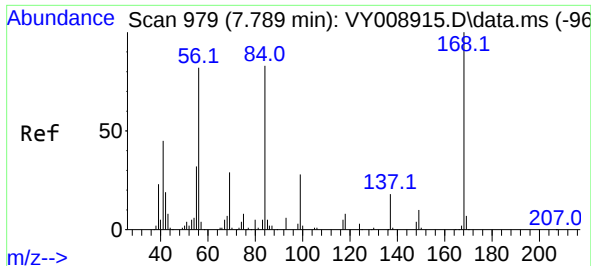

#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 7.789 min Scan# 91  
Delta R.T. -0.000 min  
Lab File: VY009041.D  
Acq: 24 May 2022 05:31




Instrument :  
MSVOA\_Y  
ClientSampleId :  
P037-SS001-1218-02


Tgt Ion:168 Resp: 110304  
Ion Ratio Lower Upper  
168 100  
99 52.9 46.9 70.3

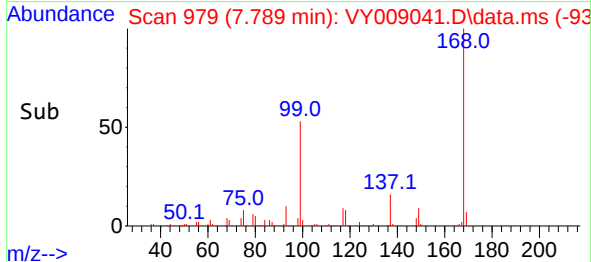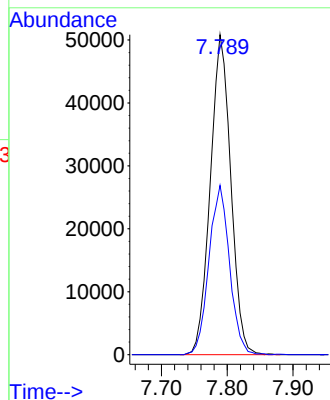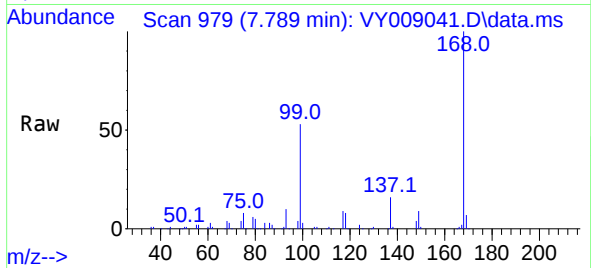

#33  
1,2-Dichloroethane-d4  
Concen: 62.882 ug/l  
RT: 8.143 min Scan# 1037  
Delta R.T. -0.000 min  
Lab File: VY009041.D  
Acq: 24 May 2022 05:31

Tgt Ion: 65 Resp: 71386  
Ion Ratio Lower Upper  
65 100  
67 53.9 0.0 99.4

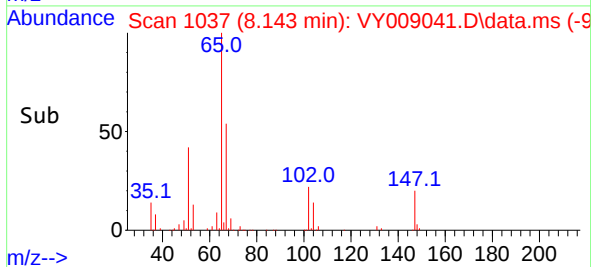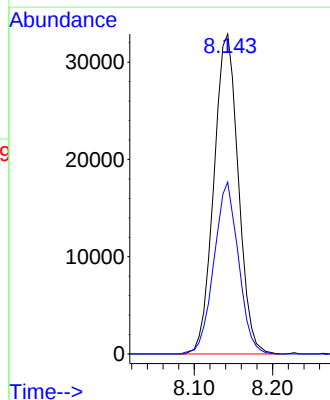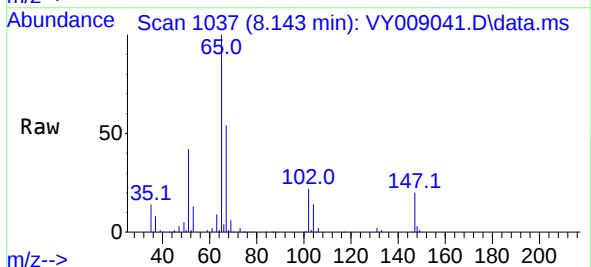

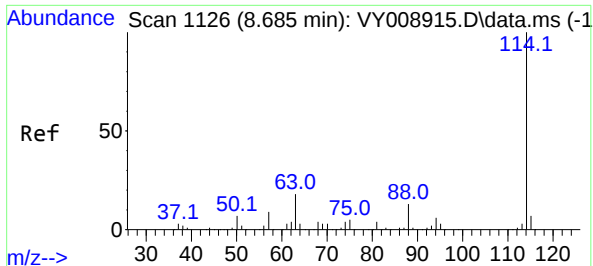

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 11

Delta R.T. 0.006 min

Lab File: VY009041.D

Acq: 24 May 2022 05:31

Instrument :

MSVOA\_Y

ClientSampleId :

P037-SS001-1218-02





Tgt Ion:114 Resp: 202870

Ion Ratio Lower Upper

114 100

63 18.1 0.0 43.2

88 13.5 0.0 31.8

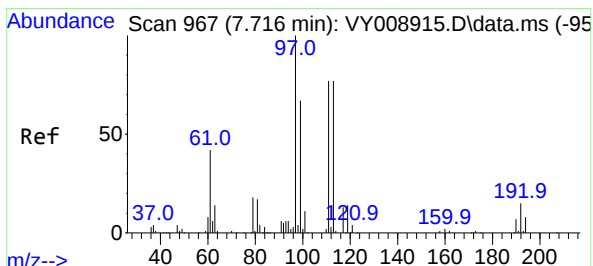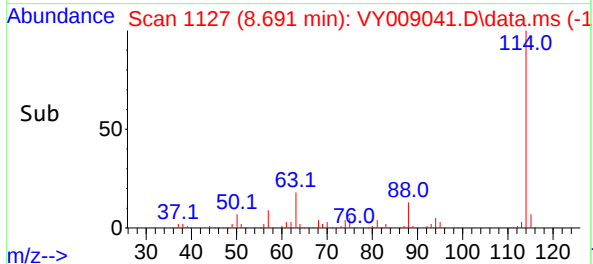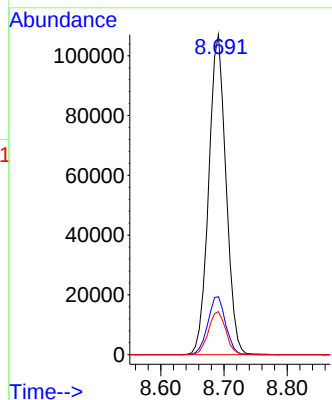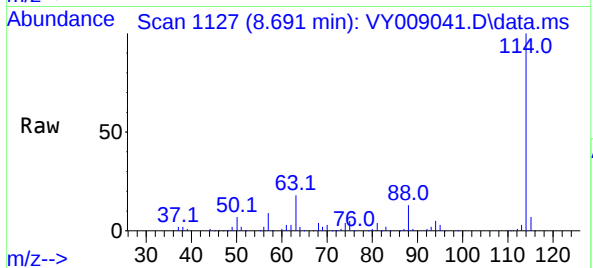

#35

Dibromofluoromethane

Concen: 51.214 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY009041.D

Acq: 24 May 2022 05:31




Tgt Ion:113 Resp: 64608


Ion Ratio Lower Upper

113 100

111 103.0 82.6 124.0

192 19.1 17.6 26.4


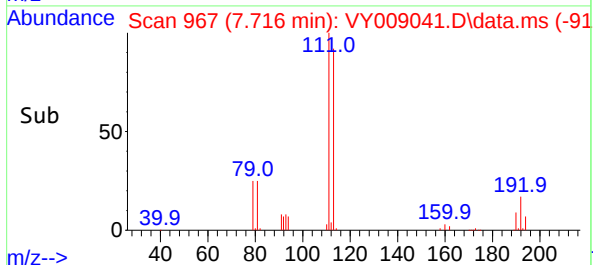
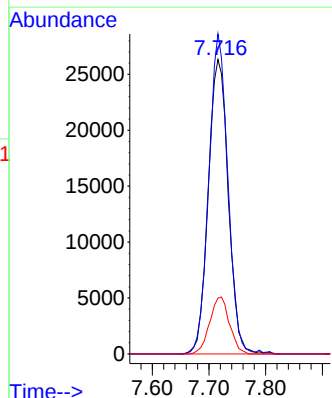
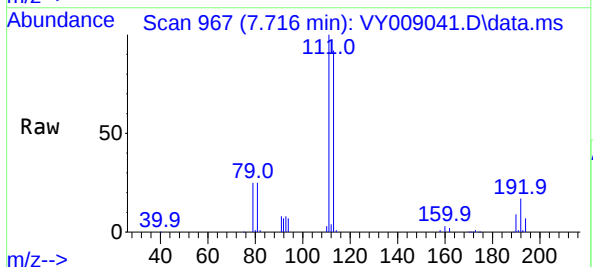


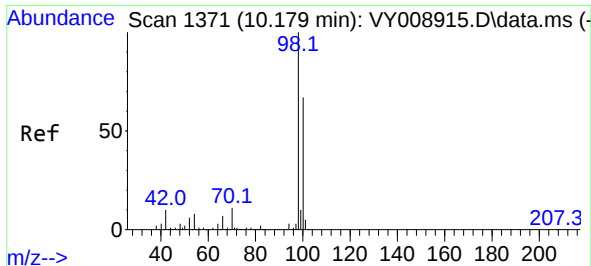

#50  
Toluene-d8  
Concen: 54.874 ug/l  
RT: 10.179 min Scan# 11  
Delta R.T. -0.000 min  
Lab File: VY009041.D  
Acq: 24 May 2022 05:31




Instrument :  
MSVOA\_Y  
ClientSampleId :  
P037-SS001-1218-02


Tgt Ion: 98 Resp: 255384  
Ion Ratio Lower Upper  
98 100  
100 63.7 50.2 75.2

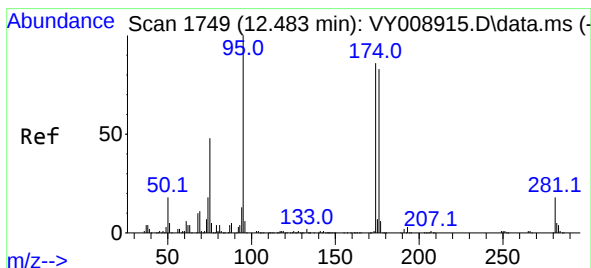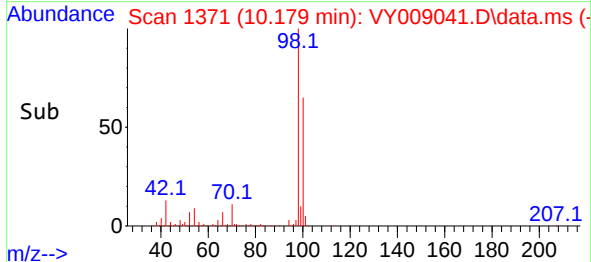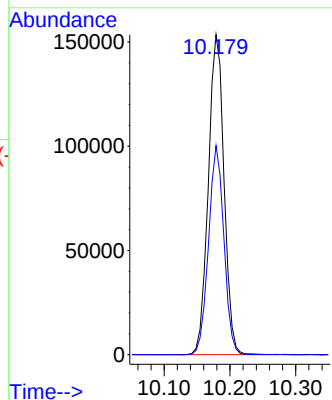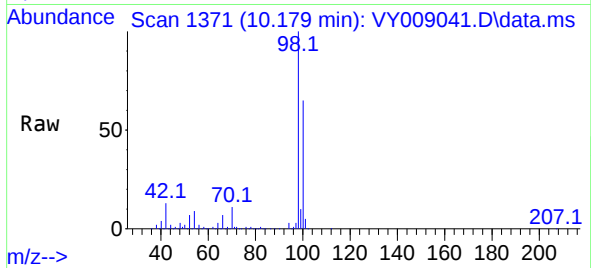

#62  
4-Bromofluorobenzene  
Concen: 39.355 ug/l  
RT: 12.477 min Scan# 1748  
Delta R.T. -0.006 min  
Lab File: VY009041.D  
Acq: 24 May 2022 05:31

Tgt Ion: 95 Resp: 73883  
Ion Ratio Lower Upper  
95 100  
174 90.6 0.0 177.0  
176 87.9 0.0 175.8


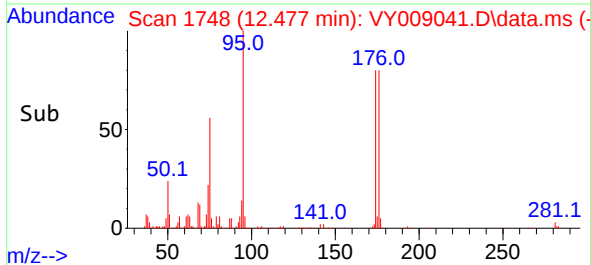
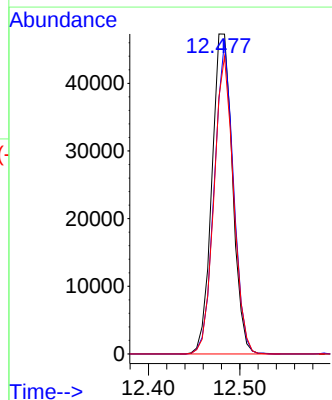
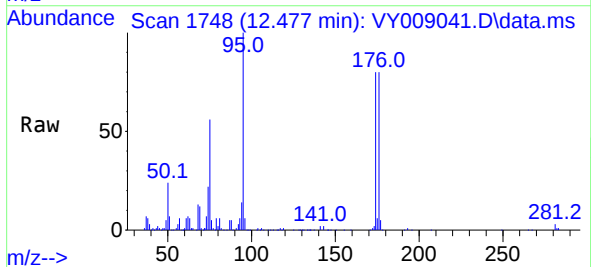


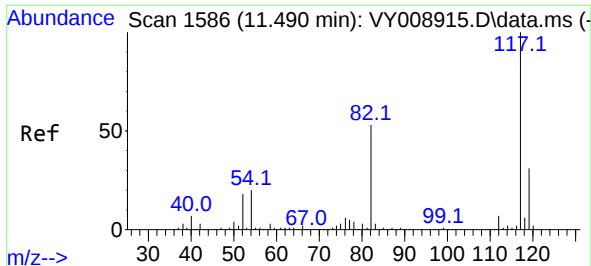

#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.490 min Scan# 11  
Delta R.T. -0.001 min  
Lab File: VY009041.D  
Acq: 24 May 2022 05:31

Instrument :  
MSVOA\_Y  
ClientSampleId :  
P037-SS001-1218-02

Tgt Ion:117 Resp: 190989  
Ion Ratio Lower Upper  
117 100  
82 52.5 43.0 64.4  
119 31.4 25.4 38.0

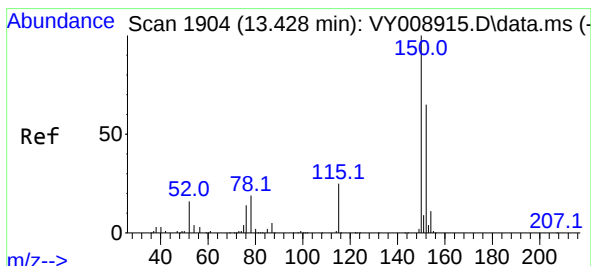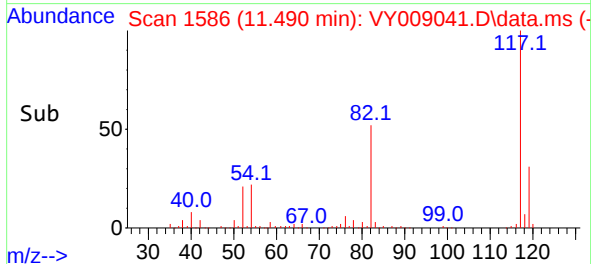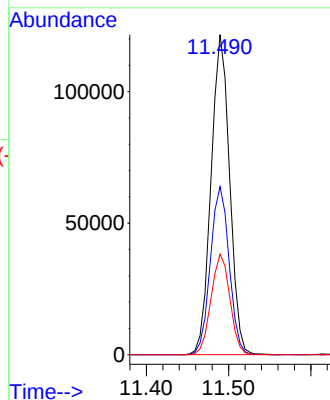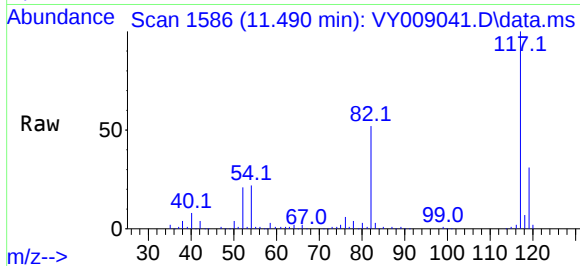

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 13.428 min Scan# 1904  
Delta R.T. 0.000 min  
Lab File: VY009041.D  
Acq: 24 May 2022 05:31

Tgt Ion:152 Resp: 84986  
Ion Ratio Lower Upper  
152 100  
115 55.3 28.2 84.7  
150 158.2 0.0 347.6

