
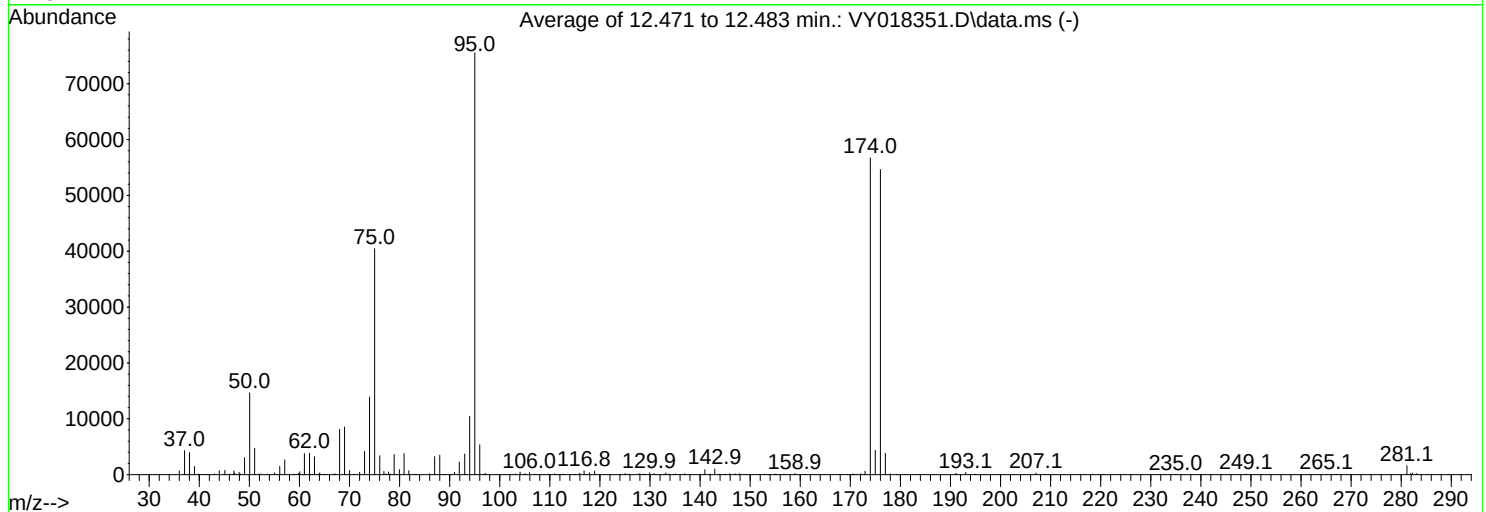


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052324\
Data File : VY018351.D
Acq On : 23 May 2024 08:40
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052224S.M
Title : SW846 8260
Last Update : Thu May 23 01:40:36 2024

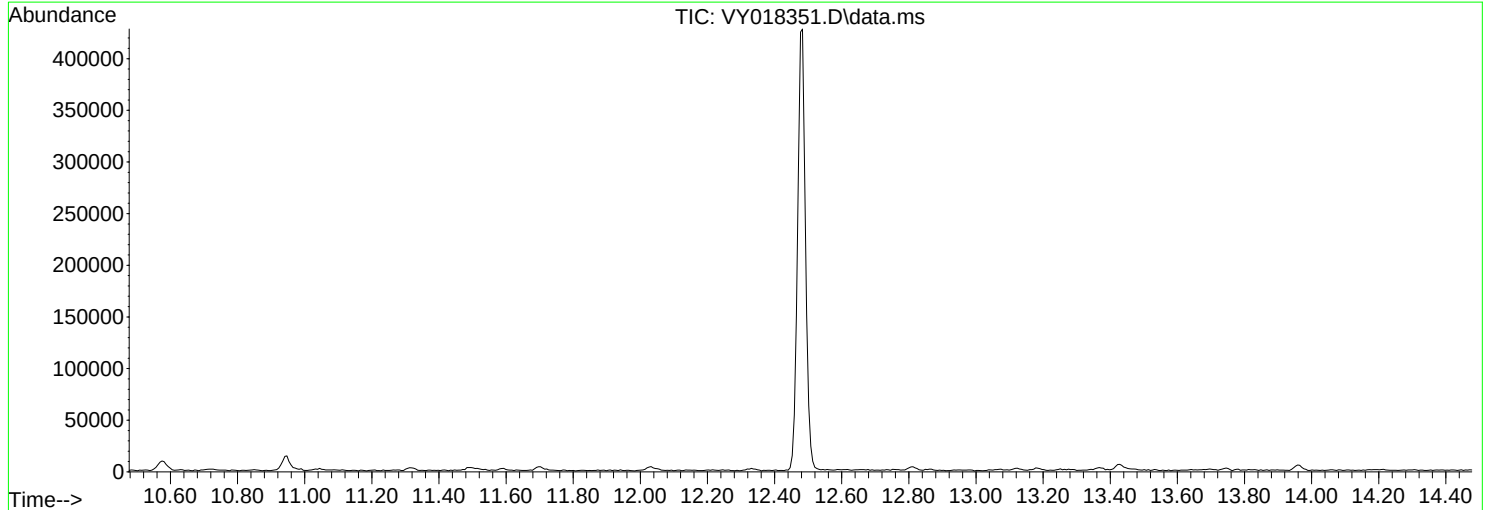

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1739

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.4	14649	PASS
75	95	30	60	53.6	40480	PASS
95	95	100	100	100.0	75525	PASS
96	95	5	9	7.1	5352	PASS
173	174	0.00	2	1.1	604	PASS
174	95	50	100	75.1	56736	PASS
175	174	5	9	7.7	4353	PASS
176	174	95	101	96.3	54640	PASS
177	176	5	9	7.0	3805	PASS