
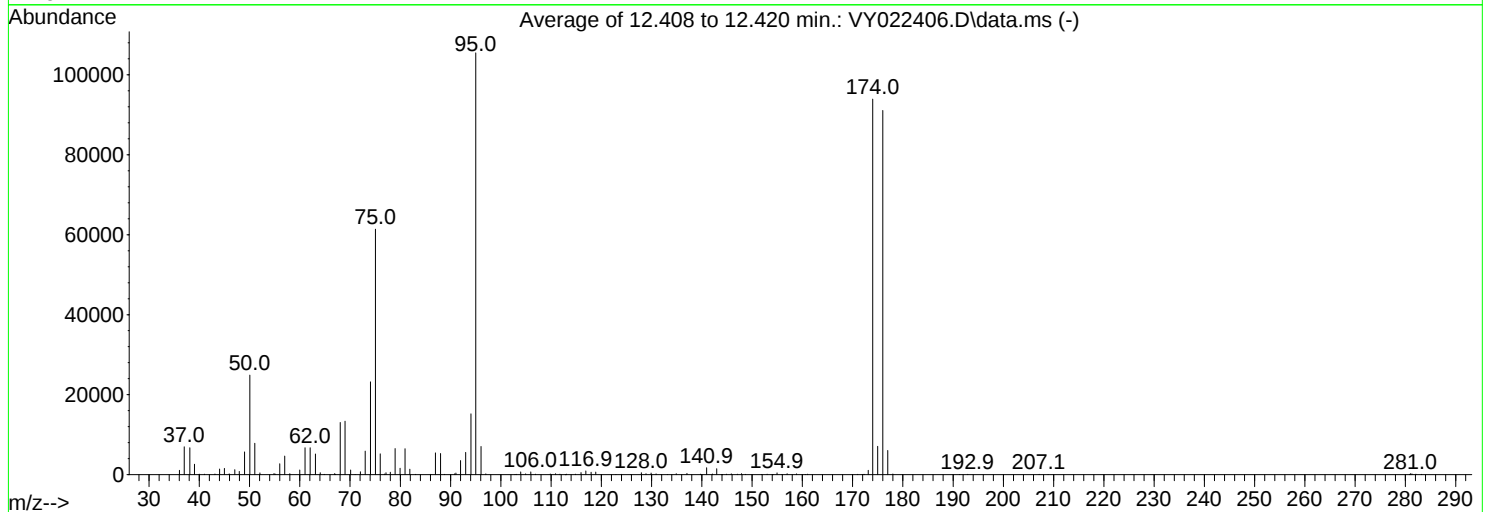


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052325\
Data File : VY022406.D
Acq On : 23 May 2025 11:40
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051525S.M
Title : SW846 8260
Last Update : Fri May 16 01:42:09 2025

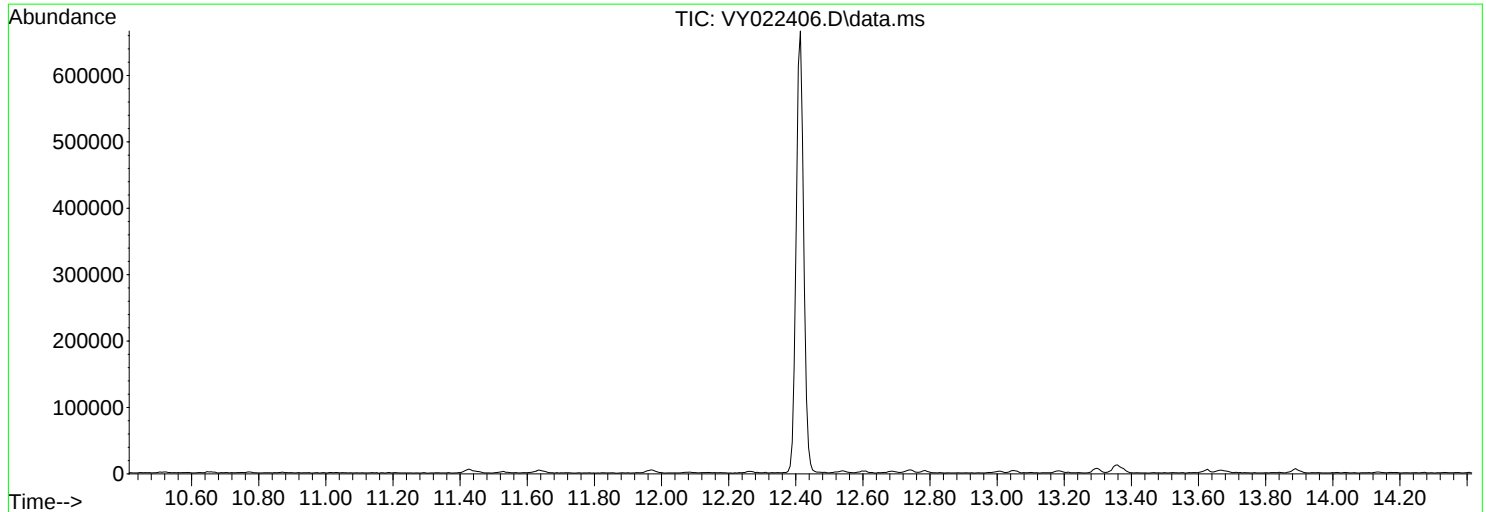

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.6	24907	PASS
75	95	30	60	58.2	61381	PASS
95	95	100	100	100.0	105501	PASS
96	95	5	9	6.7	7047	PASS
173	174	0.00	2	1.2	1085	PASS
174	95	50	100	89.0	93931	PASS
175	174	5	9	7.6	7094	PASS
176	174	95	101	97.0	91072	PASS
177	176	5	9	6.6	6044	PASS