

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052422\
 Data File : VY009050.D
 Acq On : 24 May 2022 10:23
 Operator : KP/MD
 Sample : VY0524SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0524SBL01

Quant Time: May 25 02:49:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052022S.M
 Quant Title : SW846 8260
 QLast Update : Fri May 20 23:50:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	121491	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	218885	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	201840	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	86969	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.137	65	76674	61.321	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	122.640%
35) Dibromofluoromethane	7.716	113	70064	51.475	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	102.960%
50) Toluene-d8	10.179	98	274481	54.663	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	109.320%
62) 4-Bromofluorobenzene	12.483	95	74704	36.881	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	73.760%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052422\
Data File : VY009050.D
Acq On : 24 May 2022 10:23
Operator : KP/MD
Sample : VY0524SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0524SBL01

Quant Time: May 25 02:49:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052022S.M
Quant Title : SW846 8260
QLast Update : Fri May 20 23:50:52 2022
Response via : Initial Calibration




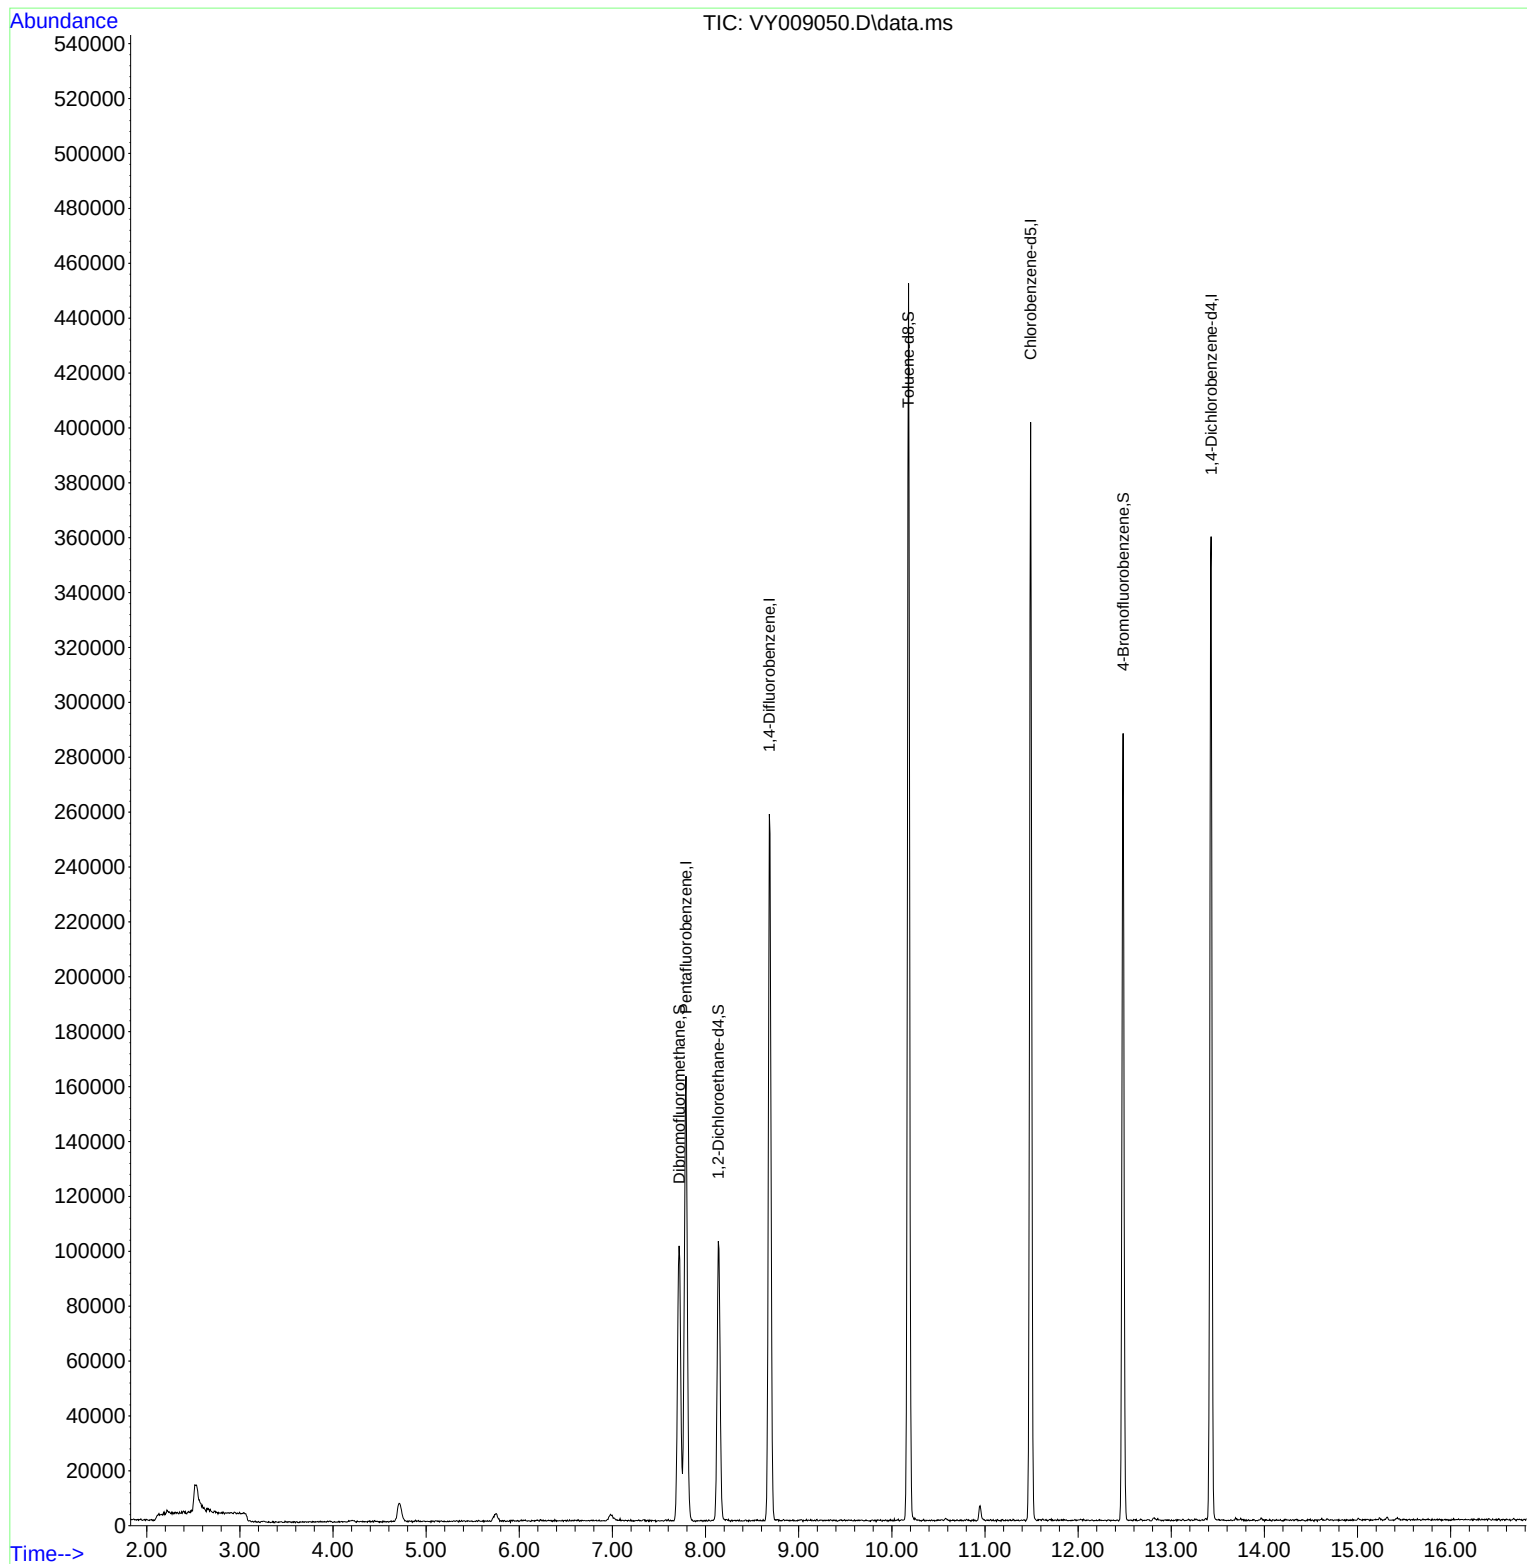


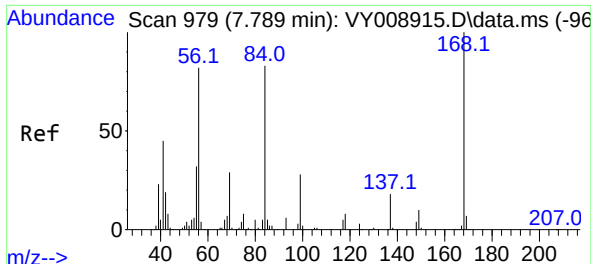

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY009050.D
Acq: 24 May 2022 10:23




Instrument :
MSVOA_Y
ClientSampleId :
VY0524SBL01


Tgt Ion:168 Resp: 121491
Ion Ratio Lower Upper
168 100
99 52.9 46.9 70.3

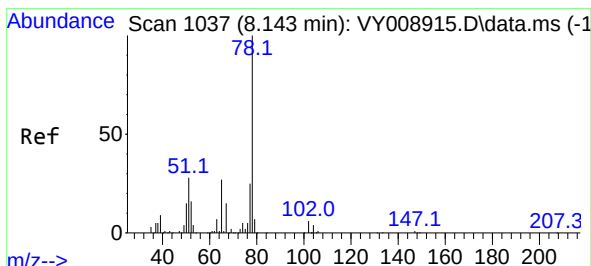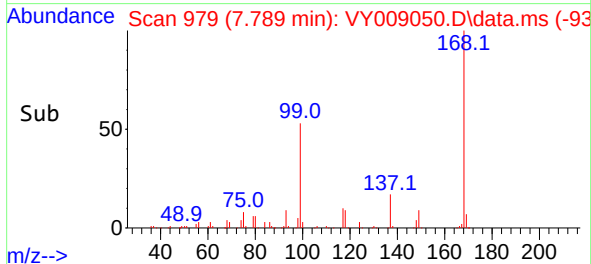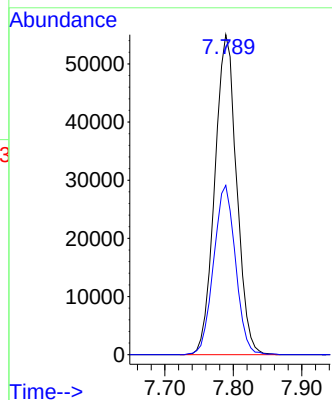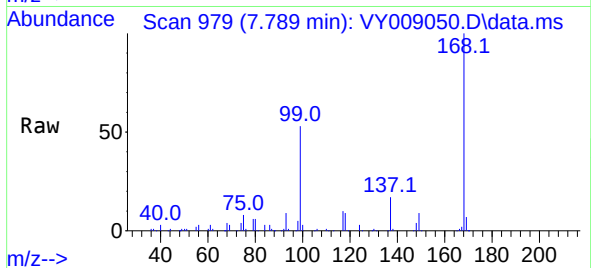

#33
1,2-Dichloroethane-d4
Concen: 61.321 ug/l
RT: 8.137 min Scan# 1036
Delta R.T. -0.006 min
Lab File: VY009050.D
Acq: 24 May 2022 10:23

Tgt Ion: 65 Resp: 76674
Ion Ratio Lower Upper
65 100
67 52.4 0.0 99.4

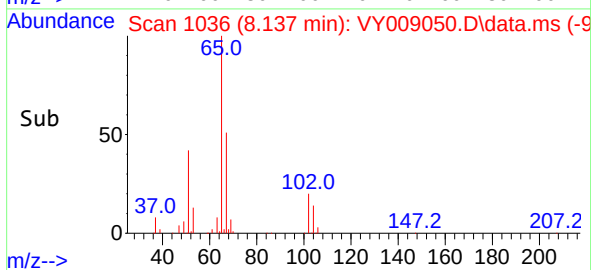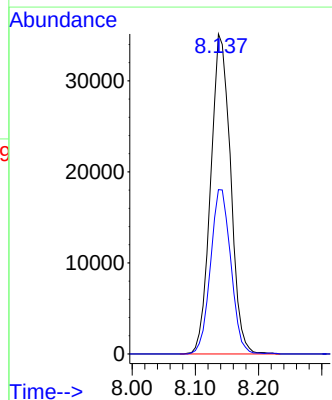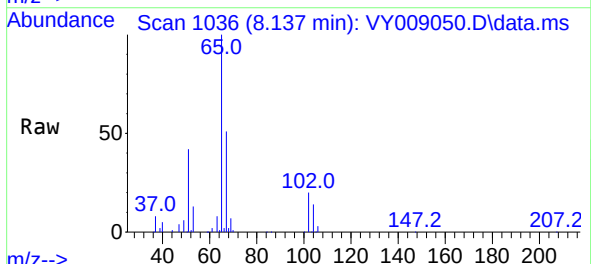

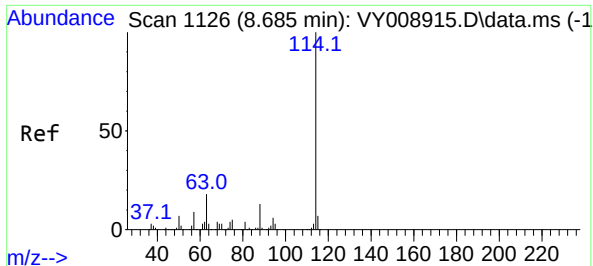

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. 0.000 min

Lab File: VY009050.D

Acq: 24 May 2022 10:23

Instrument :

MSVOA_Y

ClientSampleId :

VY0524SBL01





Tgt Ion:114 Resp: 218885

Ion Ratio Lower Upper

114 100

63 20.4 0.0 43.2

88 13.1 0.0 31.8

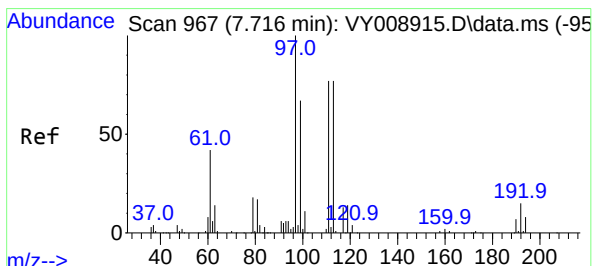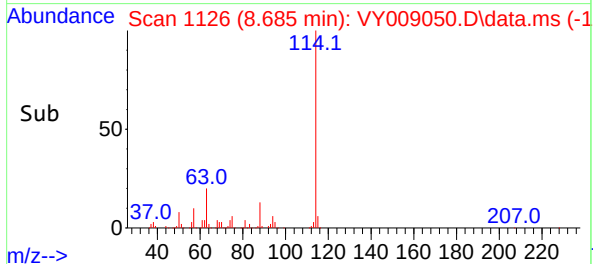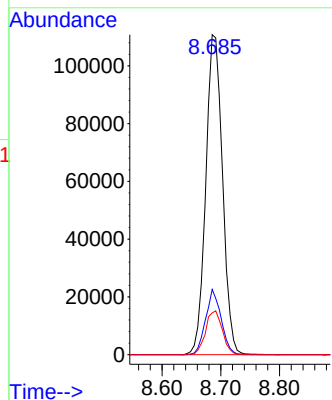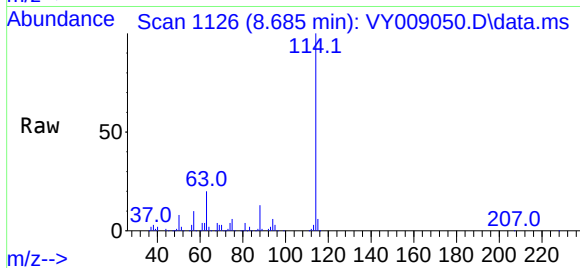

#35

Dibromofluoromethane

Concen: 51.475 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY009050.D

Acq: 24 May 2022 10:23




Tgt Ion:113 Resp: 70064


Ion Ratio Lower Upper

113 100

111 101.7 82.6 124.0

192 18.5 17.6 26.4


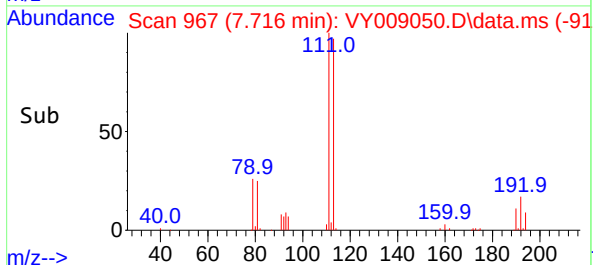
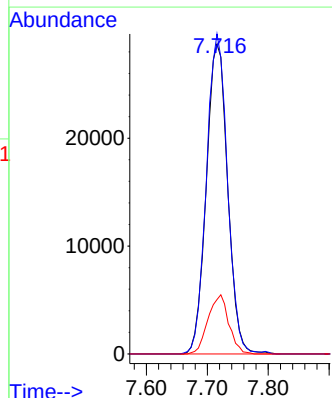
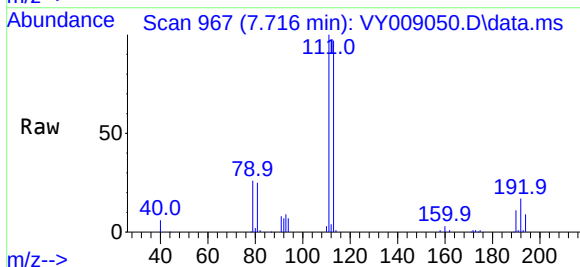


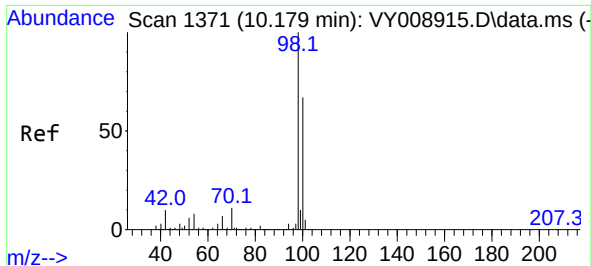

#50
Toluene-d8
Concen: 54.663 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY009050.D
Acq: 24 May 2022 10:23




Instrument :
MSVOA_Y
ClientSampleId :
VY0524SBL01


Tgt Ion: 98 Resp: 274481
Ion Ratio Lower Upper
98 100
100 64.7 50.2 75.2

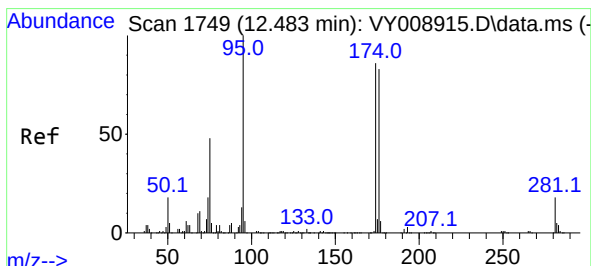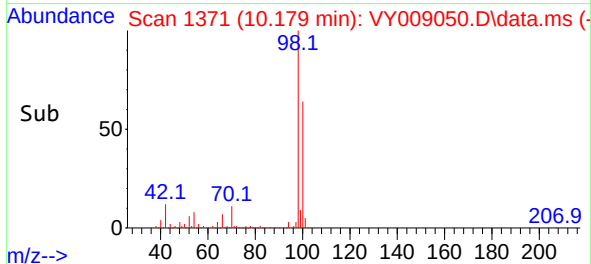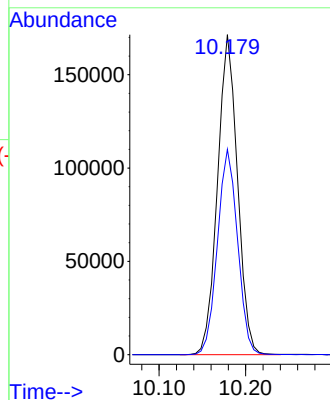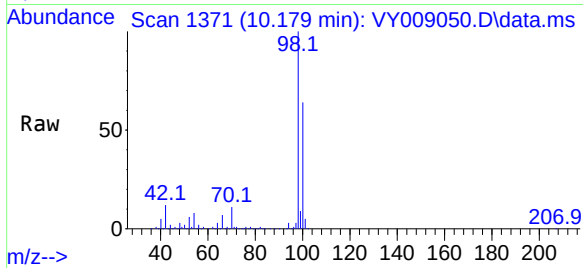

#62
4-Bromofluorobenzene
Concen: 36.881 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY009050.D
Acq: 24 May 2022 10:23

Tgt Ion: 95 Resp: 74704
Ion Ratio Lower Upper
95 100
174 92.4 0.0 177.0
176 88.5 0.0 175.8


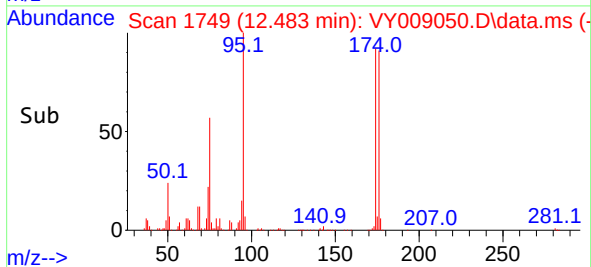
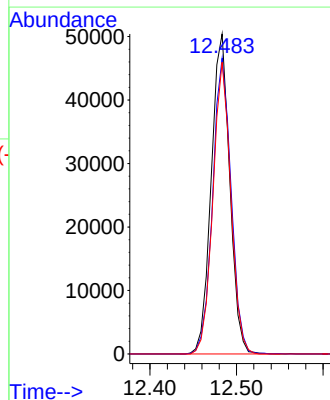
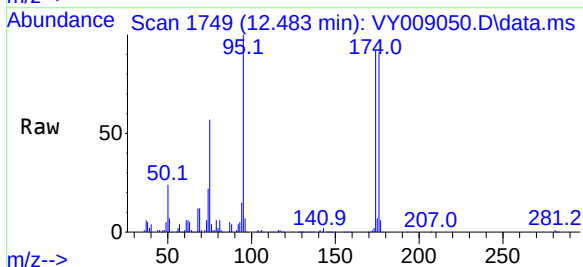


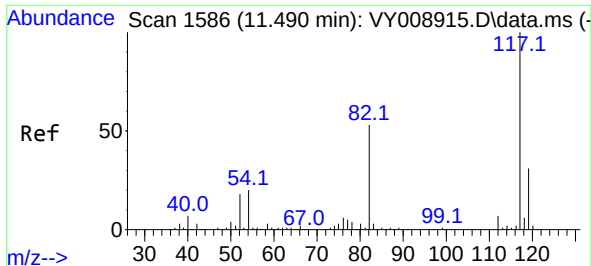

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 117
Delta R.T. -0.000 min
Lab File: VY009050.D
Acq: 24 May 2022 10:23

Instrument :
MSVOA_Y
ClientSampleId :
VY0524SBL01

Tgt Ion:117 Resp: 201840
Ion Ratio Lower Upper
117 100
82 53.3 43.0 64.4
119 31.7 25.4 38.0

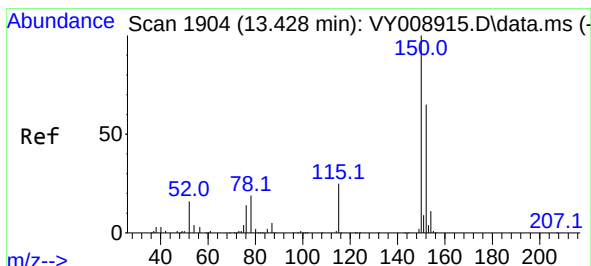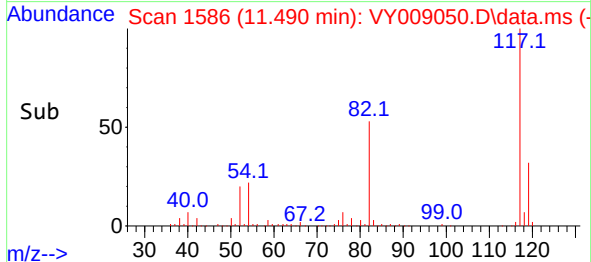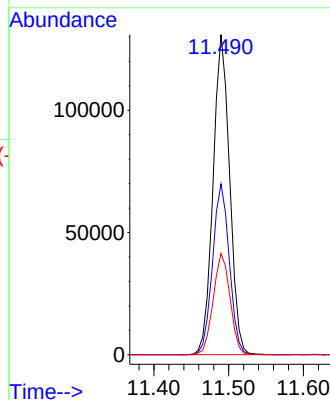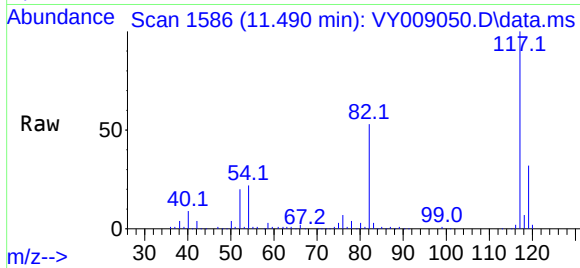

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY009050.D
Acq: 24 May 2022 10:23

Tgt Ion:152 Resp: 86969
Ion Ratio Lower Upper
152 100
115 56.1 28.2 84.7
150 157.2 0.0 347.6

