

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052422\
 Data File : VY009072.D
 Acq On : 24 May 2022 19:13
 Operator : KP/MD
 Sample : N2981-05
 Misc : 2.29g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-14(0.5-1)

Quant Time: May 25 02:56:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052022S.M
 Quant Title : SW846 8260
 QLast Update : Fri May 20 23:50:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	107948	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	194507	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	179081	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	75637	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	67373	60.643	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	121.280%
35) Dibromofluoromethane	7.716	113	61067	50.488	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	100.980%
50) Toluene-d8	10.179	98	240179	53.826	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	107.660%
62) 4-Bromofluorobenzene	12.483	95	66883	37.158	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	74.320%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052422\
Data File : VY009072.D
Acq On : 24 May 2022 19:13
Operator : KP/MD
Sample : N2981-05
Misc : 2.29g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SB-14(0.5-1)

Quant Time: May 25 02:56:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052022S.M
Quant Title : SW846 8260
QLast Update : Fri May 20 23:50:52 2022
Response via : Initial Calibration



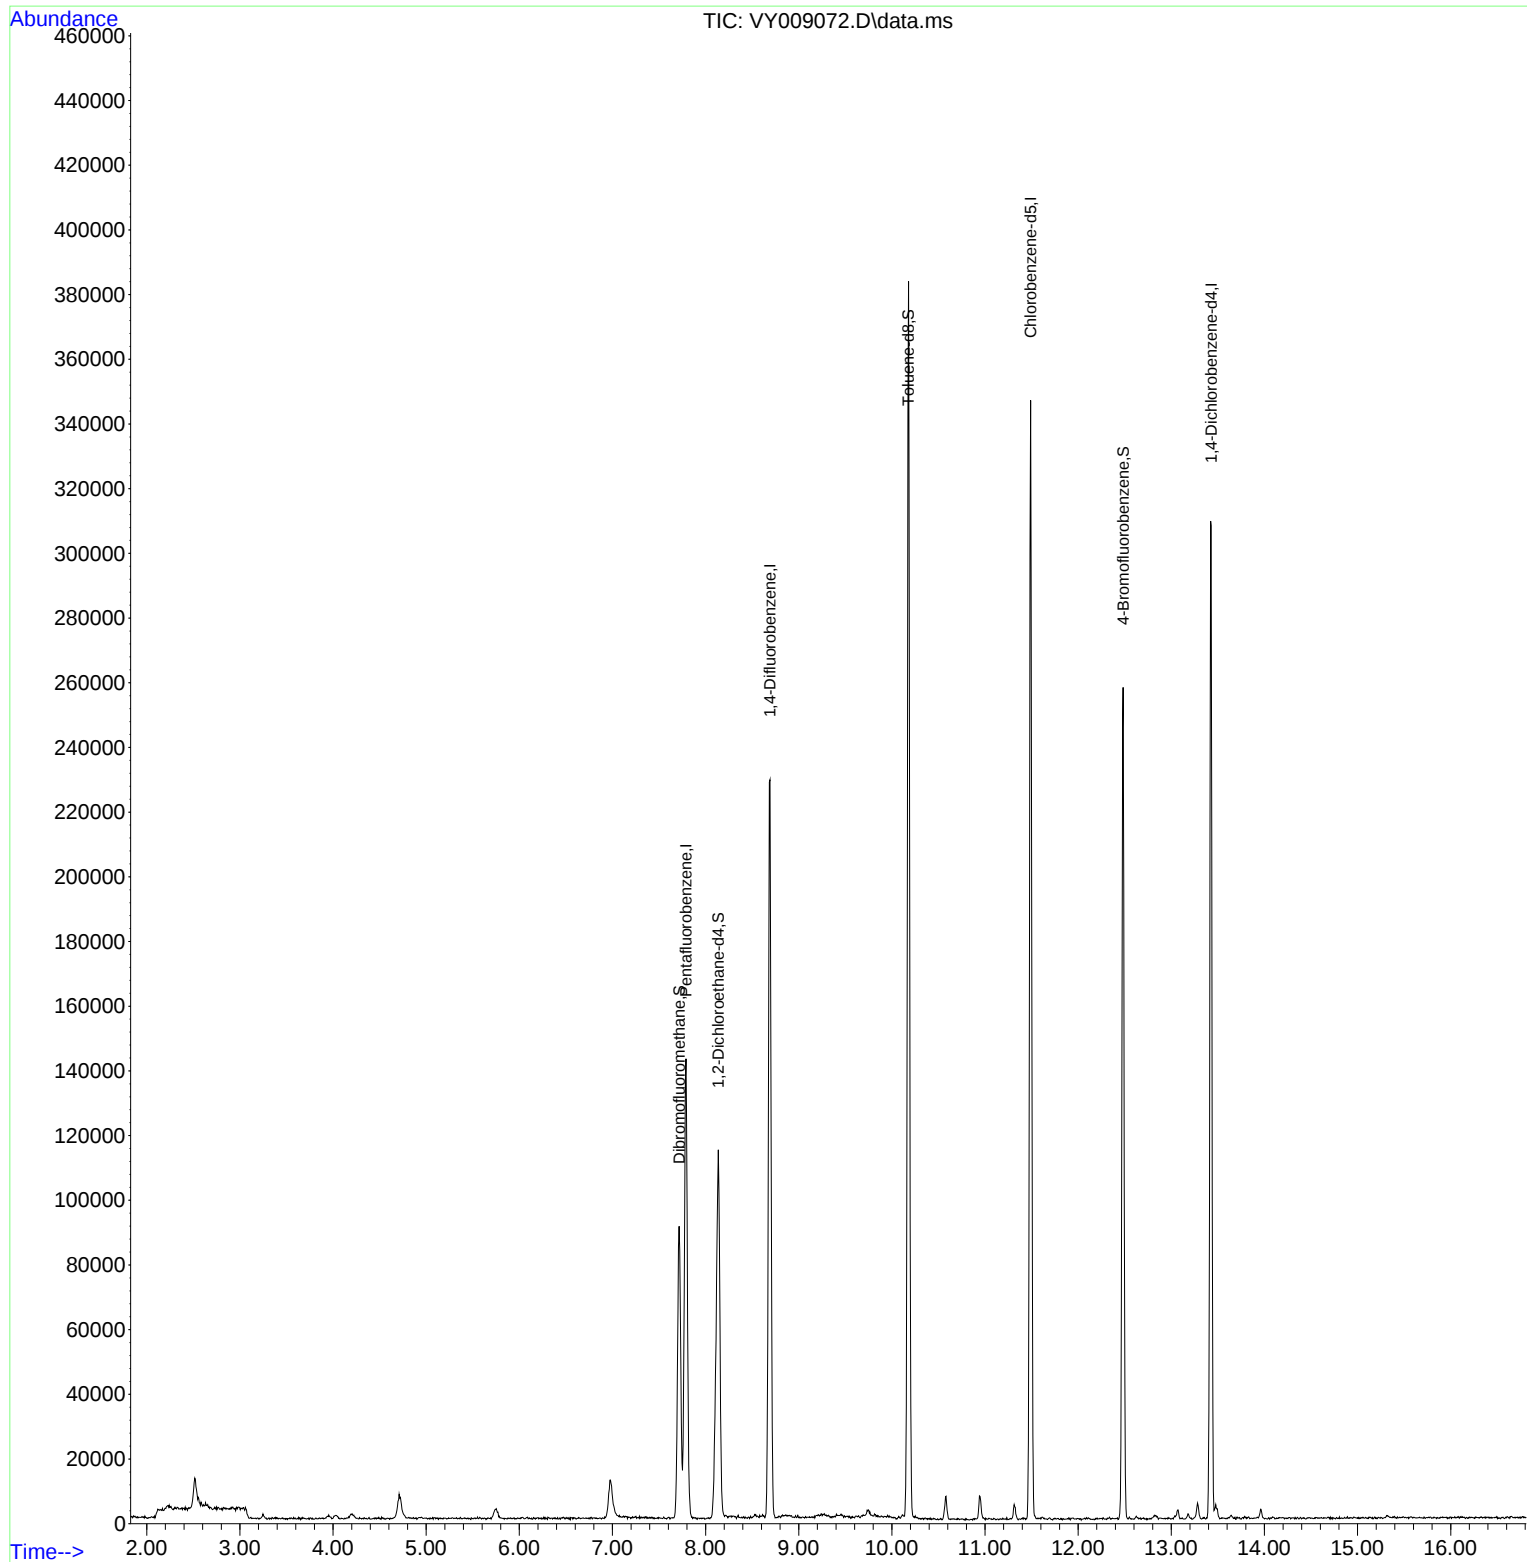


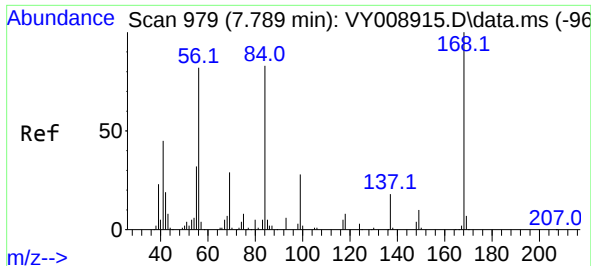

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY009072.D
Acq: 24 May 2022 19:13




Instrument :
MSVOA_Y
ClientSampleId :
SB-14(0.5-1)


Tgt Ion:168 Resp: 107948
Ion Ratio Lower Upper
168 100
99 50.9 46.9 70.3

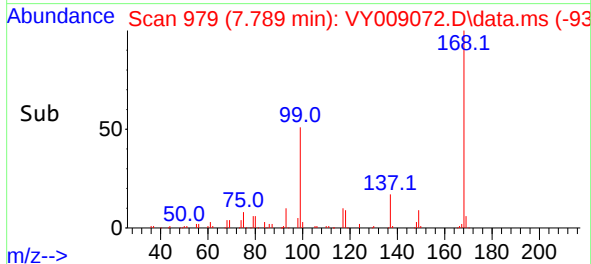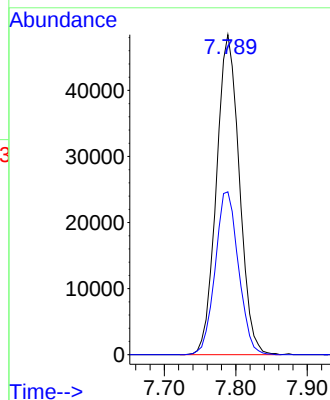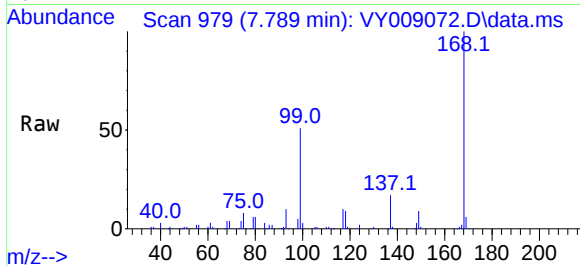

#33
1,2-Dichloroethane-d4
Concen: 60.643 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. -0.007 min
Lab File: VY009072.D
Acq: 24 May 2022 19:13

Tgt Ion: 65 Resp: 67373
Ion Ratio Lower Upper
65 100
67 54.0 0.0 99.4

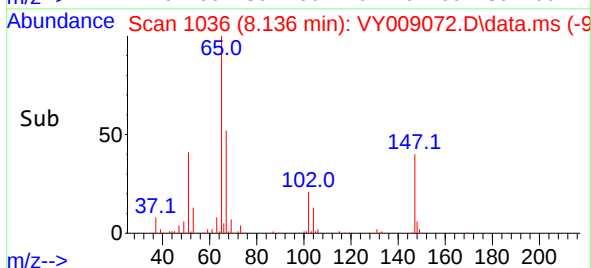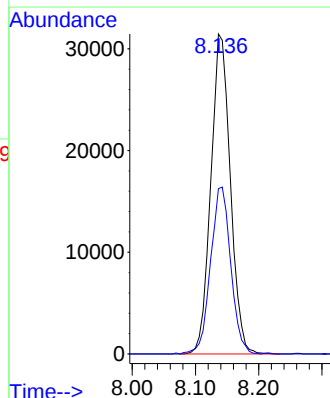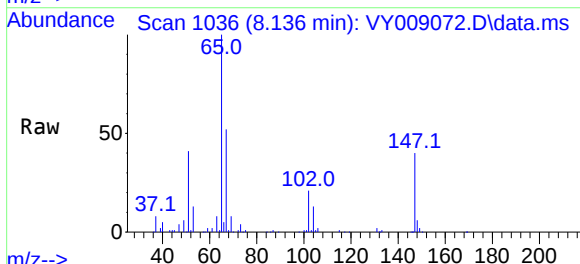

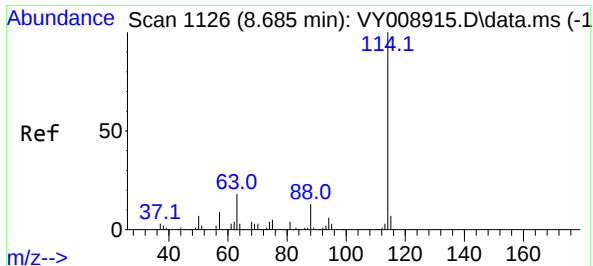

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.006 min

Lab File: VY009072.D

Acq: 24 May 2022 19:13

Instrument :

MSVOA_Y

ClientSampleId :

SB-14(0.5-1)





Tgt Ion:114 Resp: 194507

Ion Ratio Lower Upper

114 100

63 18.9 0.0 43.2

88 14.2 0.0 31.8

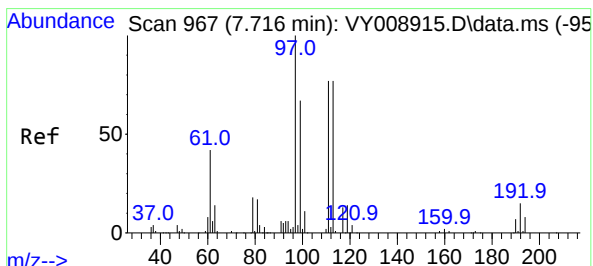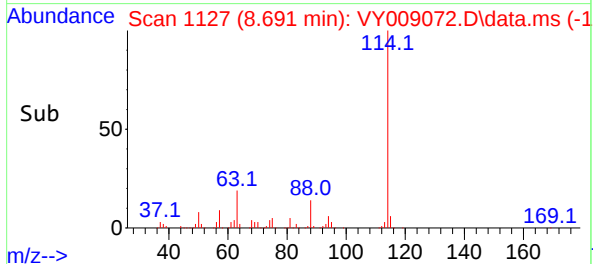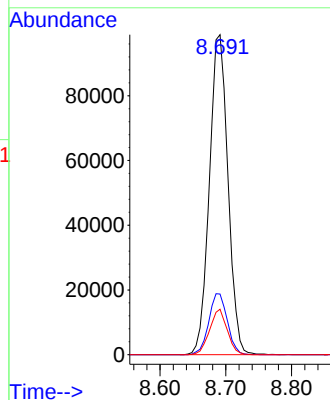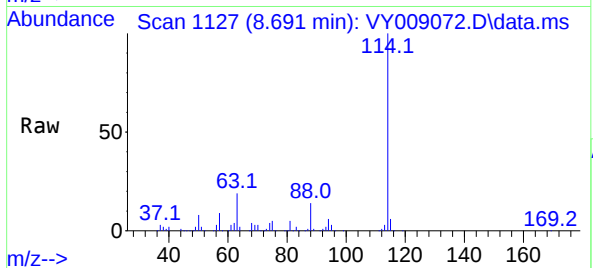

#35

Dibromofluoromethane

Concen: 50.488 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY009072.D

Acq: 24 May 2022 19:13




Tgt Ion:113 Resp: 61067


Ion Ratio Lower Upper

113 100

111 102.5 82.6 124.0

192 18.9 17.6 26.4


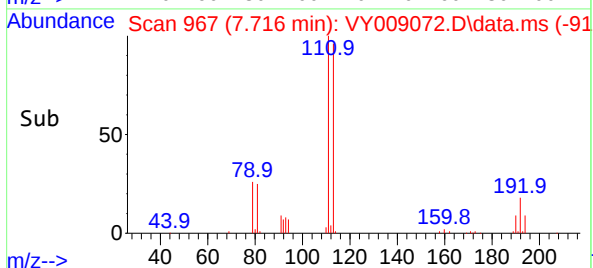
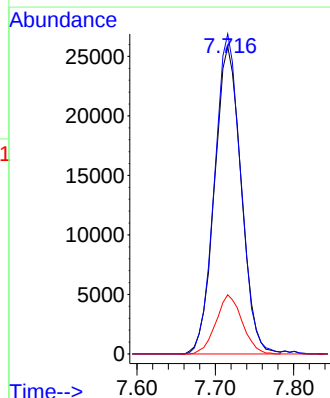
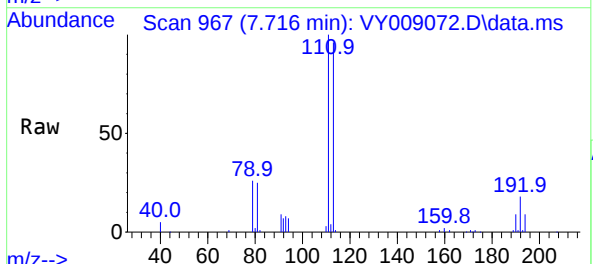


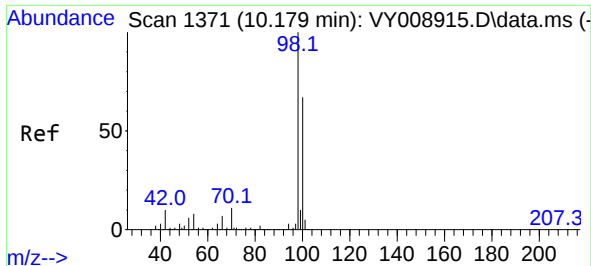

#50
Toluene-d8
Concen: 53.826 ug/l
RT: 10.179 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY009072.D
Acq: 24 May 2022 19:13




Instrument :
MSVOA_Y
ClientSampleId :
SB-14(0.5-1)


Tgt Ion: 98 Resp: 240179
Ion Ratio Lower Upper
98 100
100 63.9 50.2 75.2

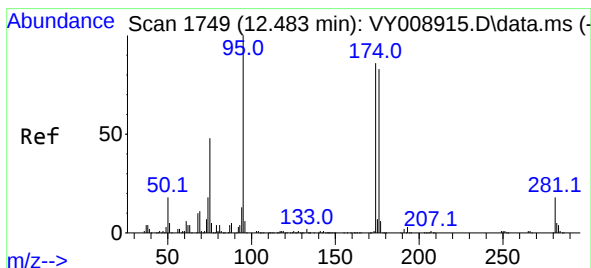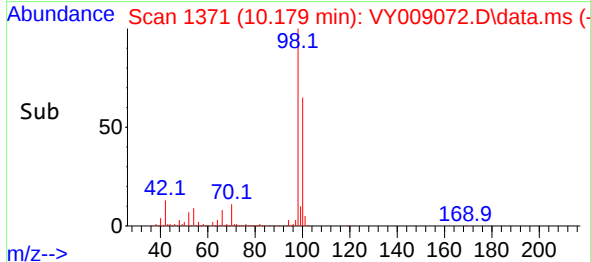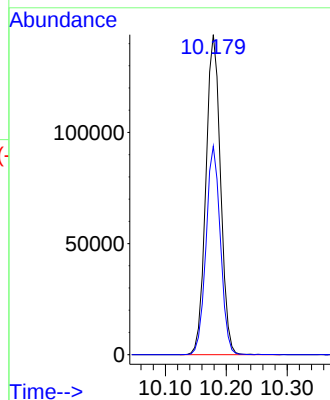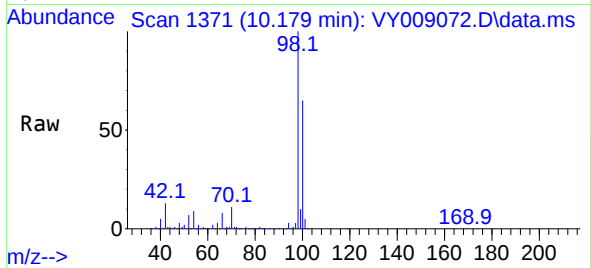

#62
4-Bromofluorobenzene
Concen: 37.158 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY009072.D
Acq: 24 May 2022 19:13

Tgt Ion: 95 Resp: 66883
Ion Ratio Lower Upper
95 100
174 90.6 0.0 177.0
176 87.4 0.0 175.8


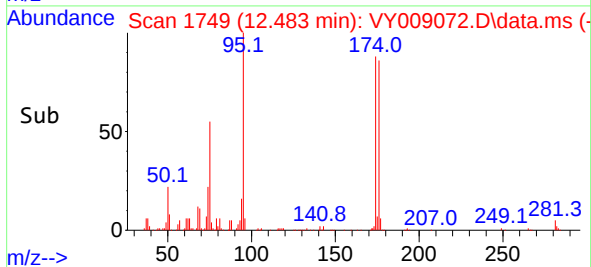
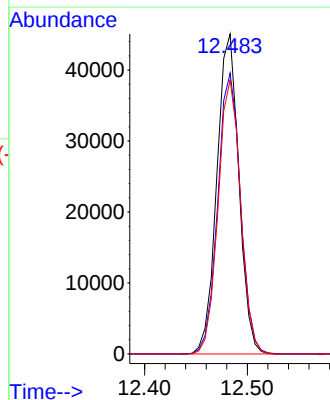
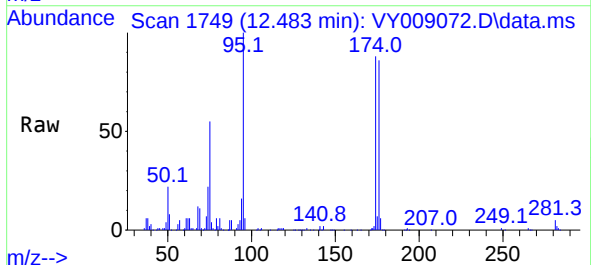


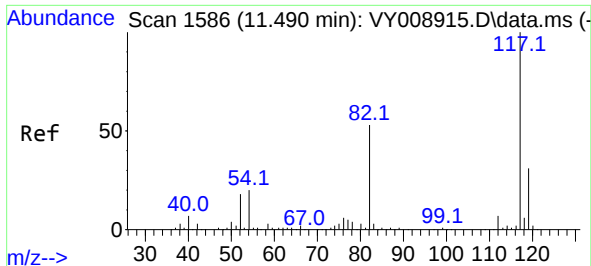

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 117
Delta R.T. -0.001 min
Lab File: VY009072.D
Acq: 24 May 2022 19:13

Instrument :
MSVOA_Y
ClientSampleId :
SB-14(0.5-1)

Tgt Ion:117 Resp: 179081
Ion Ratio Lower Upper
117 100
82 55.3 43.0 64.4
119 32.8 25.4 38.0

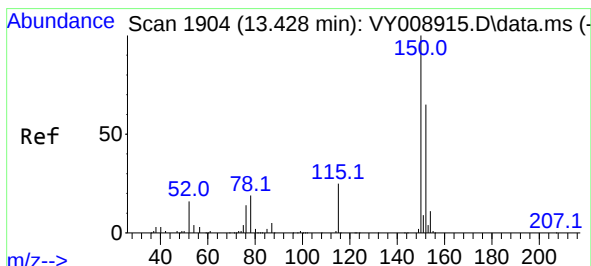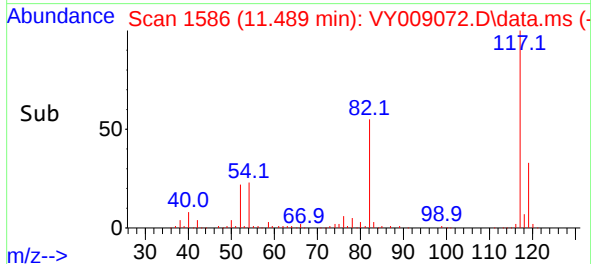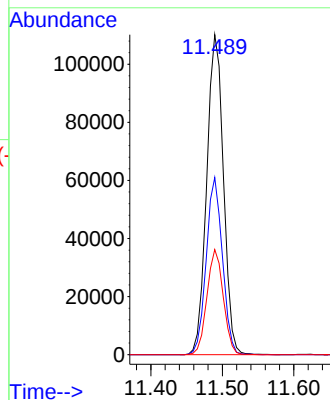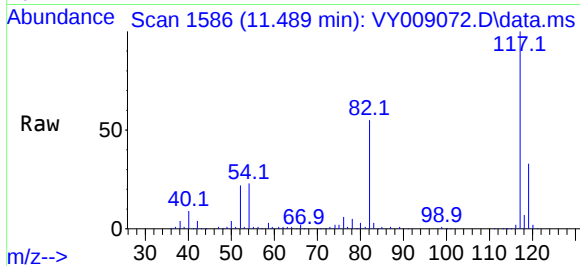

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY009072.D
Acq: 24 May 2022 19:13

Tgt Ion:152 Resp: 75637
Ion Ratio Lower Upper
152 100
115 56.1 28.2 84.7
150 157.8 0.0 347.6

