

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052521\
 Data File : VU043972.D
 Acq On : 25 May 2021 19:56
 Operator : SY/MD
 Sample : VU0525WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VBLK305

Quant Time: May 26 04:30:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM052521.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed May 26 04:28:20 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.225	114	15665	0.50	ug/L	0.00
5) Chlorobenzene-d5	9.361	117	14272	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.759	152	6489	0.50	ug/L	0.02
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.605	65	4408	0.59	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery = 118.00%			
4) 1,2-Dichloroethane-d4	5.679	65	6528	0.44	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 88.00%			
7) 1,2-Dichloropropane-d6	6.658	67	7659	0.55	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery = 110.00%			
8) Toluene-d8	7.845	98	14756	0.48	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 96.00%			
10) 1,1,2,2-Tetrachloroeth...	10.696	84	7045	0.53	ug/L	0.02
Spiked Amount 0.500	Range 65 - 120		Recovery = 106.00%			
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.924	75	22	0.01	ug/L	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052521\
Data File : VU043972.D
Acq On : 25 May 2021 19:56
Operator : SY/MD
Sample : VU0525WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VBLK305


Quant Time: May 26 04:30:38 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM052521.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed May 26 04:28:20 2021
Response via : Initial Calibration

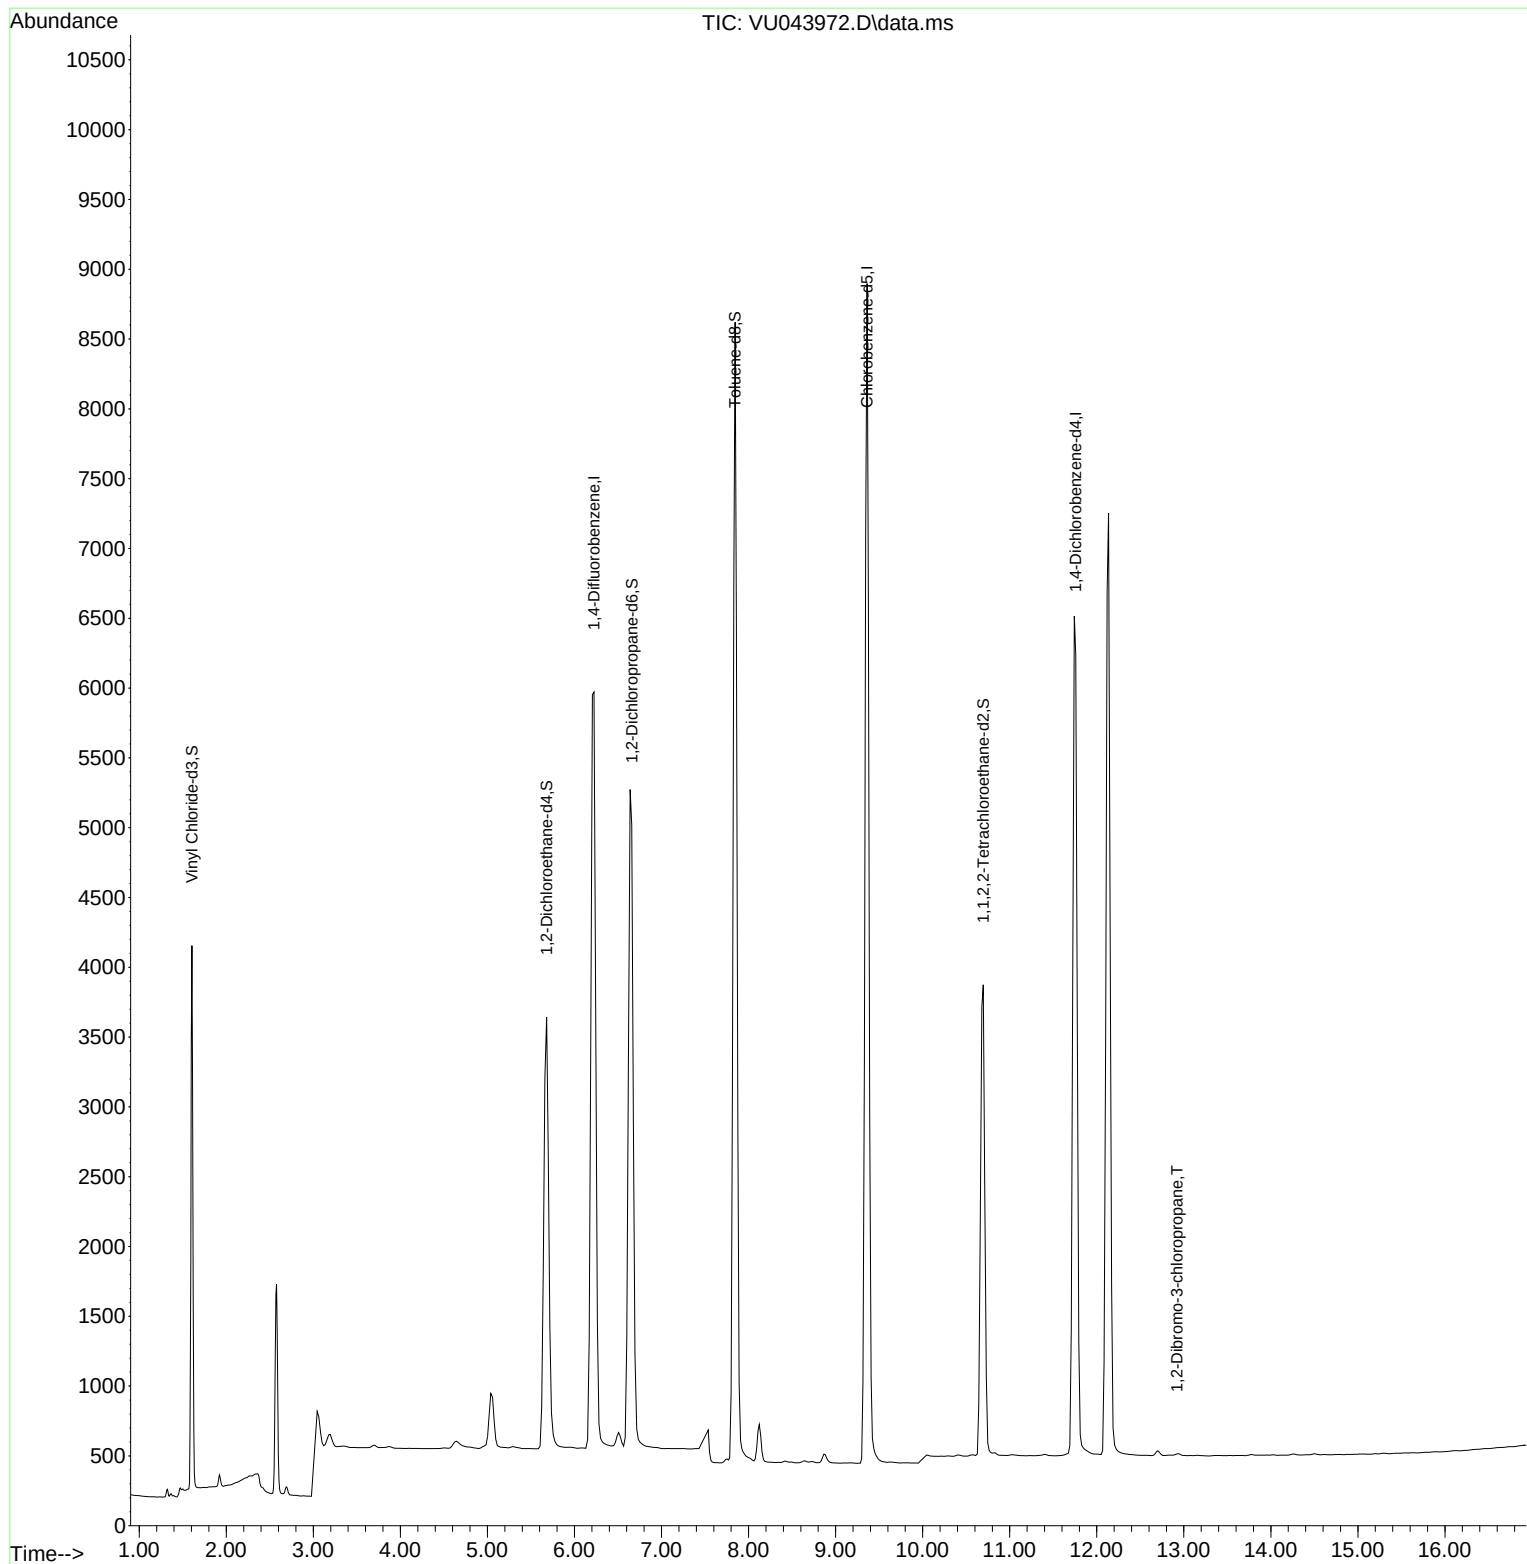

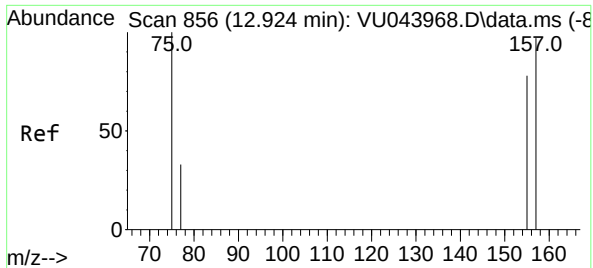

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.01 ug/L
 RT: 12.924 min Scan# 856
 Delta R.T. -0.000 min
 Lab File: VU043972.D
 Acq: 25 May 2021 19:56

Instrument :
 MSVOA_Y
 ClientSampleId :
 VBLK305

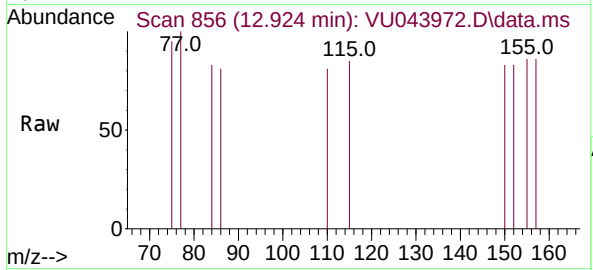

Tgt Ion:	75	Resp:	22
Ion	Ratio	Lower	Upper
75	100		
157	91.1	77.2	115.8
155	91.1	64.5	96.7

