
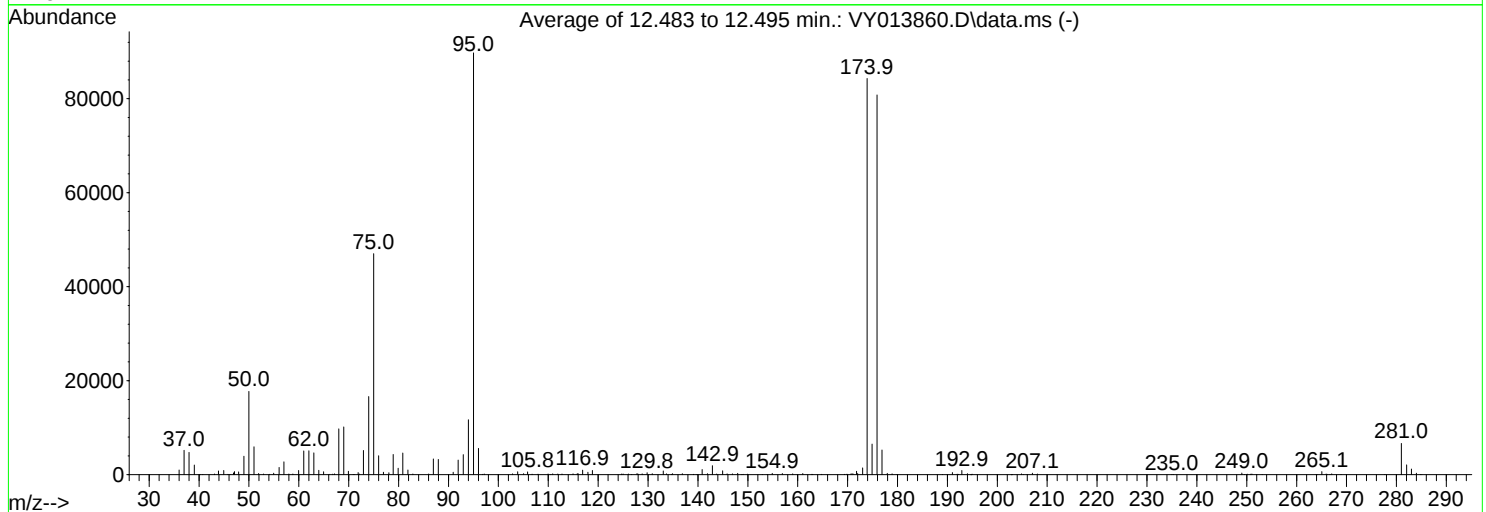


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052523\
Data File : VY013860.D
Acq On : 25 May 2023 09:14
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052323S.M
Title : SW846 8260
Last Update : Wed May 24 05:25:47 2023

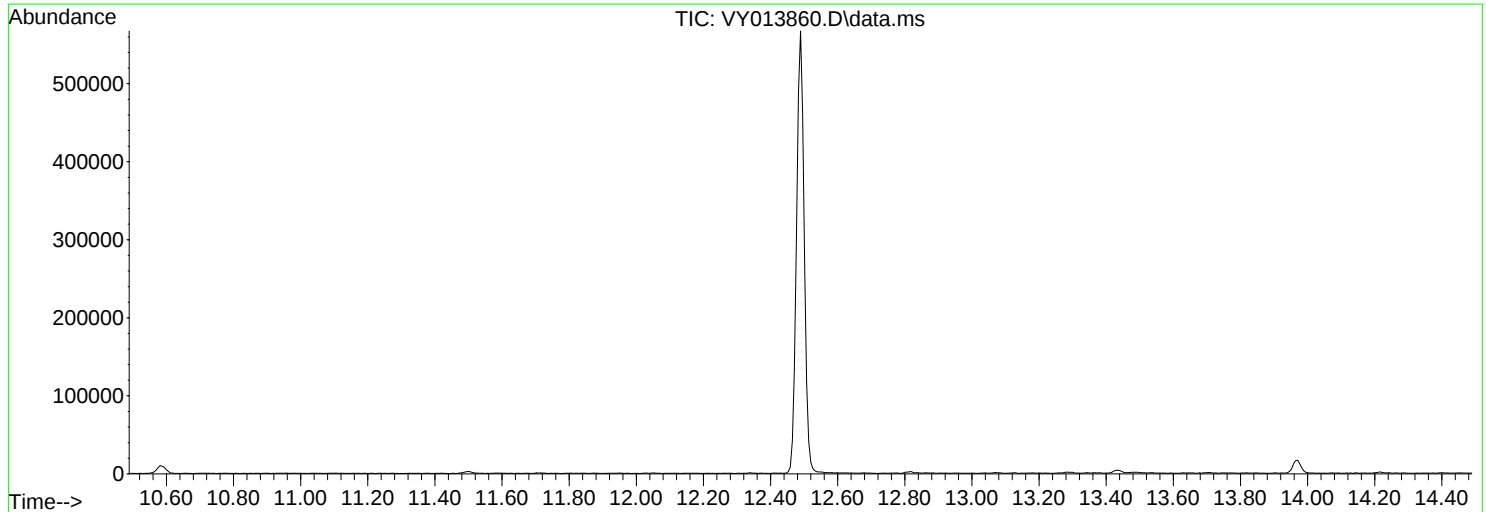

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1741

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.7	17721	PASS
75	95	30	60	52.4	47011	PASS
95	95	100	100	100.0	89760	PASS
96	95	5	9	6.2	5579	PASS
173	174	0.00	2	1.7	1427	PASS
174	95	50	100	93.9	84307	PASS
175	174	5	9	7.7	6519	PASS
176	174	95	101	95.8	80803	PASS
177	176	5	9	6.5	5254	PASS