
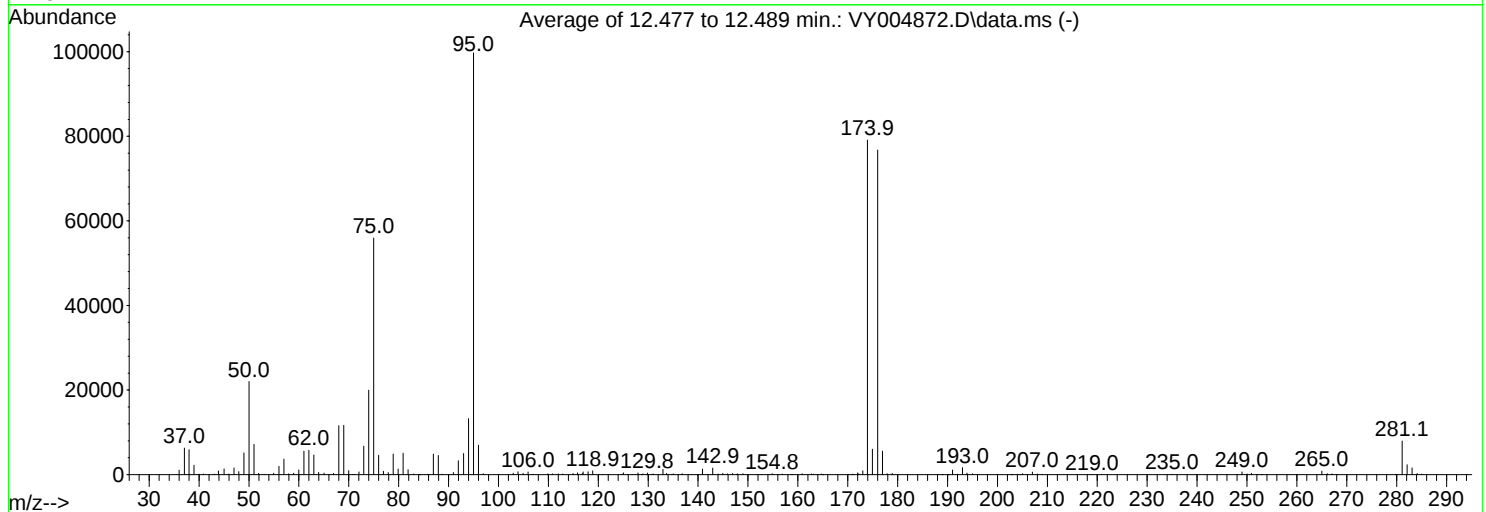


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052621\
Data File : VY004872.D
Acq On : 26 May 2021 08:55
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051021S.M
Title : SW846 8260
Last Update : Tue May 11 04:13:44 2021

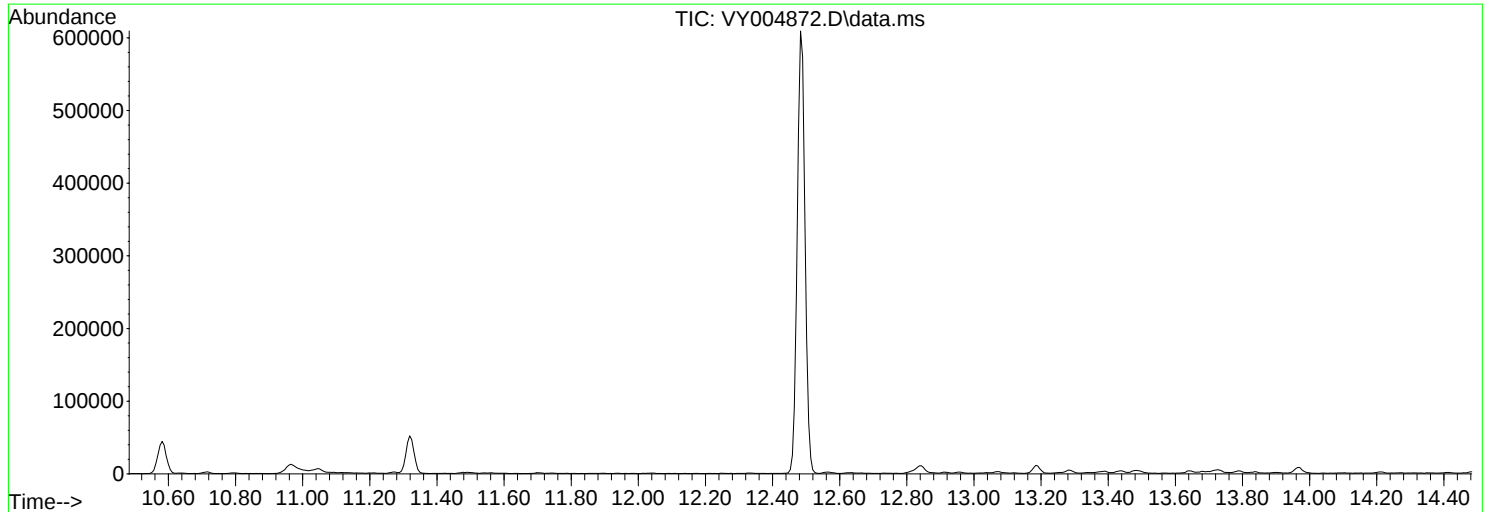

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.1	22003	PASS
75	95	30	60	56.1	55953	PASS
95	95	100	100	100.0	99728	PASS
96	95	5	9	7.0	6956	PASS
173	174	0.00	2	1.1	893	PASS
174	95	50	100	79.3	79123	PASS
175	174	5	9	7.6	6001	PASS
176	174	95	101	97.0	76752	PASS
177	176	5	9	7.2	5558	PASS