
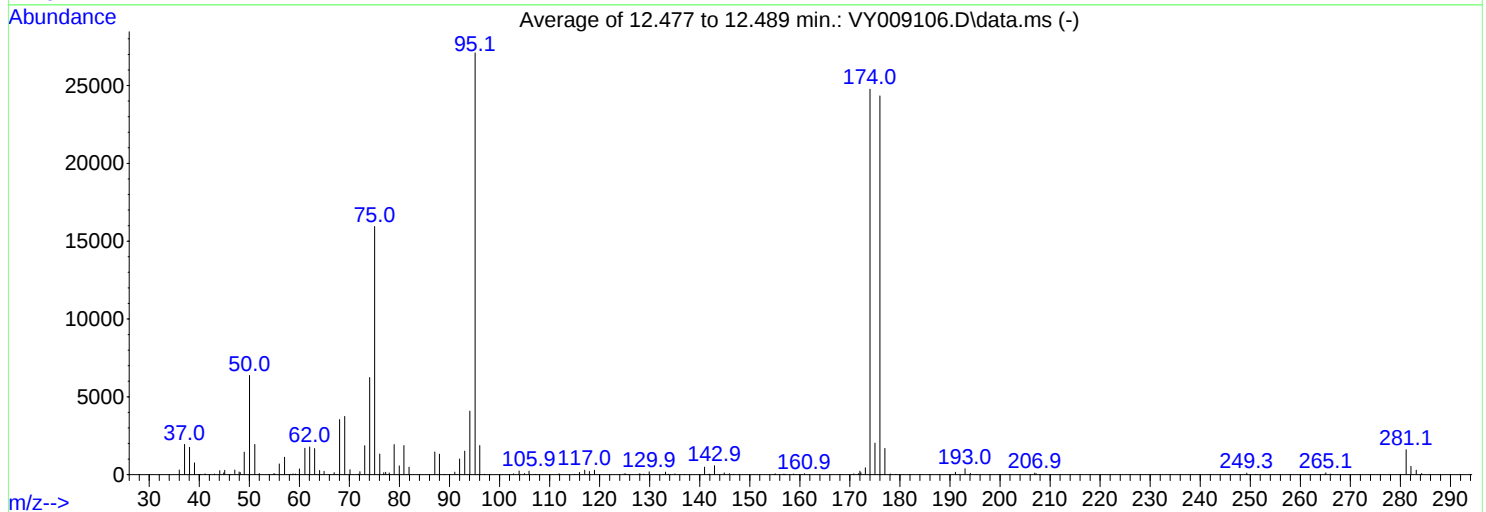


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY052622\  
 Data File : VY009106.D  
 Acq On : 26 May 2022 09:25  
 Operator : KP/MD  
 Sample : BFB  
 Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y052022S.M  
 Title : SW846 8260  
 Last Update : Fri May 20 23:50:52 2022

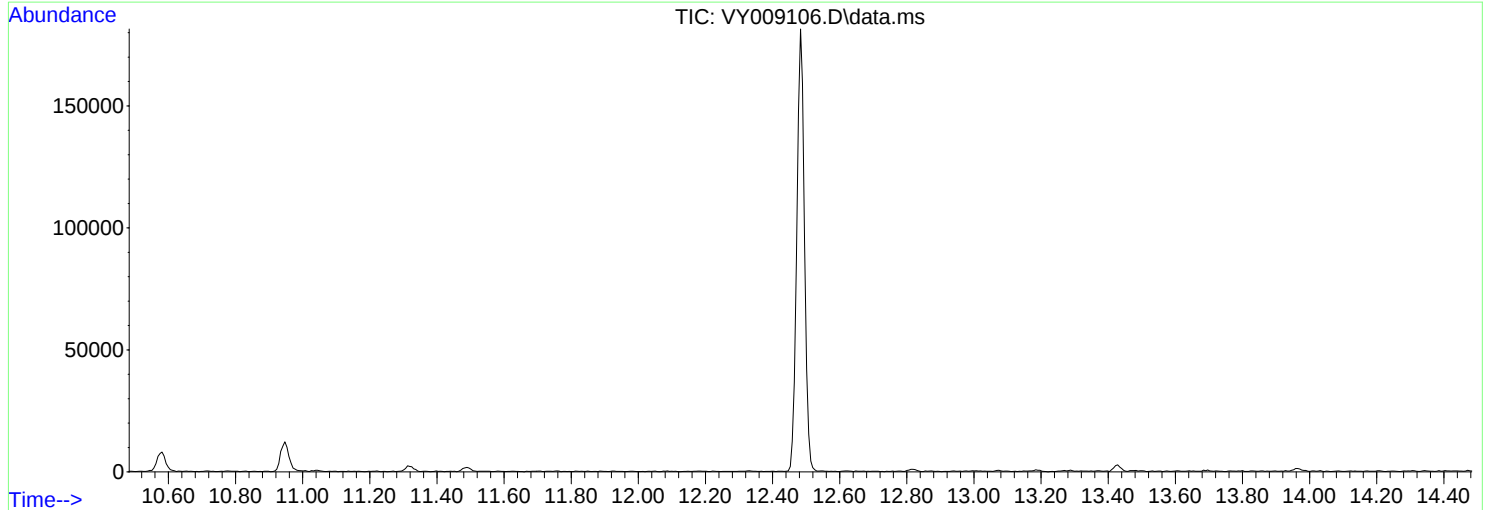

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 23.5         | 6372       | PASS                |
| 75             | 95              | 30              | 60              | 58.9         | 15949      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 27101      | PASS                |
| 96             | 95              | 5               | 9               | 6.9          | 1874       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.8          | 446        | PASS                |
| 174            | 95              | 50              | 100             | 91.4         | 24765      | PASS                |
| 175            | 174             | 5               | 9               | 8.2          | 2021       | PASS                |
| 176            | 174             | 95              | 101             | 98.3         | 24333      | PASS                |
| 177            | 176             | 5               | 9               | 6.9          | 1686       | PASS                |