

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052721\
 Data File : VY004896.D
 Acq On : 27 May 2021 13:27
 Operator : SY/MD
 Sample : M2518-01
 Misc : 3.90G/5ML/MSVOA_Y/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 115

Quant Time: May 27 14:25:29 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051021S.M
 Quant Title : SW846 8260
 QLast Update : Tue May 11 04:13:44 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.801	168	186686	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	345249	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.496	117	281985	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	98088	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	131327	59.10	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	118.20%
35) Dibromofluoromethane	7.728	113	111272	58.87	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	117.74%
50) Toluene-d8	10.185	98	414224	48.51	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	97.02%
62) 4-Bromofluorobenzene	12.483	95	114812	39.84	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	79.68%
Target Compounds						
17) Carbon Disulfide	4.210	76	7476	1.33	ug/l	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052721\
Data File : VY004896.D
Acq On : 27 May 2021 13:27
Operator : SY/MD
Sample : M2518-01
Misc : 3.90G/5ML/MSVOA_Y/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
115


Quant Time: May 27 14:25:29 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051021S.M
Quant Title : SW846 8260
QLast Update : Tue May 11 04:13:44 2021
Response via : Initial Calibration

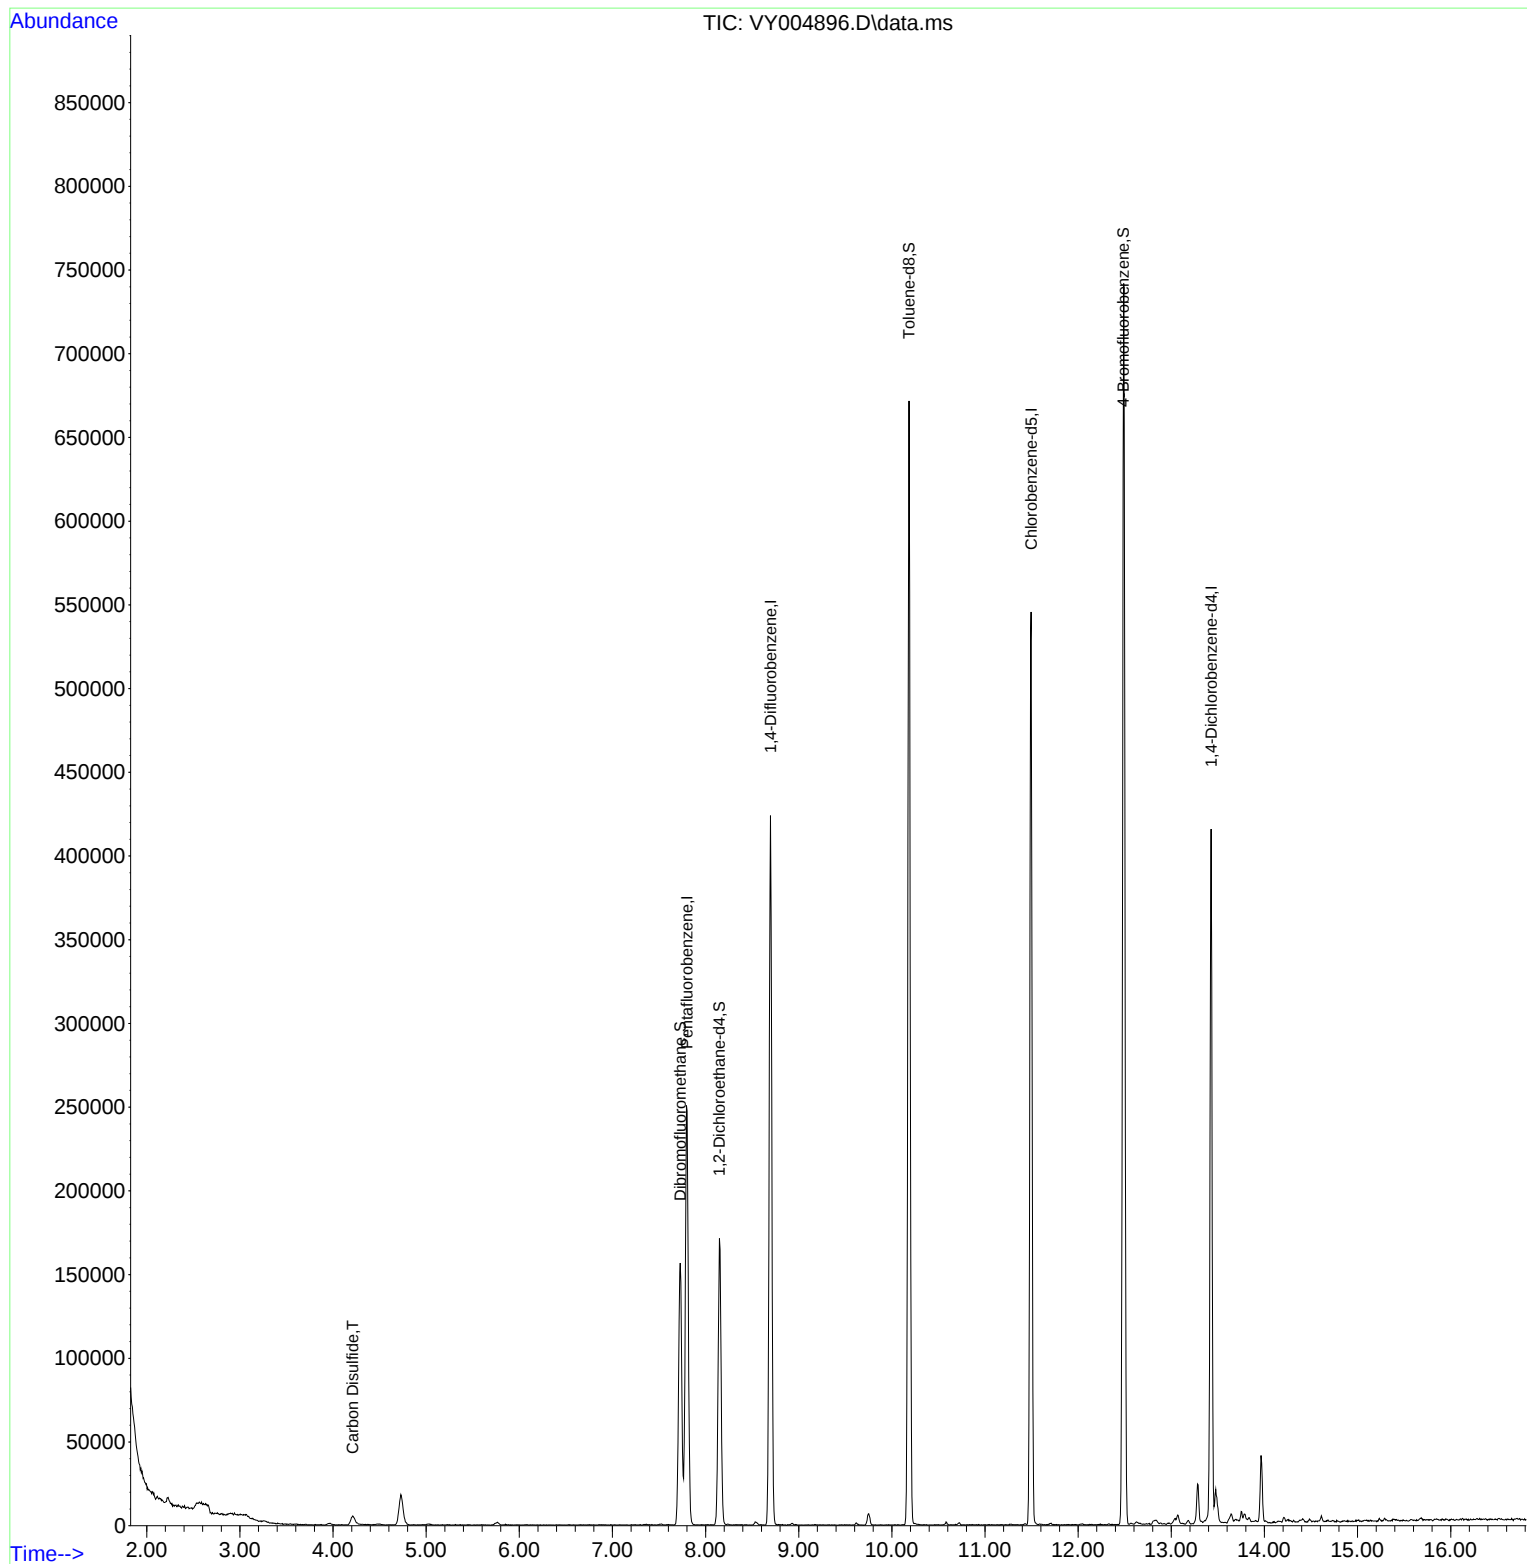



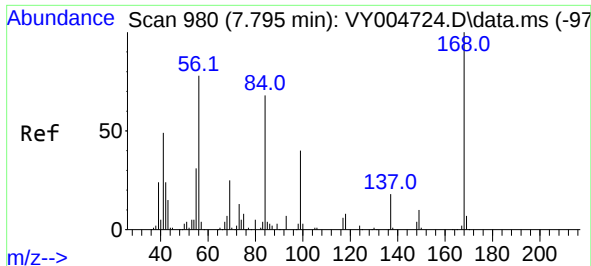


#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.801 min Scan# 981
Delta R.T. 0.006 min
Lab File: VY004896.D
Acq: 27 May 2021 13:27

Instrument :
MSVOA_Y
ClientSampled :
115



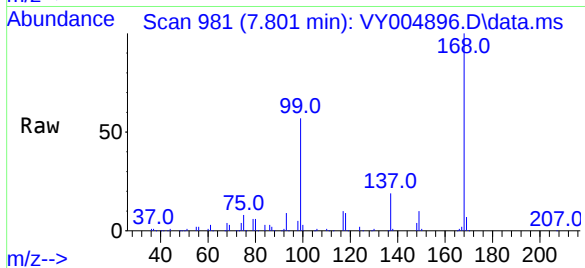



Tgt Ion:168 Resp: 186686
Ion Ratio Lower Upper
168 100
99 57.0 45.6 68.4

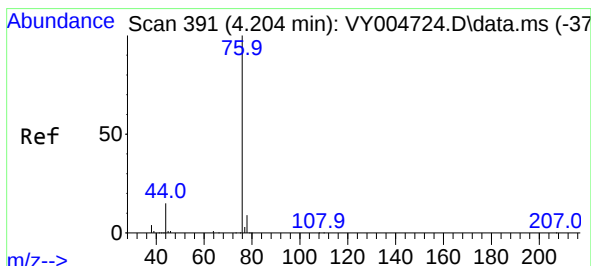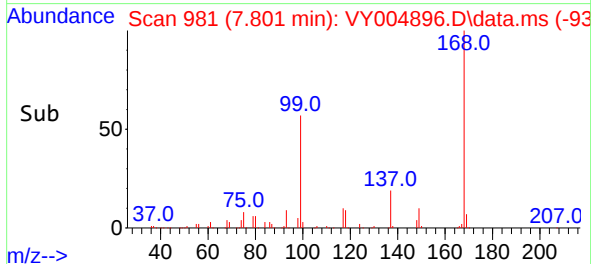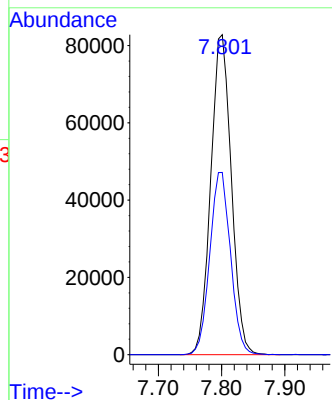

#17
Carbon Disulfide
Concen: 1.33 ug/l
RT: 4.210 min Scan# 392
Delta R.T. 0.006 min
Lab File: VY004896.D
Acq: 27 May 2021 13:27

Tgt Ion: 76 Resp: 7476
Ion Ratio Lower Upper
76 100
78 9.4 7.2 10.8


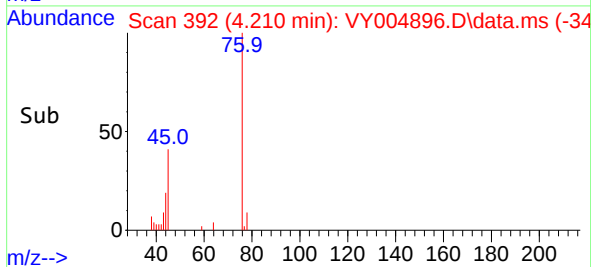
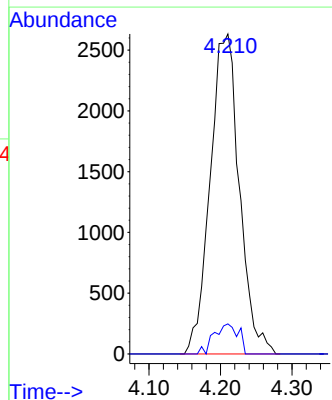
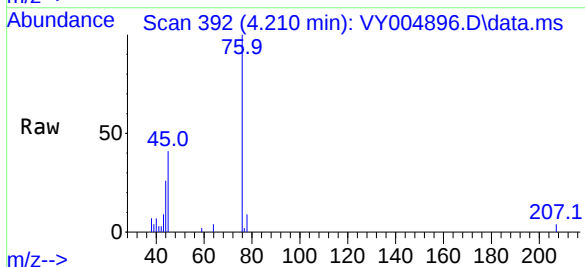


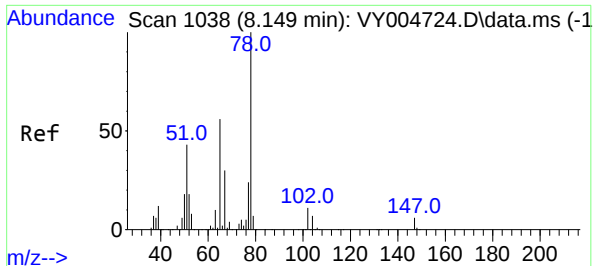

#33
1,2-Dichloroethane-d4
Concen: 59.10 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. -0.000 min
Lab File: VY004896.D
Acq: 27 May 2021 13:27




Instrument :
MSVOA_Y
ClientSampled :
115


Tgt Ion: 65 Resp: 131327
Ion Ratio Lower Upper
65 100
67 53.0 0.0 108.0

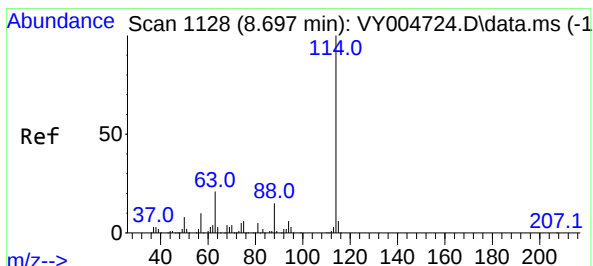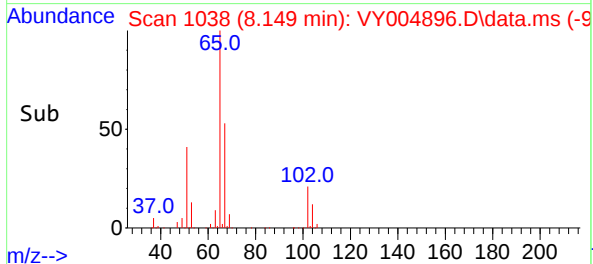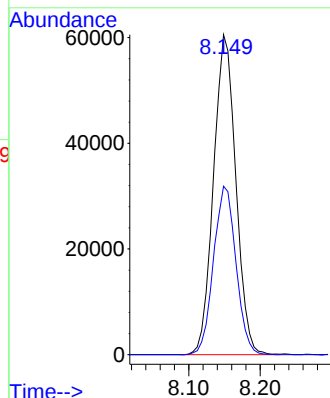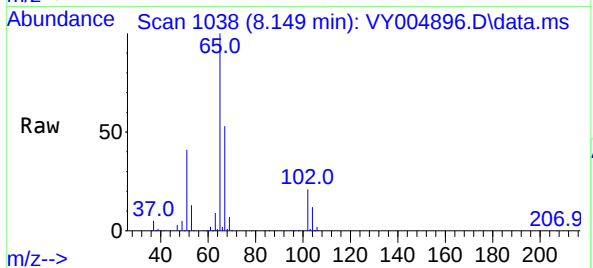

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. -0.000 min
Lab File: VY004896.D
Acq: 27 May 2021 13:27

Tgt Ion: 114 Resp: 345249
Ion Ratio Lower Upper
114 100
63 21.1 0.0 42.8
88 15.6 0.0 31.0


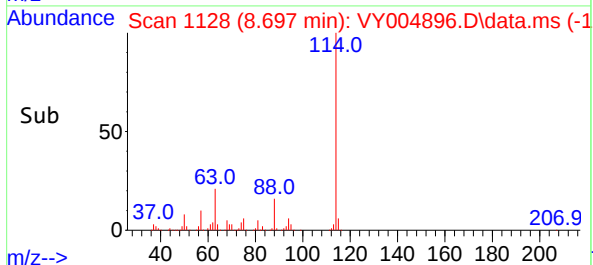
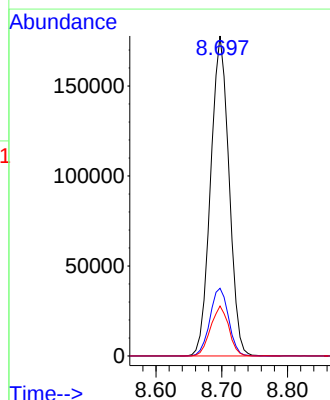
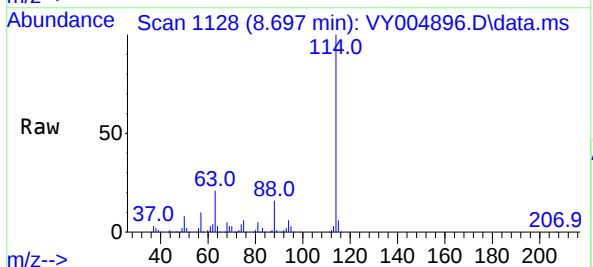


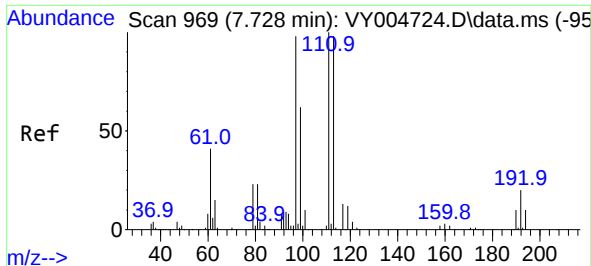

#35
Dibromofluoromethane
Concen: 58.87 ug/l
RT: 7.728 min Scan# 969
Delta R.T. -0.000 min
Lab File: VY004896.D
Acq: 27 May 2021 13:27




Instrument :
MSVOA_Y
ClientSampled :
115


Tgt Ion:113 Resp: 111272
Ion Ratio Lower Upper
113 100
111 102.6 80.5 120.7
192 18.8 15.0 22.6

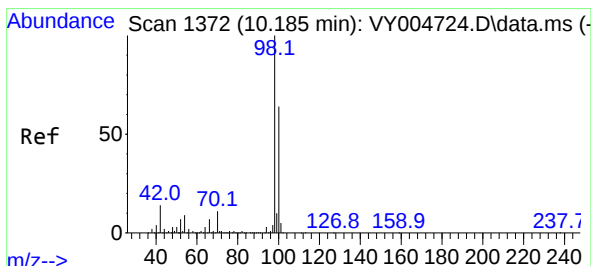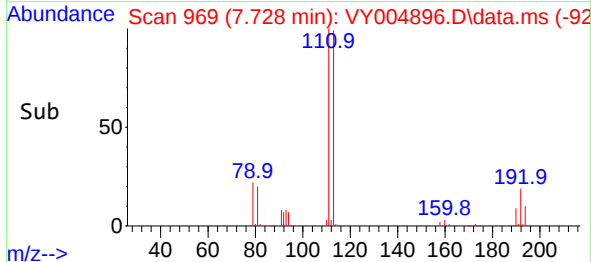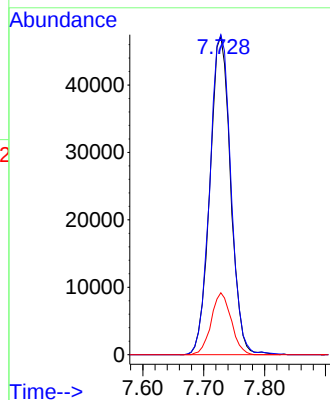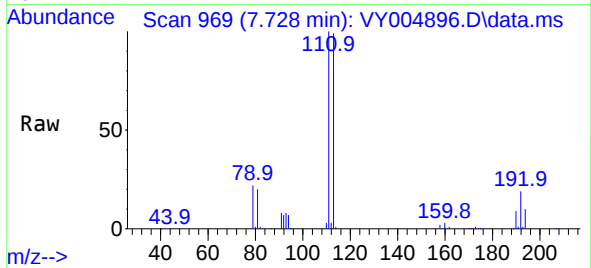

#50
Toluene-d8
Concen: 48.51 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. -0.000 min
Lab File: VY004896.D
Acq: 27 May 2021 13:27

Tgt Ion: 98 Resp: 414224
Ion Ratio Lower Upper
98 100
100 64.3 51.5 77.3

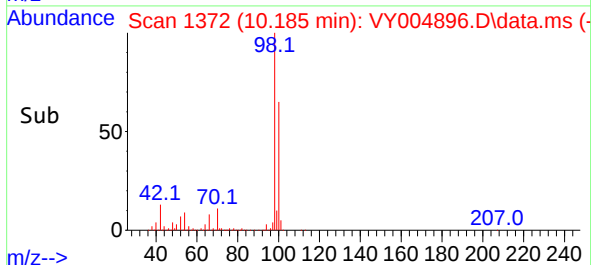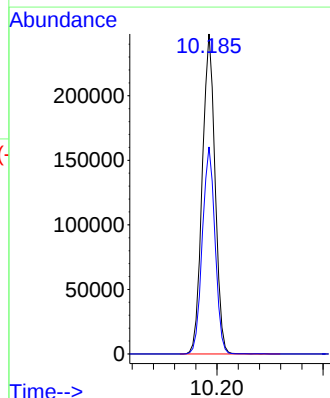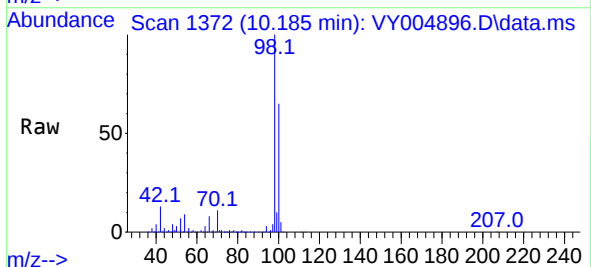




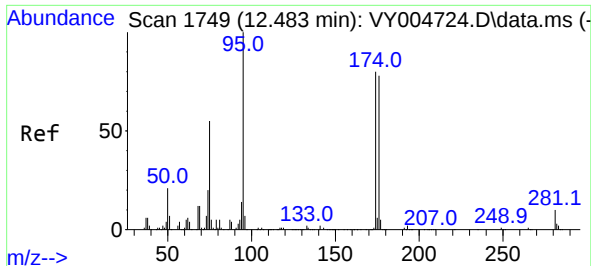


#62
4-Bromofluorobenzene
Concen: 39.84 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY004896.D
Acq: 27 May 2021 13:27

Instrument :
MSVOA_Y
ClientSampled :
115

Tgt Ion: 95 Resp: 114812




Ion	Ratio	Lower	Upper
95	100		
174	80.7	0.0	164.2
176	78.7	0.0	159.0

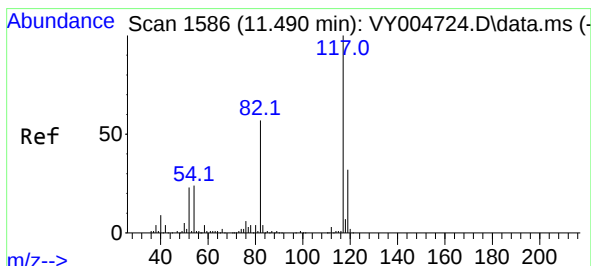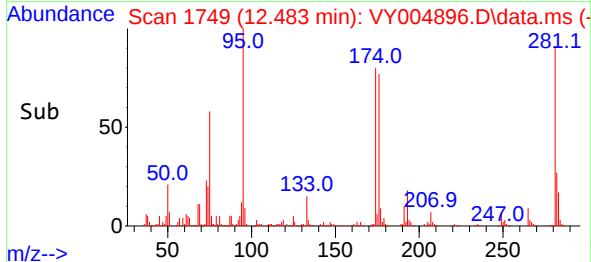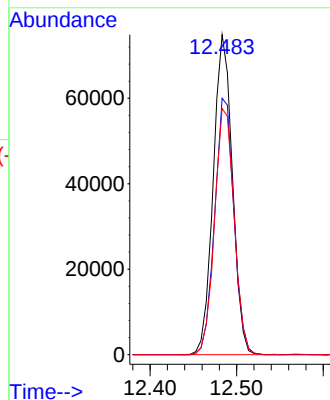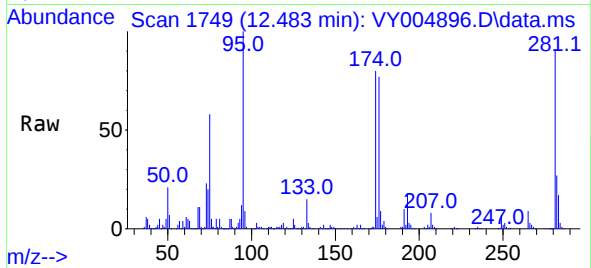


#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.496 min Scan# 1587
Delta R.T. 0.006 min
Lab File: VY004896.D
Acq: 27 May 2021 13:27

Tgt Ion: 117 Resp: 281985

Ion	Ratio	Lower	Upper
117	100		
82	56.9	45.4	68.2
119	31.5	25.8	38.6

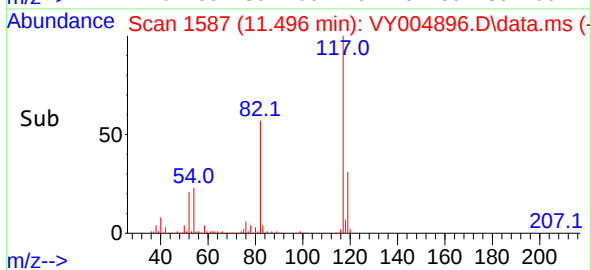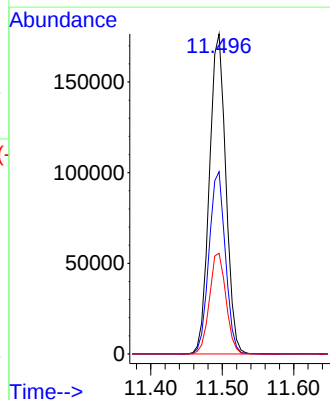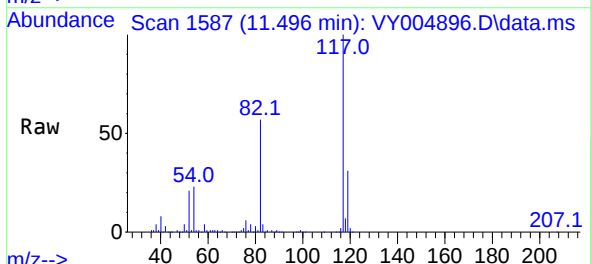

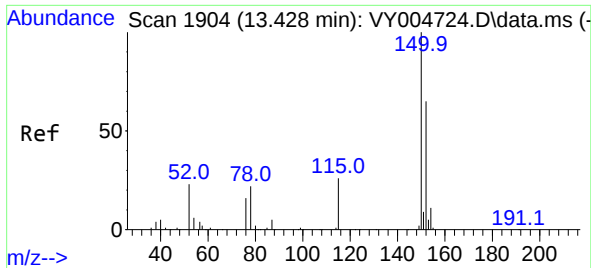

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.00 ug/l
 RT: 13.428 min Scan# 1904
 Delta R.T. -0.000 min
 Lab File: VY004896.D
 Acq: 27 May 2021 13:27

Instrument :
 MSVOA_Y
 ClientSampleId :
 115

Tgt Ion:152 Resp: 98088
 Ion Ratio Lower Upper
 152 100
 115 59.4 29.4 88.3
 150 159.3 0.0 349.8

