

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052721\
 Data File : VY004900.D
 Acq On : 27 May 2021 15:00
 Operator : SY/MD
 Sample : M2535-09
 Misc : 5.62G/5ML/MSVOA_Y/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 GHOST-5

Quant Time: May 27 15:06:55 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051021S.M
 Quant Title : SW846 8260
 QLast Update : Tue May 11 04:13:44 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.795	168	177044	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	335868	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.495	117	308164	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	126791	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.148	65	122085	57.93	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	115.86%
35) Dibromofluoromethane	7.728	113	102206	55.59	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	111.18%
50) Toluene-d8	10.185	98	415002	49.96	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	99.92%
62) 4-Bromofluorobenzene	12.483	95	125494	44.76	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	89.52%
Target Compounds						
7) Trichlorofluoromethane	3.131	101	3866	1.21	ug/l	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052721\
Data File : VY004900.D
Acq On : 27 May 2021 15:00
Operator : SY/MD
Sample : M2535-09
Misc : 5.62G/5ML/MSVOA_Y/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
GHOST-5

Quant Time: May 27 15:06:55 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051021S.M
Quant Title : SW846 8260
QLast Update : Tue May 11 04:13:44 2021
Response via : Initial Calibration




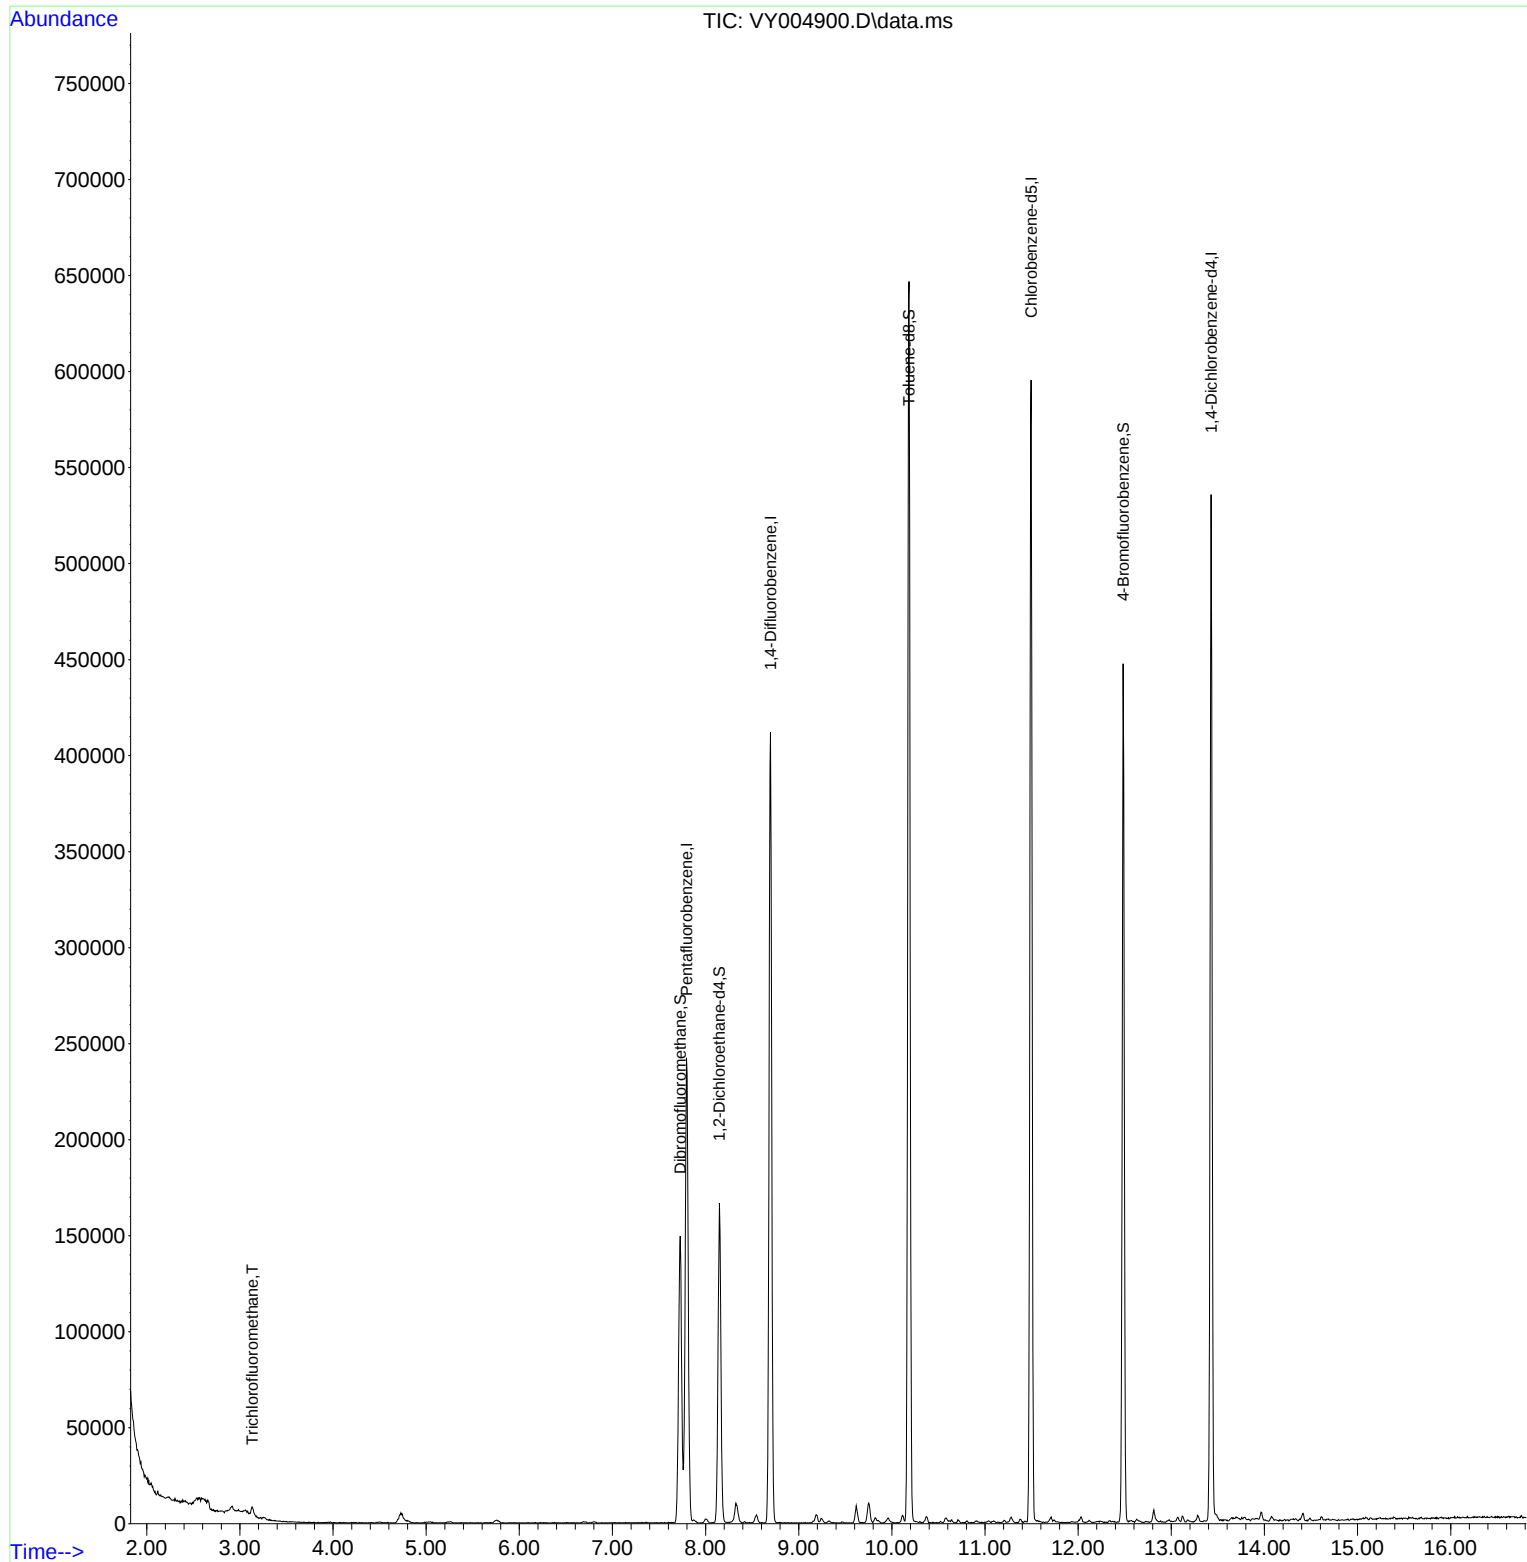


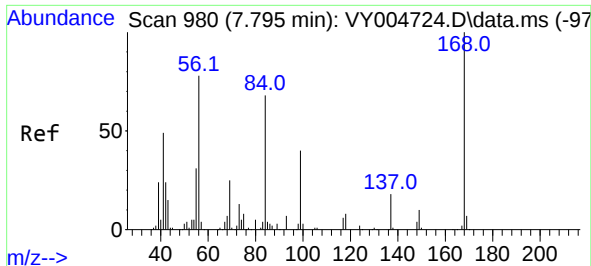

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.795 min Scan# 980
Delta R.T. -0.000 min
Lab File: VY004900.D
Acq: 27 May 2021 15:00




Instrument :
MSVOA_Y
ClientSampleId :
GHOST-5


Tgt Ion:168 Resp: 177044
Ion Ratio Lower Upper
168 100
99 57.2 45.6 68.4

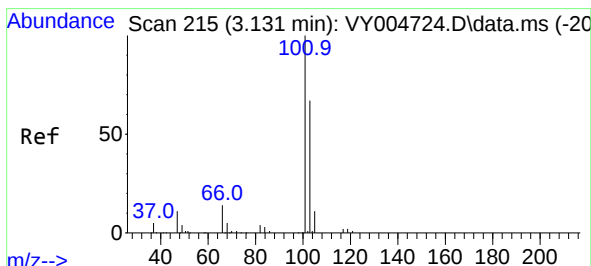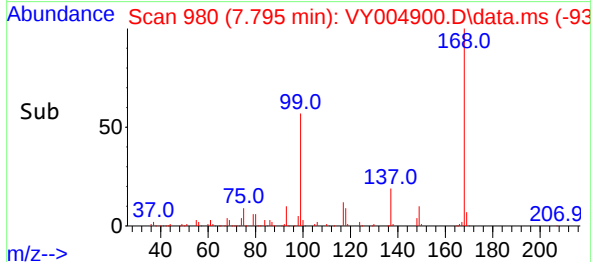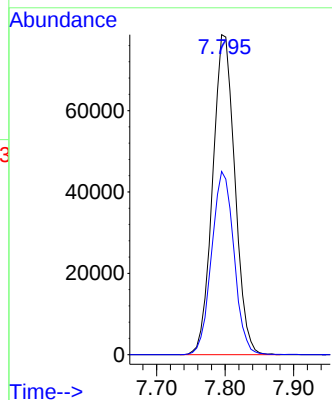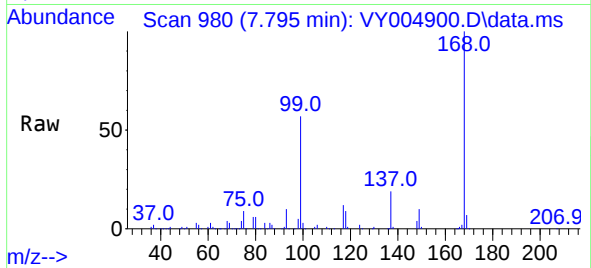

#7
Trichlorofluoromethane
Concen: 1.21 ug/l
RT: 3.131 min Scan# 215
Delta R.T. -0.000 min
Lab File: VY004900.D
Acq: 27 May 2021 15:00

Tgt Ion:101 Resp: 3866
Ion Ratio Lower Upper
101 100
103 59.6 53.4 80.2


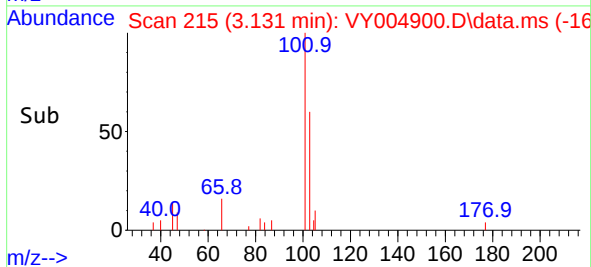
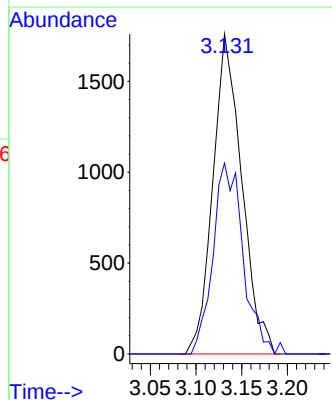
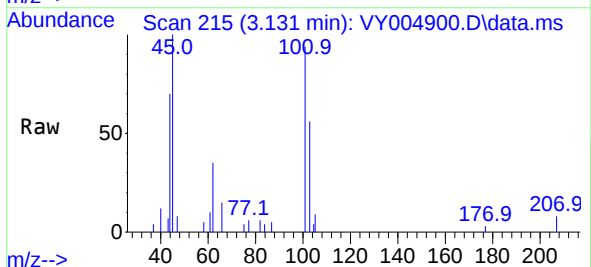


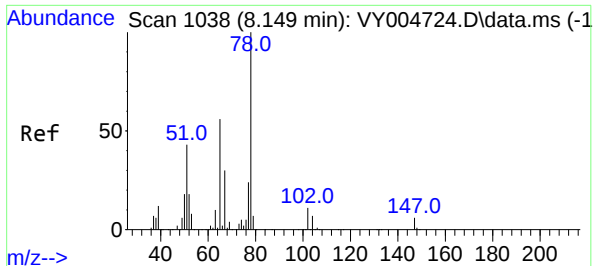

#33
1,2-Dichloroethane-d4
Concen: 57.93 ug/l
RT: 8.148 min Scan# 1038
Delta R.T. -0.000 min
Lab File: VY004900.D
Acq: 27 May 2021 15:00




Instrument :
MSVOA_Y
ClientSampleId :
GHOST-5


Tgt Ion: 65 Resp: 122085
Ion Ratio Lower Upper
65 100
67 53.1 0.0 108.0

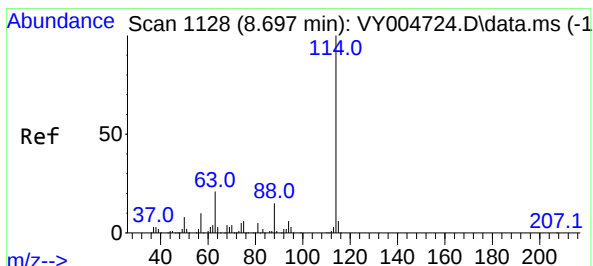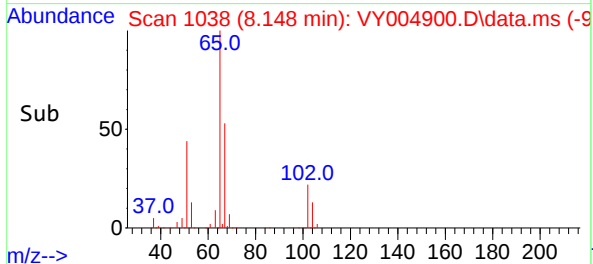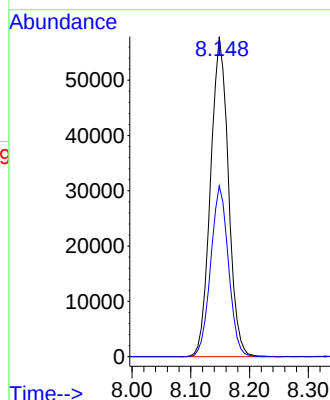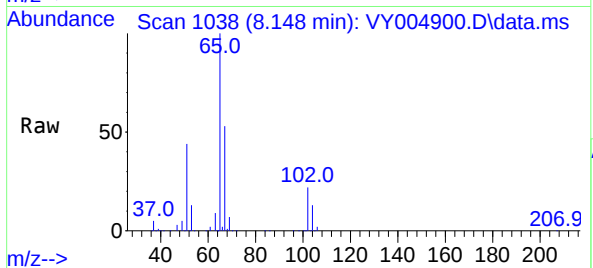

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. -0.000 min
Lab File: VY004900.D
Acq: 27 May 2021 15:00

Tgt Ion: 114 Resp: 335868
Ion Ratio Lower Upper
114 100
63 21.6 0.0 42.8
88 15.8 0.0 31.0


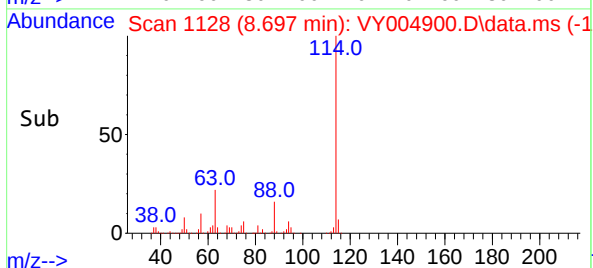
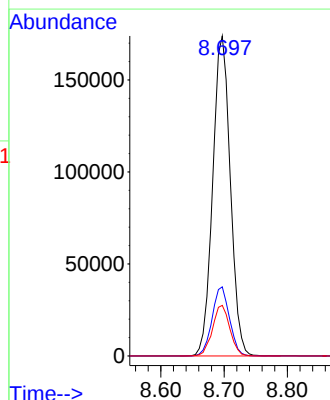
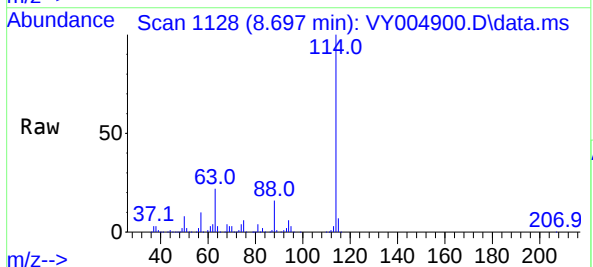


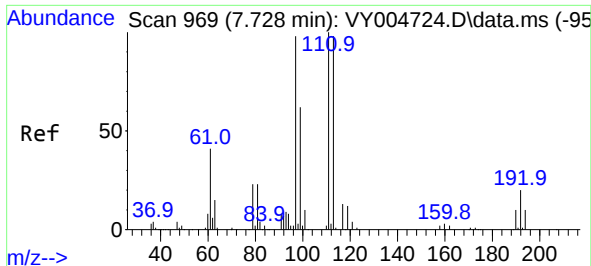

#35
Dibromofluoromethane
Concen: 55.59 ug/l
RT: 7.728 min Scan# 969
Delta R.T. -0.000 min
Lab File: VY004900.D
Acq: 27 May 2021 15:00




Instrument :
MSVOA_Y
ClientSampleId :
GHOST-5


Tgt Ion:113 Resp: 102206
Ion Ratio Lower Upper
113 100
111 103.2 80.5 120.7
192 18.6 15.0 22.6

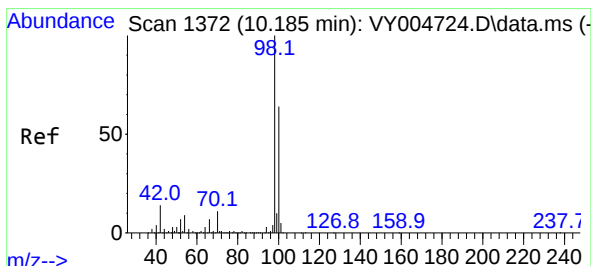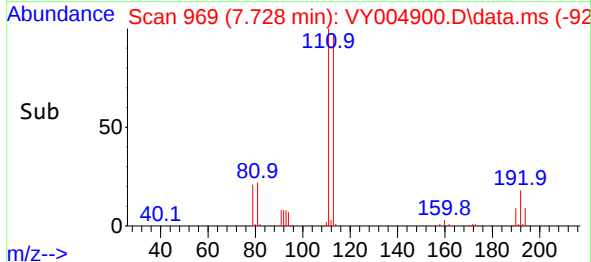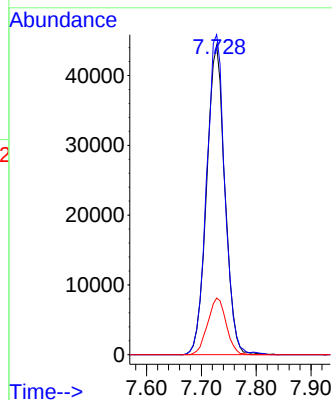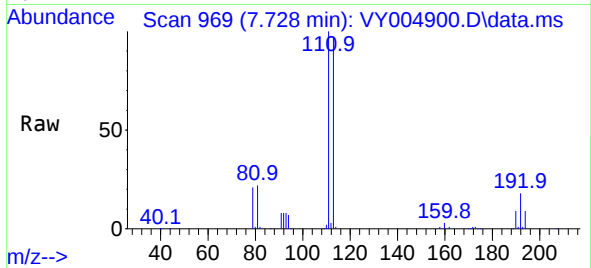

#50
Toluene-d8
Concen: 49.96 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. -0.000 min
Lab File: VY004900.D
Acq: 27 May 2021 15:00

Tgt Ion: 98 Resp: 415002
Ion Ratio Lower Upper
98 100
100 64.1 51.5 77.3


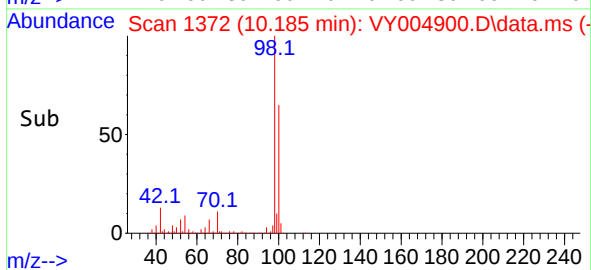
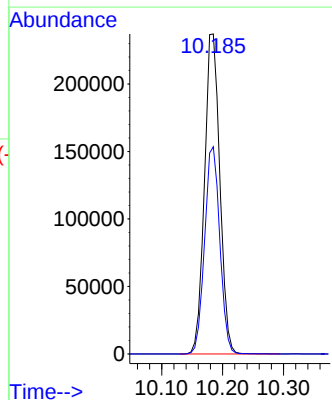
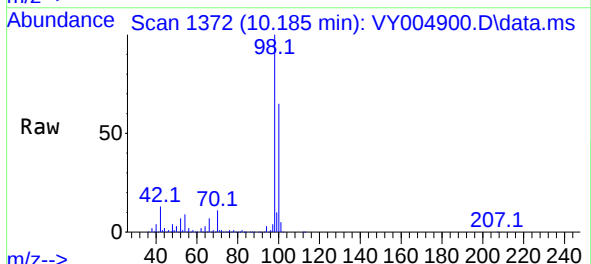


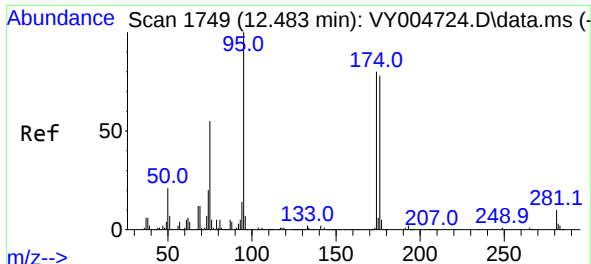

#62
4-Bromofluorobenzene
Concen: 44.76 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY004900.D
Acq: 27 May 2021 15:00




Instrument :
MSVOA_Y
ClientSampleId :
GHOST-5


Tgt Ion: 95 Resp: 125494
Ion Ratio Lower Upper
95 100
174 81.4 0.0 164.2
176 78.3 0.0 159.0

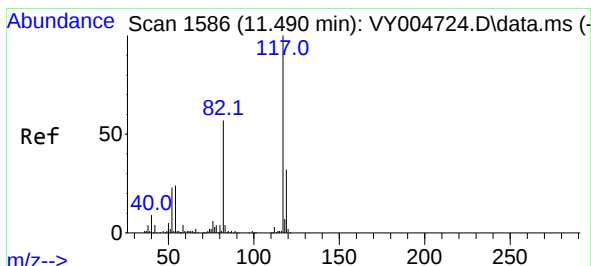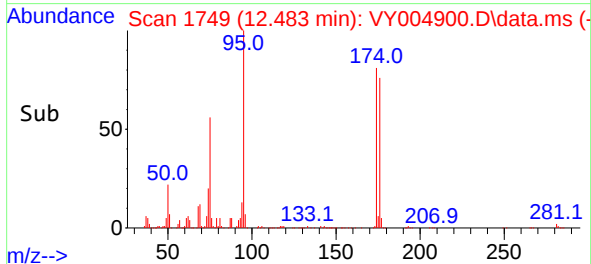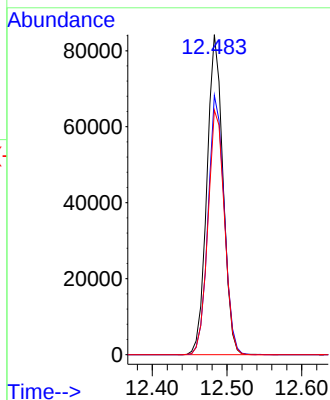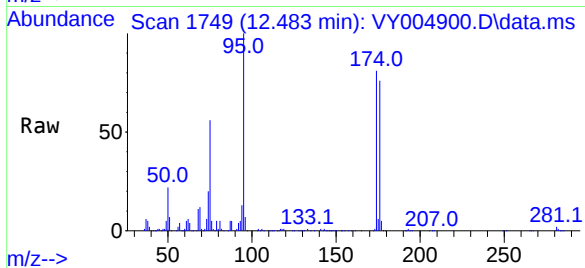

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.495 min Scan# 1587
Delta R.T. 0.006 min
Lab File: VY004900.D
Acq: 27 May 2021 15:00

Tgt Ion: 117 Resp: 308164
Ion Ratio Lower Upper
117 100
82 56.6 45.4 68.2
119 32.6 25.8 38.6

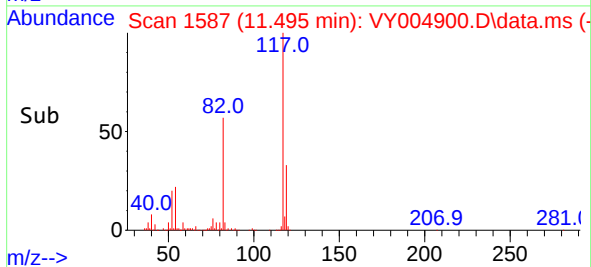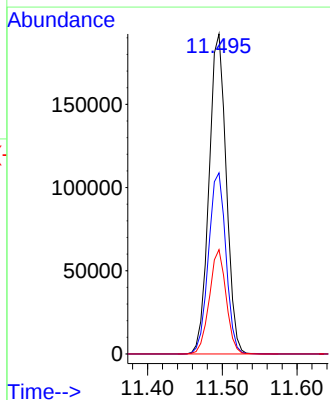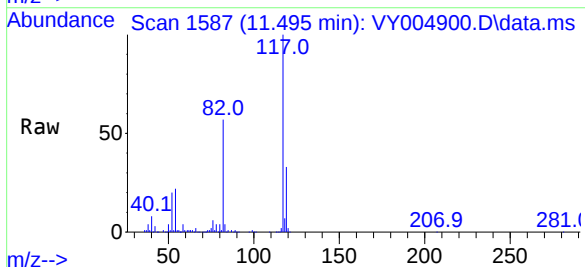

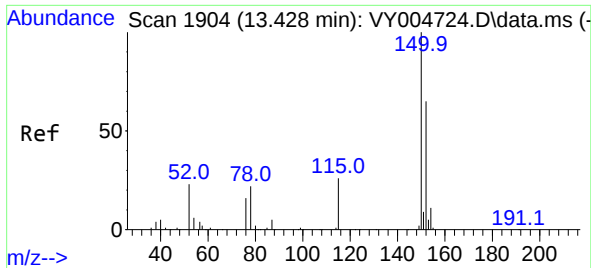

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.00 ug/l
 RT: 13.428 min Scan# 1904
 Delta R.T. -0.000 min
 Lab File: VY004900.D
 Acq: 27 May 2021 15:00

Instrument :
 MSVOA_Y
 ClientSampled :
 GHOST-5

Tgt Ion:152 Resp: 126791
 Ion Ratio Lower Upper
 152 100
 115 58.2 29.4 88.3
 150 157.3 0.0 349.8

