


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv052820\
Data File : VY002780.D
Acq On : 28 May 2020 09:36
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y052720S.M
Title : SW846 8260
Last Update : Wed May 27 13:13:33 2020

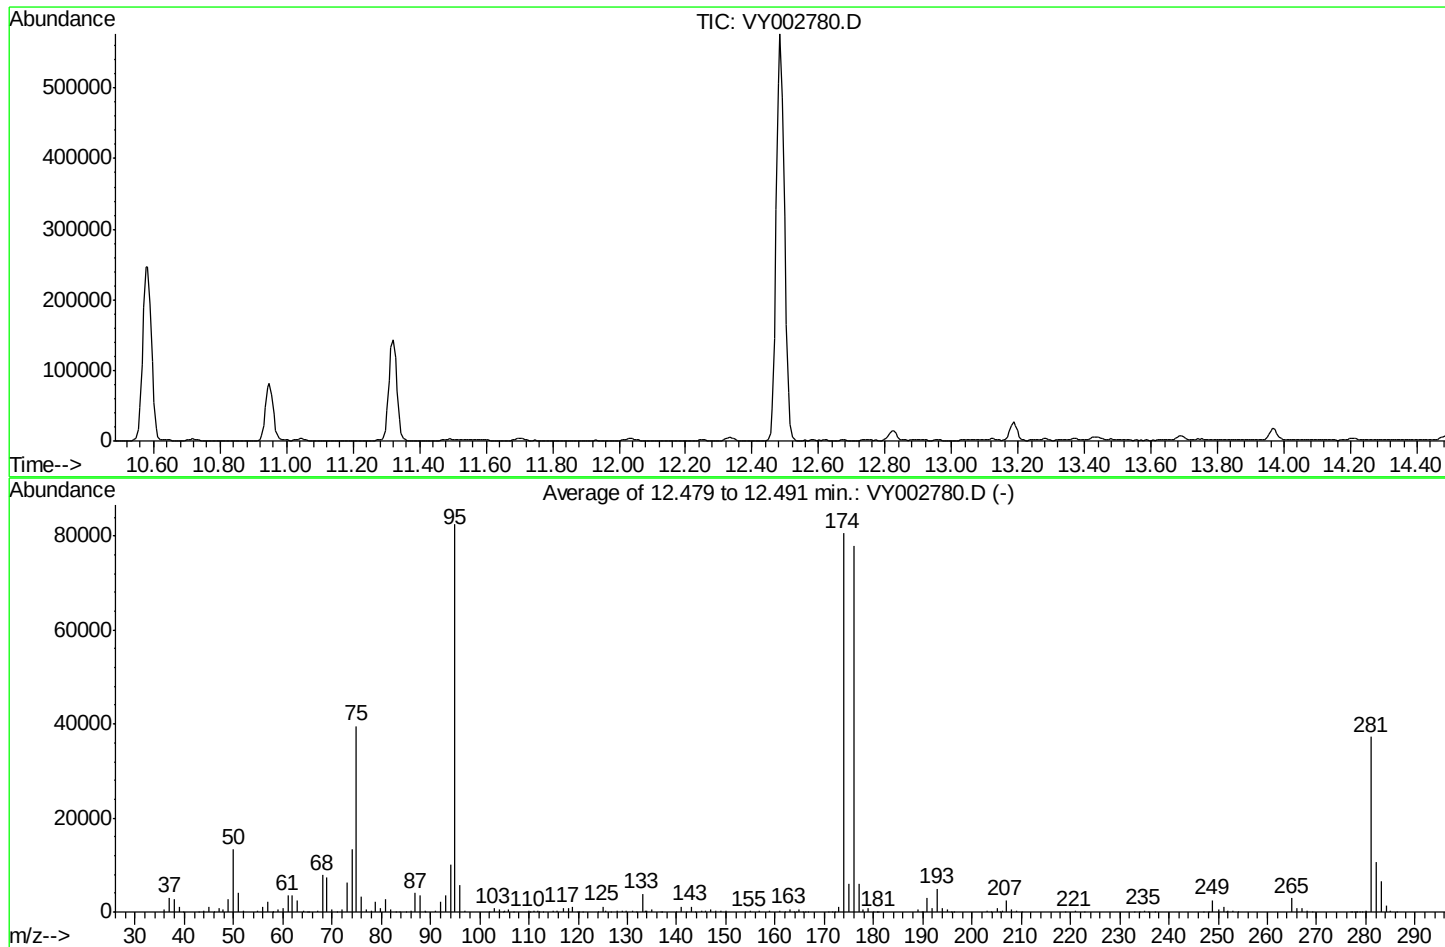

AutoFind: Scans 1762, 1763, 1764; Background Corrected with Scan 1753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	13308	PASS
75	95	30	60	47.9	39522	PASS
95	95	100	100	100.0	82482	PASS
96	95	5	9	6.8	5643	PASS
173	174	0.00	2	1.2	1005	PASS
174	95	50	100	97.7	80552	PASS
175	174	5	9	7.4	5954	PASS
176	174	95	101	96.7	77920	PASS
177	176	5	9	7.8	6076	PASS