
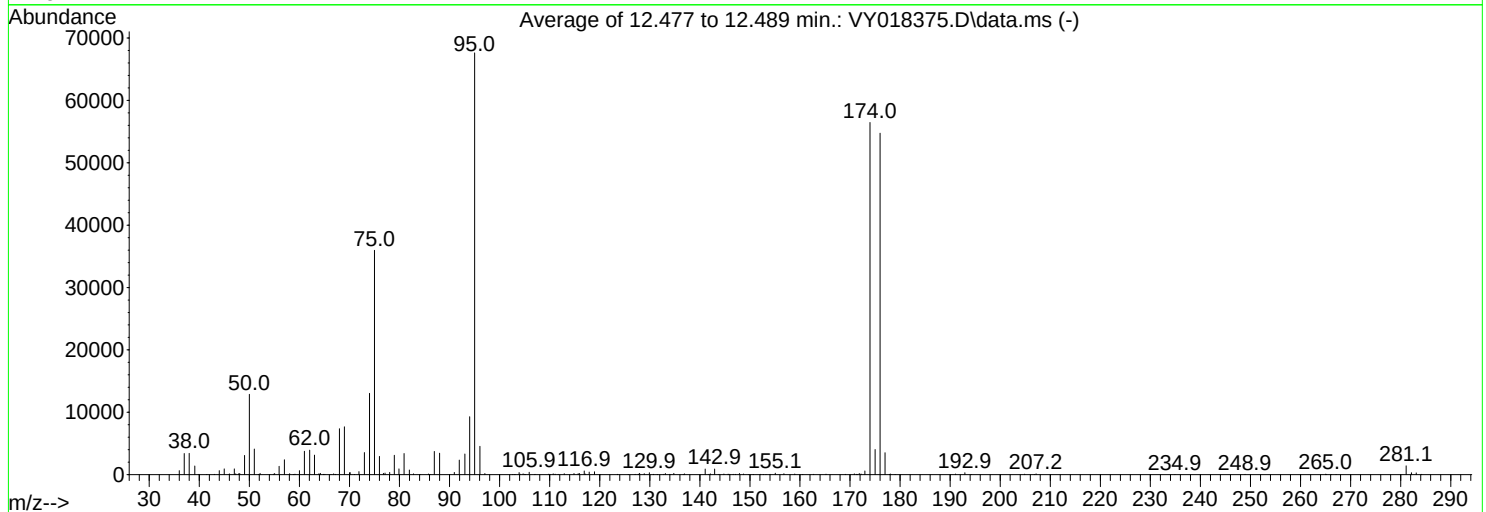


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052824\
Data File : VY018375.D
Acq On : 28 May 2024 09:33
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052224S.M
Title : SW846 8260
Last Update : Thu May 23 01:40:36 2024

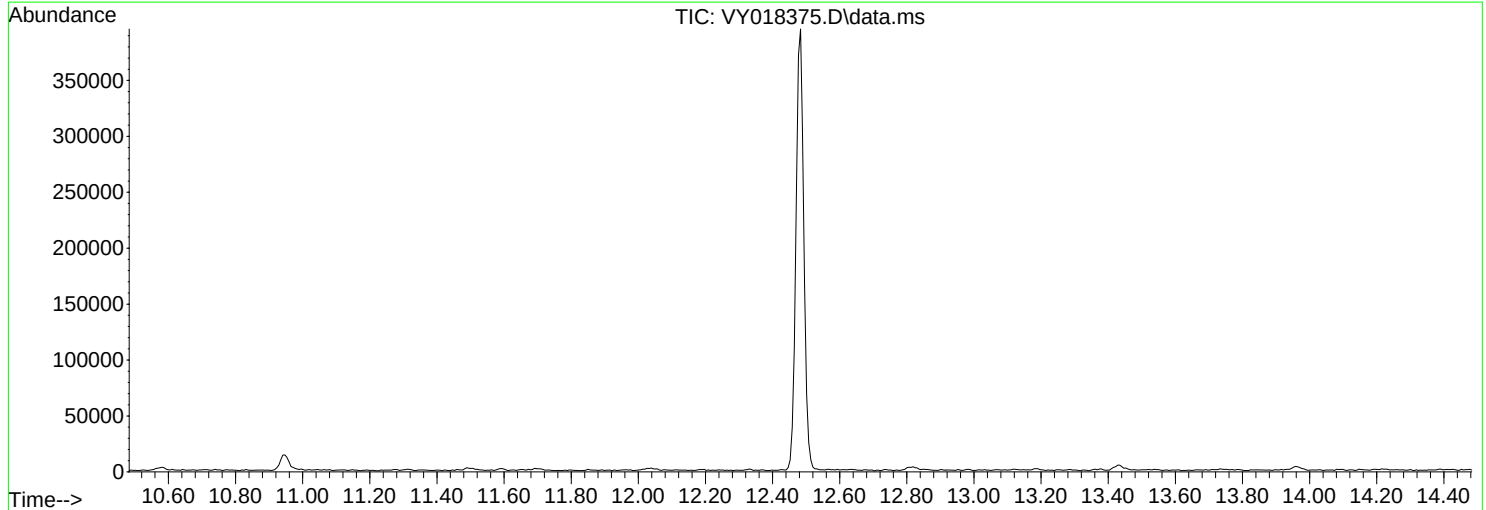

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	12876	PASS
75	95	30	60	53.2	35957	PASS
95	95	100	100	100.0	67627	PASS
96	95	5	9	6.7	4542	PASS
173	174	0.00	2	1.0	585	PASS
174	95	50	100	83.5	56453	PASS
175	174	5	9	7.2	4040	PASS
176	174	95	101	97.0	54744	PASS
177	176	5	9	6.4	3516	PASS