


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_Y\DATA\VY052920\
 Data File : VY002792.D
 Acq On : 29 May 2020 09:37
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y052720S.M
 Title : SW846 8260
 Last Update : Wed May 27 13:13:33 2020

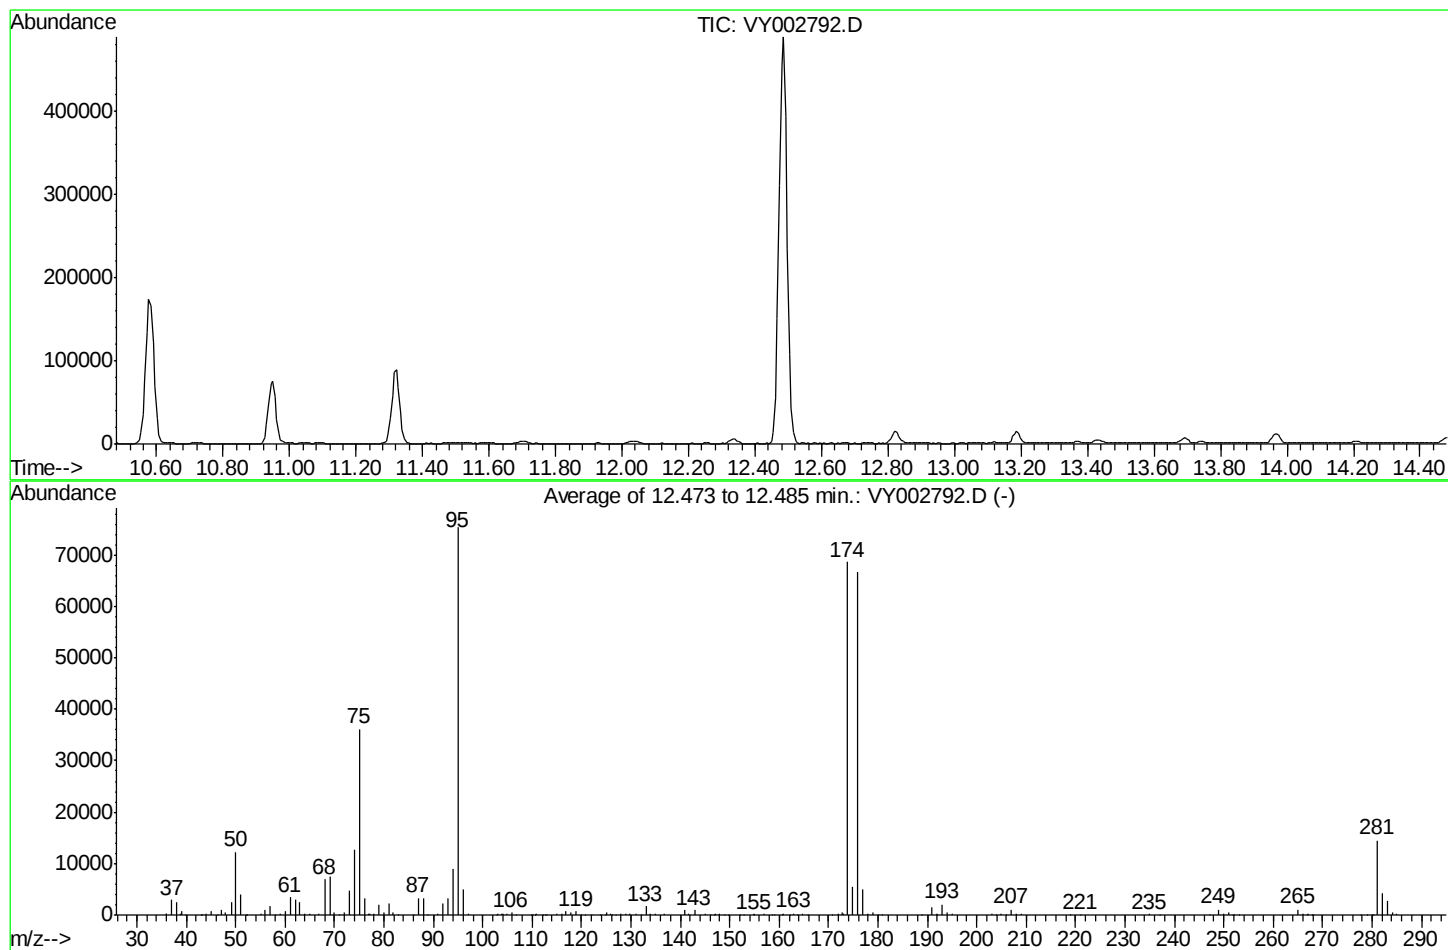

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1754

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	12215	PASS
75	95	30	60	48.0	36200	PASS
95	95	100	100	100.0	75346	PASS
96	95	5	9	6.7	5072	PASS
173	174	0.00	2	0.6	404	PASS
174	95	50	100	91.0	68557	PASS
175	174	5	9	7.8	5369	PASS
176	174	95	101	97.1	66562	PASS
177	176	5	9	7.4	4947	PASS