
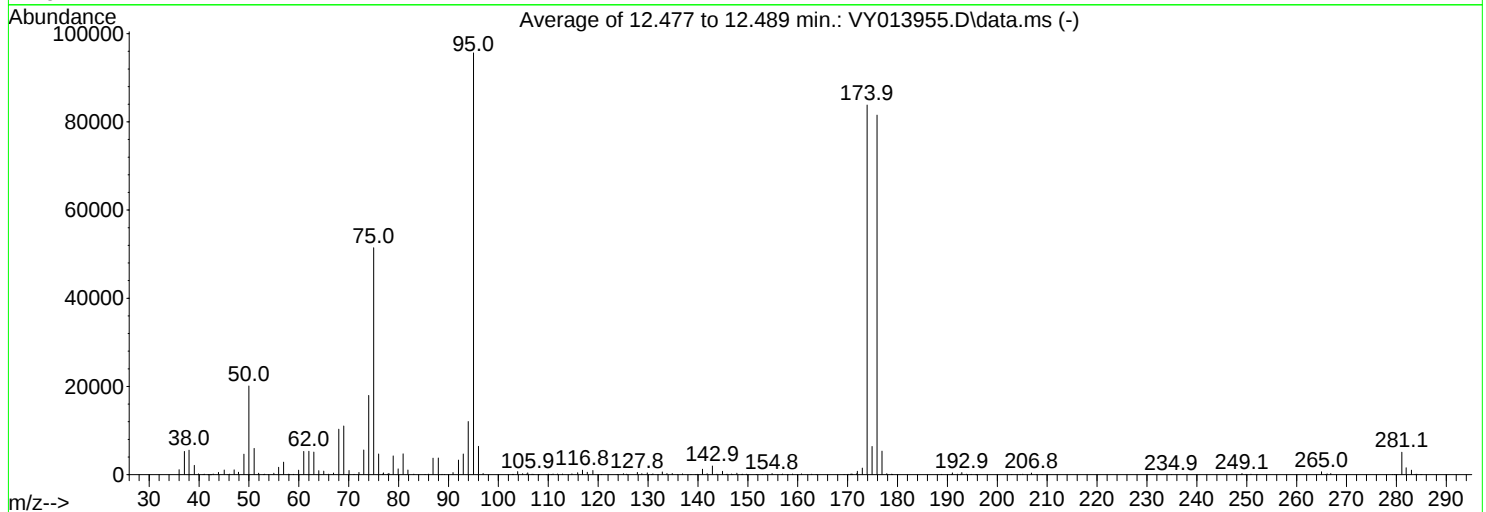


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060123\
Data File : VY013955.D
Acq On : 01 Jun 2023 09:10
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060123S.M
Title : SW846 8260
Last Update : Fri Jun 02 07:00:14 2023

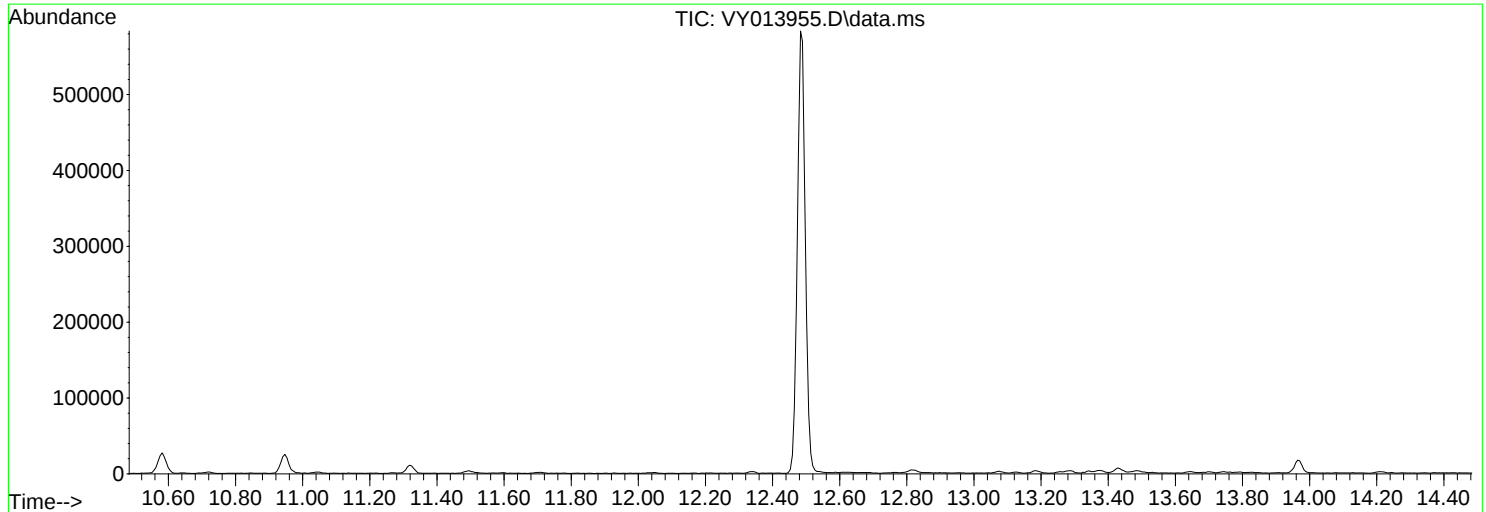

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.0	20120	PASS
75	95	30	60	53.8	51456	PASS
95	95	100	100	100.0	95656	PASS
96	95	5	9	6.7	6419	PASS
173	174	0.00	2	1.8	1483	PASS
174	95	50	100	87.6	83832	PASS
175	174	5	9	7.6	6375	PASS
176	174	95	101	97.3	81528	PASS
177	176	5	9	6.5	5324	PASS