

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060222\
 Data File : VY009125.D
 Acq On : 02 Jun 2022 14:18
 Operator : KP/MD
 Sample : N3099-03
 Misc : 3.35g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 20220426-AMENDED-COMPOSITE-F

Quant Time: Jun 03 03:12:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052022S.M
 Quant Title : SW846 8260
 QLast Update : Fri May 20 23:50:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	117435	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	206684	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	195283	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	86547	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	74037	61.257	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery = 122.520%			
35) Dibromofluoromethane	7.710	113	29223	22.737	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery = 45.480%#			
50) Toluene-d8	10.179	98	261535	55.159	ug/l	0.00
Spiked Amount 50.000	Range 49 - 140		Recovery = 110.320%			
62) 4-Bromofluorobenzene	12.483	95	76294	39.889	ug/l	0.00
Spiked Amount 50.000	Range 25 - 144		Recovery = 79.780%			
Target Compounds					Qvalue	
4) Vinyl Chloride	2.247	62	43347	19.014	ug/l	97
6) Chloroethane	2.790	64	7924	4.906	ug/l	97
11) Tert butyl alcohol	4.930	59	293	2.390	ug/l #	77
12) 1,1-Dichloroethene	3.869	96	4623	4.185	ug/l	87
13) Acrolein	3.710	56	114	2.825	ug/l #	73
16) Acetone	3.942	43	53588	213.003	ug/l	94
17) Carbon Disulfide	4.186	76	100612	27.881	ug/l	100
18) Methyl Acetate	4.686	43	2497	3.187	ug/l #	56
20) Methylene Chloride	4.716	84	6672	Below Cal	#	66
24) 1,1-Dichloroethane	6.009	63	52959	22.140	ug/l	98
25) 2-Butanone	6.984	43	14370	31.979	ug/l #	86
27) cis-1,2-Dichloroethene	6.978	96	33623	21.038	ug/l	81
31) Cyclohexane	7.783	56	11700	4.948	ug/l #	60
36) 1,1-Dichloropropene	7.783	75	10081	4.609	ug/l #	51
37) Ethyl Acetate	6.984	43	14370	12.665	ug/l #	1
38) Carbon Tetrachloride	7.789	117	11912	5.206	ug/l #	15
39) Methylcyclohexane	9.179	83	14751	5.225	ug/l	93
42) 1,2-Dichloroethane	8.234	62	1969	1.063	ug/l	97
44) Trichloroethene	8.935	130	4076	2.441	ug/l	97
49) 1,4-Dioxane	9.295	88	343	26.645	ug/l #	77
55) 1,1,2-Trichloroethane	10.618	97	2717	2.017	ug/l #	20
56) Ethyl methacrylate	10.520	69	1858	1.079	ug/l #	5
59) 2-Hexanone	10.831	43	1405	1.758	ug/l	87
65) Chlorobenzene	11.514	112	5784	1.290	ug/l	100
74) N-amyl acetate	12.099	43	2279	1.526	ug/l #	61
76) 1,2,3-Trichloropropane	12.477	75	46267	49.781	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.477	75	46267	102.176	ug/l #	8
92) 1,2-Dibromo-3-Chloropr...	14.404	75	1993	9.630	ug/l #	6


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060222\
Data File : VY009125.D
Acq On : 02 Jun 2022 14:18
Operator : KP/MD
Sample : N3099-03
Misc : 3.35g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
20220426-AMENDED-COMPOSITE-F

Quant Time: Jun 03 03:12:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052022S.M
Quant Title : SW846 8260
QLast Update : Fri May 20 23:50:52 2022
Response via : Initial Calibration




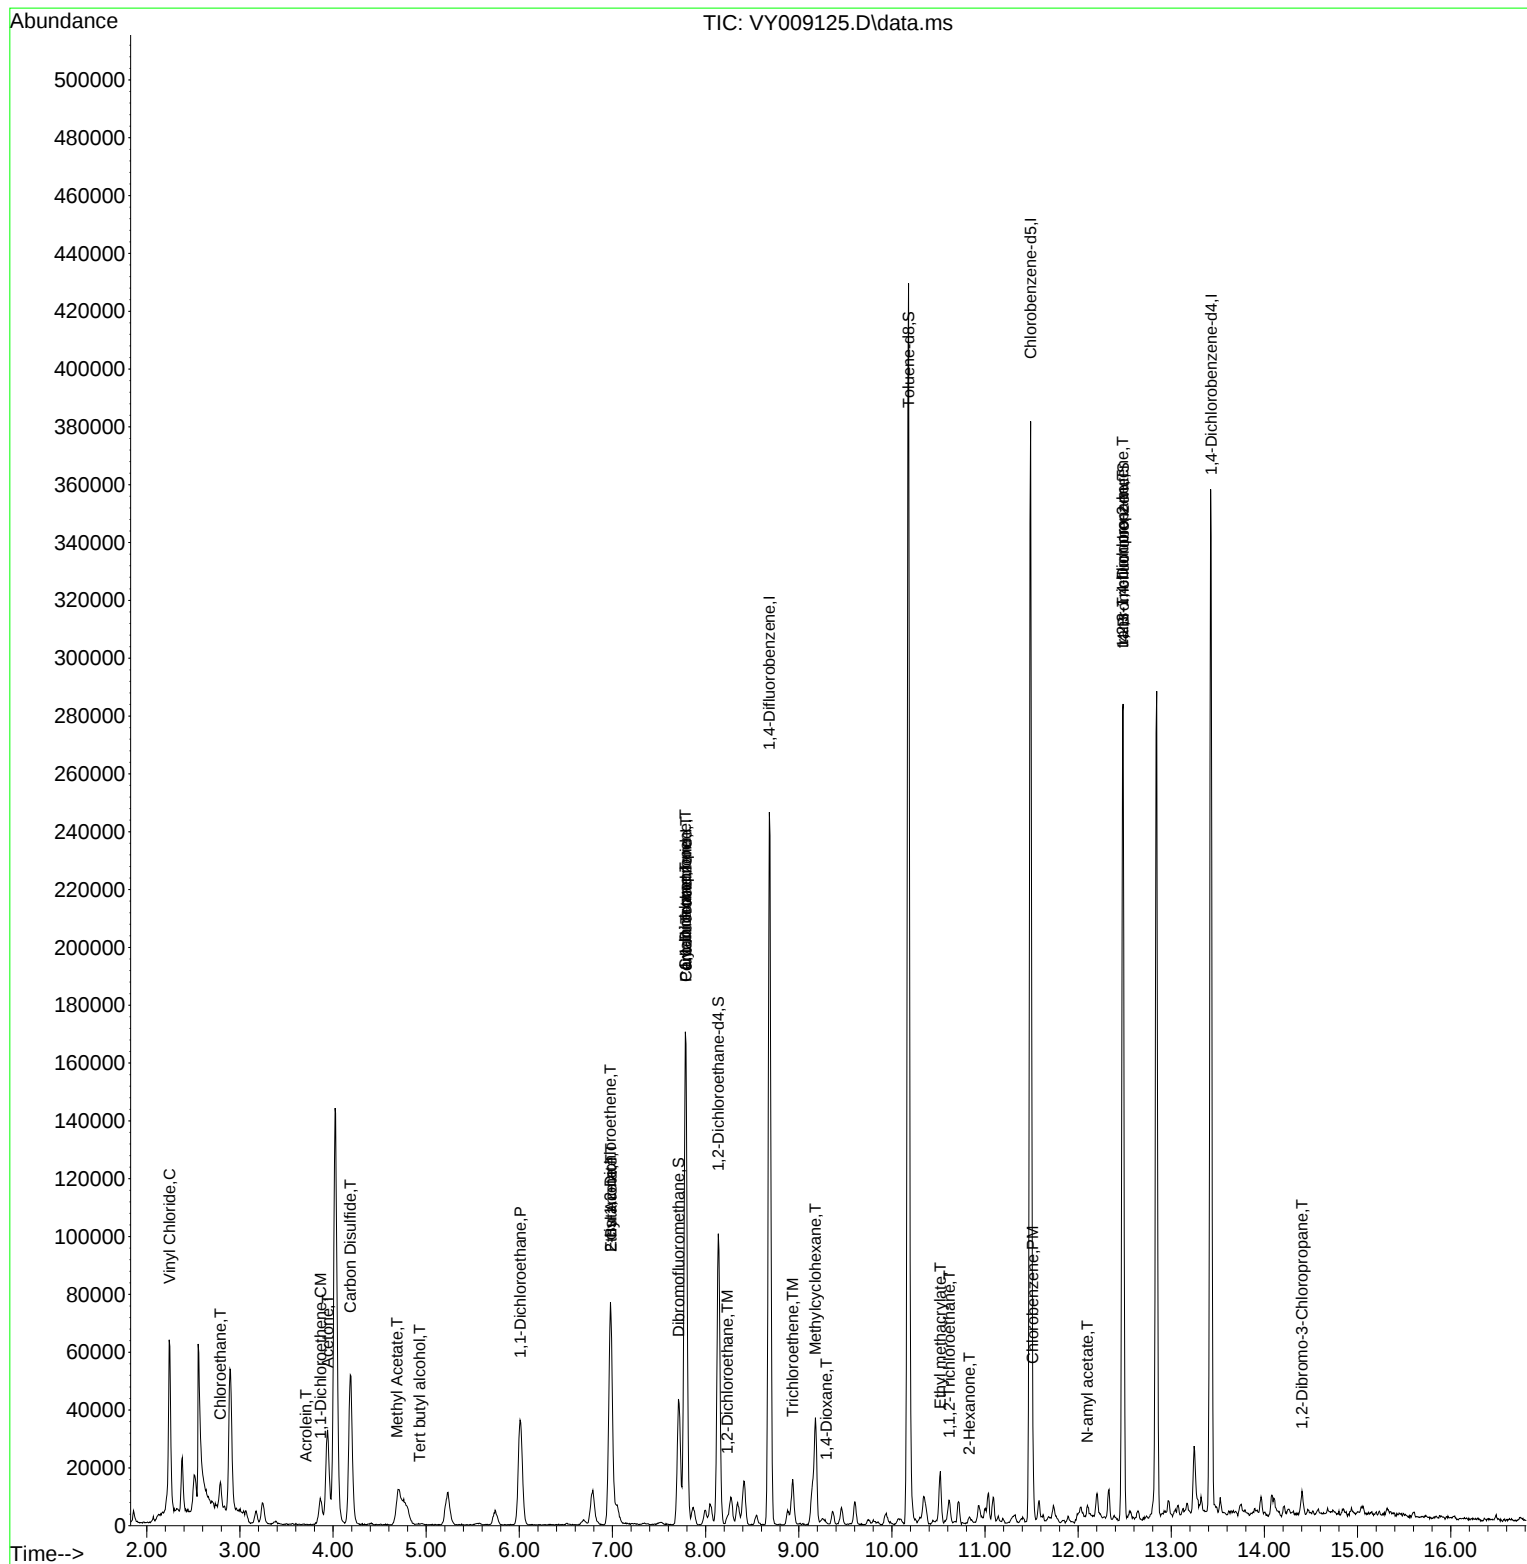




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY009125.D
Acq: 02 Jun 2022 14:18




Instrument :
MSVOA_Y
ClientSampleId :
20220426-AMENDED-COMPOSITE-F


Tgt Ion:168 Resp: 117435
Ion Ratio Lower Upper
168 100
99 51.6 46.9 70.3

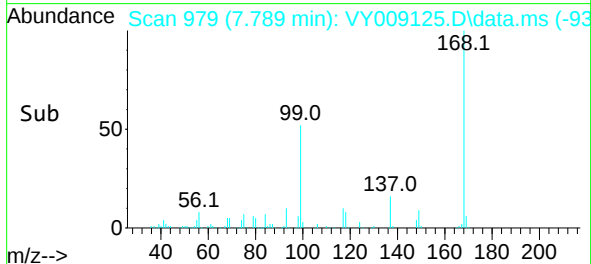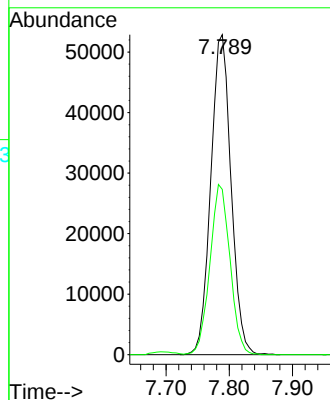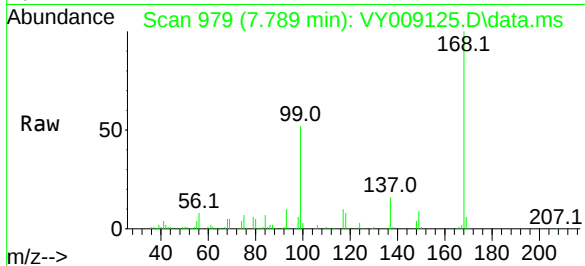

#4
Vinyl Chloride
Concen: 19.014 ug/l
RT: 2.247 min Scan# 70
Delta R.T. 0.000 min
Lab File: VY009125.D
Acq: 02 Jun 2022 14:18

Tgt Ion: 62 Resp: 43347
Ion Ratio Lower Upper
62 100
64 33.0 25.0 37.6


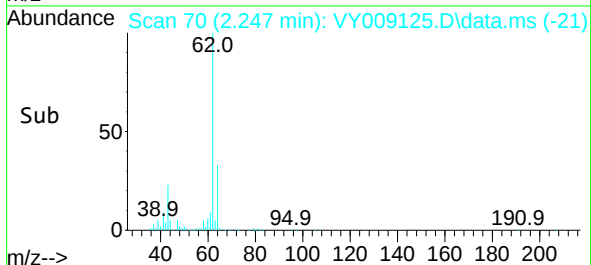
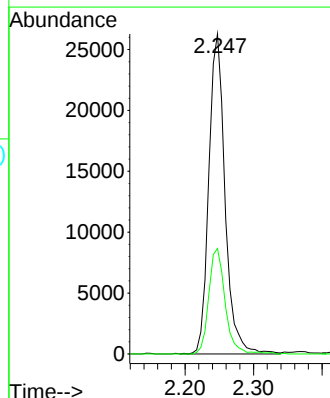
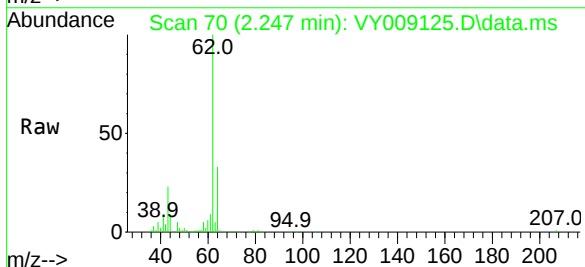


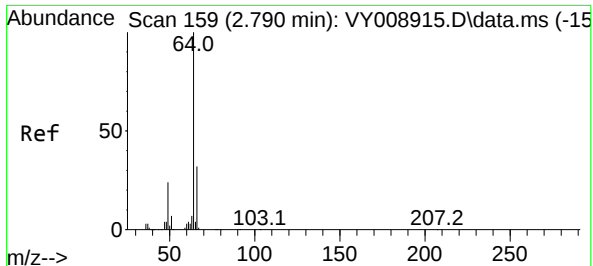

#6
Chloroethane
Concen: 4.906 ug/l
RT: 2.790 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY009125.D
Acq: 02 Jun 2022 14:18




Instrument : MSVOA_Y
ClientSampleId : 20220426-AMENDED-COMPOSITE-F


Tgt Ion: 64 Resp: 7924
Ion Ratio Lower Upper
64 100
66 33.4 25.4 38.0

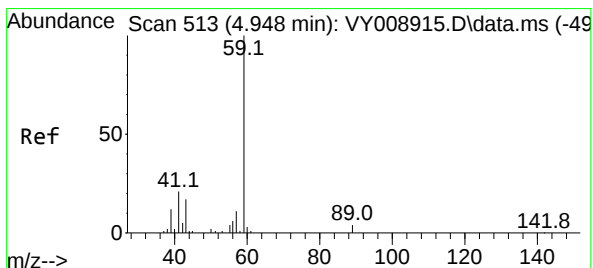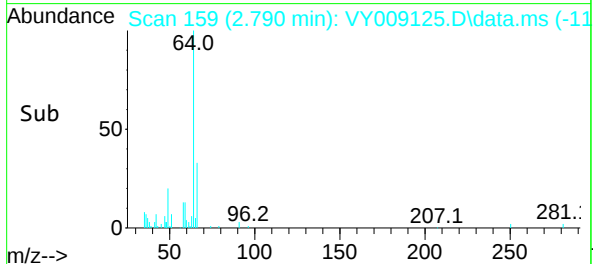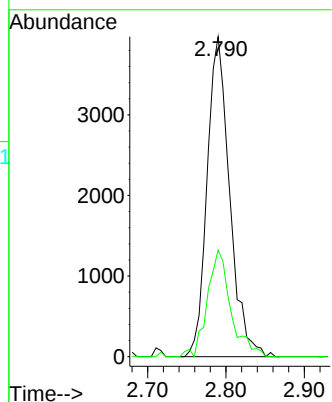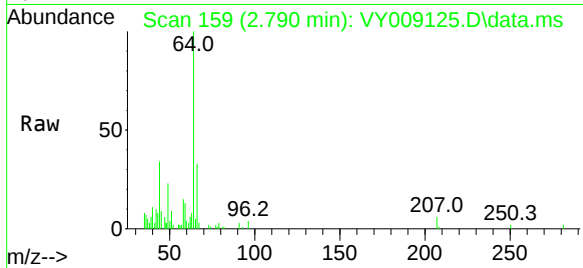

#11
Tert butyl alcohol
Concen: 2.390 ug/l
RT: 4.930 min Scan# 510
Delta R.T. -0.018 min
Lab File: VY009125.D
Acq: 02 Jun 2022 14:18

Tgt Ion: 59 Resp: 293
Ion Ratio Lower Upper
59 100
57 0.0 6.4 9.6#

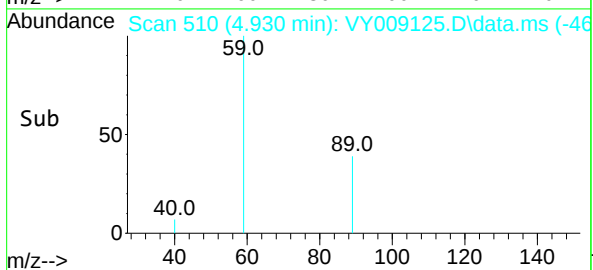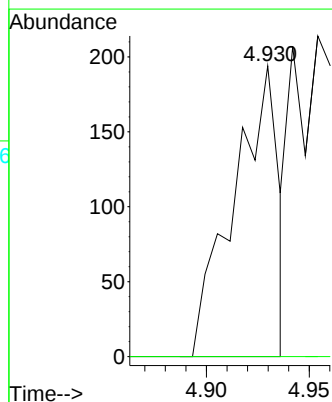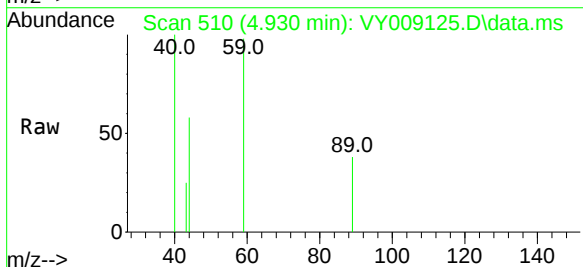



#12

1,1-Dichloroethene

Concen: 4.185 ug/l

RT: 3.869 min Scan# 310

Delta R.T. 0.006 min

Lab File: VY009125.D


Acq: 02 Jun 2022 14:18

Instrument :

MSVOA_Y

ClientSampleId :

20220426-AMENDED-COMPOSITE-F






Tgt Ion: 96 Resp: 4623

Ion Ratio Lower Upper

96 100

61 159.1 145.8 218.6

98 62.2 52.5 78.7

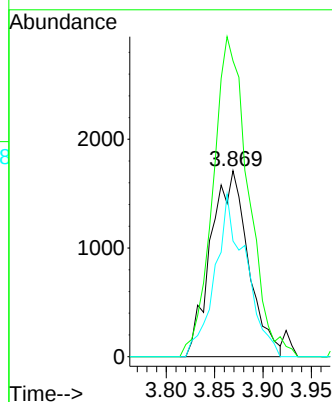

#13

Acrolein

Concen: 2.825 ug/l

RT: 3.710 min Scan# 310

Delta R.T. -0.013 min

Lab File: VY009125.D




Acq: 02 Jun 2022 14:18


Tgt Ion: 56 Resp: 114

Ion Ratio Lower Upper

56 100

55 94.7 57.6 86.4#


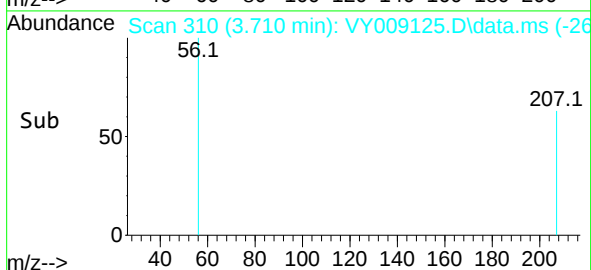






#16
Acetone
Concen: 213.003 ug/l
RT: 3.942 min Scan# 349
Delta R.T. -0.006 min
Lab File: VY009125.D
Acq: 02 Jun 2022 14:18




Instrument : MSVOA_Y
ClientSampleId : 20220426-AMENDED-COMPOSITE-F


Tgt Ion: 43 Resp: 53588
Ion Ratio Lower Upper
43 100
58 30.8 22.0 33.0

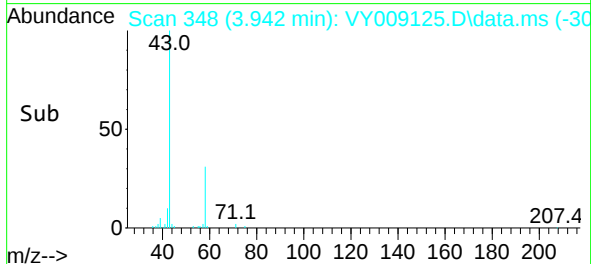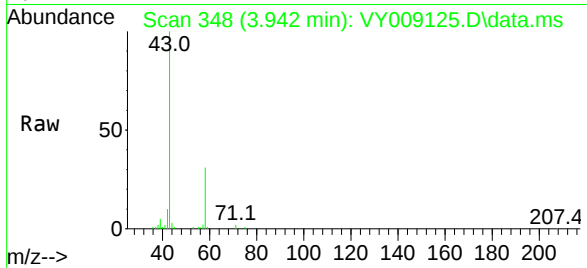

#17
Carbon Disulfide
Concen: 27.881 ug/l
RT: 4.186 min Scan# 388
Delta R.T. 0.000 min
Lab File: VY009125.D
Acq: 02 Jun 2022 14:18

Tgt Ion: 76 Resp: 100612
Ion Ratio Lower Upper
76 100
78 9.2 7.4 11.0




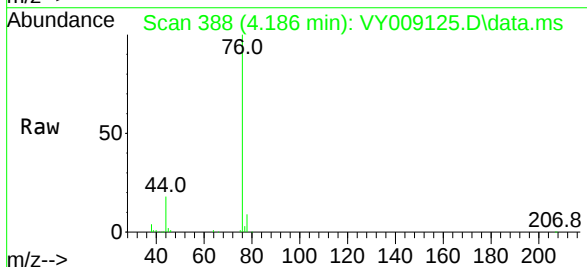




#18
Methyl Acetate
Concen: 3.187 ug/l
RT: 4.686 min Scan# 41
Delta R.T. 0.213 min
Lab File: VY009125.D
Acq: 02 Jun 2022 14:18




Instrument :
MSVOA_Y
ClientSampleId :
20220426-AMENDED-COMPOSITE-F


Tgt Ion: 43 Resp: 2497
Ion Ratio Lower Upper
43 100
74 0.0 16.6 24.8#

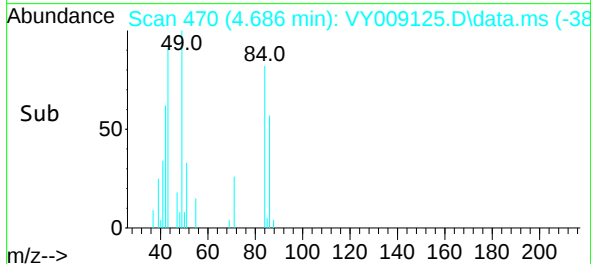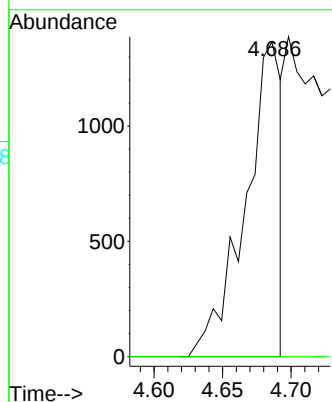

#20
Methylene Chloride
Concen: Below Cal
RT: 4.716 min Scan# 475
Delta R.T. 0.006 min
Lab File: VY009125.D
Acq: 02 Jun 2022 14:18

Tgt Ion: 84 Resp: 6672
Ion Ratio Lower Upper
84 100
49 84.3 114.4 171.6#
51 32.4 35.3 52.9#
86 55.3 53.7 80.5


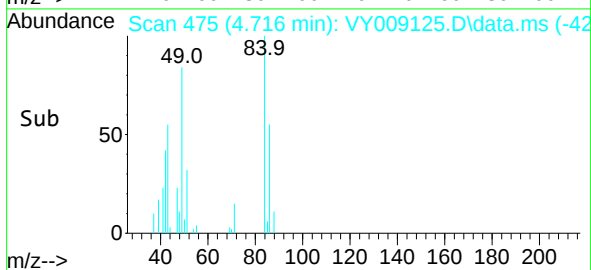

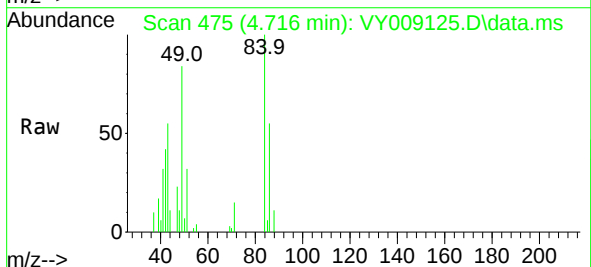




#24
1,1-Dichloroethane
Concen: 22.140 ug/l
RT: 6.009 min Scan# 61
Delta R.T. -0.006 min
Lab File: VY009125.D
Acq: 02 Jun 2022 14:18




Instrument :
MSVOA_Y
ClientSampleId :
20220426-AMENDED-COMPOSITE-F


Tgt Ion: 63 Resp: 52959
Ion Ratio Lower Upper
63 100
98 7.0 3.6 10.8
100 5.2 2.0 5.8

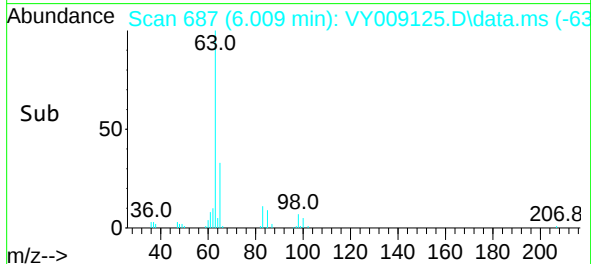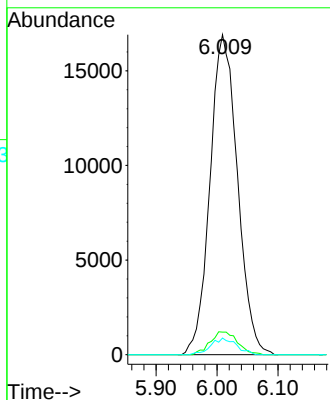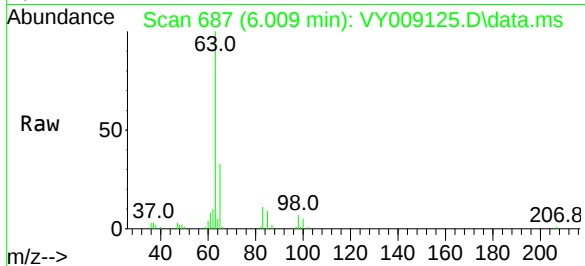

#25
2-Butanone
Concen: 31.979 ug/l
RT: 6.984 min Scan# 847
Delta R.T. 0.000 min
Lab File: VY009125.D
Acq: 02 Jun 2022 14:18

Tgt Ion: 43 Resp: 14370
Ion Ratio Lower Upper
43 100
72 28.6 17.7 26.5#

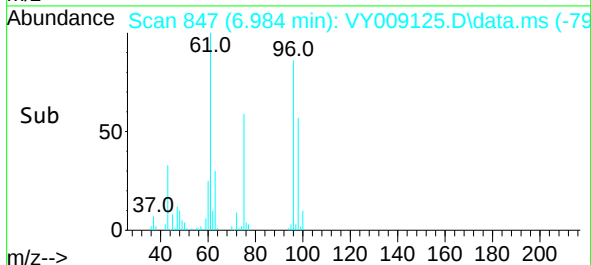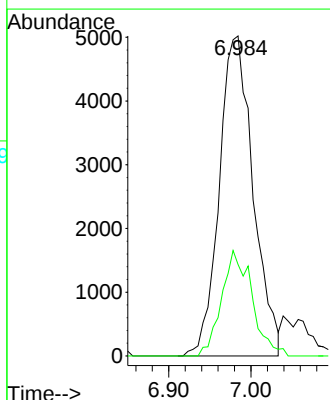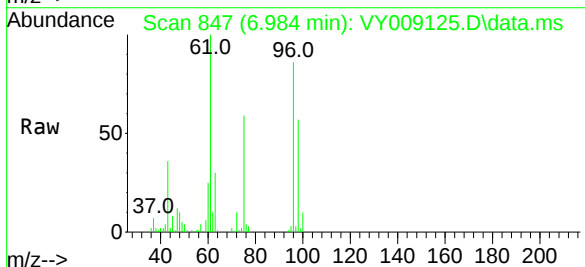



#27

cis-1,2-Dichloroethene

Concen: 21.038 ug/l

RT: 6.978 min Scan# 847

Delta R.T. -0.006 min

Lab File: VY009125.D


Acq: 02 Jun 2022 14:18

Instrument :

MSVOA_Y

ClientSampleId :

20220426-AMENDED-COMPOSITE-F

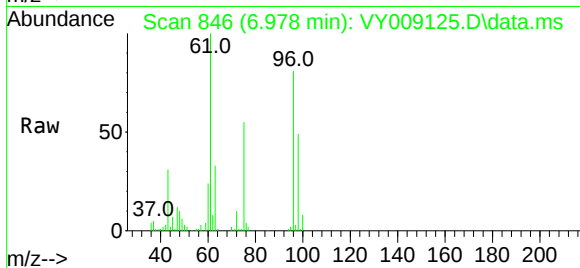




Tgt Ion: 96 Resp: 33623

Ion Ratio Lower Upper

96 100

61 124.6 0.0 319.8

98 63.0 0.0 127.0

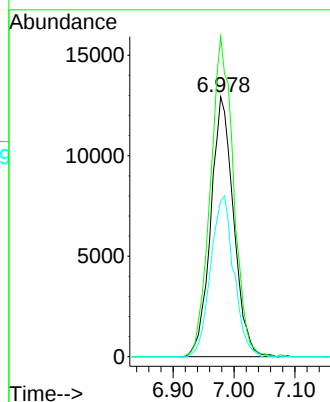

#31

Cyclohexane

Concen: 4.948 ug/l

RT: 7.783 min Scan# 978

Delta R.T. -0.000 min

Lab File: VY009125.D

Acq: 02 Jun 2022 14:18




Tgt Ion: 56 Resp: 11700


Ion Ratio Lower Upper

56 100

69 62.1 26.7 40.1#

84 115.9 67.2 100.8#

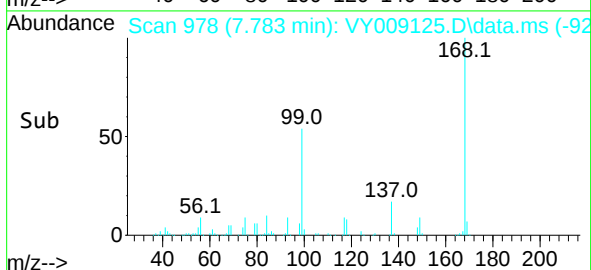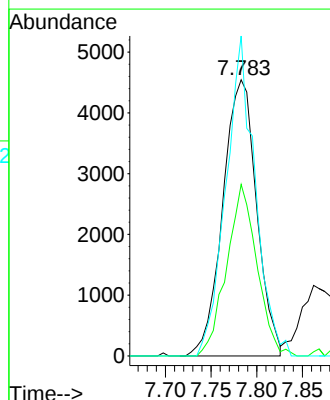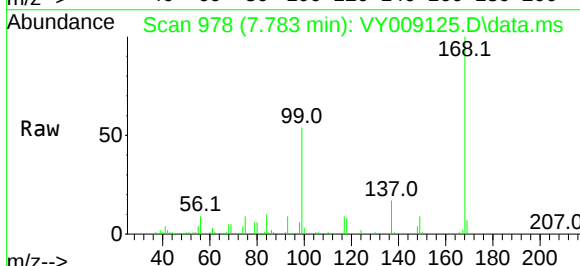



#33

1,2-Dichloroethane-d4

Concen: 61.257 ug/l

RT: 8.136 min Scan# 1036

Delta R.T. -0.007 min

Lab File: VY009125.D

Acq: 02 Jun 2022 14:18

Instrument :

MSVOA_Y

ClientSampleId :





20220426-AMENDED-COMPOSITE-F

Tgt Ion: 65 Resp: 74037

Ion Ratio Lower Upper

65 100

67 53.0 0.0 99.4

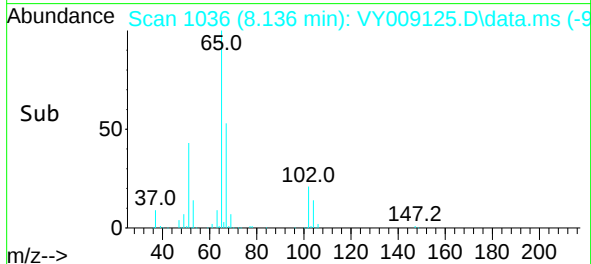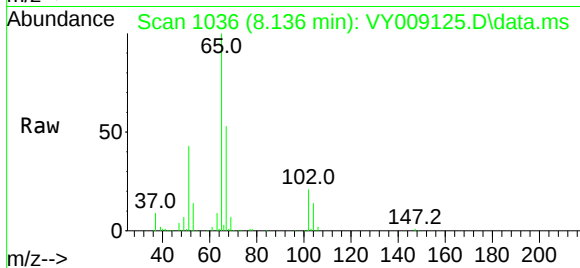

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. 0.000 min

Lab File: VY009125.D

Acq: 02 Jun 2022 14:18




Tgt Ion: 114 Resp: 206684


Ion Ratio Lower Upper

114 100

63 19.8 0.0 43.2

88 13.0 0.0 31.8


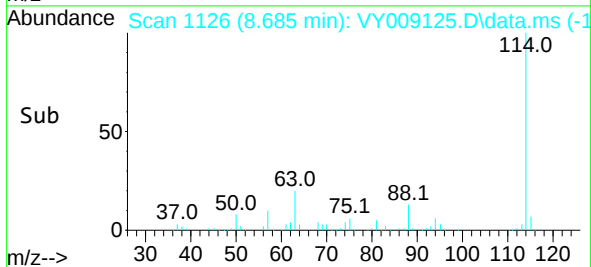

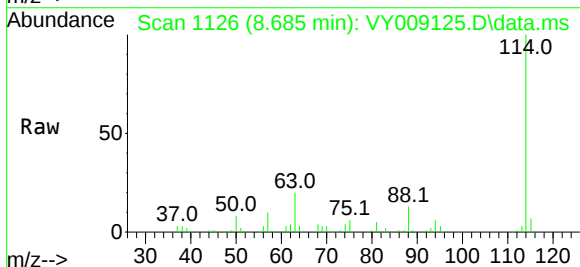




#35
Dibromofluoromethane
Concen: 22.737 ug/l
RT: 7.710 min Scan# 910
Delta R.T. -0.006 min
Lab File: VY009125.D
Acq: 02 Jun 2022 14:18




Instrument : MSVOA_Y
ClientSampleId : 20220426-AMENDED-COMPOSITE-F


Tgt Ion:113 Resp: 29223
Ion Ratio Lower Upper
113 100
111 102.8 82.6 124.0
192 19.1 17.6 26.4

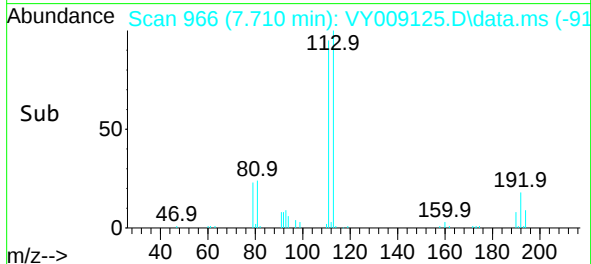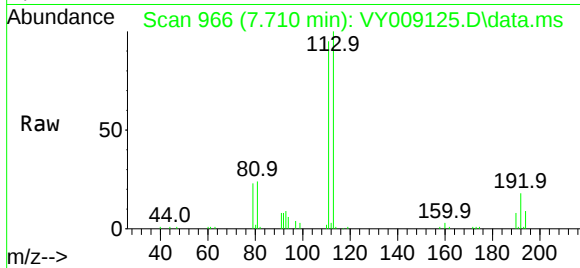

#36
1,1-Dichloropropene
Concen: 4.609 ug/l
RT: 7.783 min Scan# 978
Delta R.T. -0.128 min
Lab File: VY009125.D
Acq: 02 Jun 2022 14:18

Tgt Ion: 75 Resp: 10081
Ion Ratio Lower Upper
75 100
110 8.9 17.1 51.2#
77 0.6 24.4 36.6#



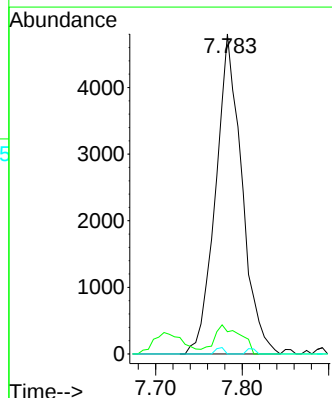
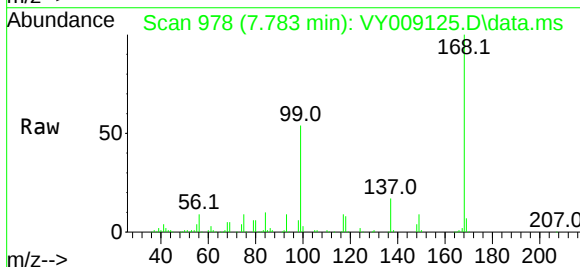




#37
Ethyl Acetate
Concen: 12.665 ug/l
RT: 6.984 min Scan# 847
Delta R.T. -0.092 min
Lab File: VY009125.D
Acq: 02 Jun 2022 14:18




Instrument : MSVOA_Y
ClientSampleId : 20220426-AMENDED-COMPOSITE-F


Tgt Ion: 43 Resp: 14370
Ion Ratio Lower Upper
43 100
61 291.5 9.7 14.5#
70 5.0 7.1 10.7#

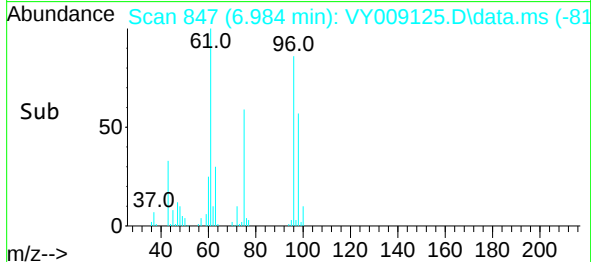

#38
Carbon Tetrachloride
Concen: 5.206 ug/l
RT: 7.789 min Scan# 979
Delta R.T. -0.110 min
Lab File: VY009125.D
Acq: 02 Jun 2022 14:18

Tgt Ion: 117 Resp: 11912
Ion Ratio Lower Upper
117 100
119 4.3 77.9 116.9#
121 0.0 24.8 37.2#

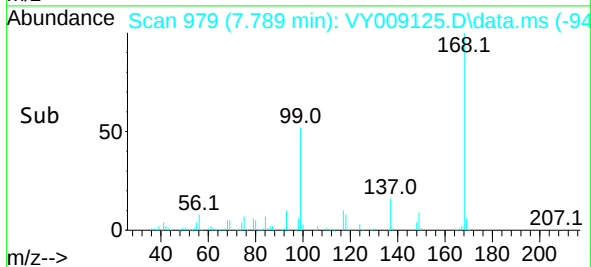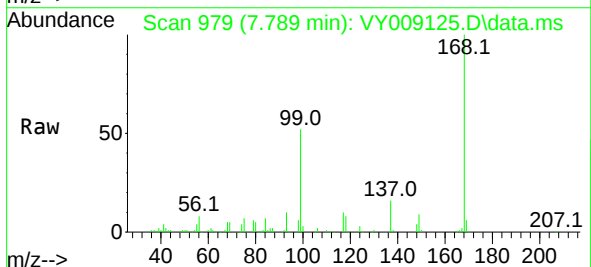

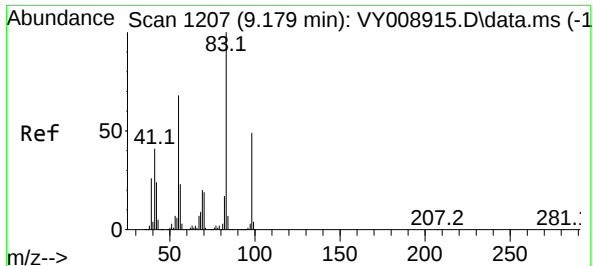

#39

Methylcyclohexane

Concen: 5.225 ug/l

RT: 9.179 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY009125.D

Acq: 02 Jun 2022 14:18

Instrument :

MSVOA_Y

ClientSampleId :

20220426-AMENDED-COMPOSITE-F





Tgt Ion: 83 Resp: 14751

Ion Ratio Lower Upper

83 100

55 77.0 66.5 99.7

98 53.2 37.9 56.9

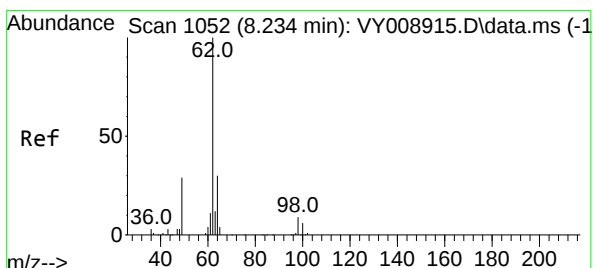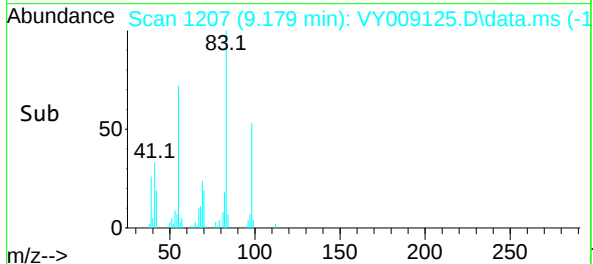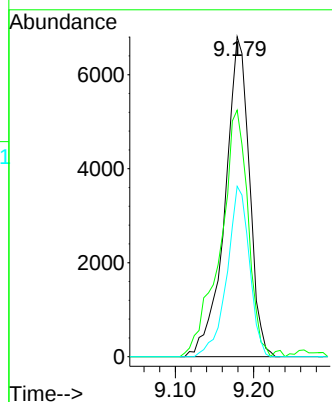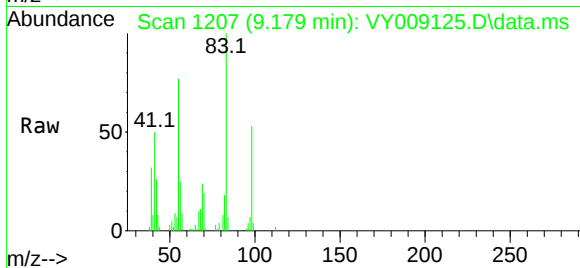

#42

1,2-Dichloroethane

Concen: 1.063 ug/l

RT: 8.234 min Scan# 1052

Delta R.T. 0.000 min

Lab File: VY009125.D




Acq: 02 Jun 2022 14:18


Tgt Ion: 62 Resp: 1969

Ion Ratio Lower Upper

62 100

98 6.4 0.0 14.8


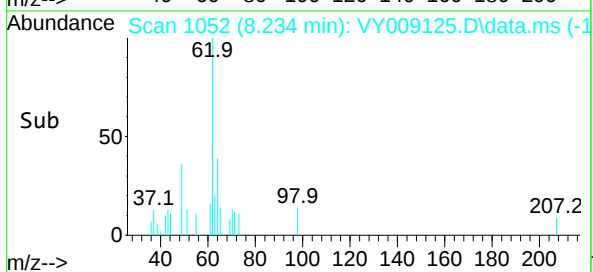
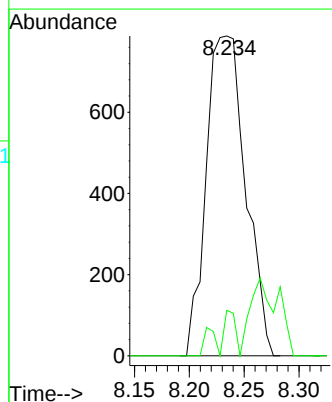
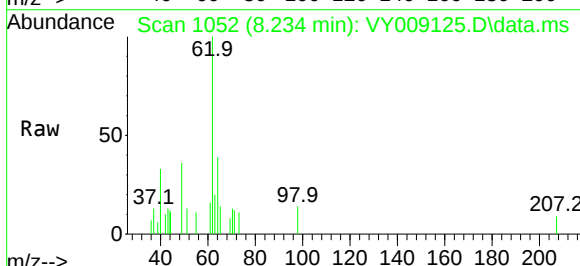




#44
Trichloroethene
Concen: 2.441 ug/l
RT: 8.935 min Scan# 1167
Delta R.T. 0.000 min
Lab File: VY009125.D
Acq: 02 Jun 2022 14:18




Instrument : MSVOA_Y
ClientSampleId : 20220426-AMENDED-COMPOSITE-F


Tgt Ion: 130 Resp: 4076
Ion Ratio Lower Upper
130 100
95 90.8 0.0 188.2

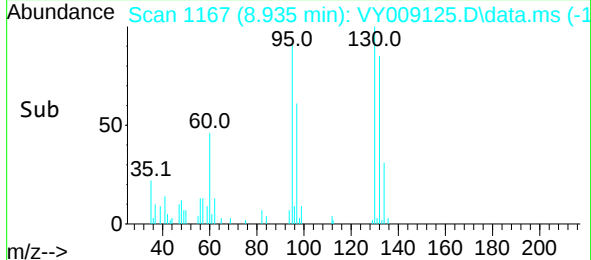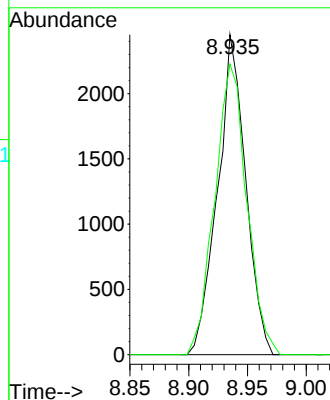

#49
1,4-Dioxane
Concen: 26.645 ug/l
RT: 9.295 min Scan# 1226
Delta R.T. 0.006 min
Lab File: VY009125.D
Acq: 02 Jun 2022 14:18

Tgt Ion: 88 Resp: 343
Ion Ratio Lower Upper
88 100
43 0.0 32.8 49.2#
58 74.9 59.8 89.6


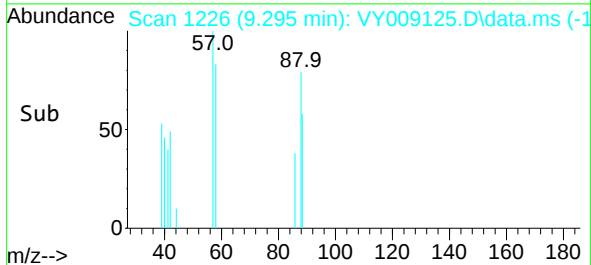
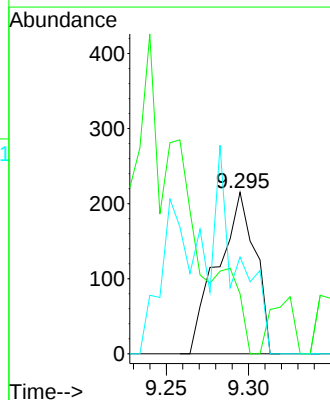
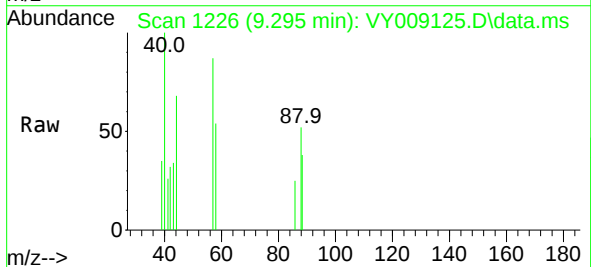




#50
Toluene-d8
Concen: 55.159 ug/l
RT: 10.179 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY009125.D
Acq: 02 Jun 2022 14:18




Instrument : MSVOA_Y
ClientSampleId : 20220426-AMENDED-COMPOSITE-F


Tgt Ion: 98 Resp: 261535
Ion Ratio Lower Upper
98 100
100 63.7 50.2 75.2

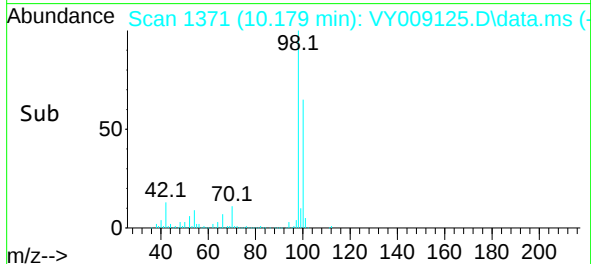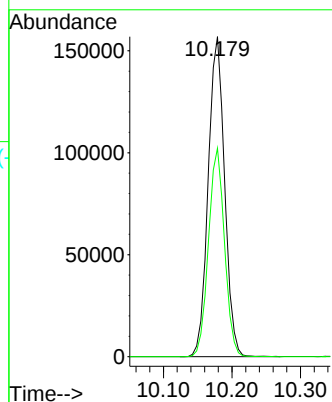

#55
1,1,2-Trichloroethane
Concen: 2.017 ug/l
RT: 10.618 min Scan# 1443
Delta R.T. -0.024 min
Lab File: VY009125.D
Acq: 02 Jun 2022 14:18

Tgt Ion: 97 Resp: 2717
Ion Ratio Lower Upper
97 100
83 10.6 69.8 104.8#
85 0.0 44.3 66.5#
99 0.0 49.8 74.6#


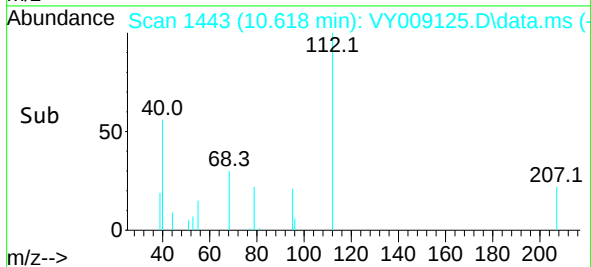

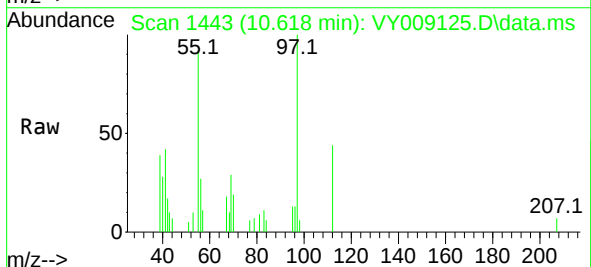


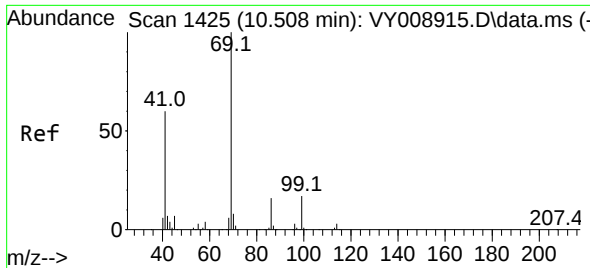

#56
Ethyl methacrylate
Concen: 1.079 ug/l
RT: 10.520 min Scan# 1425
Delta R.T. 0.012 min
Lab File: VY009125.D
Acq: 02 Jun 2022 14:18




Instrument : MSVOA_Y
ClientSampleId : 20220426-AMENDED-COMPOSITE-F


Tgt Ion: 69 Resp: 1858
Ion Ratio Lower Upper
69 100
41 171.9 63.4 95.0#
39 93.8 35.8 53.8#

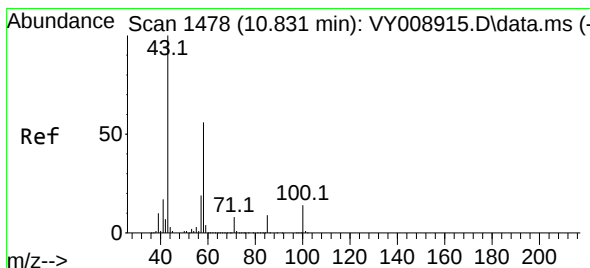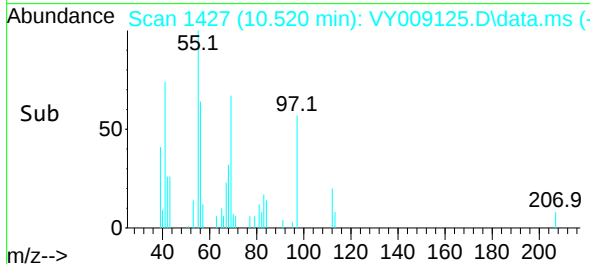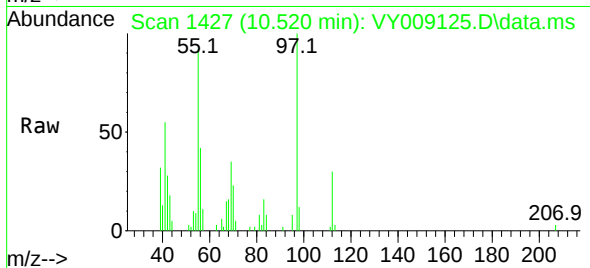

#59
2-Hexanone
Concen: 1.758 ug/l
RT: 10.831 min Scan# 1478
Delta R.T. 0.000 min
Lab File: VY009125.D
Acq: 02 Jun 2022 14:18

Tgt Ion: 43 Resp: 1405
Ion Ratio Lower Upper
43 100
58 39.9 24.4 73.4


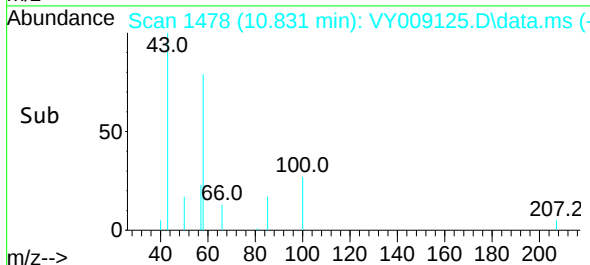

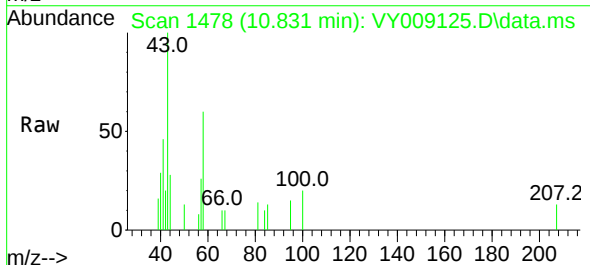




#62
4-Bromofluorobenzene
Concen: 39.889 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY009125.D
Acq: 02 Jun 2022 14:18




Instrument :
MSVOA_Y
ClientSampleId :
20220426-AMENDED-COMPOSITE-F


Tgt Ion: 95 Resp: 76294
Ion Ratio Lower Upper
95 100
174 91.1 0.0 177.0
176 87.8 0.0 175.8

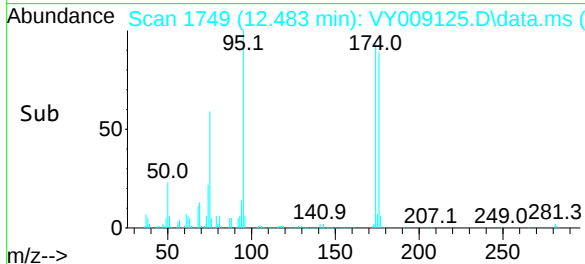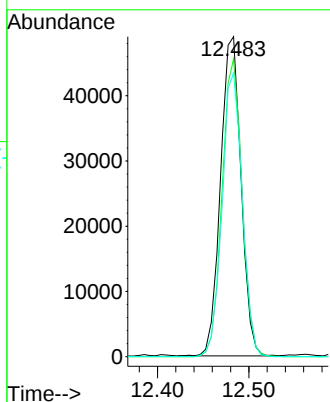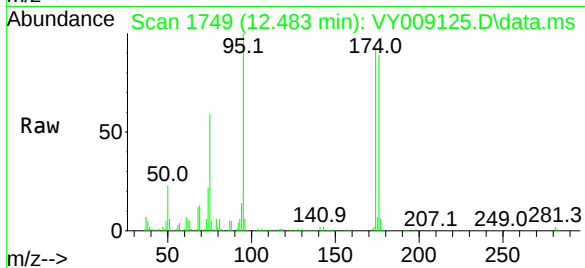

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 1586
Delta R.T. -0.000 min
Lab File: VY009125.D
Acq: 02 Jun 2022 14:18

Tgt Ion: 117 Resp: 195283
Ion Ratio Lower Upper
117 100
82 54.1 43.0 64.4
119 31.2 25.4 38.0


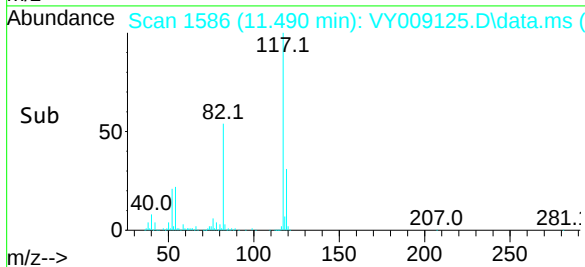
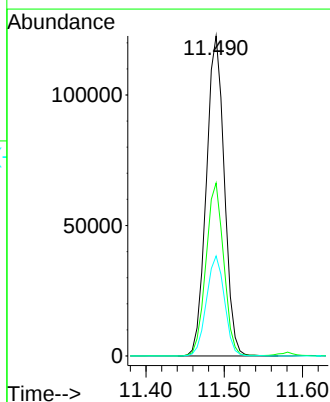
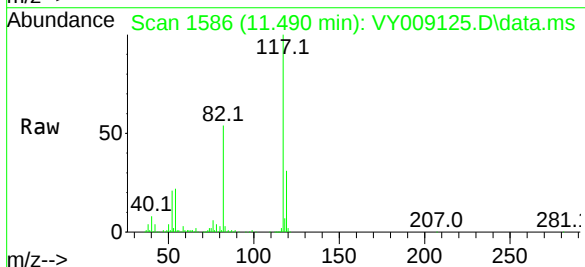


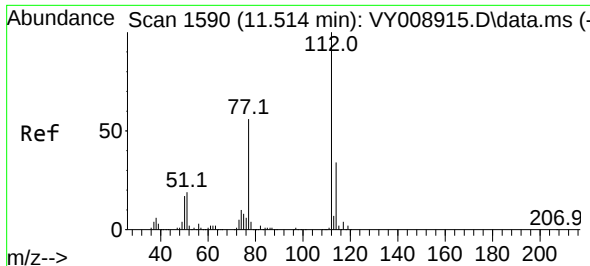

#65
Chlorobenzene
Concen: 1.290 ug/l
RT: 11.514 min Scan# 11590
Delta R.T. -0.000 min
Lab File: VY009125.D
Acq: 02 Jun 2022 14:18




Instrument : MSVOA_Y
ClientSampleId : 20220426-AMENDED-COMPOSITE-F


Tgt Ion:112 Resp: 5784
Ion Ratio Lower Upper
112 100
114 31.9 25.8 38.6

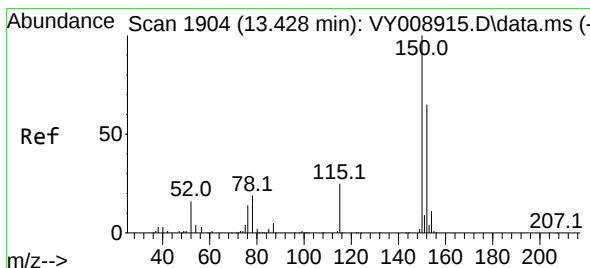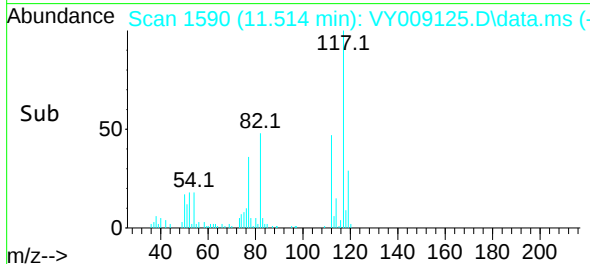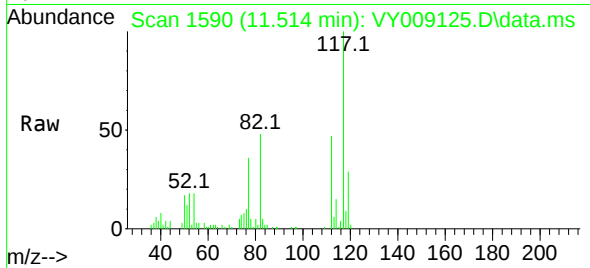

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY009125.D
Acq: 02 Jun 2022 14:18

Tgt Ion:152 Resp: 86547
Ion Ratio Lower Upper
152 100
115 56.6 28.2 84.7
150 154.2 0.0 347.6

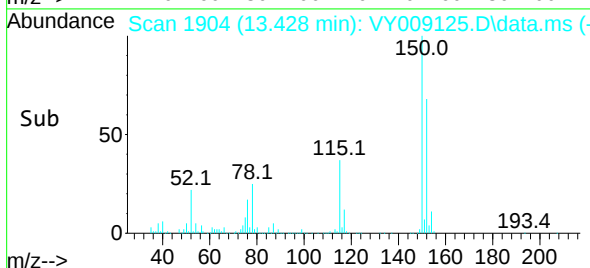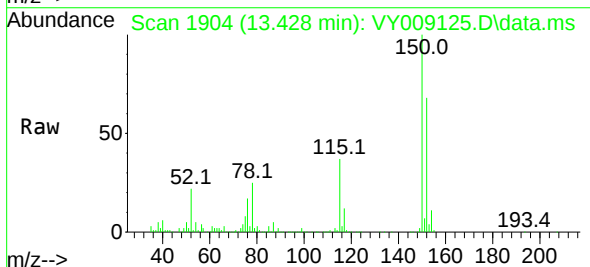



#74

N-ethyl acetate

Concen: 1.526 ug/l

RT: 12.099 min Scan# 1

Delta R.T. -0.043 min

Lab File: VY009125.D


Acq: 02 Jun 2022 14:18

Instrument :

MSVOA_Y

ClientSampleId :

20220426-AMENDED-COMPOSITE-F

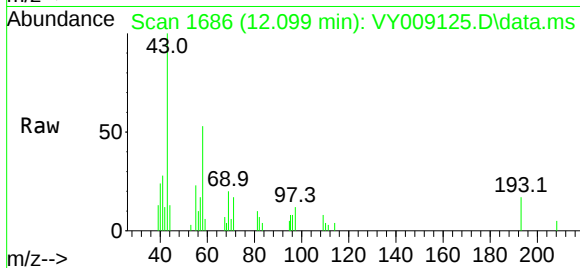

Tgt Ion: 43 Resp: 2279




Ion Ratio Lower Upper

43 100

70 5.5 28.7 43.1#

55 26.3 17.3 25.9#

61 0.0 17.0 25.6#

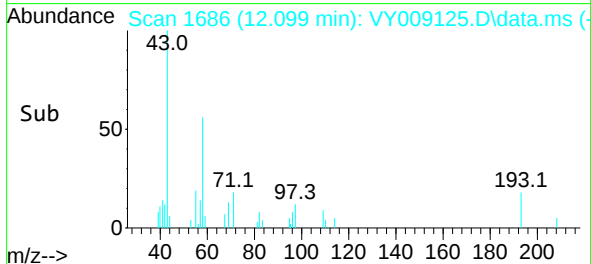

#76

1,2,3-Trichloropropane

Concen: 49.781 ug/l

RT: 12.477 min Scan# 1748

Delta R.T. -0.153 min

Lab File: VY009125.D




Acq: 02 Jun 2022 14:18


Tgt Ion: 75 Resp: 46267

Ion Ratio Lower Upper

75 100

77 1.7 0.0 0.0#


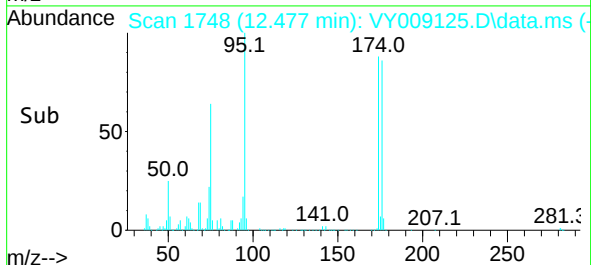
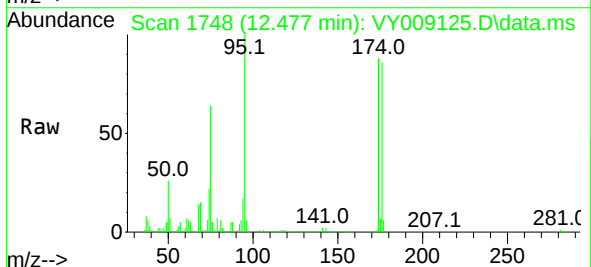





#81
trans-1,4-Dichloro-2-butene
Concen: 102.176 ug/l
RT: 12.477 min Scan# 11
Delta R.T. 0.097 min
Lab File: VY009125.D
Acq: 02 Jun 2022 14:18

Instrument :
MSVOA_Y
ClientSampleId :
20220426-AMENDED-COMPOSITE-F

Tgt Ion: 75 Resp: 46267
Ion Ratio Lower Upper
75 100
53 0.3 85.3 127.9#
89 0.3 37.0 55.4#

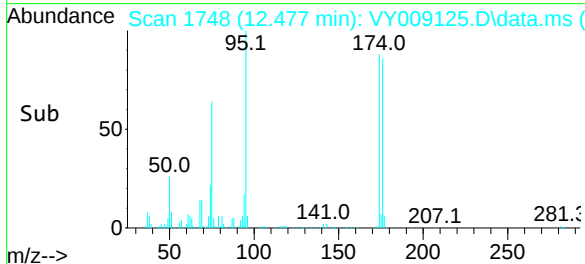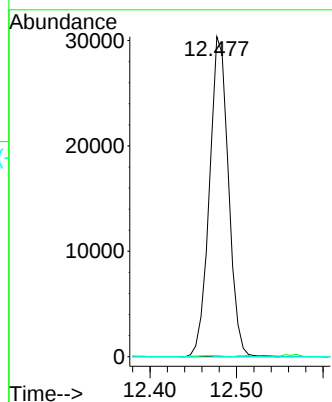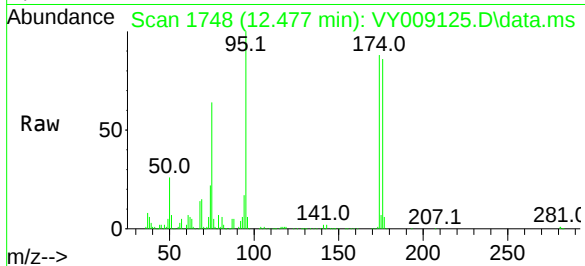

#92
1,2-Dibromo-3-Chloropropane
Concen: 9.630 ug/l
RT: 14.404 min Scan# 2064
Delta R.T. 0.049 min
Lab File: VY009125.D
Acq: 02 Jun 2022 14:18

Tgt Ion: 75 Resp: 1993
Ion Ratio Lower Upper
75 100
155 0.0 38.0 113.9#
157 0.0 47.8 143.3#

