

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060421\
 Data File : VY004959.D
 Acq On : 04 Jun 2021 13:12
 Operator : SY/MD
 Sample : M2597-01
 Misc : 5.57G/5ML/MSVOA_Y/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 124019

Quant Time: Jun 05 01:32:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060221S.M
 Quant Title : SW846 8260
 QLast Update : Thu Jun 03 04:43:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.801	168	168009	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	280737	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	230289	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	96981	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	84236	47.426	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	94.860%
35) Dibromofluoromethane	7.728	113	78690	52.099	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	104.200%
50) Toluene-d8	10.185	98	338167	53.909	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	107.820%
62) 4-Bromofluorobenzene	12.483	95	99391	46.071	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	92.140%
Target Compounds						
					Qvalue	
16) Acetone	3.954	43	34585	80.888	ug/l	98
95) Naphthalene	15.239	128	13880	3.652	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060421\
Data File : VY004959.D
Acq On : 04 Jun 2021 13:12
Operator : SY/MD
Sample : M2597-01
Misc : 5.57G/5ML/MSVOA_Y/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
124019


Quant Time: Jun 05 01:32:36 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060221S.M
Quant Title : SW846 8260
QLast Update : Thu Jun 03 04:43:33 2021
Response via : Initial Calibration

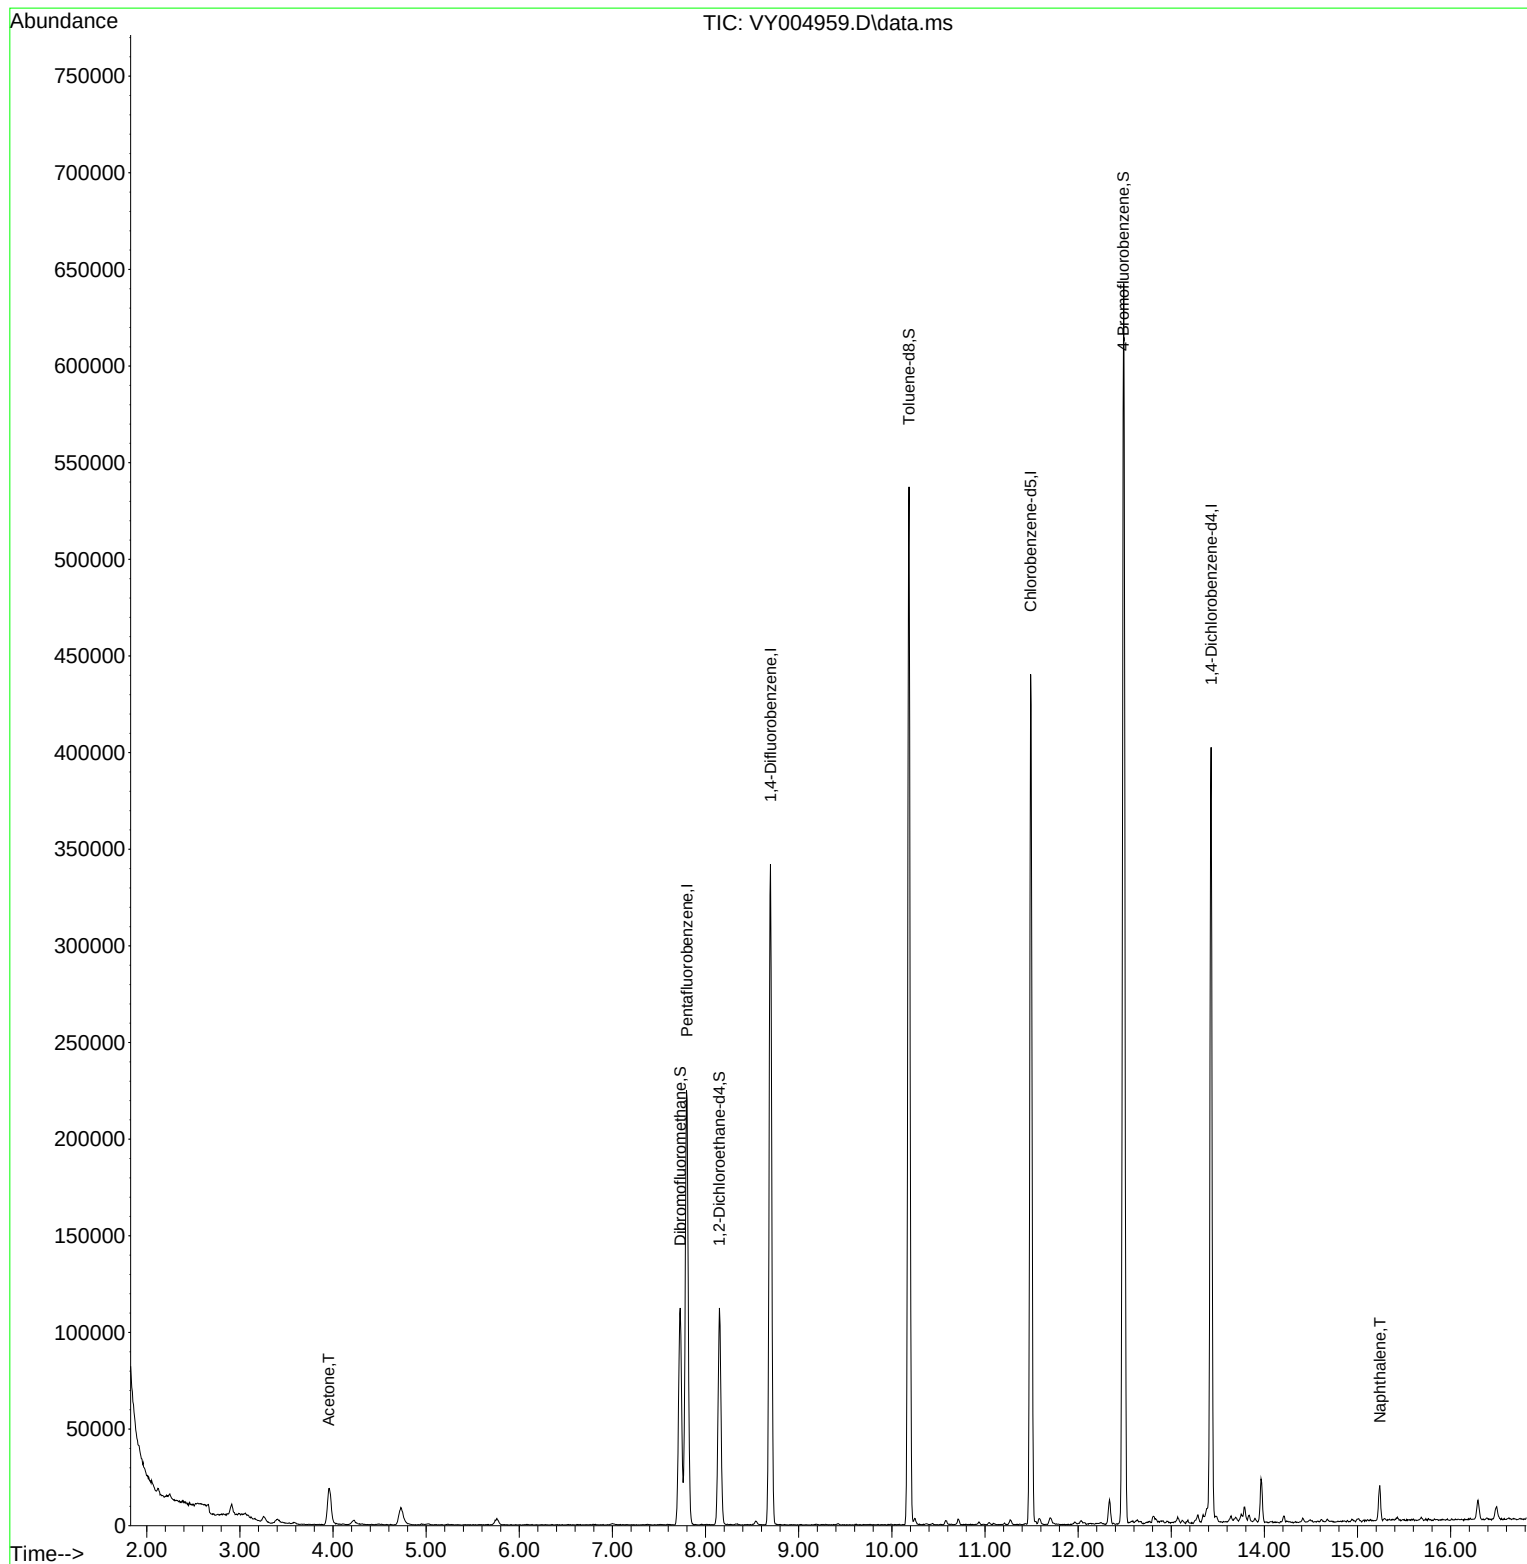



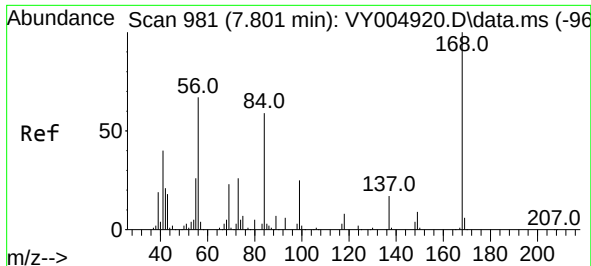


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.801 min Scan# 981
Delta R.T. 0.000 min
Lab File: VY004959.D
Acq: 04 Jun 2021 13:12

Instrument :
MSVOA_Y
ClientSampleId :
124019



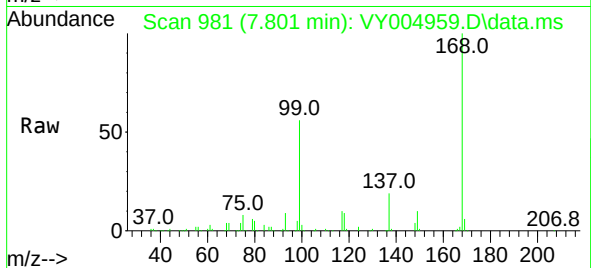



Tgt Ion:168 Resp: 168009
Ion Ratio Lower Upper
168 100
99 56.2 43.9 65.9

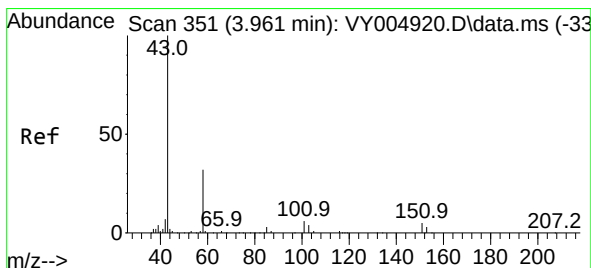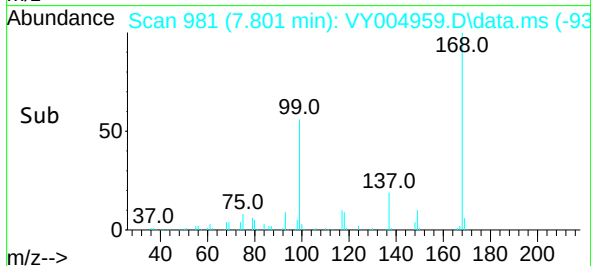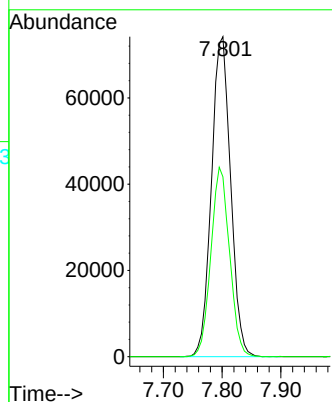

#16
Acetone
Concen: 80.888 ug/l
RT: 3.954 min Scan# 350
Delta R.T. -0.006 min
Lab File: VY004959.D
Acq: 04 Jun 2021 13:12

Tgt Ion: 43 Resp: 34585
Ion Ratio Lower Upper
43 100
58 30.7 25.3 37.9


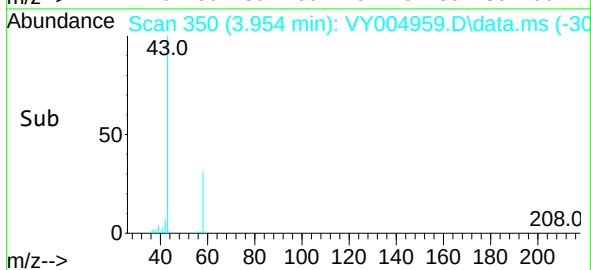
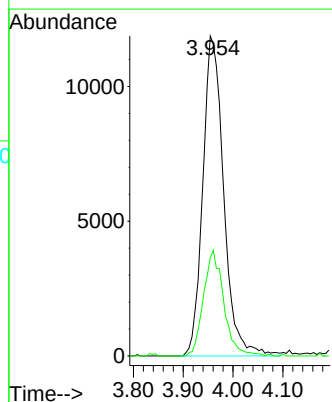
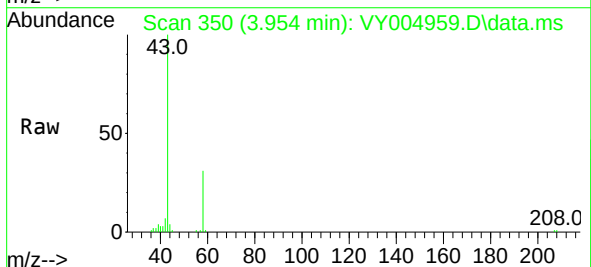


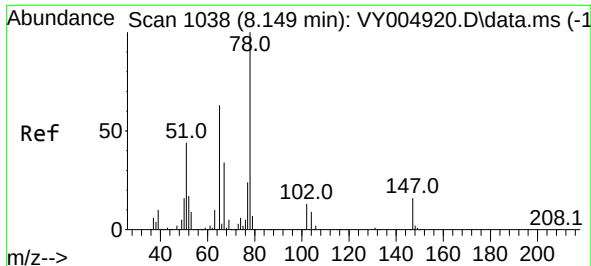

#33
1,2-Dichloroethane-d4
Concen: 47.426 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. -0.000 min
Lab File: VY004959.D
Acq: 04 Jun 2021 13:12




Instrument :
MSVOA_Y
ClientSampleId :
124019


Tgt Ion: 65 Resp: 84236
Ion Ratio Lower Upper
65 100
67 53.8 0.0 110.6

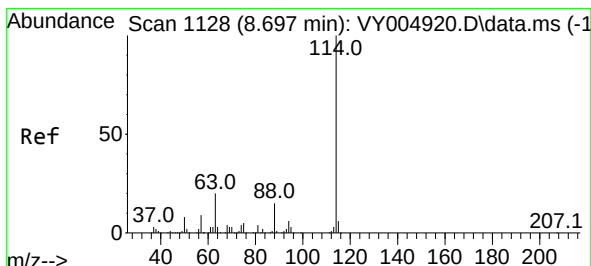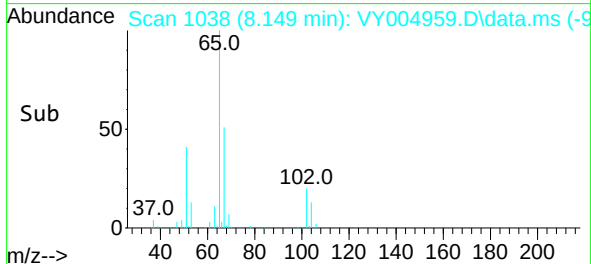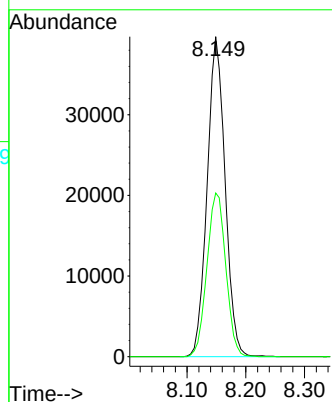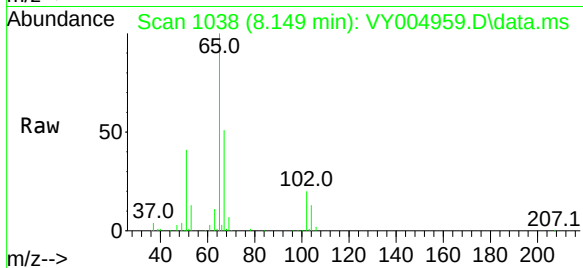

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. -0.000 min
Lab File: VY004959.D
Acq: 04 Jun 2021 13:12

Tgt Ion: 114 Resp: 280737
Ion Ratio Lower Upper
114 100
63 20.2 0.0 41.0
88 15.5 0.0 30.6


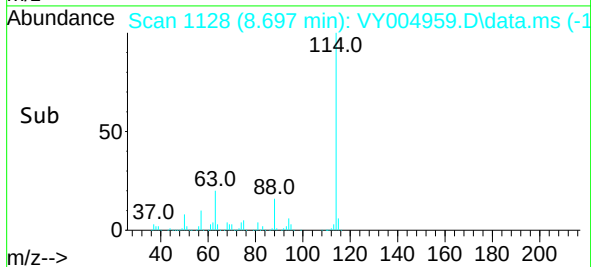
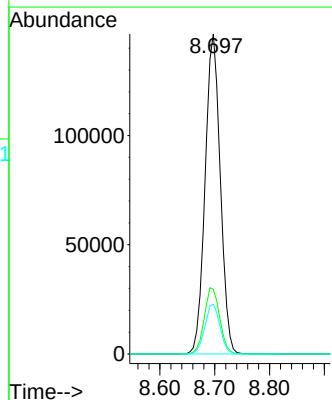
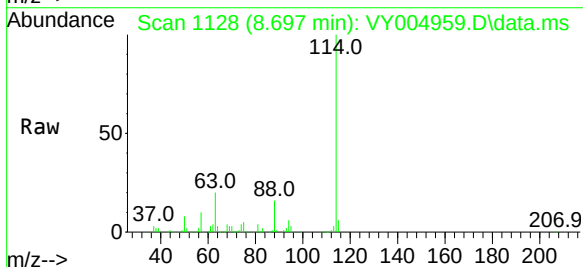


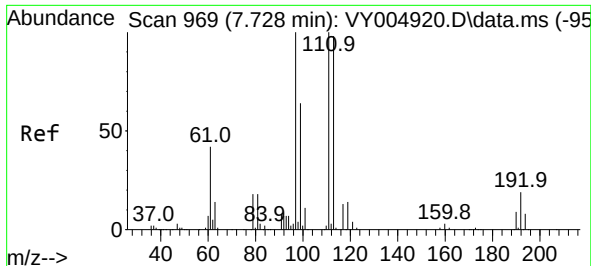

#35
Dibromofluoromethane
Concen: 52.099 ug/l
RT: 7.728 min Scan# 969
Delta R.T. -0.000 min
Lab File: VY004959.D
Acq: 04 Jun 2021 13:12




Instrument :
MSVOA_Y
ClientSampleId :
124019


Tgt Ion:	113	Resp:	78690
Ion	Ratio	Lower	Upper
113	100		
111	103.8	81.8	122.8
192	18.4	15.3	22.9

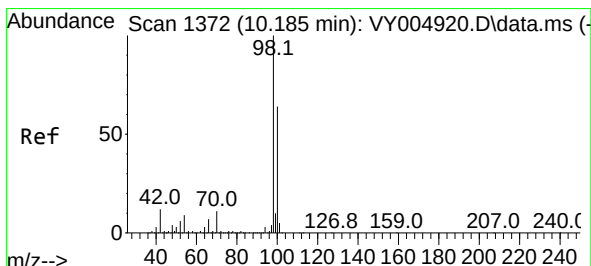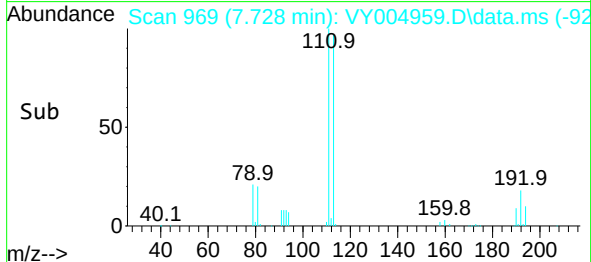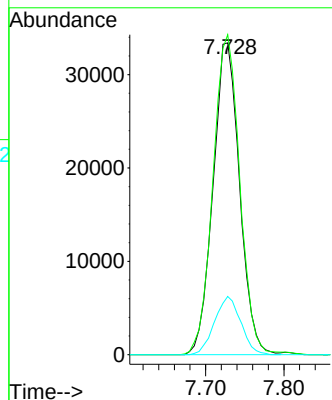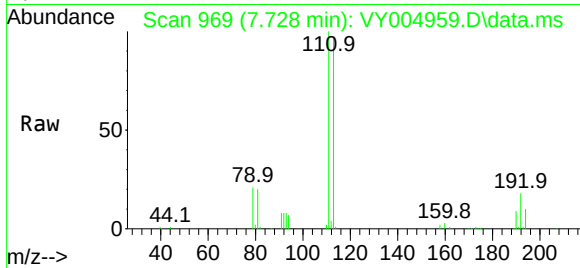

#50
Toluene-d8
Concen: 53.909 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. -0.000 min
Lab File: VY004959.D
Acq: 04 Jun 2021 13:12

Tgt Ion:	98	Resp:	338167
Ion	Ratio	Lower	Upper
98	100		
100	64.2	51.8	77.6


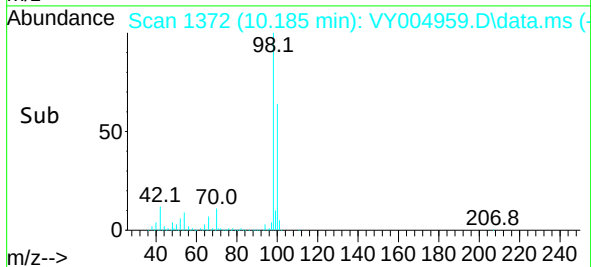
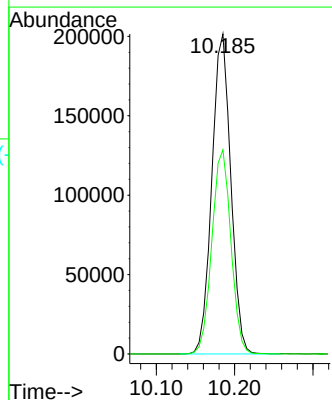
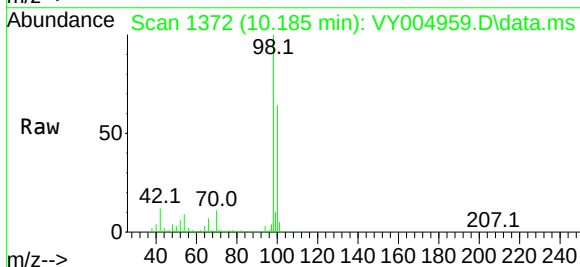


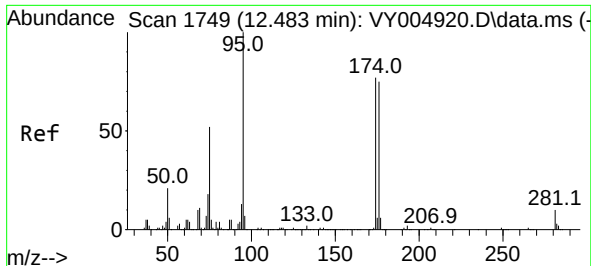

#62
4-Bromofluorobenzene
Concen: 46.071 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY004959.D
Acq: 04 Jun 2021 13:12




Instrument :
MSVOA_Y
ClientSampleId :
124019


Tgt Ion:	95	Resp:	99391
Ion Ratio	Lower	Upper	
95	100		
174	79.3	0.0	160.8
176	77.5	0.0	155.6

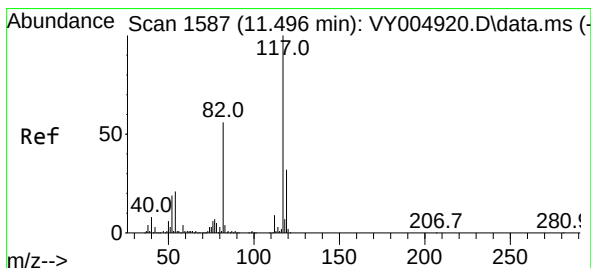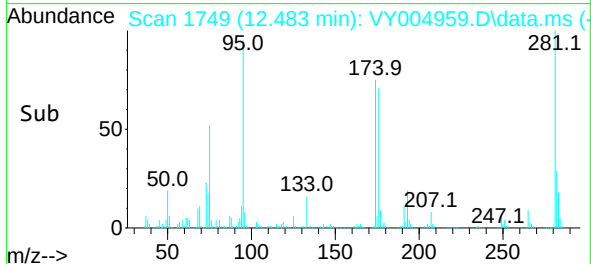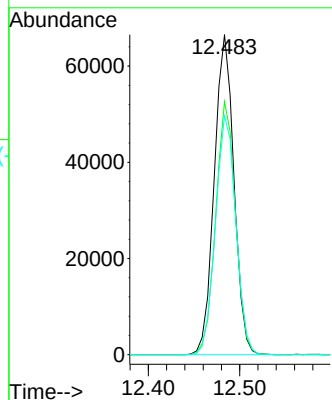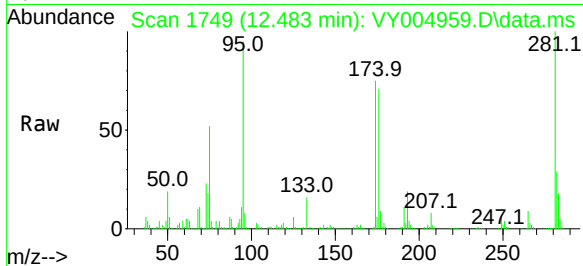

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 1586
Delta R.T. -0.006 min
Lab File: VY004959.D
Acq: 04 Jun 2021 13:12

Tgt Ion:	117	Resp:	230289
Ion Ratio	Lower	Upper	
117	100		
82	56.5	44.8	67.2
119	31.5	25.2	37.8


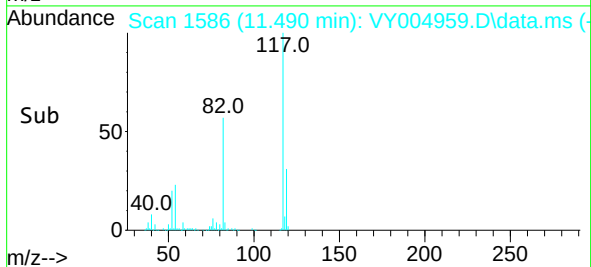
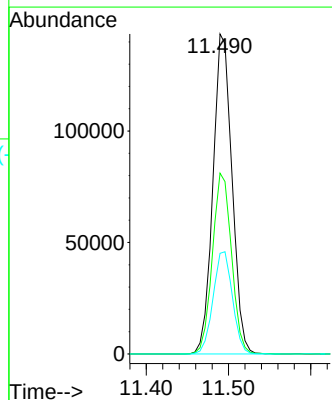
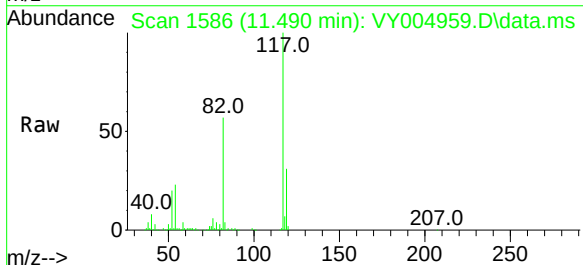


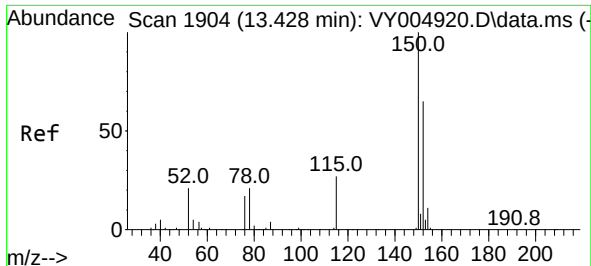

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY004959.D
Acq: 04 Jun 2021 13:12

Instrument :
MSVOA_Y
ClientSampleId :
124019

Tgt Ion:152 Resp: 96981
Ion Ratio Lower Upper
152 100
115 59.0 29.9 89.7
150 159.3 0.0 347.8

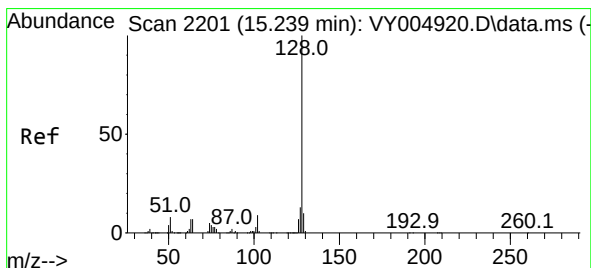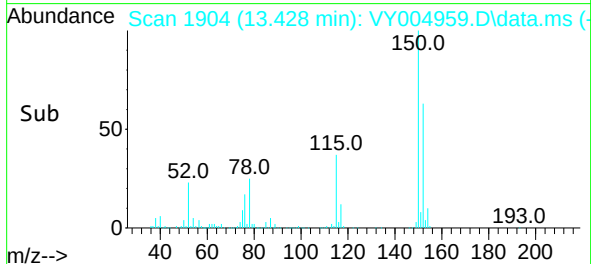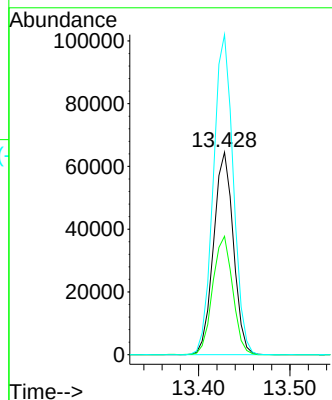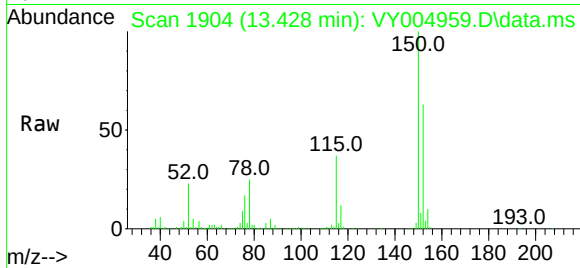

#95
Naphthalene
Concen: 3.652 ug/l
RT: 15.239 min Scan# 2201
Delta R.T. -0.000 min
Lab File: VY004959.D
Acq: 04 Jun 2021 13:12

Tgt Ion:128 Resp: 13880
Ion Ratio Lower Upper
128 100
127 13.1 10.2 15.2
129 11.3 8.7 13.1

