

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060523\
 Data File : VY014002.D
 Acq On : 05 Jun 2023 13:12
 Operator : KP/MD
 Sample : 03002-04
 Misc : 5.01g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB04

Quant Time: Jun 05 15:33:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060123S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 02 07:00:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	172856	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	287837	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	293266	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	138655	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	120127	52.498	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 105.000%	
35) Dibromofluoromethane	7.716	113	97893	53.516	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 107.040%	
50) Toluene-d8	10.179	98	358566	51.389	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	= 102.780%	
62) 4-Bromofluorobenzene	12.483	95	121353	51.015	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	= 102.040%	
Target Compounds						
16) Acetone	3.954	43	26666	34.062	ug/l	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060523\
Data File : VY014002.D
Acq On : 05 Jun 2023 13:12
Operator : KP/MD
Sample : 03002-04
Misc : 5.01g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SB04

Quant Time: Jun 05 15:33:03 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060123S.M
Quant Title : SW846 8260
QLast Update : Fri Jun 02 07:00:14 2023
Response via : Initial Calibration




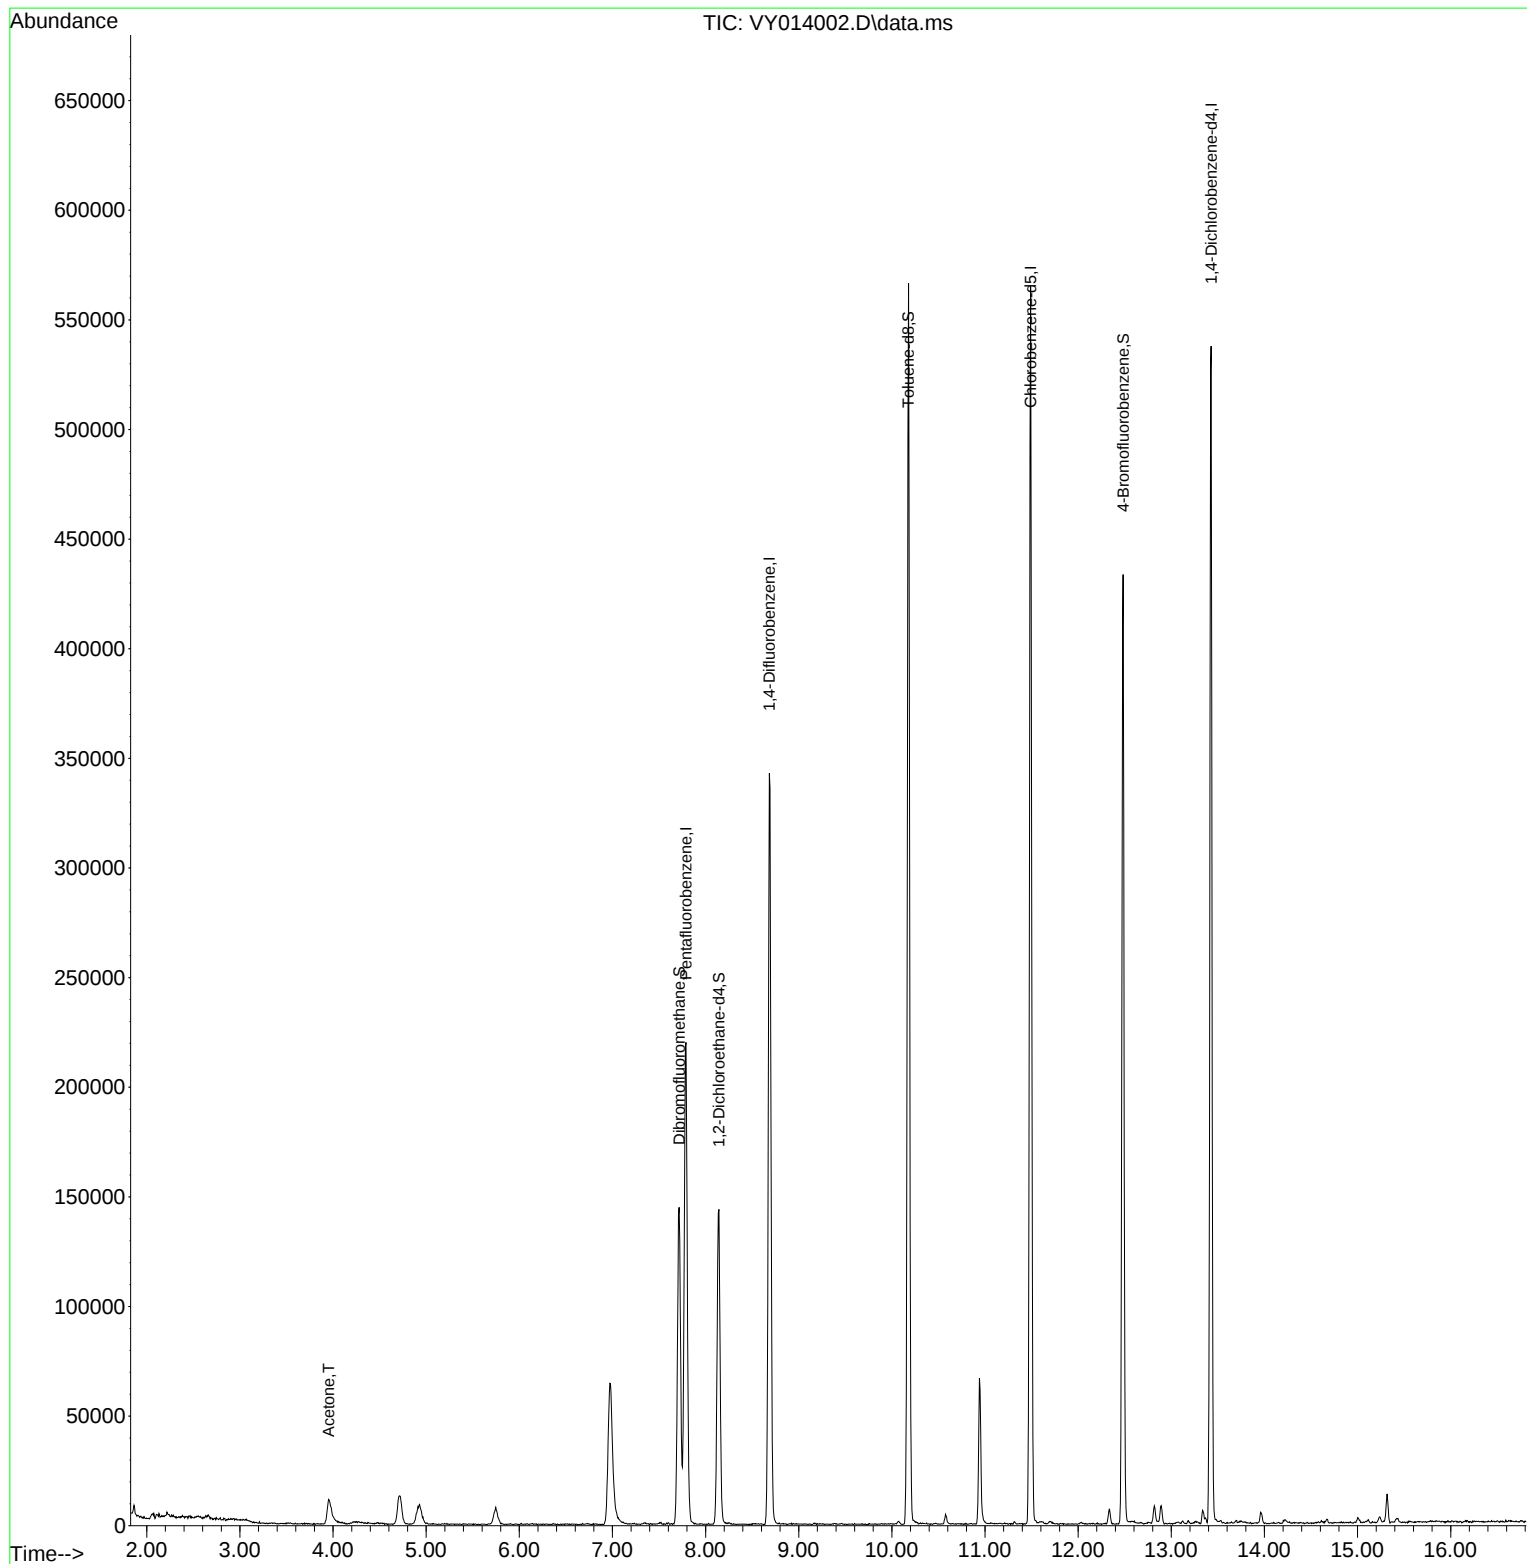


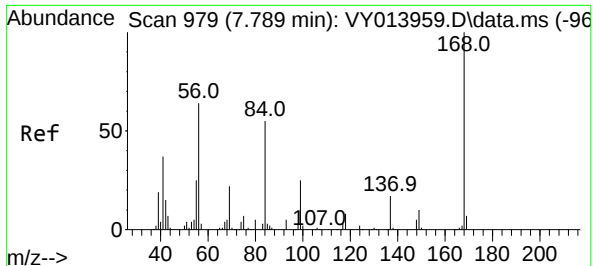

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY014002.D
Acq: 05 Jun 2023 13:12




Instrument :
MSVOA_Y
ClientSampleId :
SB04


Tgt Ion:168 Resp: 172856
Ion Ratio Lower Upper
168 100
99 52.5 43.4 65.0

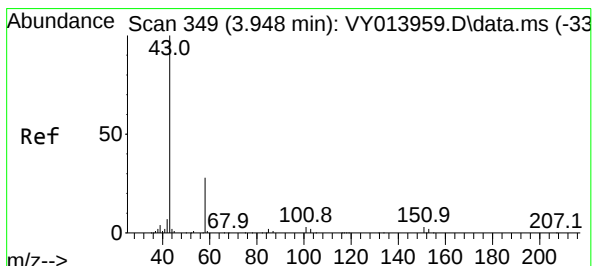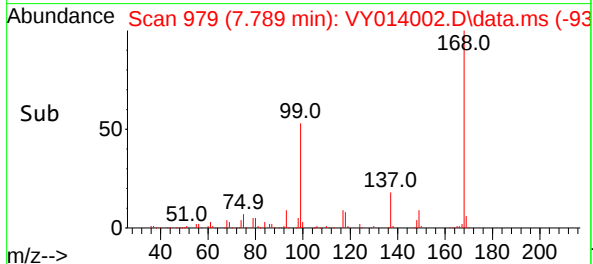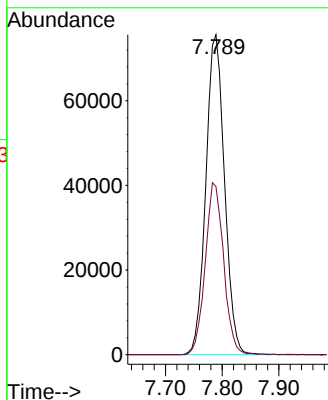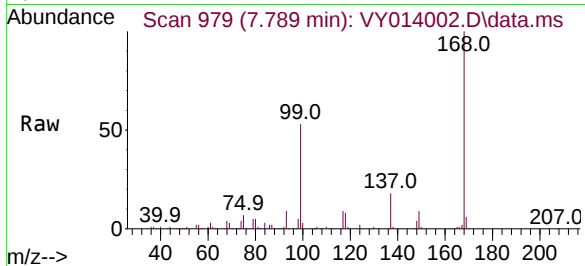

#16
Acetone
Concen: 34.062 ug/l
RT: 3.954 min Scan# 350
Delta R.T. 0.006 min
Lab File: VY014002.D
Acq: 05 Jun 2023 13:12

Tgt Ion: 43 Resp: 26666
Ion Ratio Lower Upper
43 100
58 29.9 22.7 34.1

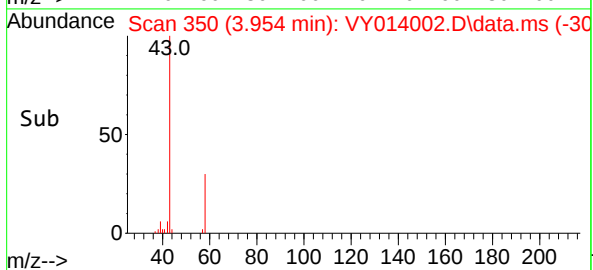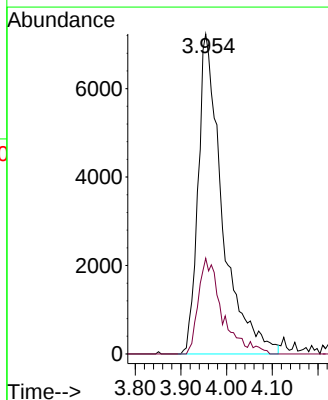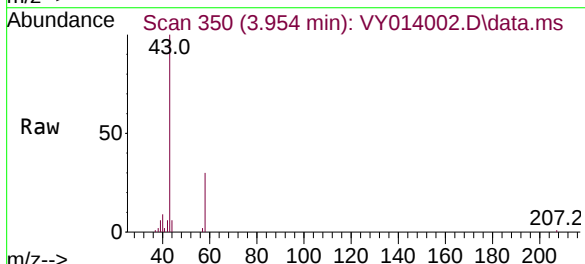

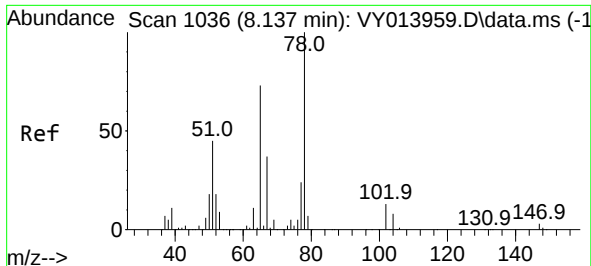

#33

1,2-Dichloroethane-d4

Concen: 52.498 ug/l

RT: 8.143 min Scan# 110

Delta R.T. 0.006 min

Lab File: VY014002.D

Acq: 05 Jun 2023 13:12

Instrument :

MSVOA_Y

ClientSampleId :





SB04

Tgt Ion: 65 Resp: 120127

Ion Ratio Lower Upper

65 100

67 50.2 0.0 101.8

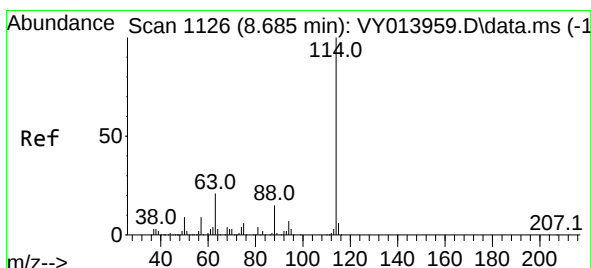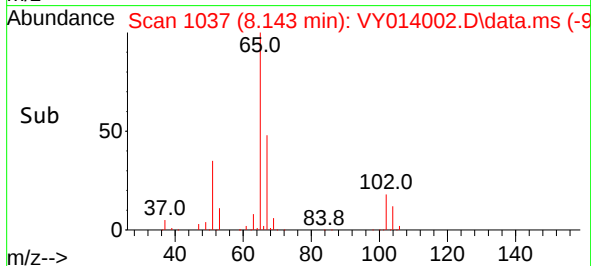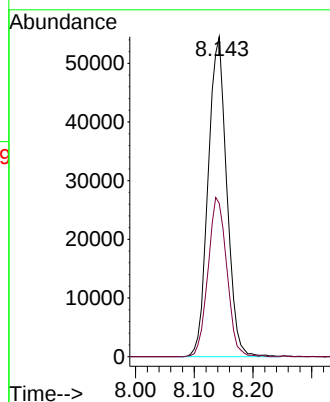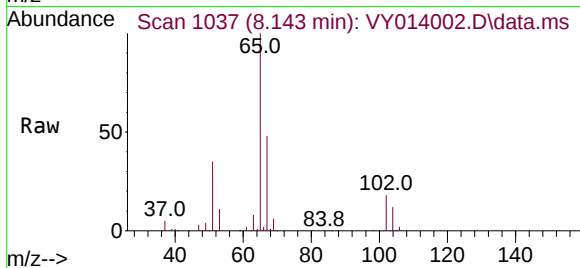

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. 0.000 min

Lab File: VY014002.D

Acq: 05 Jun 2023 13:12




Tgt Ion: 114 Resp: 287837


Ion Ratio Lower Upper

114 100

63 20.7 0.0 42.4

88 14.6 0.0 30.6


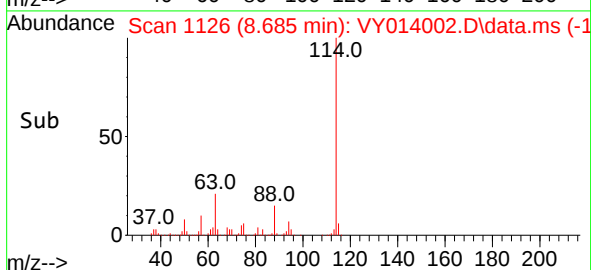
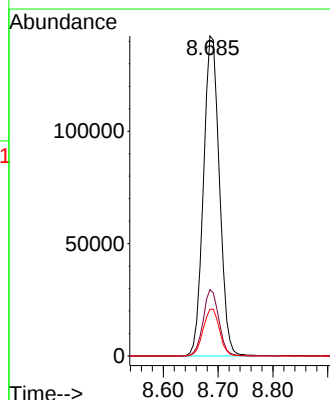
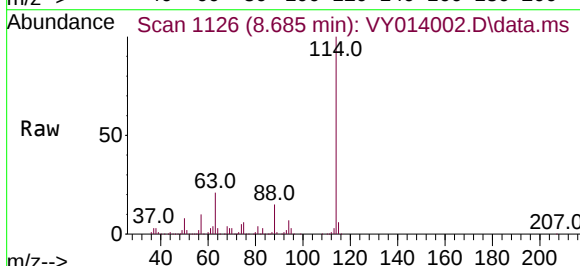


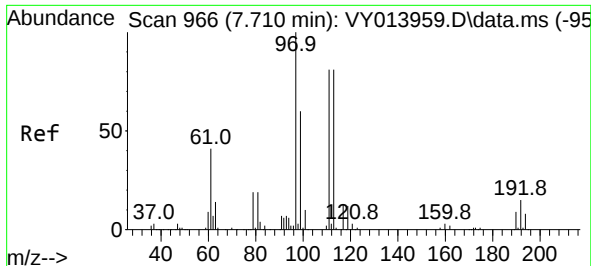

#35
Dibromofluoromethane
Concen: 53.516 ug/l
RT: 7.716 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY014002.D
Acq: 05 Jun 2023 13:12




Instrument :
MSVOA_Y
ClientSampleId :
SB04


Tgt Ion:113 Resp: 97893
Ion Ratio Lower Upper
113 100
111 104.0 81.3 121.9
192 20.7 16.9 25.3

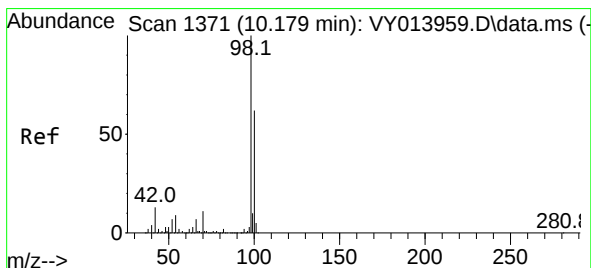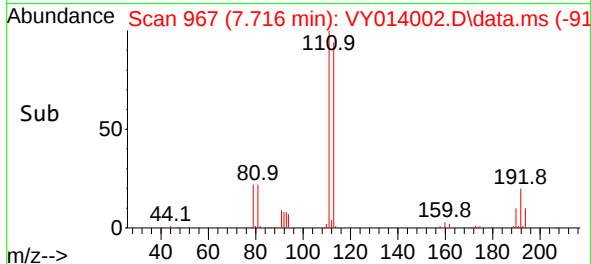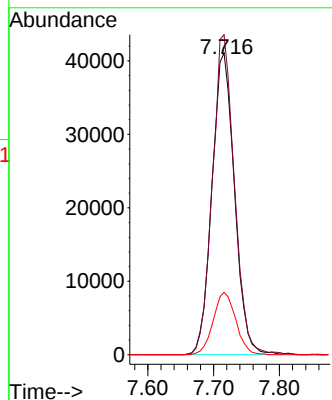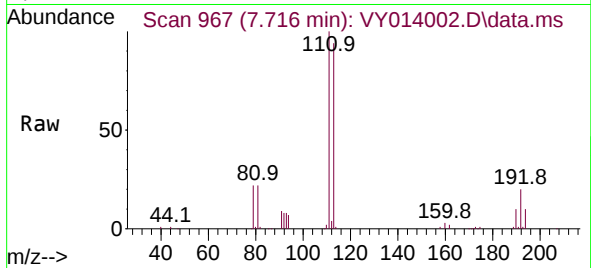

#50
Toluene-d8
Concen: 51.389 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY014002.D
Acq: 05 Jun 2023 13:12

Tgt Ion: 98 Resp: 358566
Ion Ratio Lower Upper
98 100
100 62.1 50.1 75.1


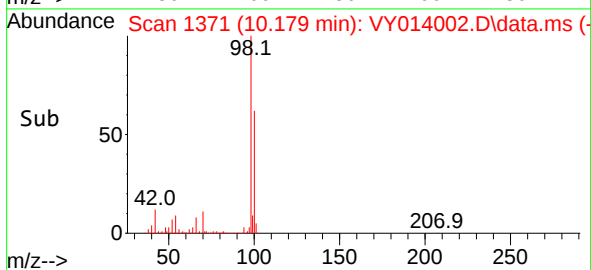
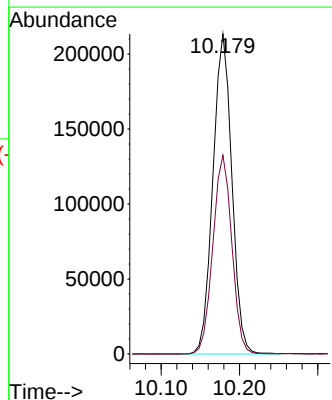
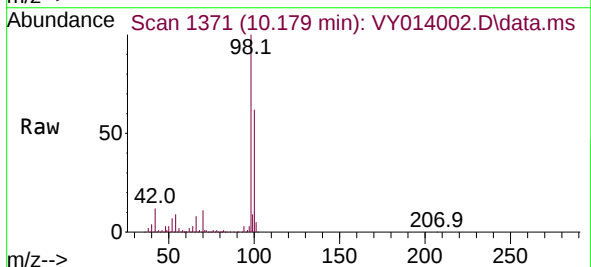


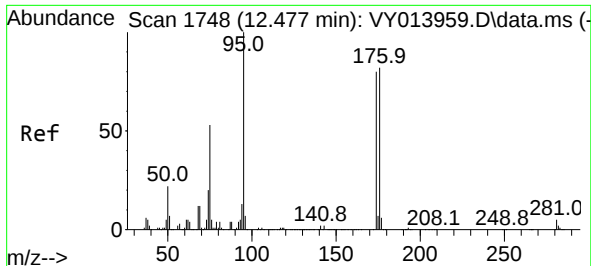

#62
4-Bromofluorobenzene
Concen: 51.015 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.006 min
Lab File: VY014002.D
Acq: 05 Jun 2023 13:12




Instrument :
MSVOA_Y
ClientSampleId :
SB04


Tgt Ion: 95 Resp: 121353
Ion Ratio Lower Upper
95 100
174 95.0 0.0 178.2
176 90.5 0.0 173.8

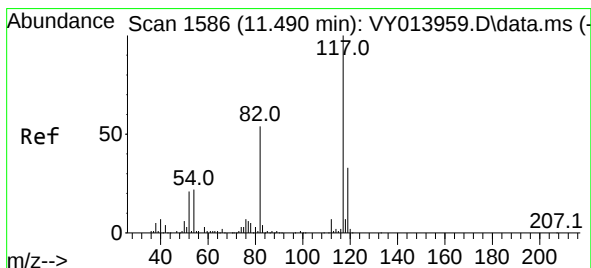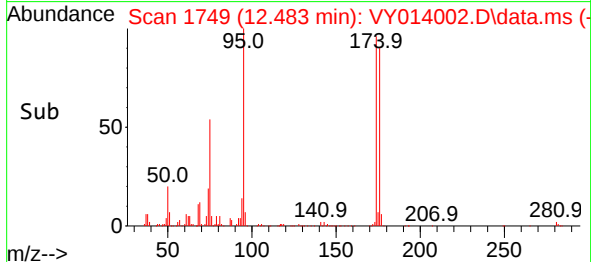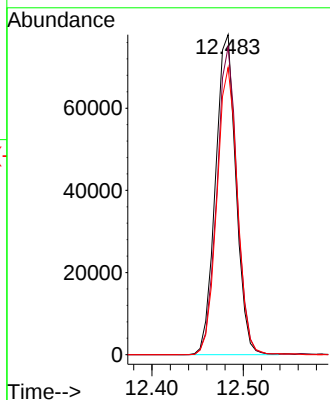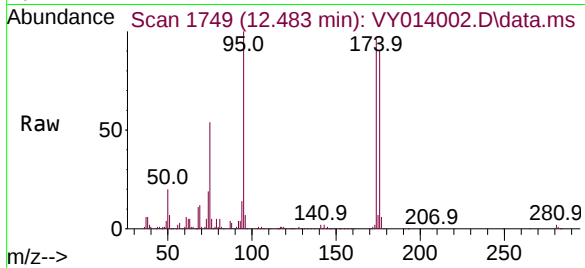

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 1586
Delta R.T. -0.000 min
Lab File: VY014002.D
Acq: 05 Jun 2023 13:12

Tgt Ion: 117 Resp: 293266
Ion Ratio Lower Upper
117 100
82 53.9 43.4 65.0
119 32.9 26.3 39.5

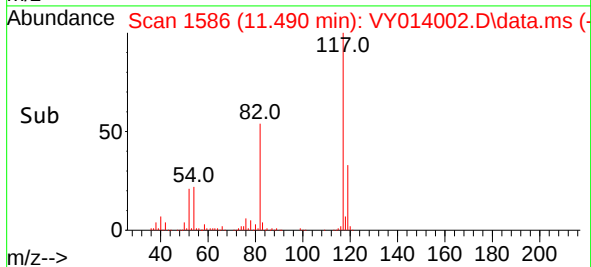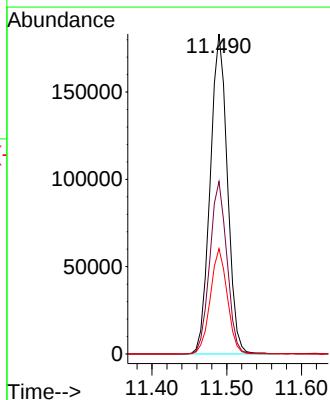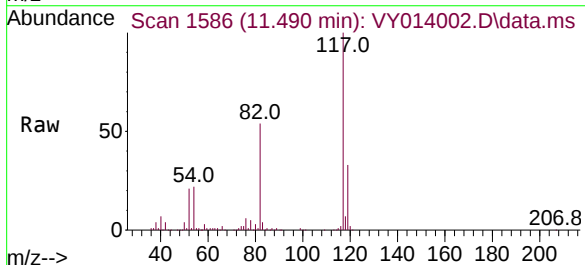

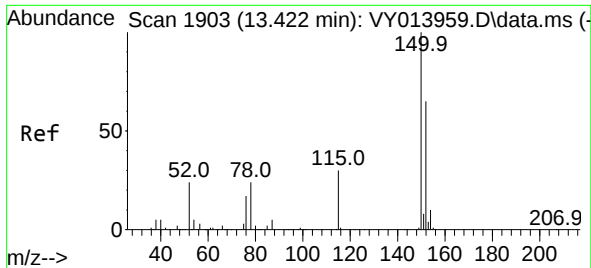

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.428 min Scan# 1904

Delta R.T. 0.006 min

Lab File: VY014002.D


Acq: 05 Jun 2023 13:12

Instrument :

MSVOA_Y

ClientSampleId :

SB04

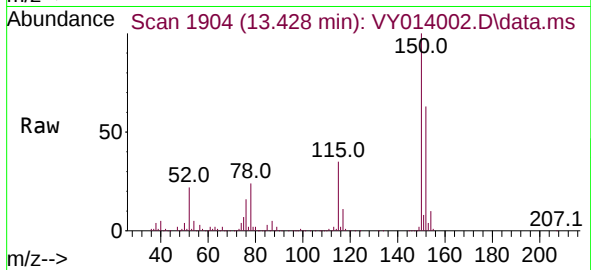

Tgt Ion:152 Resp: 138655

Ion Ratio Lower Upper

152 100

115 56.6 28.8 86.5

150 157.3 0.0 348.8

