
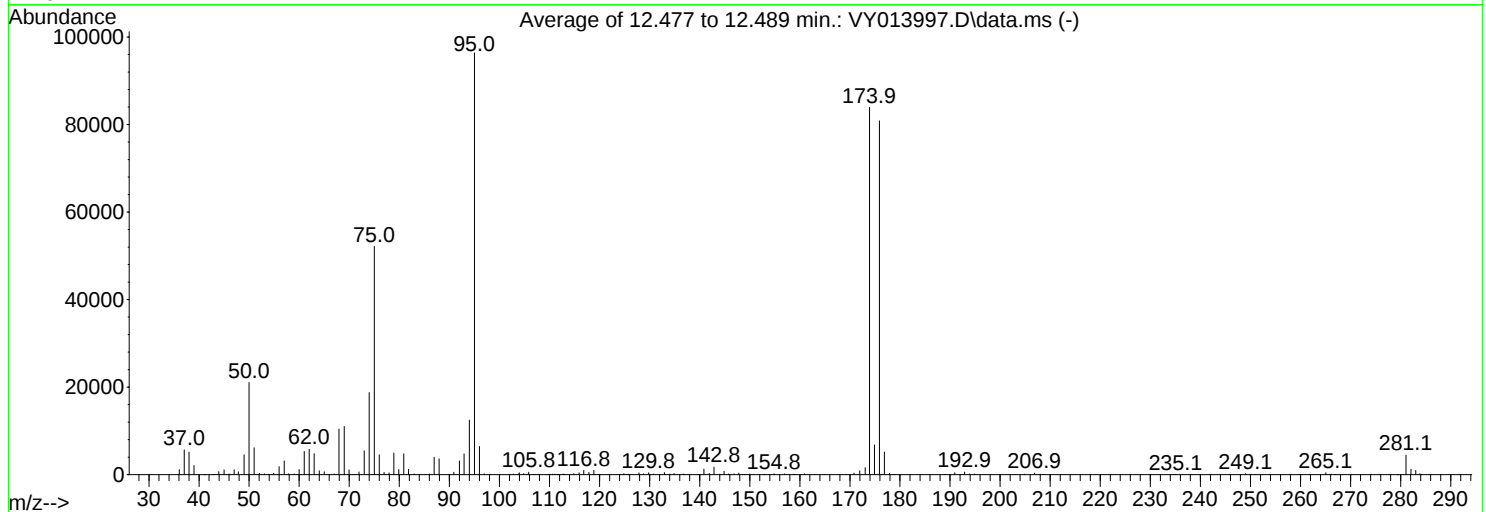


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060523\
Data File : VY013997.D
Acq On : 05 Jun 2023 09:17
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060123S.M
Title : SW846 8260
Last Update : Fri Jun 02 07:00:14 2023

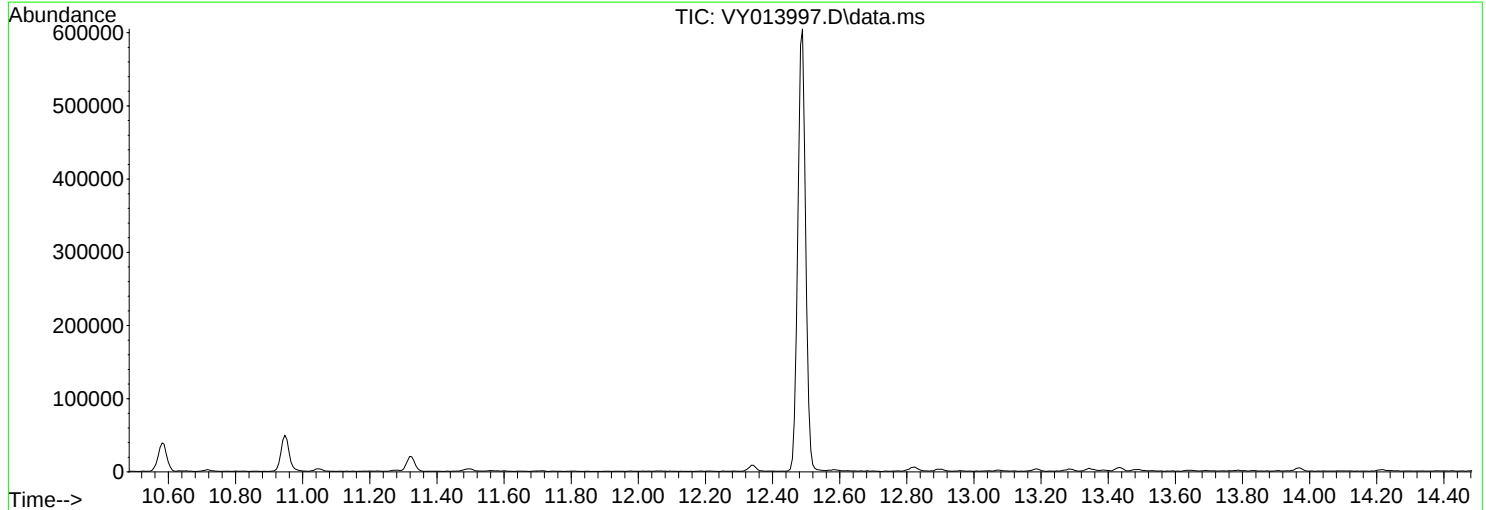

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.9	21069	PASS
75	95	30	60	54.1	52173	PASS
95	95	100	100	100.0	96384	PASS
96	95	5	9	6.7	6449	PASS
173	174	0.00	2	1.9	1614	PASS
174	95	50	100	87.0	83899	PASS
175	174	5	9	8.1	6806	PASS
176	174	95	101	96.4	80843	PASS
177	176	5	9	6.4	5161	PASS