

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060721\
 Data File : VY005004.D
 Acq On : 07 Jun 2021 19:38
 Operator : SY/MD
 Sample : M2626-01
 Misc : 7.25G/5ML/MSVOA_Y/SOIL
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 18-B12(218-222)

Quant Time: Jun 08 02:10:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060221S.M
 Quant Title : SW846 8260
 QLast Update : Thu Jun 03 04:43:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.801	168	171431	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	327725	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.496	117	322835	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	145722	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	117433	64.797	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 129.600%	
35) Dibromofluoromethane	7.728	113	103914	58.935	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 117.860%	
50) Toluene-d8	10.185	98	418232	57.114	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 114.220%	
62) 4-Bromofluorobenzene	12.483	95	142773	56.691	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 113.380%	
Target Compounds						
16) Acetone	3.967	43	4363	10.001	ug/l	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060721\
Data File : VY005004.D
Acq On : 07 Jun 2021 19:38
Operator : SY/MD
Sample : M2626-01
Misc : 7.25G/5ML/MSVOA_Y/SOIL
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
18-B12(218-222)

Quant Time: Jun 08 02:10:53 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060221S.M
Quant Title : SW846 8260
QLast Update : Thu Jun 03 04:43:33 2021
Response via : Initial Calibration




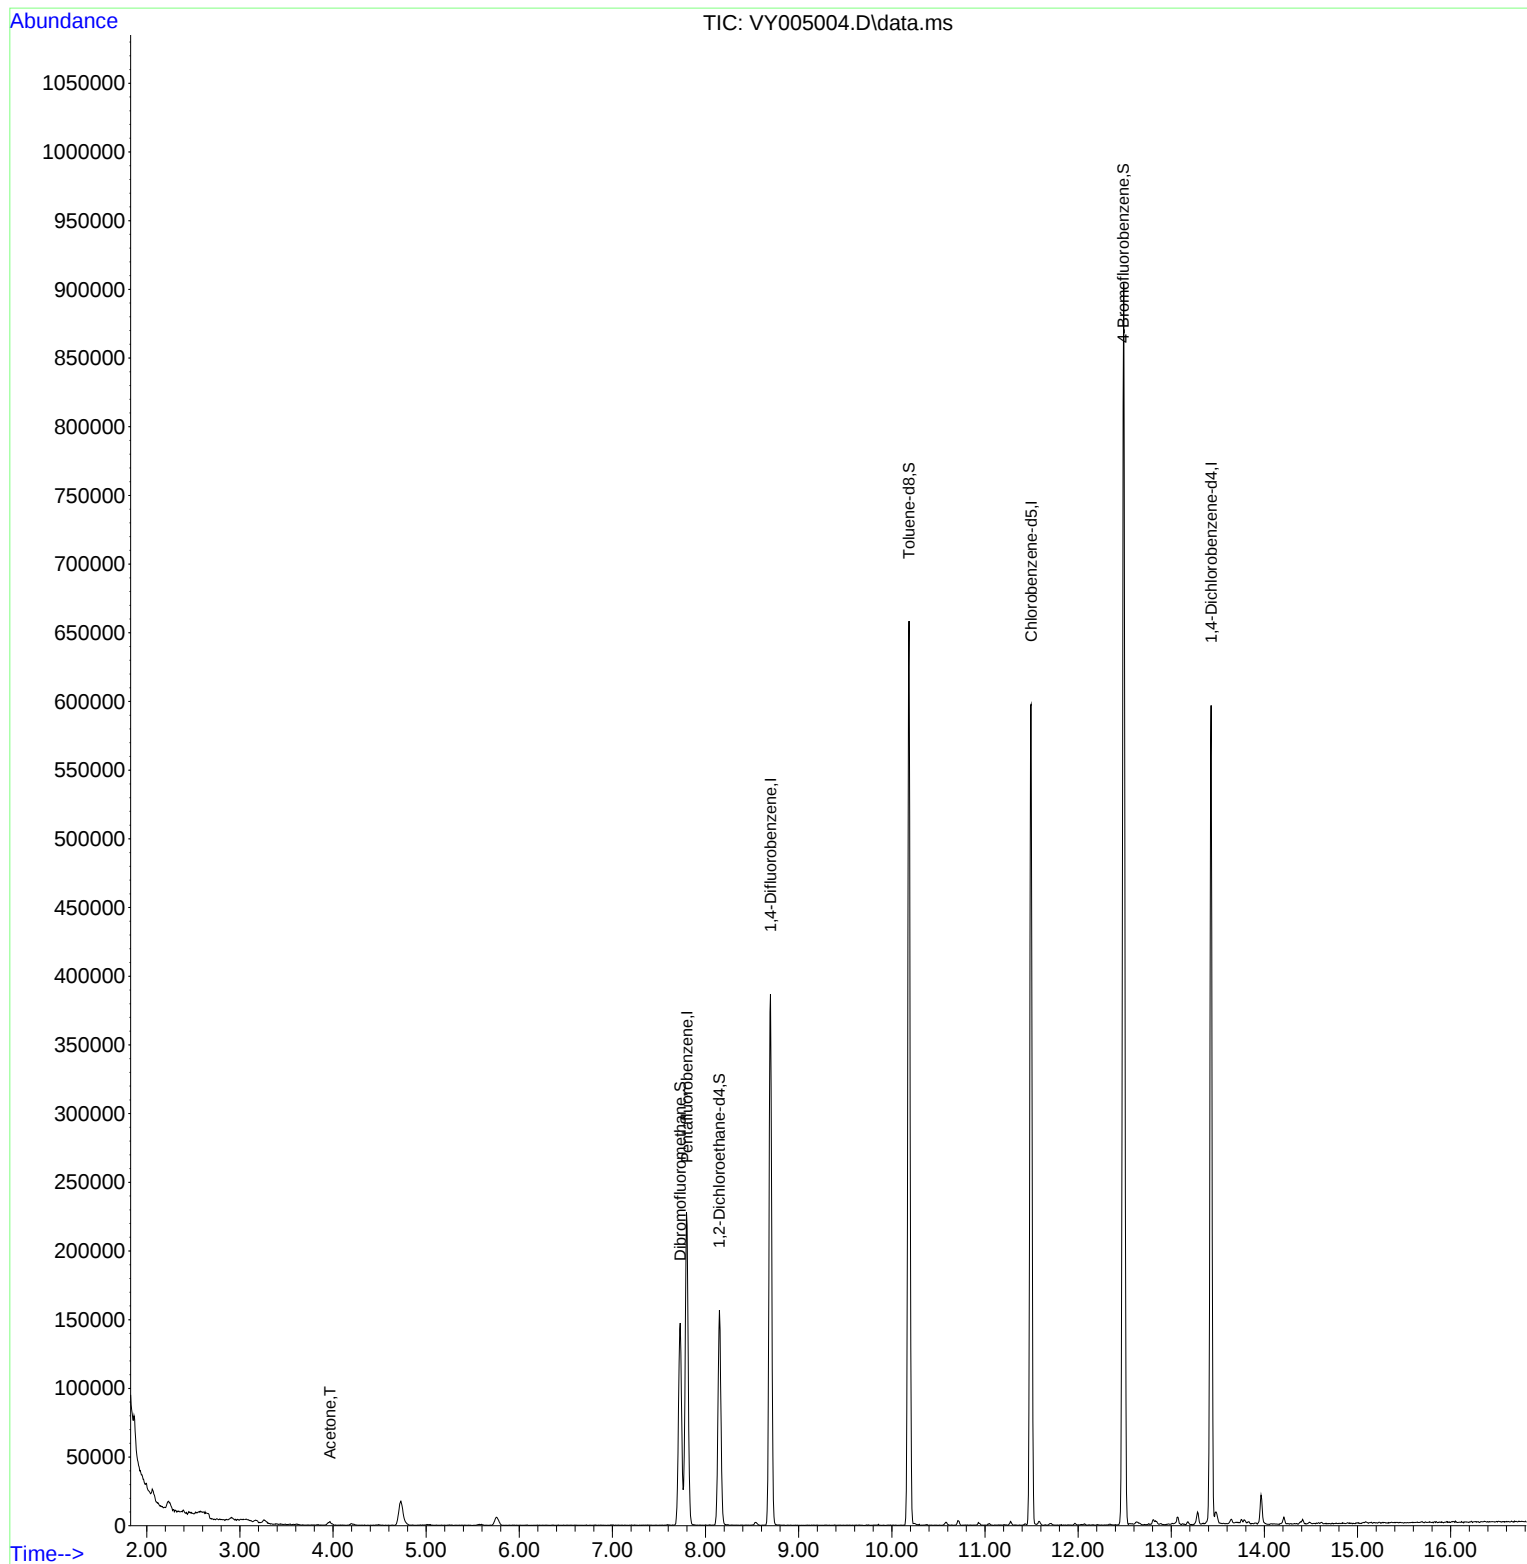


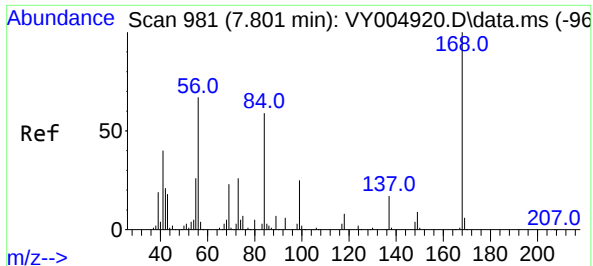

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.801 min Scan# 981
Delta R.T. 0.000 min
Lab File: VY005004.D
Acq: 07 Jun 2021 19:38




Instrument :
MSVOA_Y
ClientSampleId :
18-B12(218-222)


Tgt Ion:168 Resp: 171431
Ion Ratio Lower Upper
168 100
99 52.4 43.9 65.9

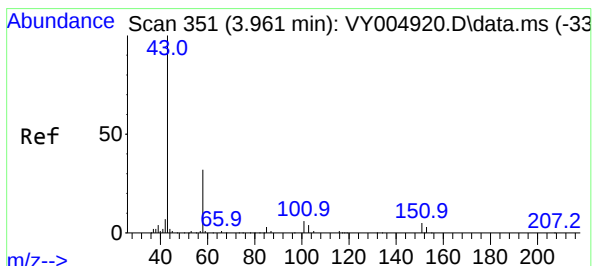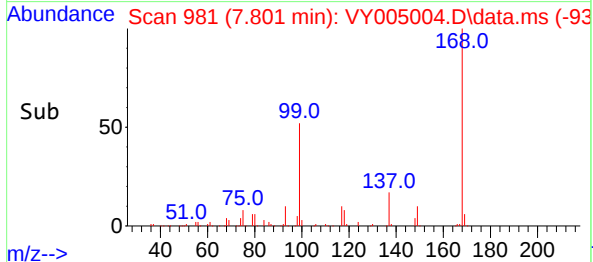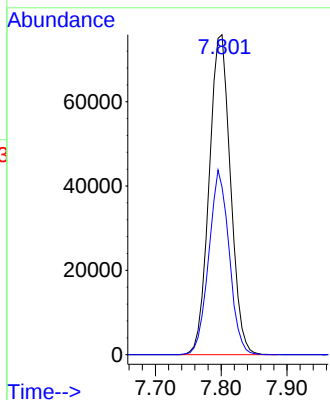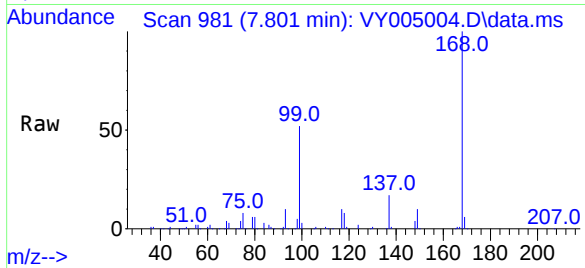

#16
Acetone
Concen: 10.001 ug/l
RT: 3.967 min Scan# 352
Delta R.T. 0.006 min
Lab File: VY005004.D
Acq: 07 Jun 2021 19:38

Tgt Ion: 43 Resp: 4363
Ion Ratio Lower Upper
43 100
58 34.4 25.3 37.9


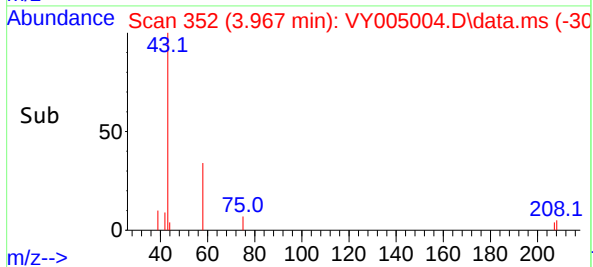
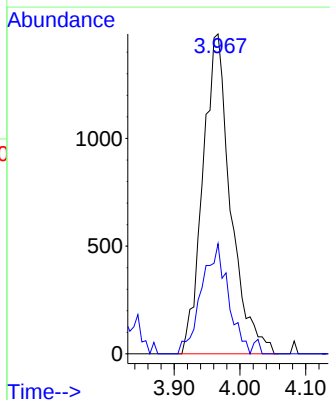
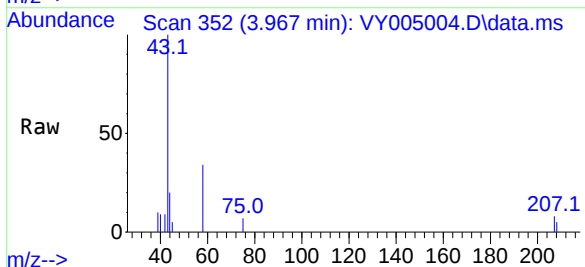


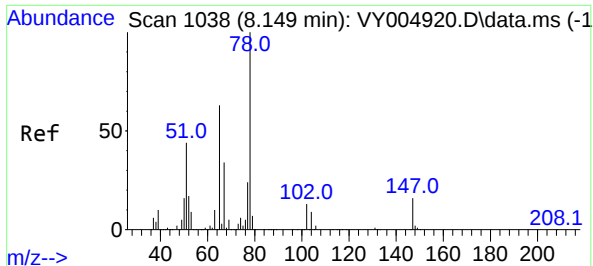

#33
1,2-Dichloroethane-d4
Concen: 64.797 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. -0.000 min
Lab File: VY005004.D
Acq: 07 Jun 2021 19:38




Instrument :
MSVOA_Y
ClientSampleId :
18-B12(218-222)


Tgt Ion: 65 Resp: 117433
Ion Ratio Lower Upper
65 100
67 54.0 0.0 110.6

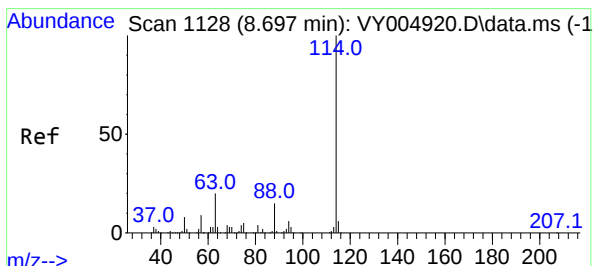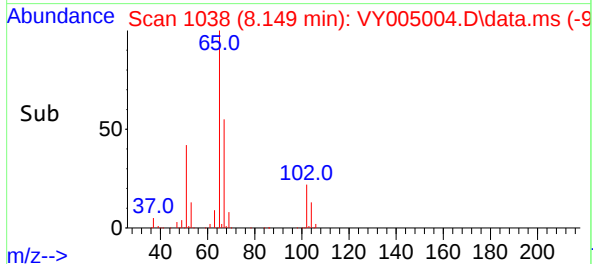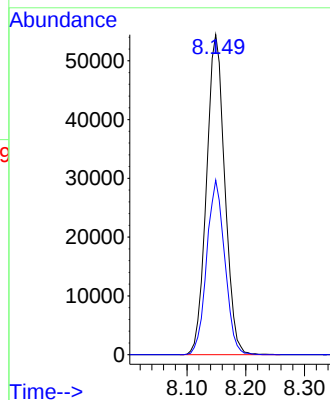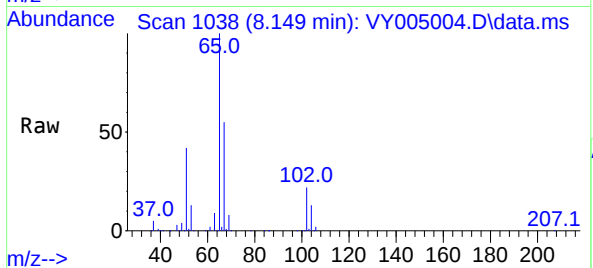

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. -0.000 min
Lab File: VY005004.D
Acq: 07 Jun 2021 19:38

Tgt Ion: 114 Resp: 327725
Ion Ratio Lower Upper
114 100
63 20.5 0.0 41.0
88 15.3 0.0 30.6


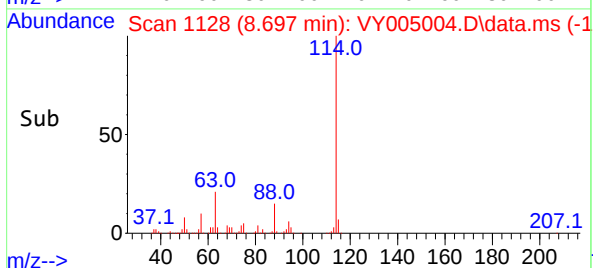
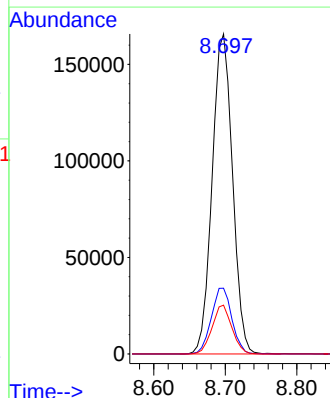
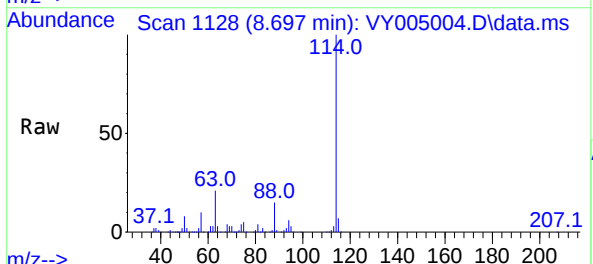


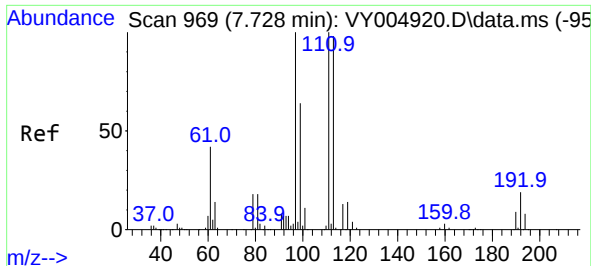

#35
Dibromofluoromethane
Concen: 58.935 ug/l
RT: 7.728 min Scan# 969
Delta R.T. -0.000 min
Lab File: VY005004.D
Acq: 07 Jun 2021 19:38




Instrument :
MSVOA_Y
ClientSampleId :
18-B12(218-222)


Tgt Ion:	113	Resp:	103914
Ion	Ratio	Lower	Upper
113	100		
111	103.6	81.8	122.8
192	18.7	15.3	22.9

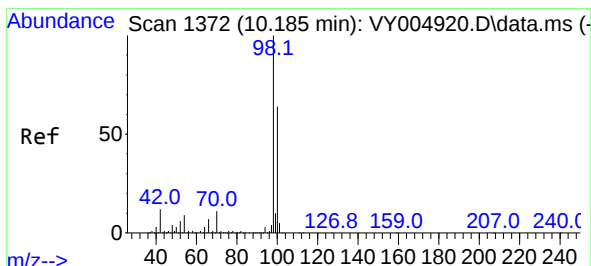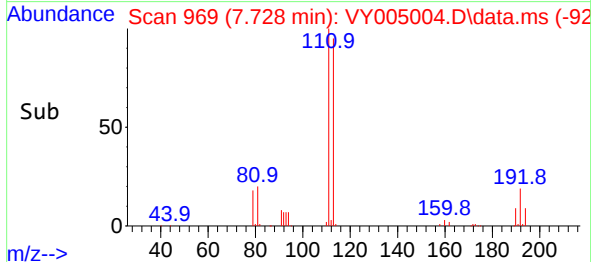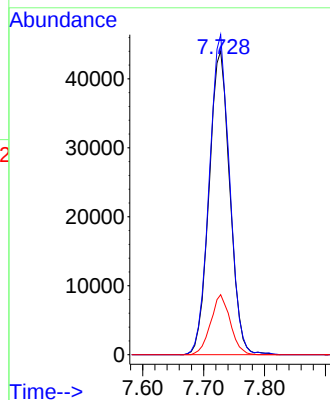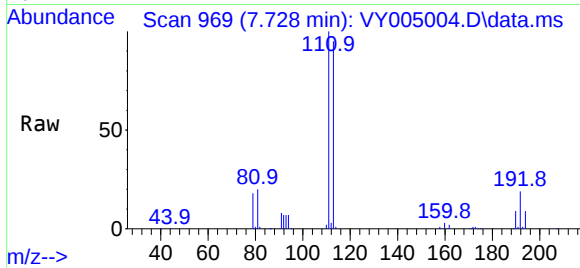

#50
Toluene-d8
Concen: 57.114 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. -0.000 min
Lab File: VY005004.D
Acq: 07 Jun 2021 19:38

Tgt Ion:	98	Resp:	418232
Ion	Ratio	Lower	Upper
98	100		
100	63.6	51.8	77.6


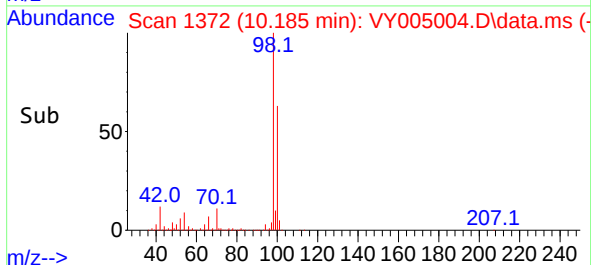
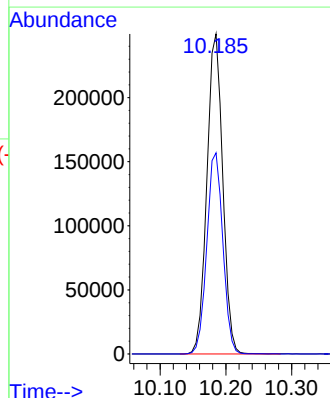
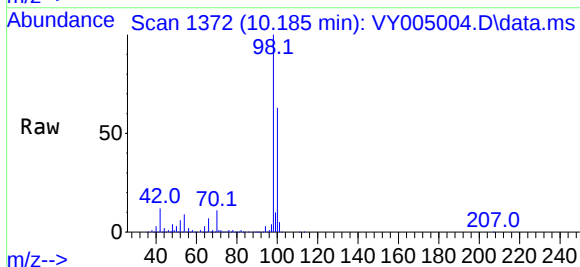


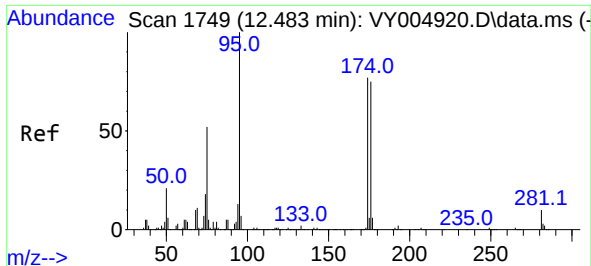

#62
4-Bromofluorobenzene
Concen: 56.691 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY005004.D
Acq: 07 Jun 2021 19:38




Instrument :
MSVOA_Y
ClientSampleId :
18-B12(218-222)


Tgt Ion: 95 Resp: 142773
Ion Ratio Lower Upper
95 100
174 79.8 0.0 160.8
176 78.9 0.0 155.6

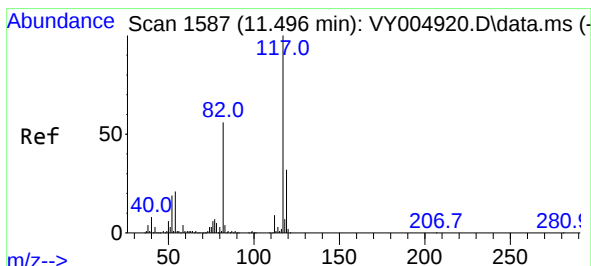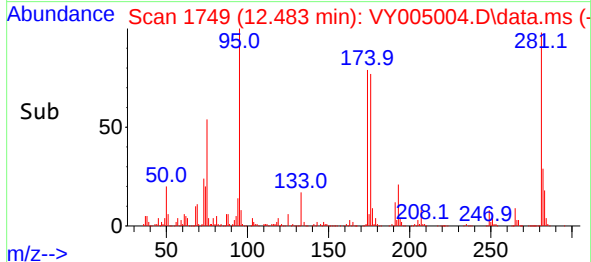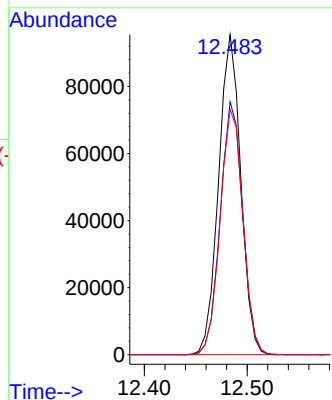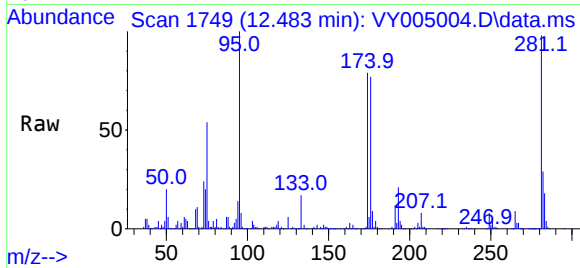

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.496 min Scan# 1587
Delta R.T. -0.000 min
Lab File: VY005004.D
Acq: 07 Jun 2021 19:38


Tgt Ion: 117 Resp: 322835
Ion Ratio Lower Upper
117 100
82 54.2 44.8 67.2
119 31.5 25.2 37.8

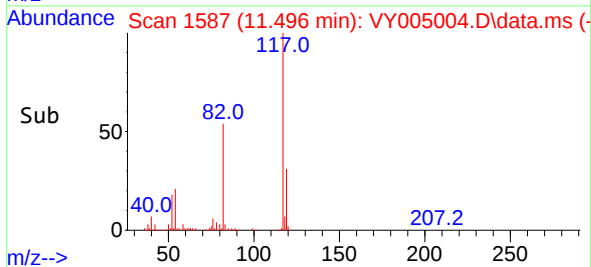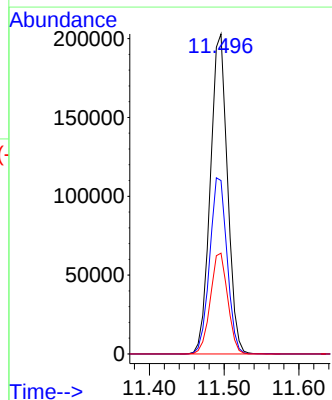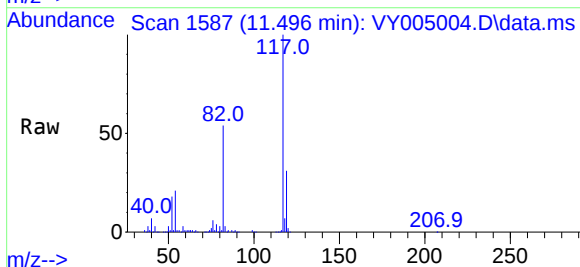

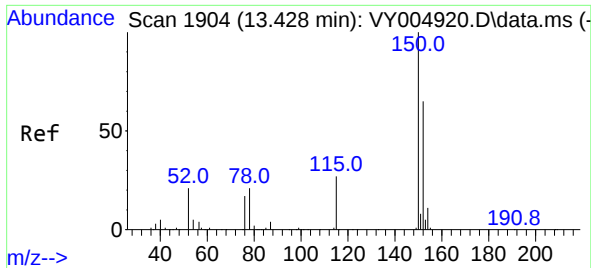

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.428 min Scan# 1904
 Delta R.T. -0.000 min
 Lab File: VY005004.D
 Acq: 07 Jun 2021 19:38

Instrument :
 MSVOA_Y
 ClientSampleId :
 18-B12(218-222)

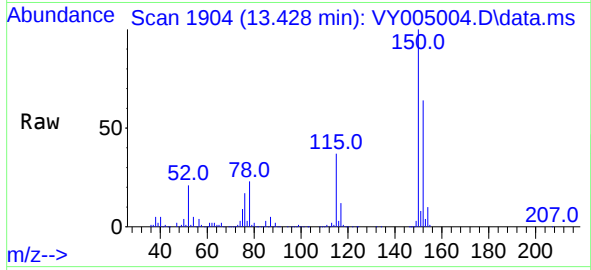

Tgt Ion:	152	Resp:	145722
Ion	Ratio	Lower	Upper
152	100		
115	58.4	29.9	89.7
150	156.6	0.0	347.8

