

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060722\
 Data File : VY009165.D
 Acq On : 07 Jun 2022 15:41
 Operator : KP/MD
 Sample : N3189-03RE
 Misc : 5.03g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 20220423-AMENDED-COMPOSITE-CRE

Quant Time: Jun 08 07:57:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052022S.M
 Quant Title : SW846 8260
 QLast Update : Fri May 20 23:50:52 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.783	168	108707	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	195184	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	180137	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	77069	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	68005	60.784	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 121.560%	
35) Dibromofluoromethane	7.710	113	26530	21.858	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 43.720%#	
50) Toluene-d8	10.179	98	240797	53.778	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 107.560%	
62) 4-Bromofluorobenzene	12.477	95	67673	37.466	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 74.940%	
Target Compounds						
						Qvalue
16) Acetone	3.942	43	58165	249.759	ug/l	91
17) Carbon Disulfide	4.186	76	108464	32.470	ug/l	99
25) 2-Butanone	6.978	43	15703	37.751	ug/l #	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060722\
Data File : VY009165.D
Acq On : 07 Jun 2022 15:41
Operator : KP/MD
Sample : N3189-03RE
Misc : 5.03g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
20220423-AMENDED-COMPOSITE-CRE

Quant Time: Jun 08 07:57:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052022S.M
Quant Title : SW846 8260
QLast Update : Fri May 20 23:50:52 2022
Response via : Initial Calibration




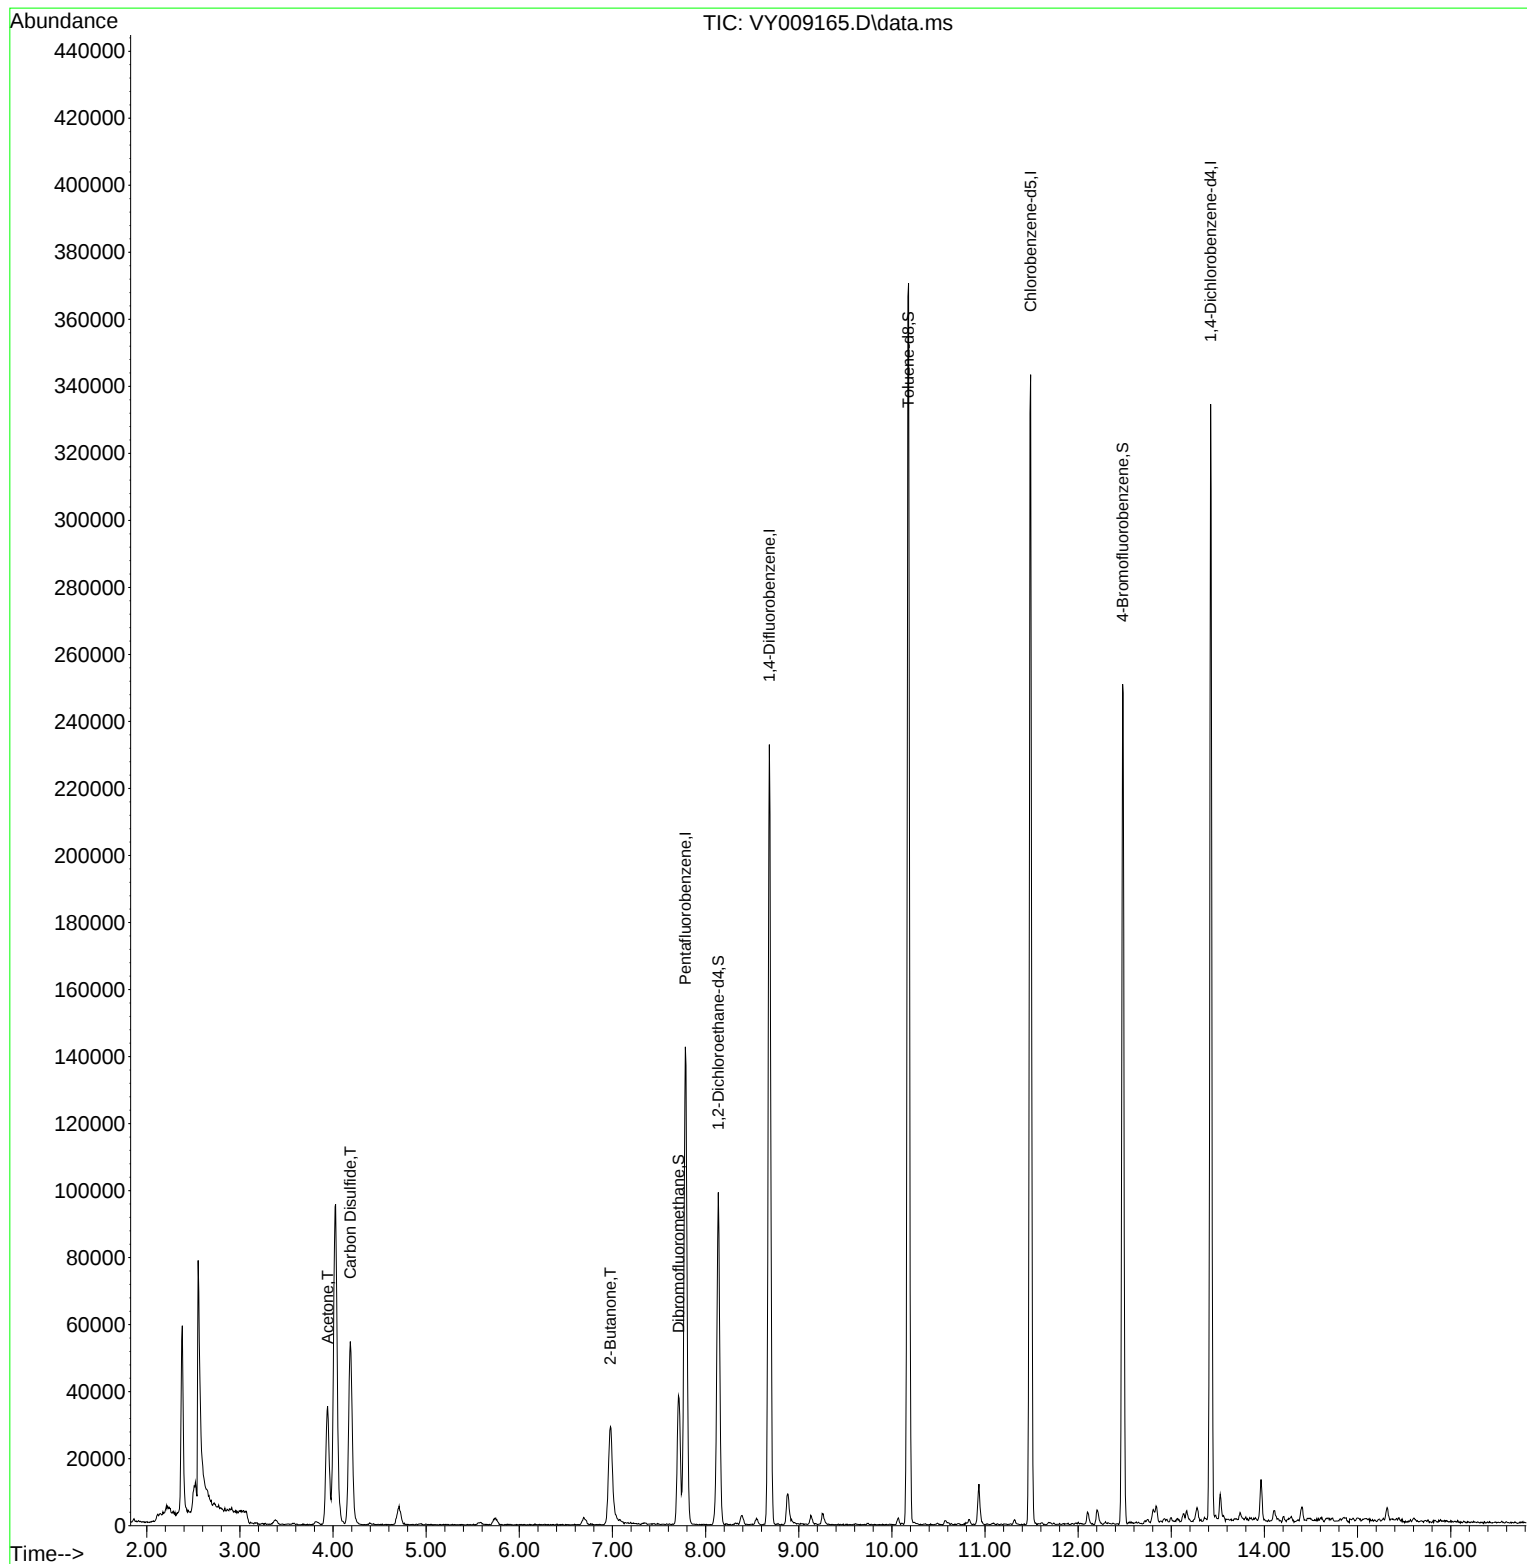


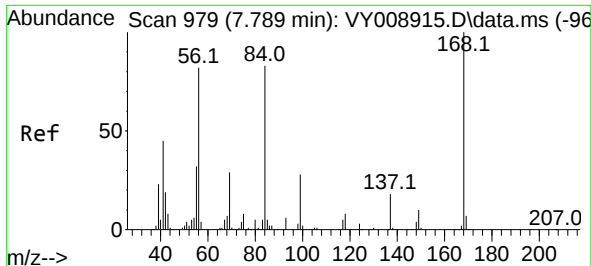

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY009165.D
Acq: 07 Jun 2022 15:41




Instrument :
MSVOA_Y
ClientSampleId :
20220423-AMENDED-COMPOSITE-CRE


Tgt Ion:168 Resp: 108707
Ion Ratio Lower Upper
168 100
99 52.2 46.9 70.3

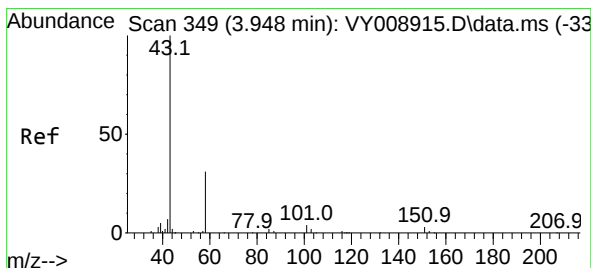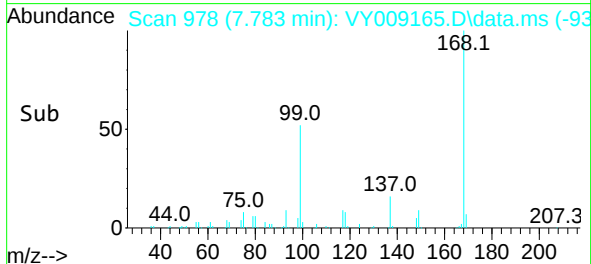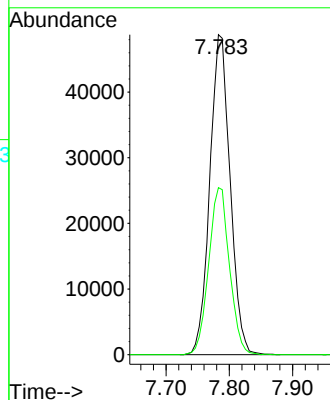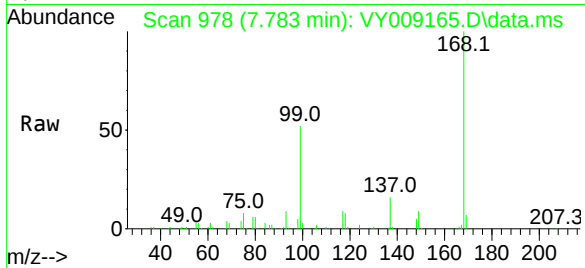

#16
Acetone
Concen: 249.759 ug/l
RT: 3.942 min Scan# 348
Delta R.T. -0.006 min
Lab File: VY009165.D
Acq: 07 Jun 2022 15:41

Tgt Ion: 43 Resp: 58165
Ion Ratio Lower Upper
43 100
58 32.1 22.0 33.0


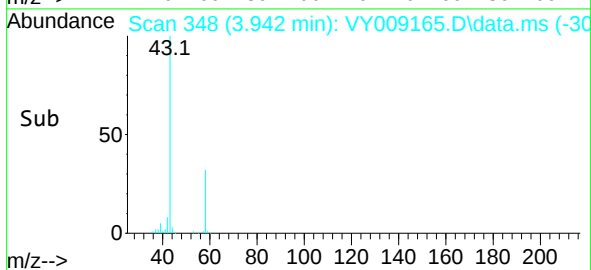
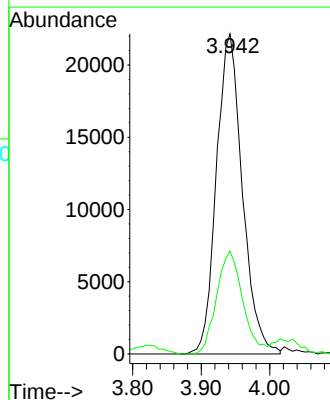
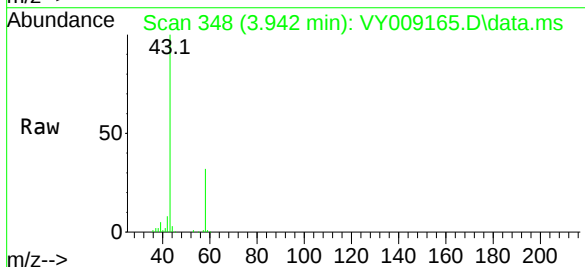


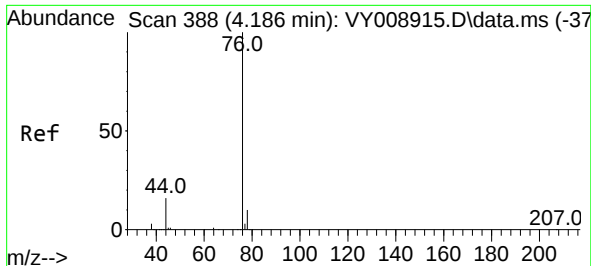

#17
Carbon Disulfide
Concen: 32.470 ug/l
RT: 4.186 min Scan# 388
Delta R.T. -0.000 min
Lab File: VY009165.D
Acq: 07 Jun 2022 15:41




Instrument : MSVOA_Y
ClientSampleId : 20220423-AMENDED-COMPOSITE-CRE


Tgt Ion: 76 Resp: 108464
Ion Ratio Lower Upper
76 100
78 8.9 7.4 11.0

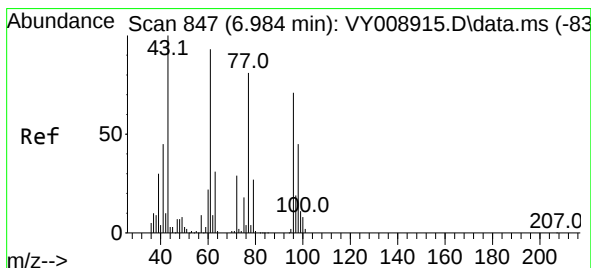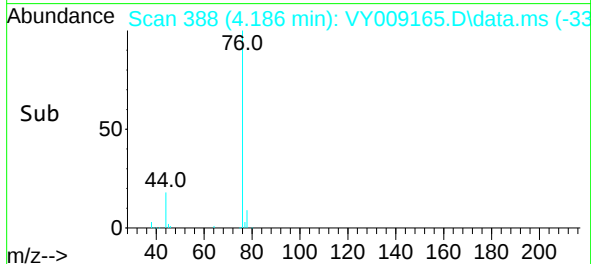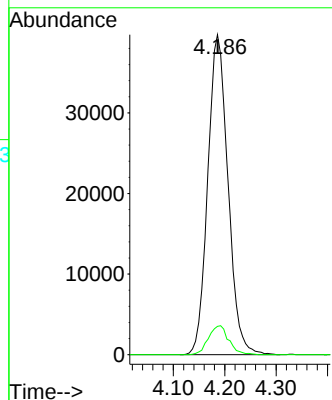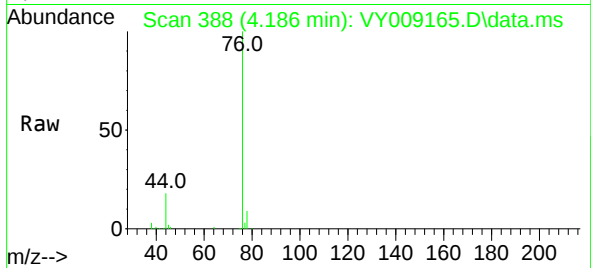

#25
2-Butanone
Concen: 37.751 ug/l
RT: 6.978 min Scan# 846
Delta R.T. -0.006 min
Lab File: VY009165.D
Acq: 07 Jun 2022 15:41

Tgt Ion: 43 Resp: 15703
Ion Ratio Lower Upper
43 100
72 28.2 17.7 26.5#

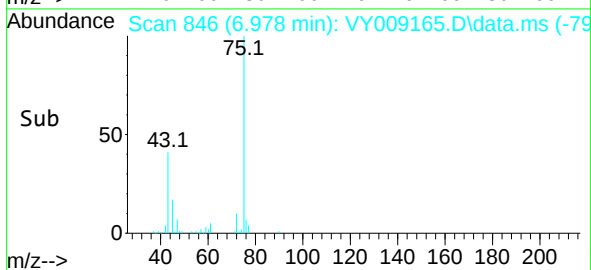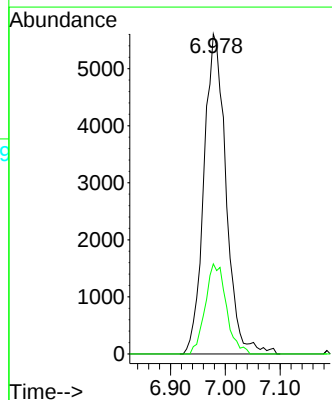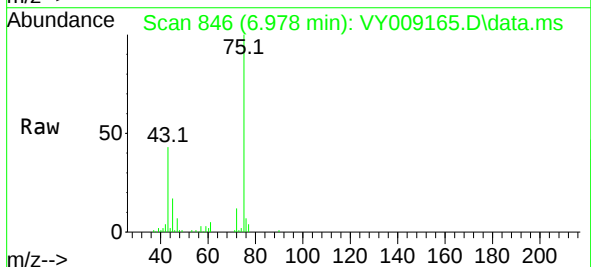

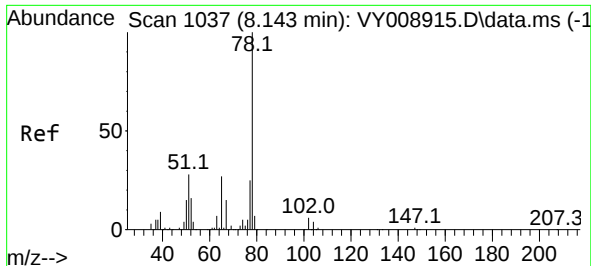

#33

1,2-Dichloroethane-d4

Concen: 60.784 ug/l

RT: 8.136 min Scan# 1

Delta R.T. -0.007 min

Lab File: VY009165.D

Acq: 07 Jun 2022 15:41

Instrument :

MSVOA_Y

ClientSampleId :





20220423-AMENDED-COMPOSITE-CRE

Tgt Ion: 65 Resp: 68005

Ion Ratio Lower Upper

65 100

67 52.2 0.0 99.4

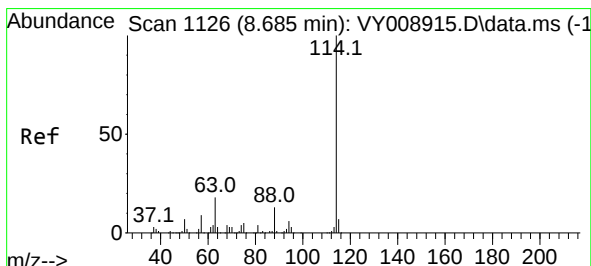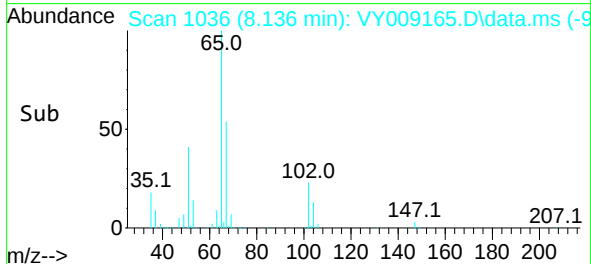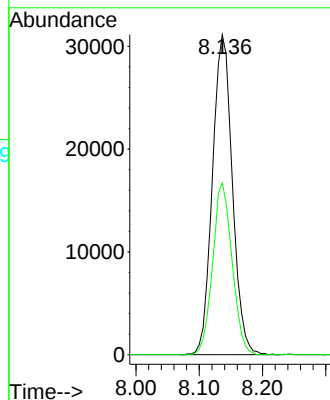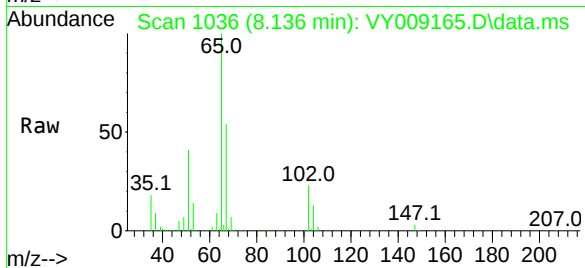

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. 0.000 min

Lab File: VY009165.D

Acq: 07 Jun 2022 15:41




Tgt Ion: 114 Resp: 195184


Ion Ratio Lower Upper

114 100

63 18.6 0.0 43.2

88 13.5 0.0 31.8


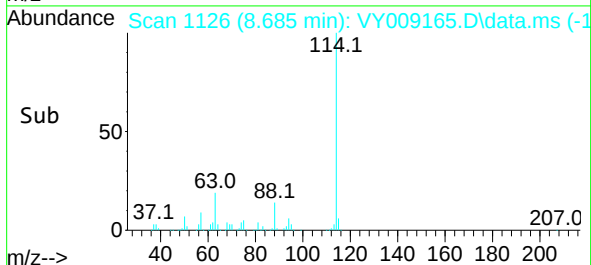
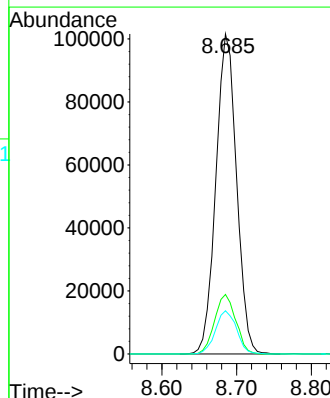
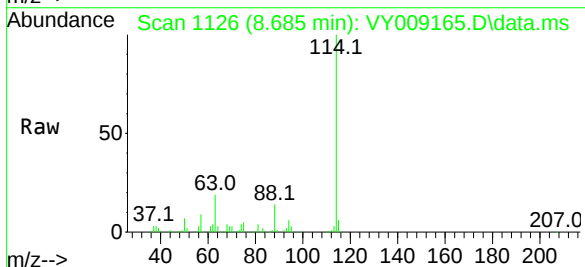


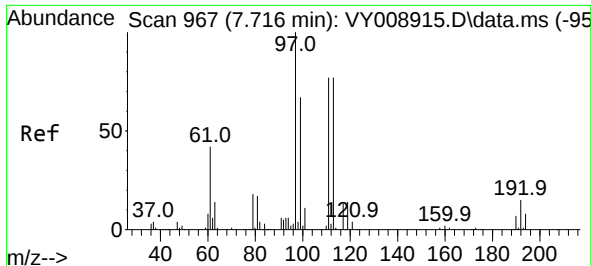

#35
Dibromofluoromethane
Concen: 21.858 ug/l
RT: 7.710 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY009165.D
Acq: 07 Jun 2022 15:41




Instrument :
MSVOA_Y
ClientSampleId :
20220423-AMENDED-COMPOSITE-CRE


Tgt Ion:113 Resp: 26530
Ion Ratio Lower Upper
113 100
111 103.4 82.6 124.0
192 19.7 17.6 26.4

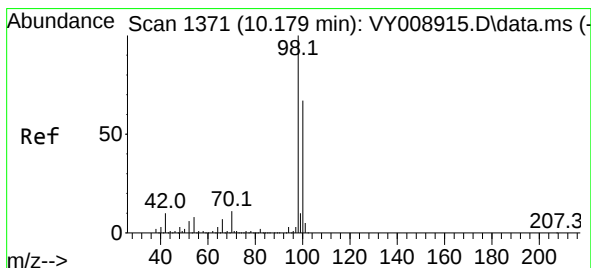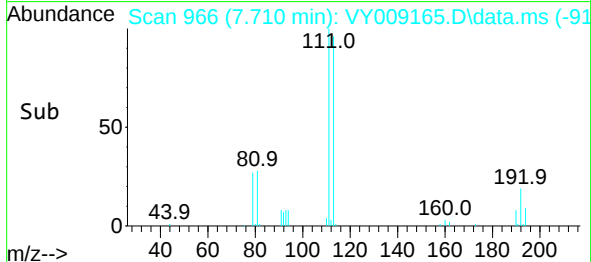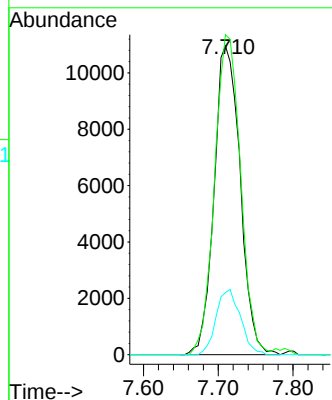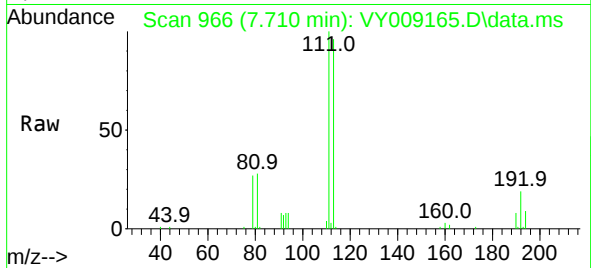

#50
Toluene-d8
Concen: 53.778 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY009165.D
Acq: 07 Jun 2022 15:41

Tgt Ion: 98 Resp: 240797
Ion Ratio Lower Upper
98 100
100 64.8 50.2 75.2


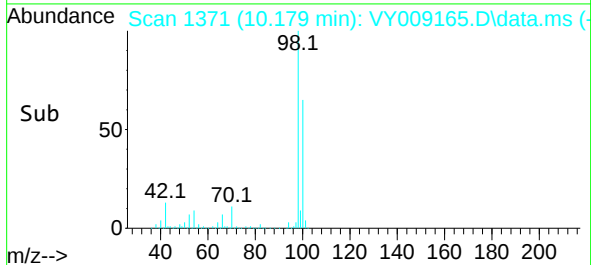
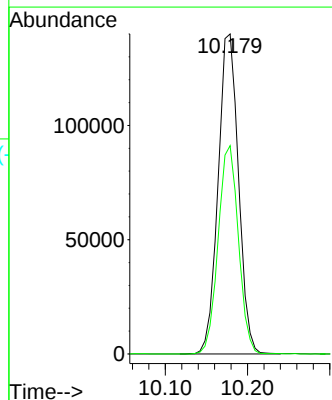
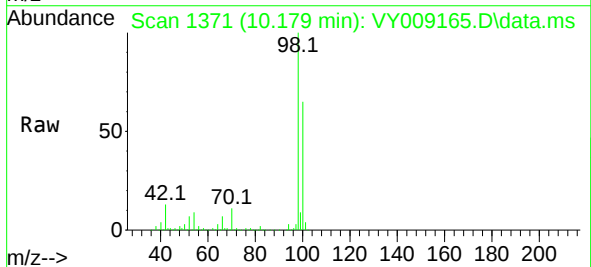


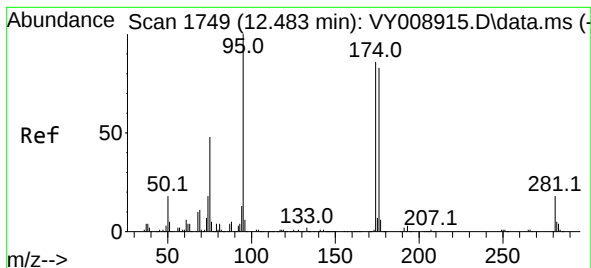

#62
4-Bromofluorobenzene
Concen: 37.466 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.006 min
Lab File: VY009165.D
Acq: 07 Jun 2022 15:41




Instrument : MSVOA_Y
ClientSampleId : 20220423-AMENDED-COMPOSITE-CRE


Tgt Ion: 95 Resp: 67673
Ion Ratio Lower Upper
95 100
174 93.1 0.0 177.0
176 88.8 0.0 175.8

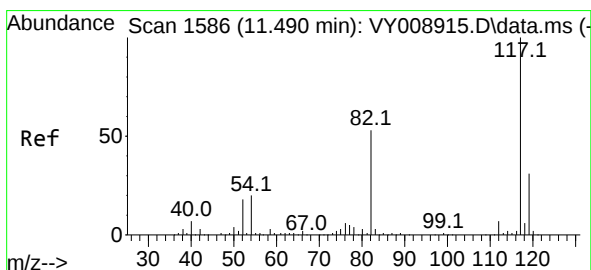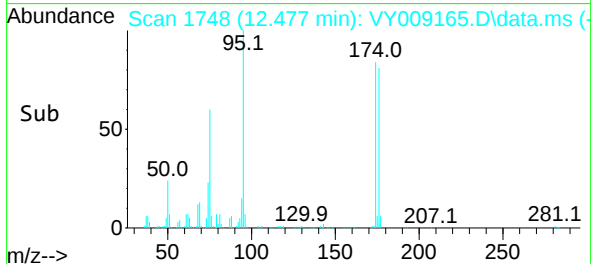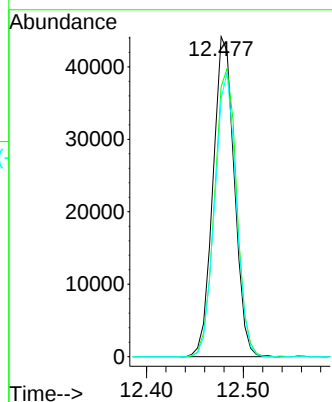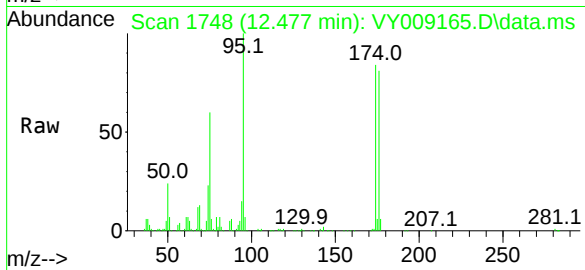

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 1586
Delta R.T. -0.001 min
Lab File: VY009165.D
Acq: 07 Jun 2022 15:41


Tgt Ion: 117 Resp: 180137
Ion Ratio Lower Upper
117 100
82 51.1 43.0 64.4
119 32.4 25.4 38.0

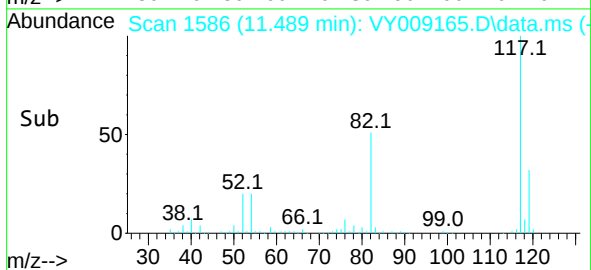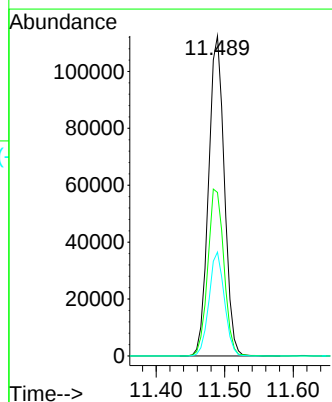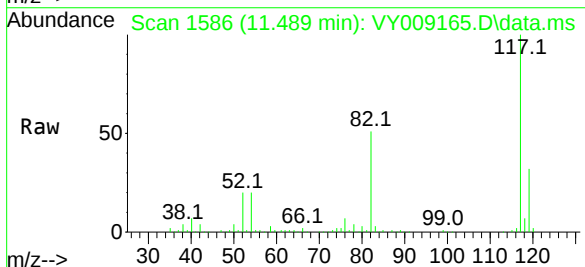

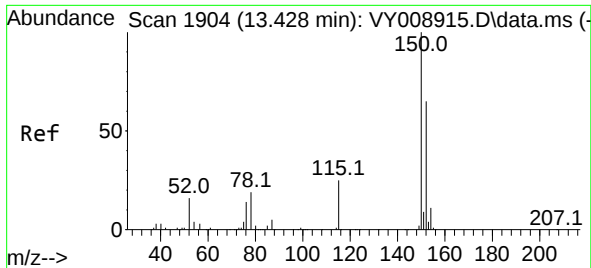

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.422 min Scan# 1903
 Delta R.T. -0.006 min
 Lab File: VY009165.D
 Acq: 07 Jun 2022 15:41

Instrument :
 MSVOA_Y
 ClientSampleId :
 20220423-AMENDED-COMPOSITE-CRE

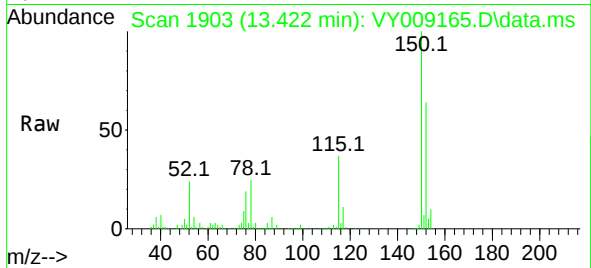

Tgt Ion:152 Resp: 77069
 Ion Ratio Lower Upper
 152 100
 115 55.9 28.2 84.7
 150 158.7 0.0 347.6

