
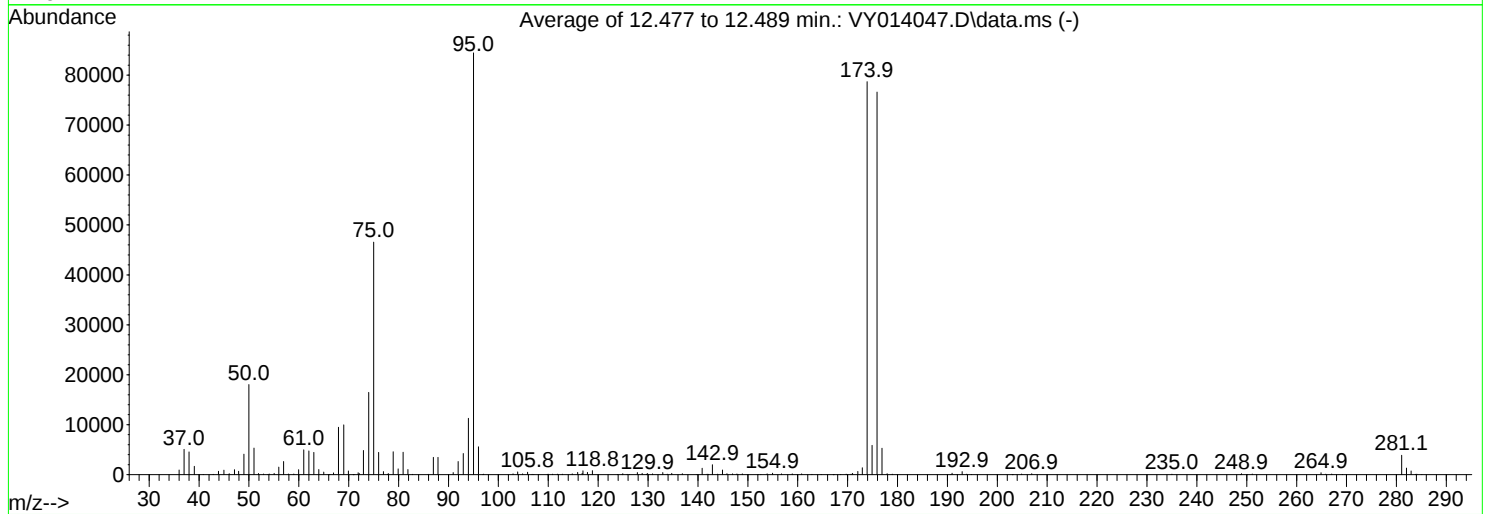


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060723\
Data File : VY014047.D
Acq On : 07 Jun 2023 09:04
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X052323W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Tue May 23 11:36:37 2023

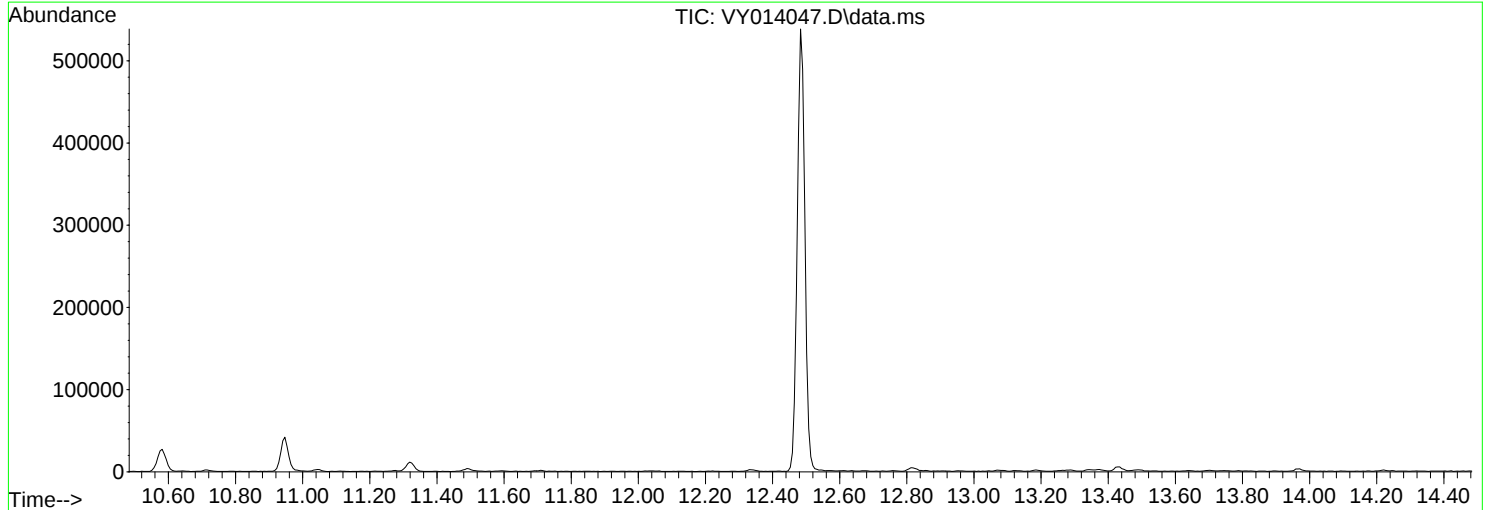

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	18047	PASS
75	95	30	60	55.1	46565	PASS
95	95	100	100	100.0	84461	PASS
96	95	5	9	6.6	5565	PASS
173	174	0.00	2	1.8	1385	PASS
174	95	50	100	93.2	78693	PASS
175	174	5	9	7.5	5873	PASS
176	174	95	101	97.3	76605	PASS
177	176	5	9	6.9	5276	PASS