
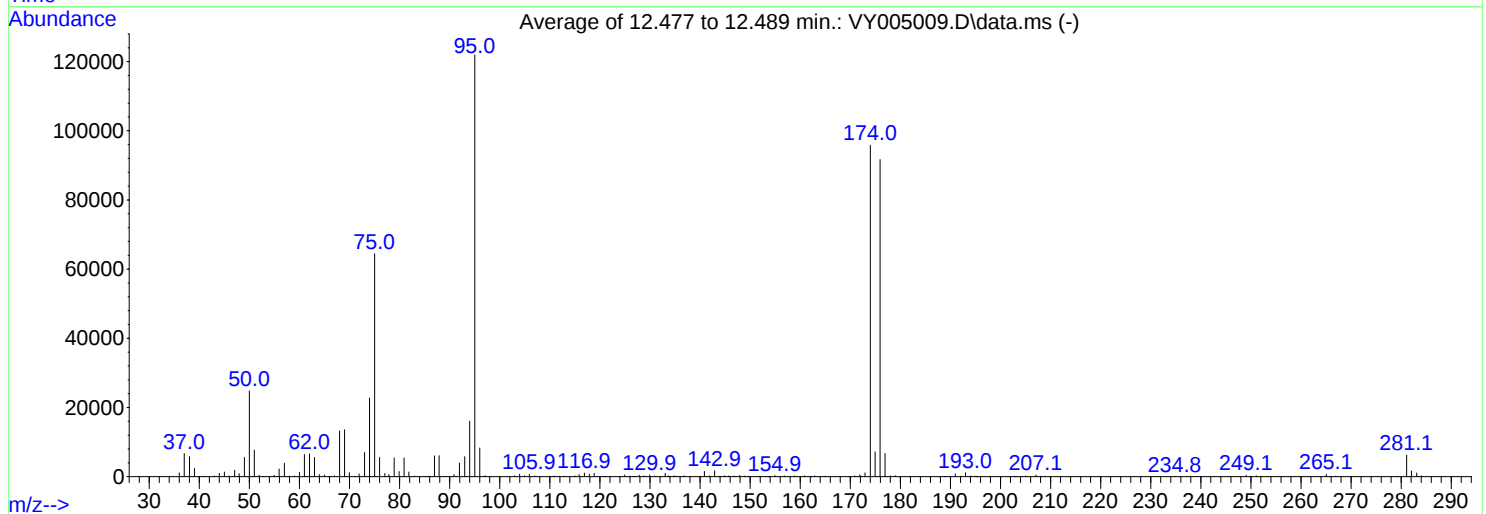


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060821\
 Data File : VY005009.D
 Acq On : 08 Jun 2021 09:18
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060221S.M
 Title : SW846 8260
 Last Update : Thu Jun 03 04:43:33 2021

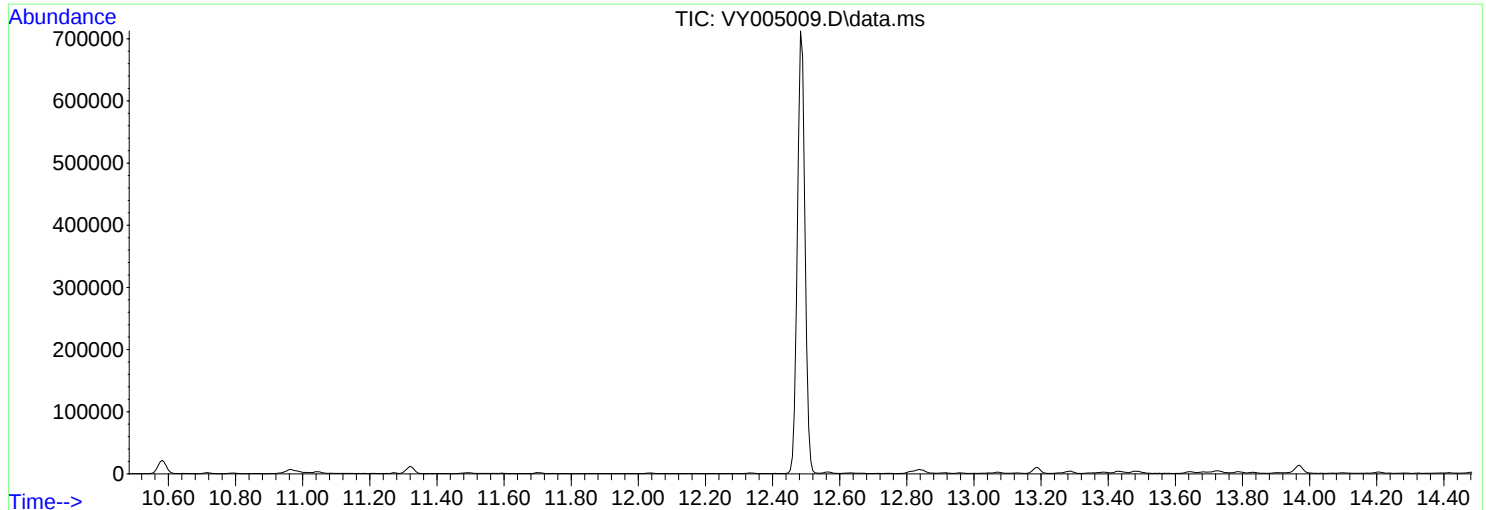

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	24789	PASS
75	95	30	60	52.8	64453	PASS
95	95	100	100	100.0	121960	PASS
96	95	5	9	6.8	8263	PASS
173	174	0.00	2	1.2	1122	PASS
174	95	50	100	78.6	95803	PASS
175	174	5	9	7.5	7186	PASS
176	174	95	101	95.7	91677	PASS
177	176	5	9	7.3	6690	PASS