

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY060920\
 Data File : VY002867.D
 Acq On : 09 Jun 2020 12:33
 Operator : SY/MD
 Sample : L2951-01
 Misc : 5.17G/5ML/MSVOA Y/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 239988

Quant Time: Jun 10 05:47:25 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y052720S.M
 Quant Title : SW846 8260
 QLast Update : Wed May 27 13:13:33 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.80	168	247001	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.69	114	398097	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.49	117	373274	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.42	152	189157	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.15	65	124638	58.12	ug/l	0.00
Spiked Amount 50.000			Recovery	=	116.24%	
35) Dibromofluoromethane	7.72	113	121628	52.13	ug/l	0.00
Spiked Amount 50.000			Recovery	=	104.26%	
50) Toluene-d8	10.18	98	471176	49.95	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.90%	
62) 4-Bromofluorobenzene	12.48	95	161436	50.08	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.16%	
Target Compounds						
20) Methylene Chloride	4.72	84	27940	11.369	ug/l	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY060920\
Data File : VY002867.D
Acq On : 09 Jun 2020 12:33
Operator : SY/MD
Sample : L2951-01
Misc : 5.17G/5ML/MSVOA Y/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
239988

Quant Time: Jun 10 05:47:25 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y052720S.M
Quant Title : SW846 8260
QLast Update : Wed May 27 13:13:33 2020
Response via : Initial Calibration

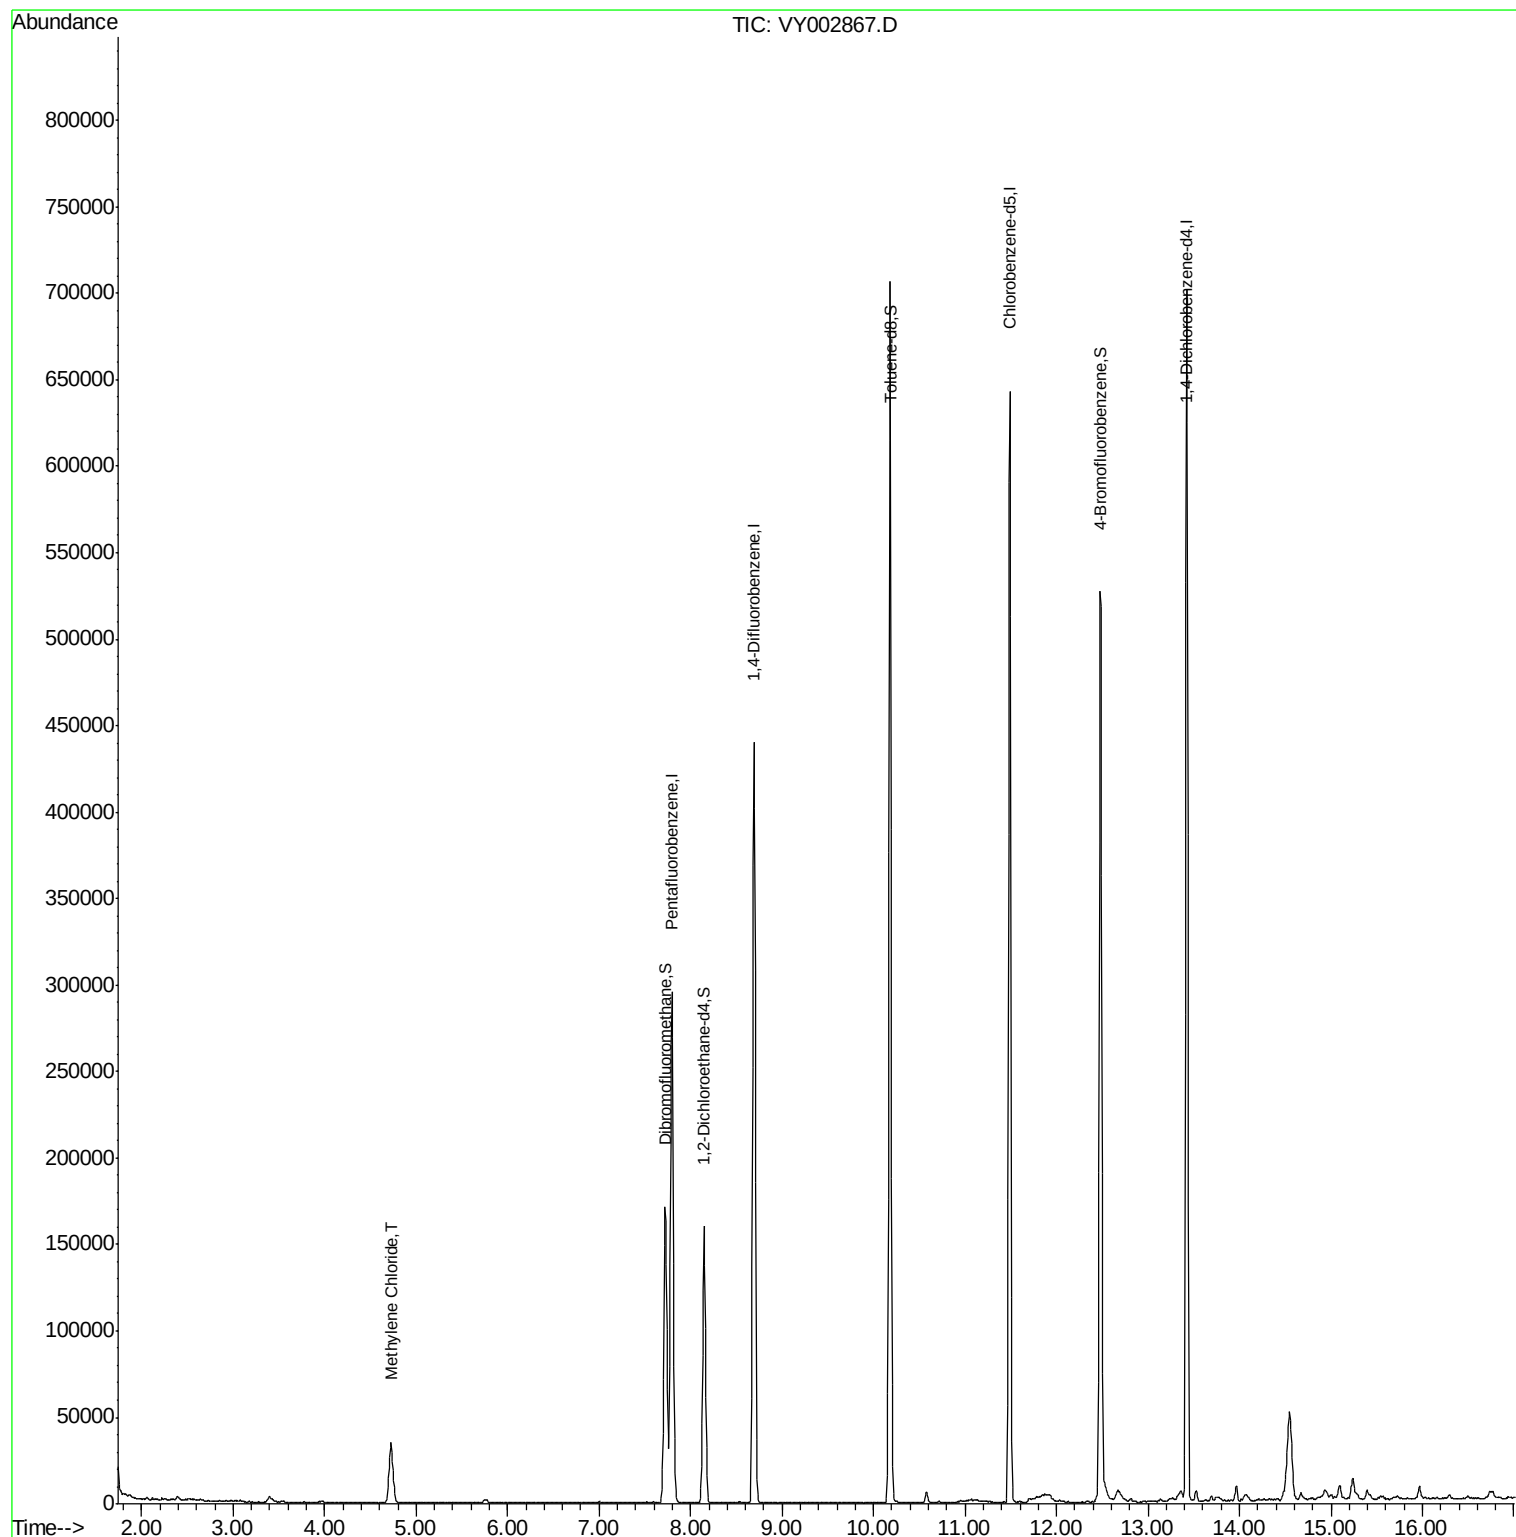

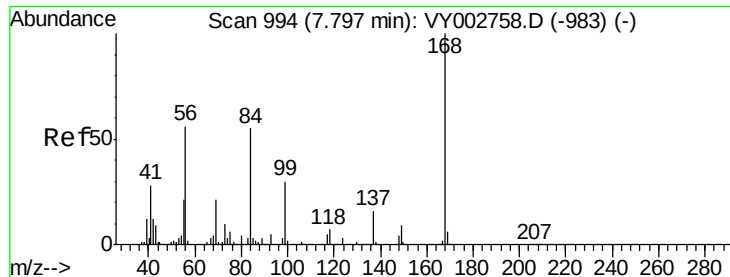

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.80 min Scan# 994

Delta R.T. -0.00 min

Lab File: VY002867.D

Acq: 09 Jun 2020 12:33

Instrument :

MSVOA_Y

ClientSampleId :


239988

Tot Ion:168 Resp: 247001

Ion Ratio Lower Upper

168 100

99 46.8 39.0 58.4

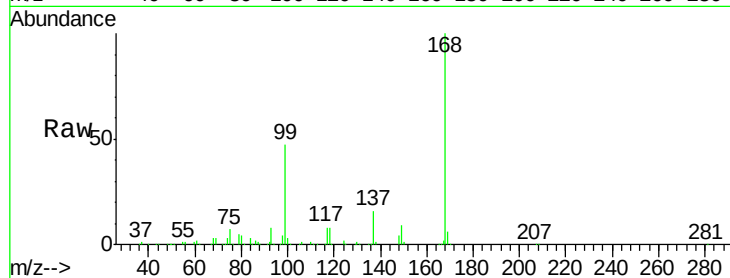

Abundance Ion 167.90 (167.60 to 168.60): VY002758.D (-983) (-)

Ion 98.90 (98.60 to 99.60): VY002758.D (-983) (-)

7.80

120000

100000

80000



60000

40000

20000

0

Time-->

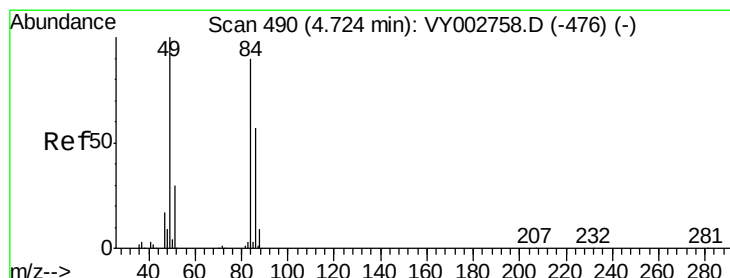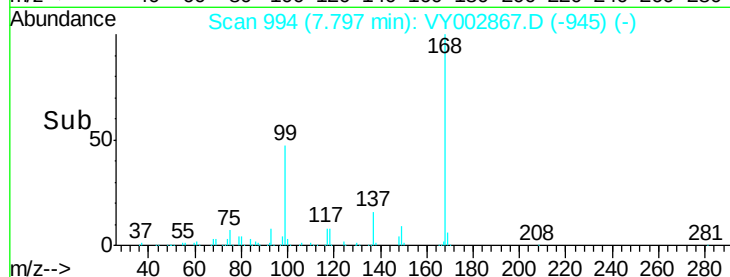

#20

Methylene Chloride

Concen: 11.369 ug/l

RT: 4.72 min Scan# 490

Delta R.T. -0.00 min

Lab File: VY002867.D

Acq: 09 Jun 2020 12:33

Tgt Ion: 84 Resp: 27940


Ion Ratio Lower Upper

84 100

49 112.5 88.5 132.7

51 36.7 26.8 40.2

86 69.0 50.6 75.8

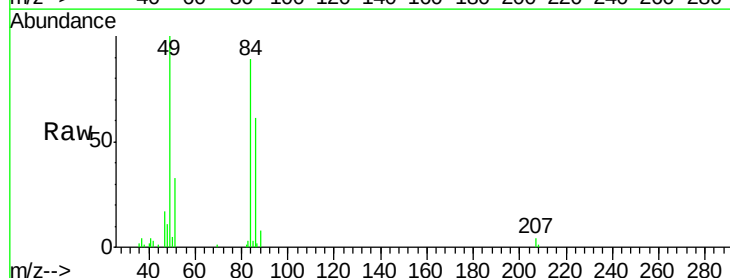

Abundance Ion 83.90 (83.60 to 84.60): VY002758.D (-476) (-)

Ion 48.90 (48.60 to 49.60): VY002758.D (-476) (-)

Ion 50.90 (50.60 to 51.60): VY002758.D (-476) (-)

Ion 85.90 (85.60 to 86.60): VY002758.D (-476) (-)


15000


10000

5000

0

Time-->




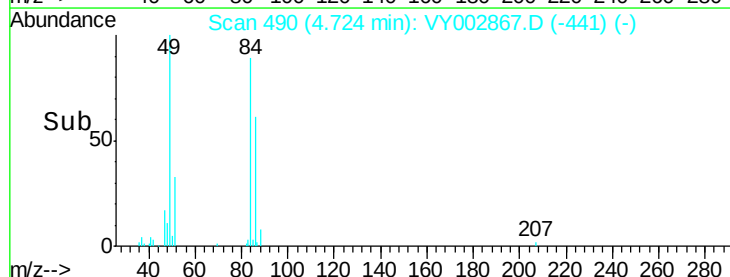


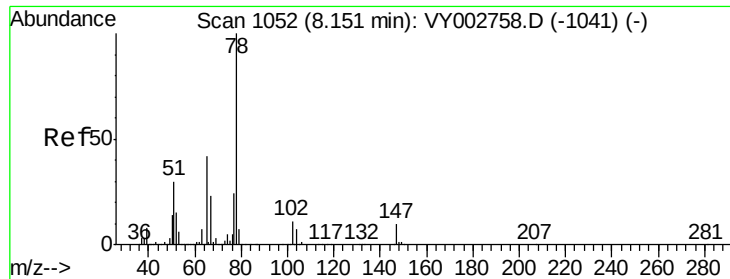

#33
 1,2-Dichloroethane-d4
 Concen: 58.116 ug/l
 RT: 8.15 min Scan# 1052
 Delta R.T. -0.00 min
 Lab File: VY002867.D
 Acq: 09 Jun 2020 12:33




Instrument :
 MSVOA_Y
 ClientSampleId :
 239988


Tot Ion: 65 Resp: 124638
 Ion Ratio Lower Upper
 65 100
 67 53.6 0.0 111.0

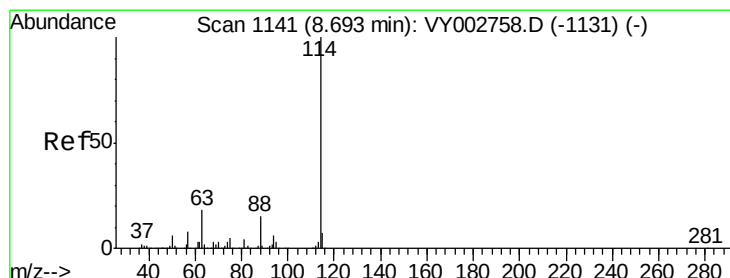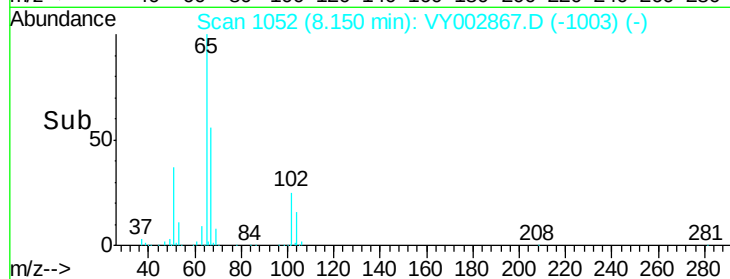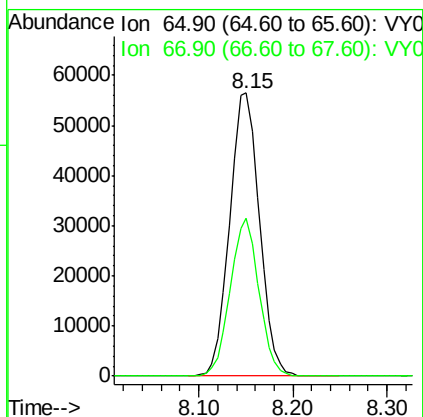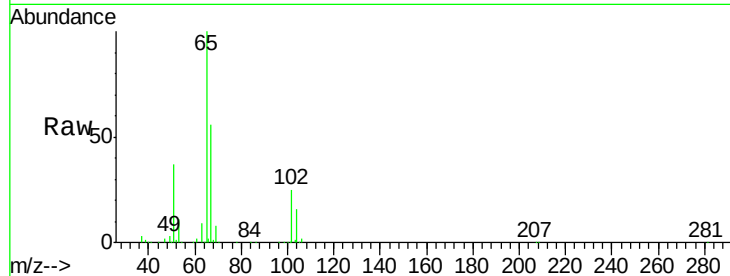

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.69 min Scan# 1141
 Delta R.T. -0.00 min
 Lab File: VY002867.D
 Acq: 09 Jun 2020 12:33

Tgt Ion: 114 Resp: 398097
 Ion Ratio Lower Upper
 114 100
 63 17.6 0.0 35.2
 88 14.4 0.0 29.2


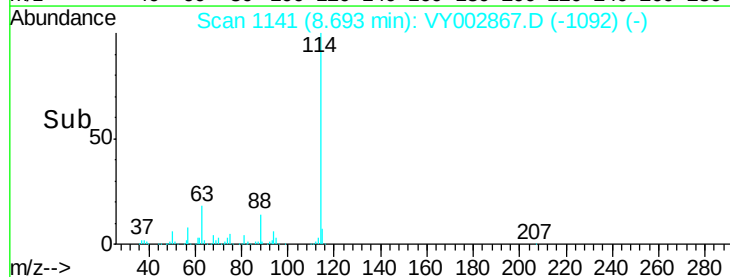
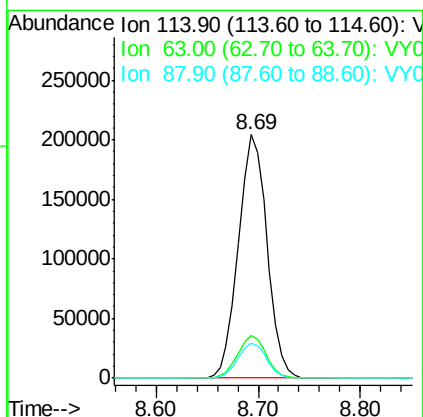
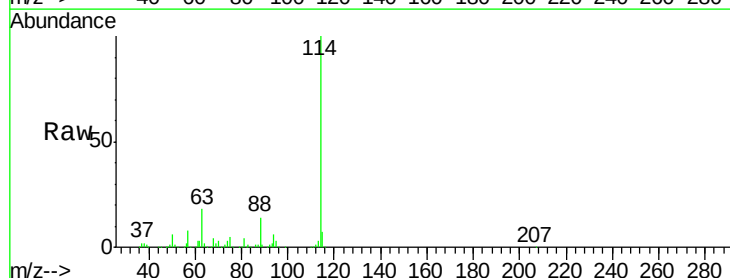


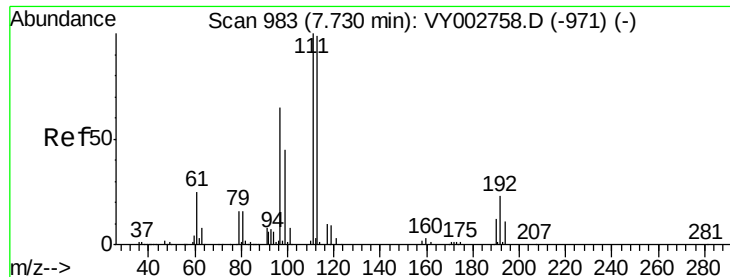

#35
 Dibromofluoromethane
 Concen: 52.133 ug/l
 RT: 7.72 min Scan# 982
 Delta R.T. -0.01 min
 Lab File: VY002867.D
 Acq: 09 Jun 2020 12:33




Instrument :
 MSVOA_Y
 ClientSampleId :
 239988


Tot Ion	Ratio	Lower	Upper
113	100		
111	103.2	82.0	123.0
192	23.5	18.9	28.3

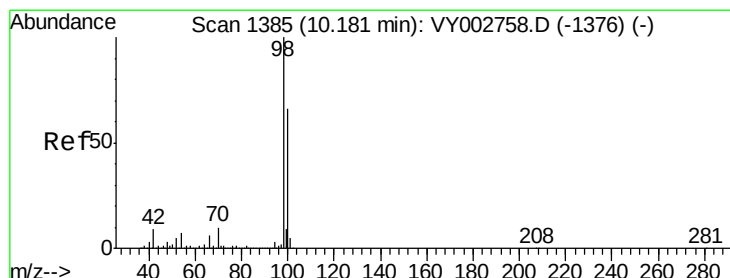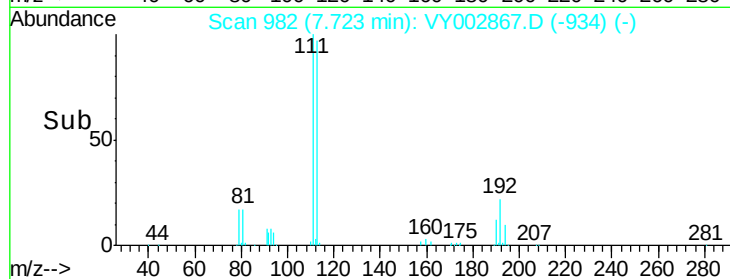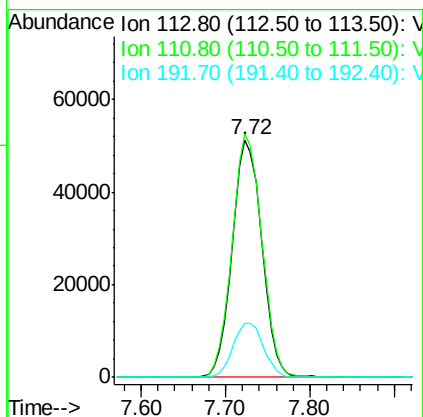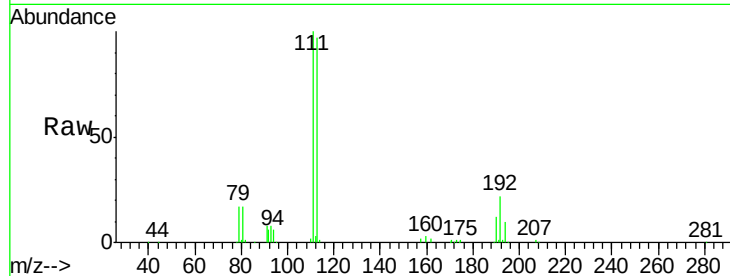

#50
 Toluene-d8
 Concen: 49.949 ug/l
 RT: 10.18 min Scan# 1385
 Delta R.T. -0.00 min
 Lab File: VY002867.D
 Acq: 09 Jun 2020 12:33

Tgt Ion	Ratio	Lower	Upper
98	100		
100	64.5	52.2	78.2

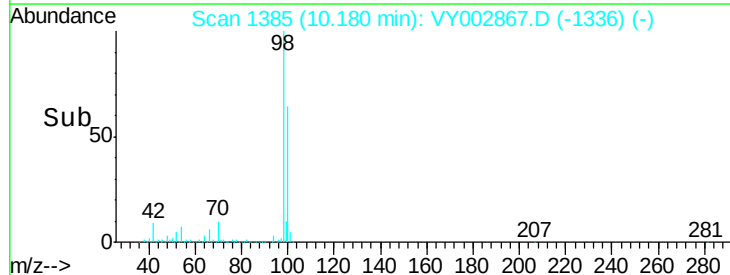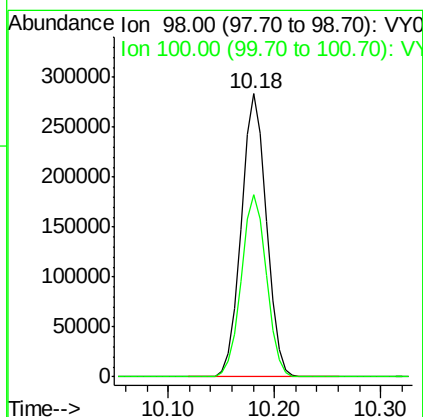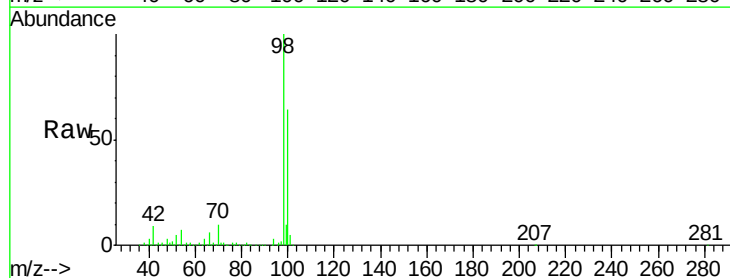

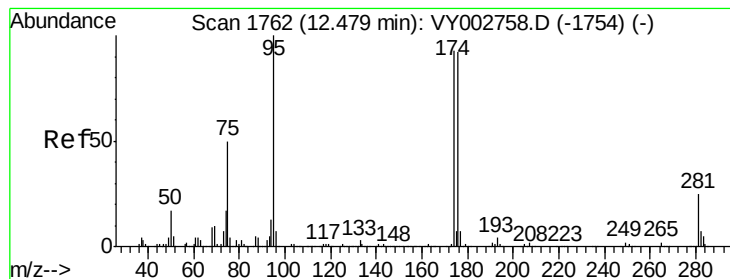

#62

4-Bromofluorobenzene

Concen: 50.077 ug/l

RT: 12.48 min Scan# 1762

Delta R.T. -0.00 min

Lab File: VY002867.D

Acq: 09 Jun 2020 12:33

Instrument :

MSVOA_Y

ClientSampled :

239988


Tot Ion: 95 Resp: 161436

Ion Ratio Lower Upper

95 100

174 95.8 0.0 191.2




176 92.4 0.0 188.8

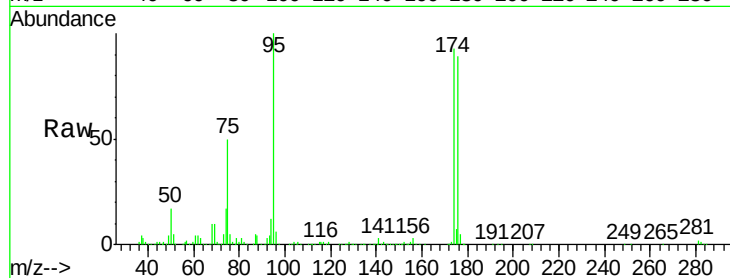

Abundance Ion 94.90 (94.60 to 95.60): VY002867.D (-1713) (-)

Ion 173.80 (173.50 to 174.50): VY002867.D (-1713) (-)

Ion 175.80 (175.50 to 176.50): VY002867.D (-1713) (-)

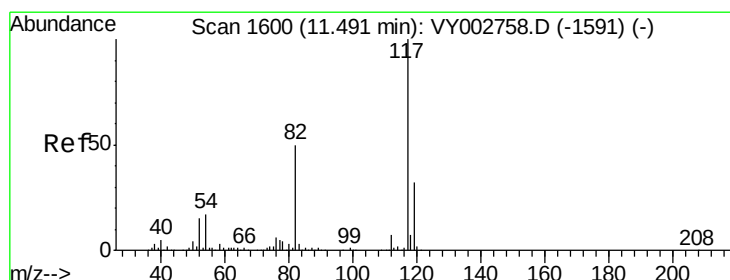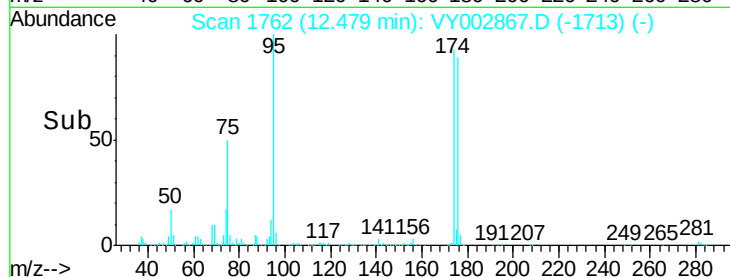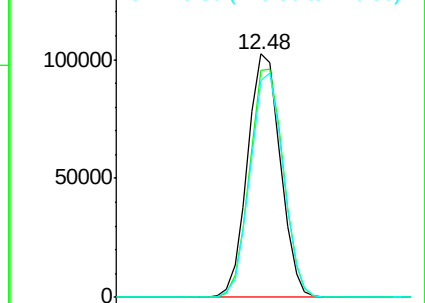

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.49 min Scan# 1600

Delta R.T. -0.00 min

Lab File: VY002867.D

Acq: 09 Jun 2020 12:33


Tgt Ion: 117 Resp: 373274

Ion Ratio Lower Upper

117 100

82 50.4 40.2 60.4



119 32.0 25.8 38.8

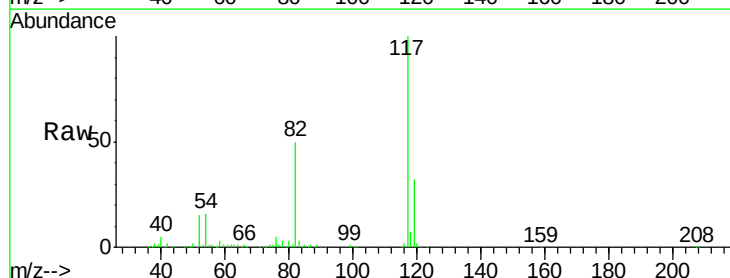


Abundance Ion 116.90 (116.60 to 117.60): VY002867.D (-1551) (-)

Ion 82.00 (81.70 to 82.70): VY002867.D (-1551) (-)

Ion 118.90 (118.60 to 119.60): VY002867.D (-1551) (-)

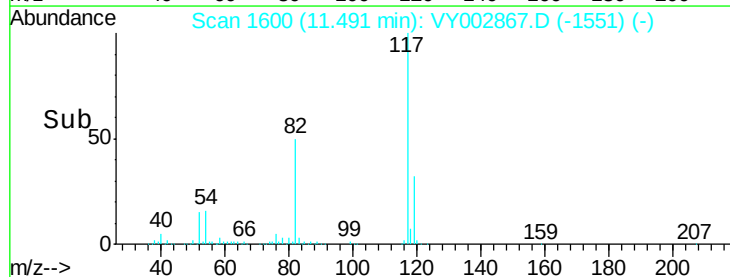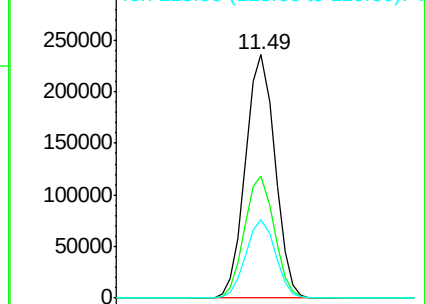

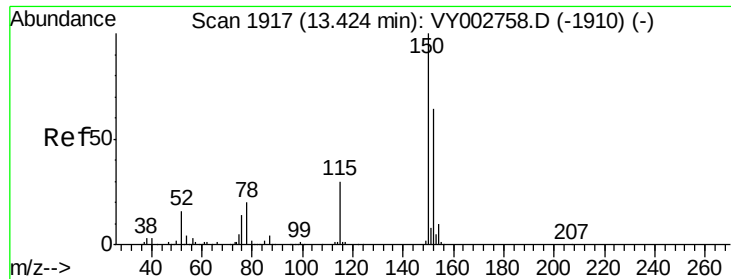

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.42 min Scan# 1917

Delta R.T. -0.00 min

Lab File: VY002867.D

Acq: 09 Jun 2020 12:33

Instrument :

MSVOA_Y

ClientSampleId :

239988


Tot Ion:152 Resp: 189157

Ion Ratio Lower Upper

152 100

115 53.9 27.0 81.0

150 158.9 0.0 344.8

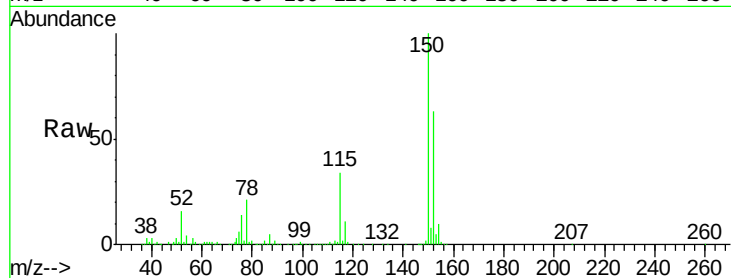

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

