

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY061021\
 Data File : VY005087.D
 Acq On : 10 Jun 2021 19:11
 Operator : SY/MD
 Sample : M2672-10
 Misc : 6.52G/5ML/MSVOA_Y/SOIL
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 17-B6(44-48)

Quant Time: Jun 11 05:08:14 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060221S.M
 Quant Title : SW846 8260
 QLast Update : Thu Jun 03 04:43:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.801	168	177353	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	325227	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.495	117	316009	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	143215	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	113324	60.442	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	120.880%
35) Dibromofluoromethane	7.728	113	100399	57.379	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	114.760%
50) Toluene-d8	10.185	98	402190	55.345	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	110.680%
62) 4-Bromofluorobenzene	12.483	95	139557	55.840	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	111.680%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY061021\
Data File : VY005087.D
Acq On : 10 Jun 2021 19:11
Operator : SY/MD
Sample : M2672-10
Misc : 6.52G/5ML/MSVOA_Y/SOIL
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
17-B6(44-48)

Quant Time: Jun 11 05:08:14 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060221S.M
Quant Title : SW846 8260
QLast Update : Thu Jun 03 04:43:33 2021
Response via : Initial Calibration




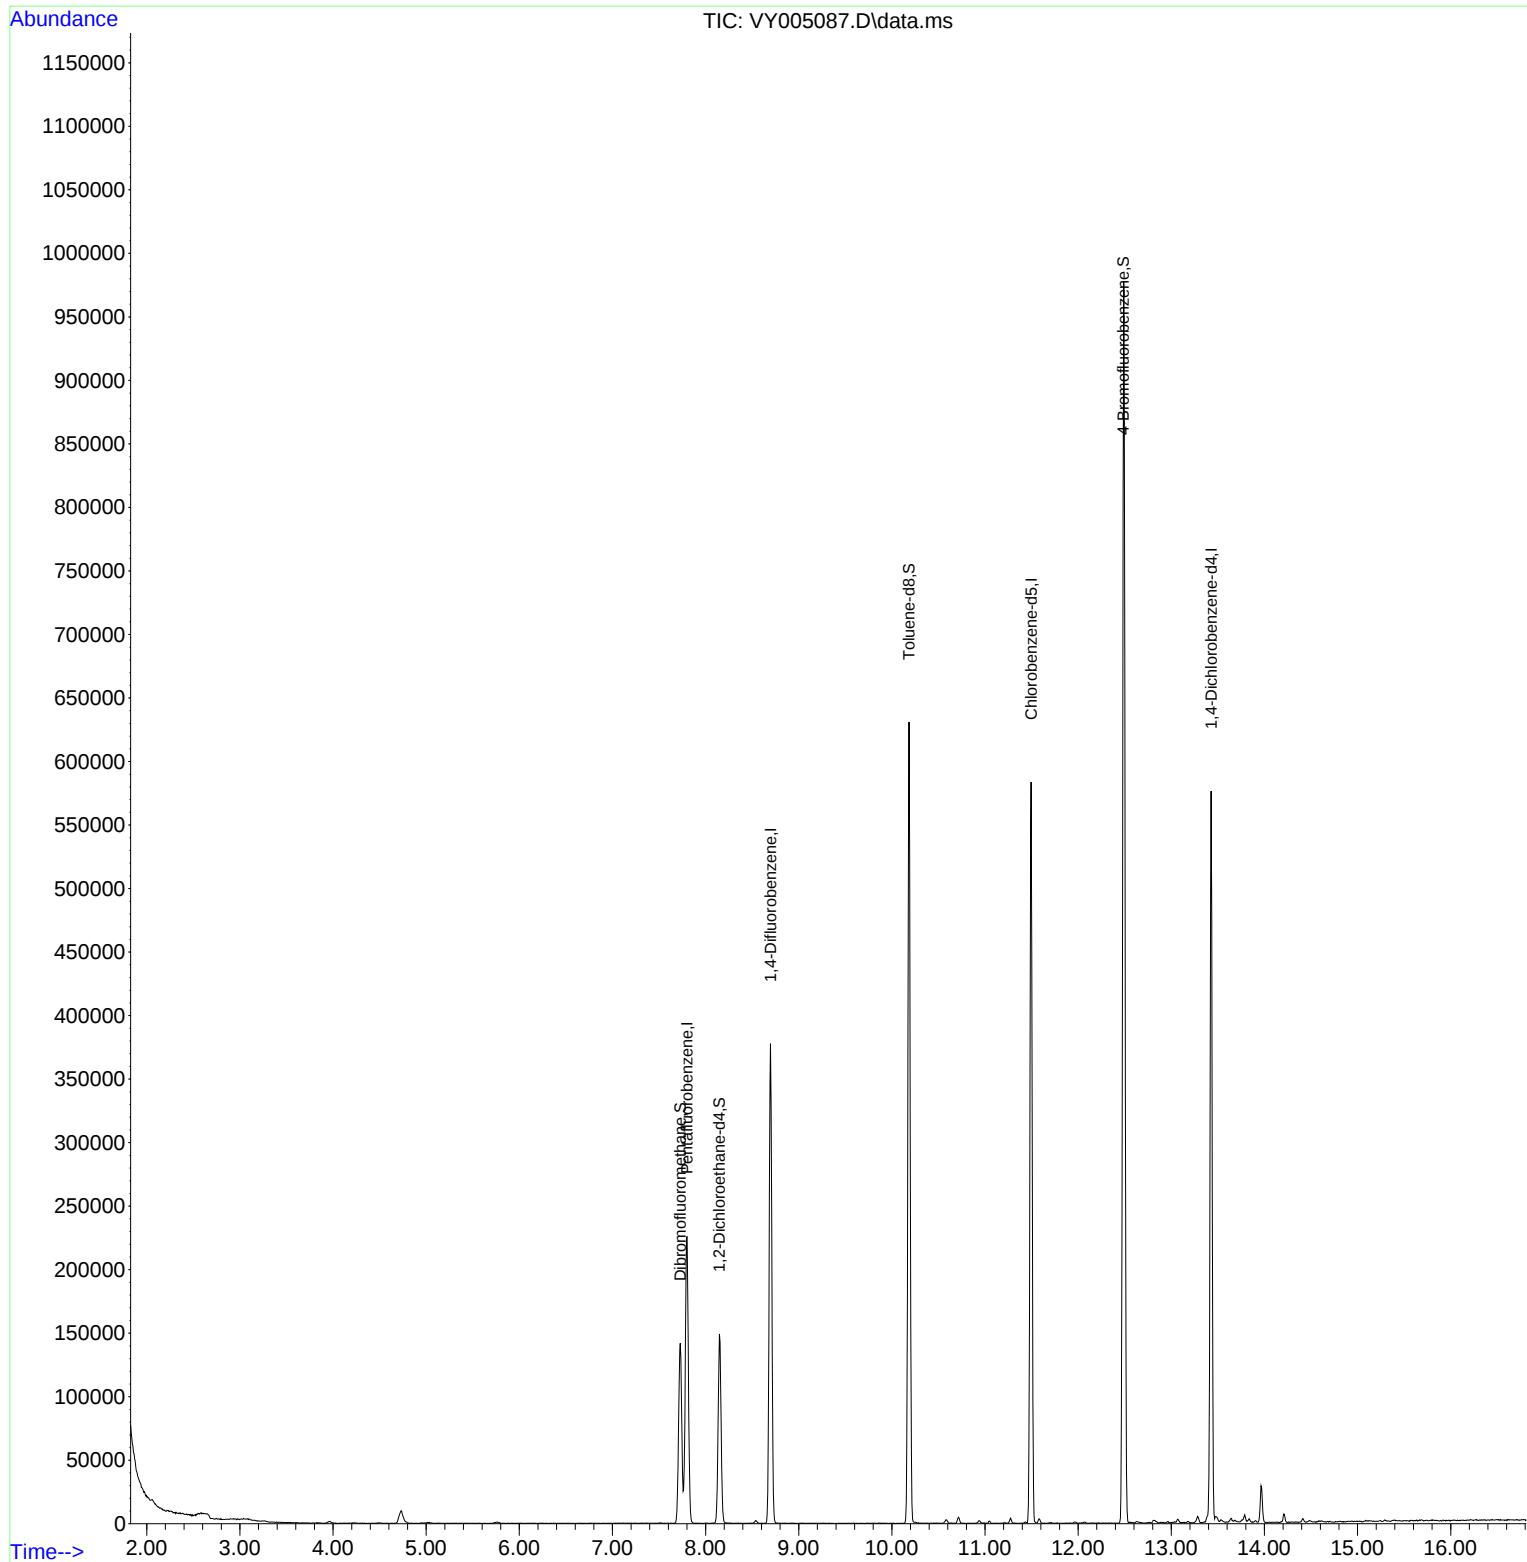


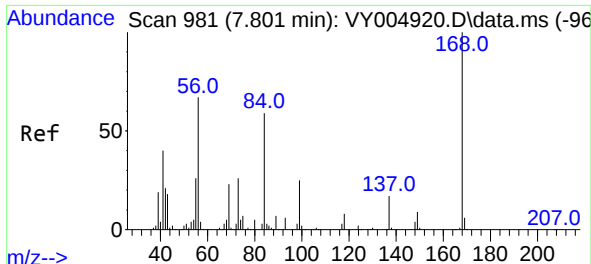

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.801 min Scan# 981
Delta R.T. 0.000 min
Lab File: VY005087.D
Acq: 10 Jun 2021 19:11




Instrument :
MSVOA_Y
ClientSampleId :
17-B6(44-48)


Tgt Ion:168 Resp: 177353
Ion Ratio Lower Upper
168 100
99 54.0 43.9 65.9

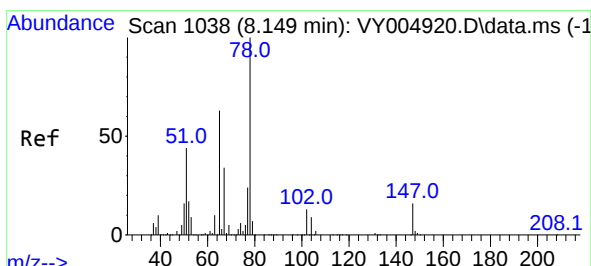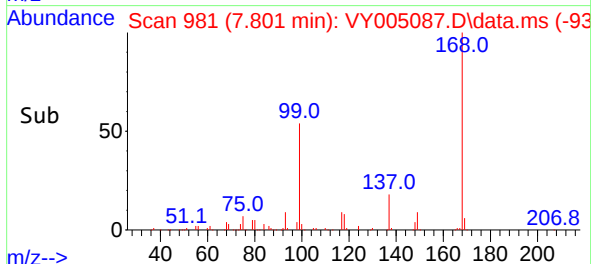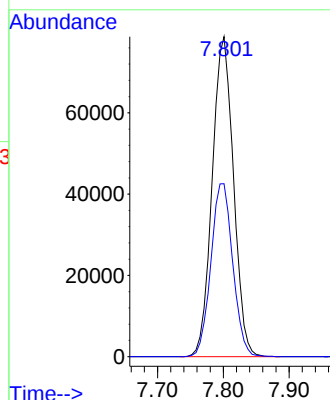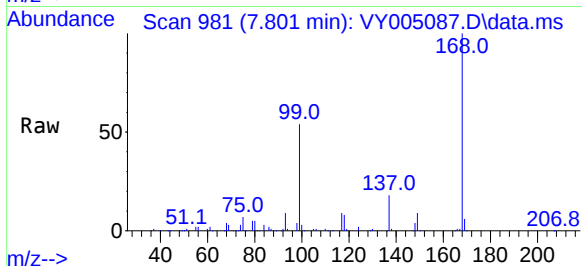

#33
1,2-Dichloroethane-d4
Concen: 60.442 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. -0.000 min
Lab File: VY005087.D
Acq: 10 Jun 2021 19:11


Tgt Ion: 65 Resp: 113324
Ion Ratio Lower Upper
65 100
67 53.6 0.0 110.6

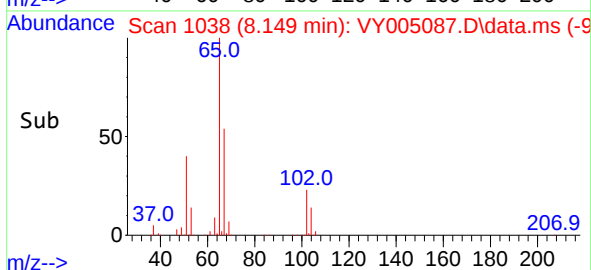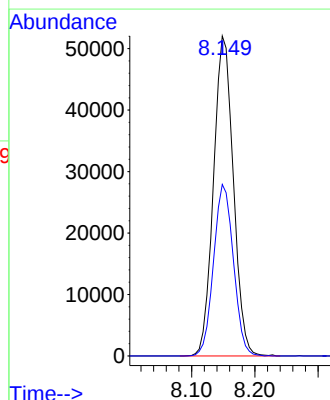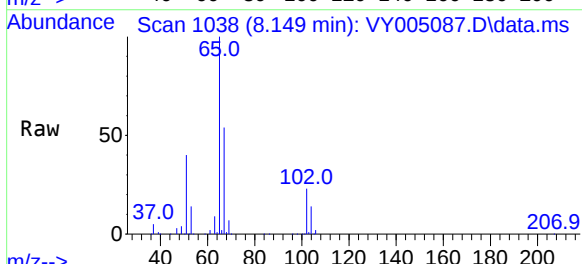

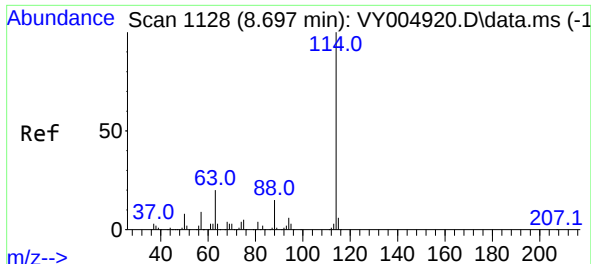




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. -0.000 min
Lab File: VY005087.D
Acq: 10 Jun 2021 19:11

Instrument :
MSVOA_Y
ClientSampleId :
17-B6(44-48)

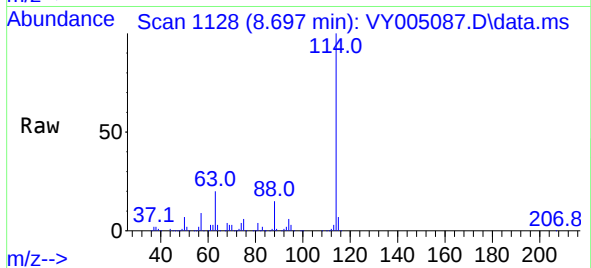

Tgt Ion:114 Resp: 325227




Ion	Ratio	Lower	Upper
114	100		
63	19.6	0.0	41.0
88	15.2	0.0	30.6

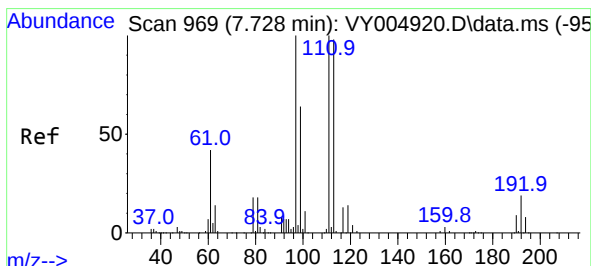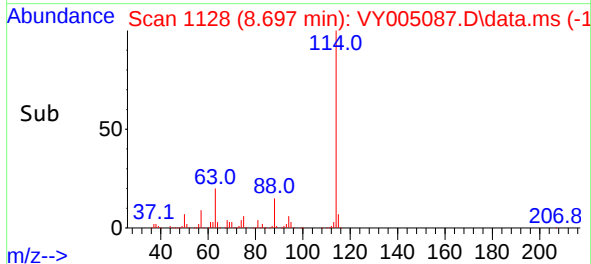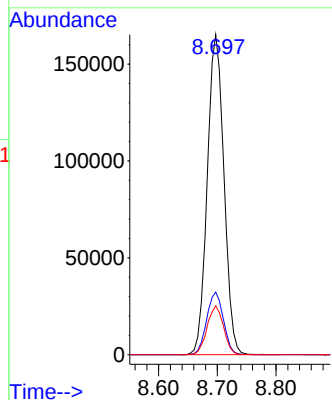


#35
Dibromofluoromethane
Concen: 57.379 ug/l
RT: 7.728 min Scan# 969
Delta R.T. -0.000 min
Lab File: VY005087.D
Acq: 10 Jun 2021 19:11

Tgt Ion:113 Resp: 100399

Ion	Ratio	Lower	Upper
113	100		
111	104.6	81.8	122.8
192	19.2	15.3	22.9


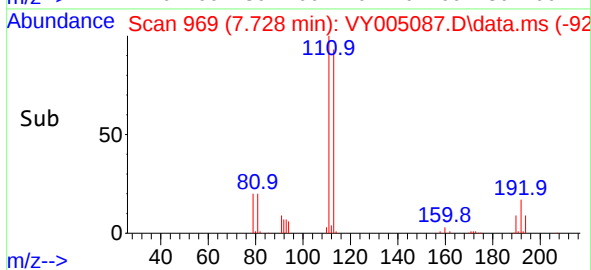
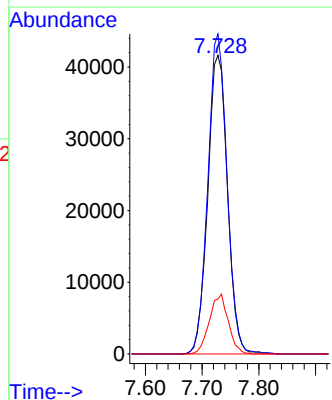
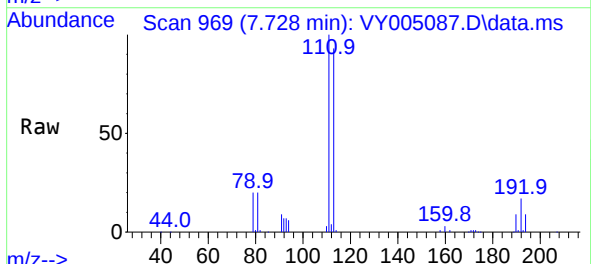


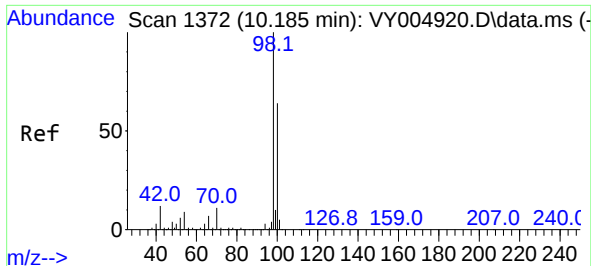

#50
Toluene-d8
Concen: 55.345 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. -0.000 min
Lab File: VY005087.D
Acq: 10 Jun 2021 19:11




Instrument :
MSVOA_Y
ClientSampleId :
17-B6(44-48)


Tgt Ion: 98 Resp: 402190
Ion Ratio Lower Upper
98 100
100 64.6 51.8 77.6

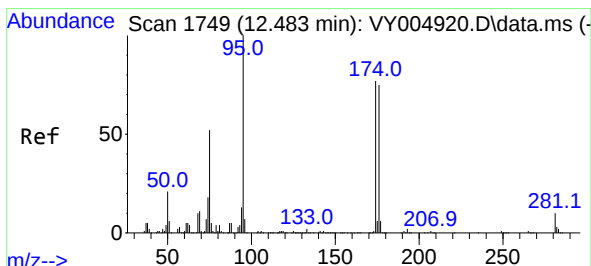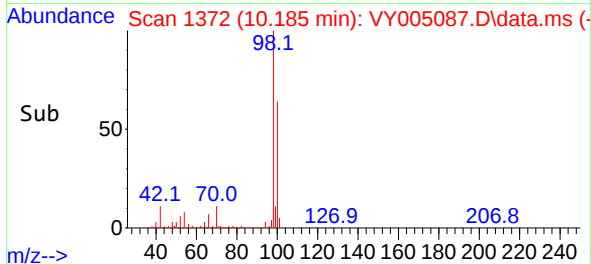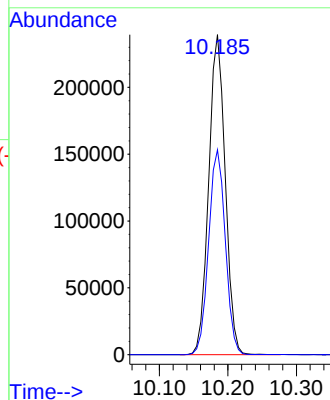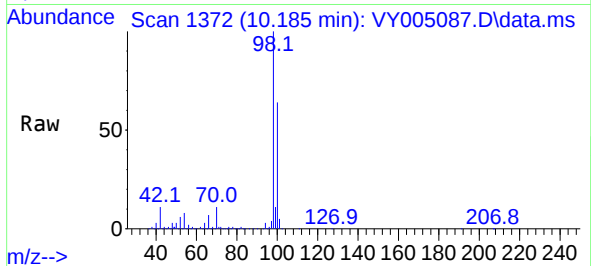

#62
4-Bromofluorobenzene
Concen: 55.840 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY005087.D
Acq: 10 Jun 2021 19:11

Tgt Ion: 95 Resp: 139557
Ion Ratio Lower Upper
95 100
174 83.4 0.0 160.8
176 81.5 0.0 155.6


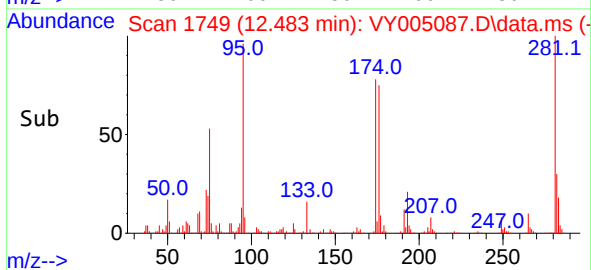
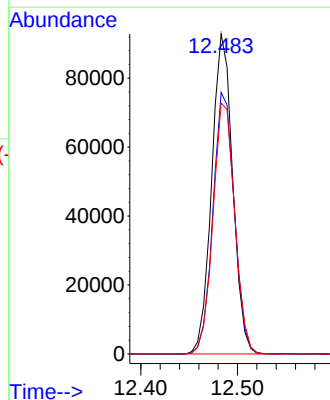
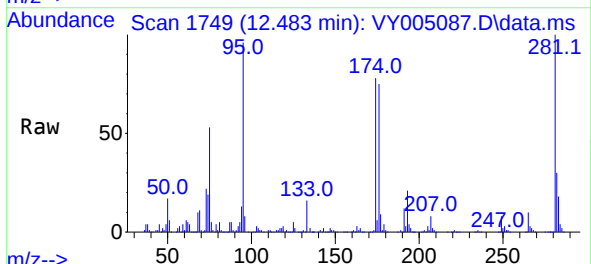


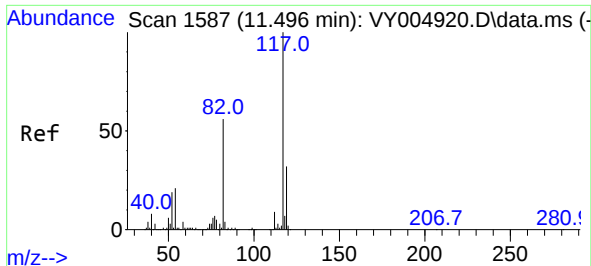

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.495 min Scan# 1587
Delta R.T. -0.000 min
Lab File: VY005087.D
Acq: 10 Jun 2021 19:11

Instrument :
MSVOA_Y
ClientSampleId :
17-B6(44-48)

Tgt Ion:117 Resp: 316009
Ion Ratio Lower Upper
117 100
82 52.6 44.8 67.2
119 32.2 25.2 37.8

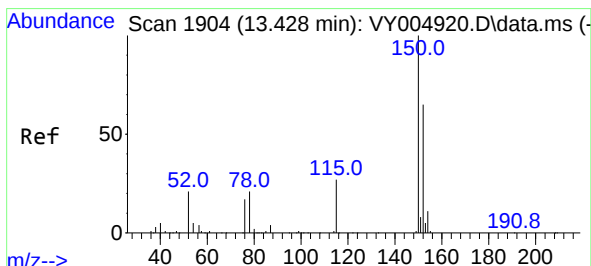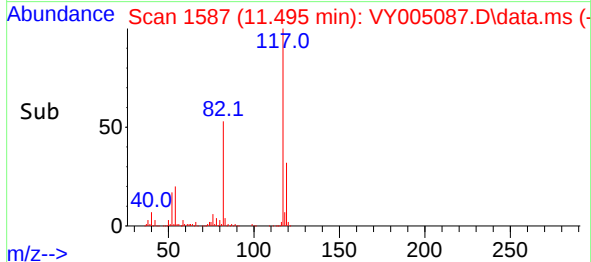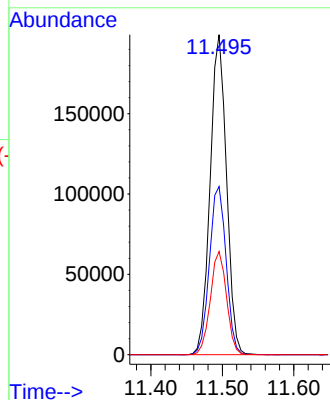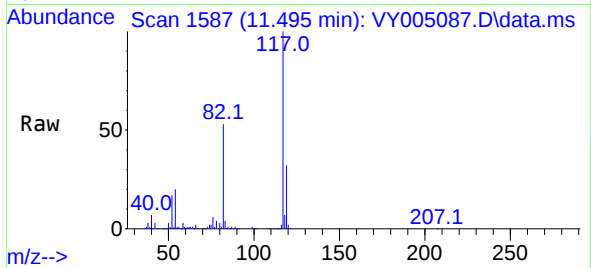

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY005087.D
Acq: 10 Jun 2021 19:11

Tgt Ion:152 Resp: 143215
Ion Ratio Lower Upper
152 100
115 59.5 29.9 89.7
150 160.7 0.0 347.8

