

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY061121\
 Data File : VY005119.D
 Acq On : 11 Jun 2021 13:11
 Operator : SY/MD
 Sample : M2672-08
 Misc : 9.96G/5ML/MSVOA_Y/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 17-B6(36-40)

Quant Time: Jun 12 00:35:48 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060221S.M
 Quant Title : SW846 8260
 QLast Update : Thu Jun 03 04:43:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.801	168	157584	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	282070	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.496	117	277473	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	132477	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	101504	60.929	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	121.860%
35) Dibromofluoromethane	7.728	113	87611	57.731	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	115.460%
50) Toluene-d8	10.185	98	349202	55.405	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	110.820%
62) 4-Bromofluorobenzene	12.483	95	119864	55.298	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	110.600%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY061121\
Data File : VY005119.D
Acq On : 11 Jun 2021 13:11
Operator : SY/MD
Sample : M2672-08
Misc : 9.96G/5ML/MSVOA_Y/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
17-B6(36-40)


Quant Time: Jun 12 00:35:48 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060221S.M
Quant Title : SW846 8260
QLast Update : Thu Jun 03 04:43:33 2021
Response via : Initial Calibration

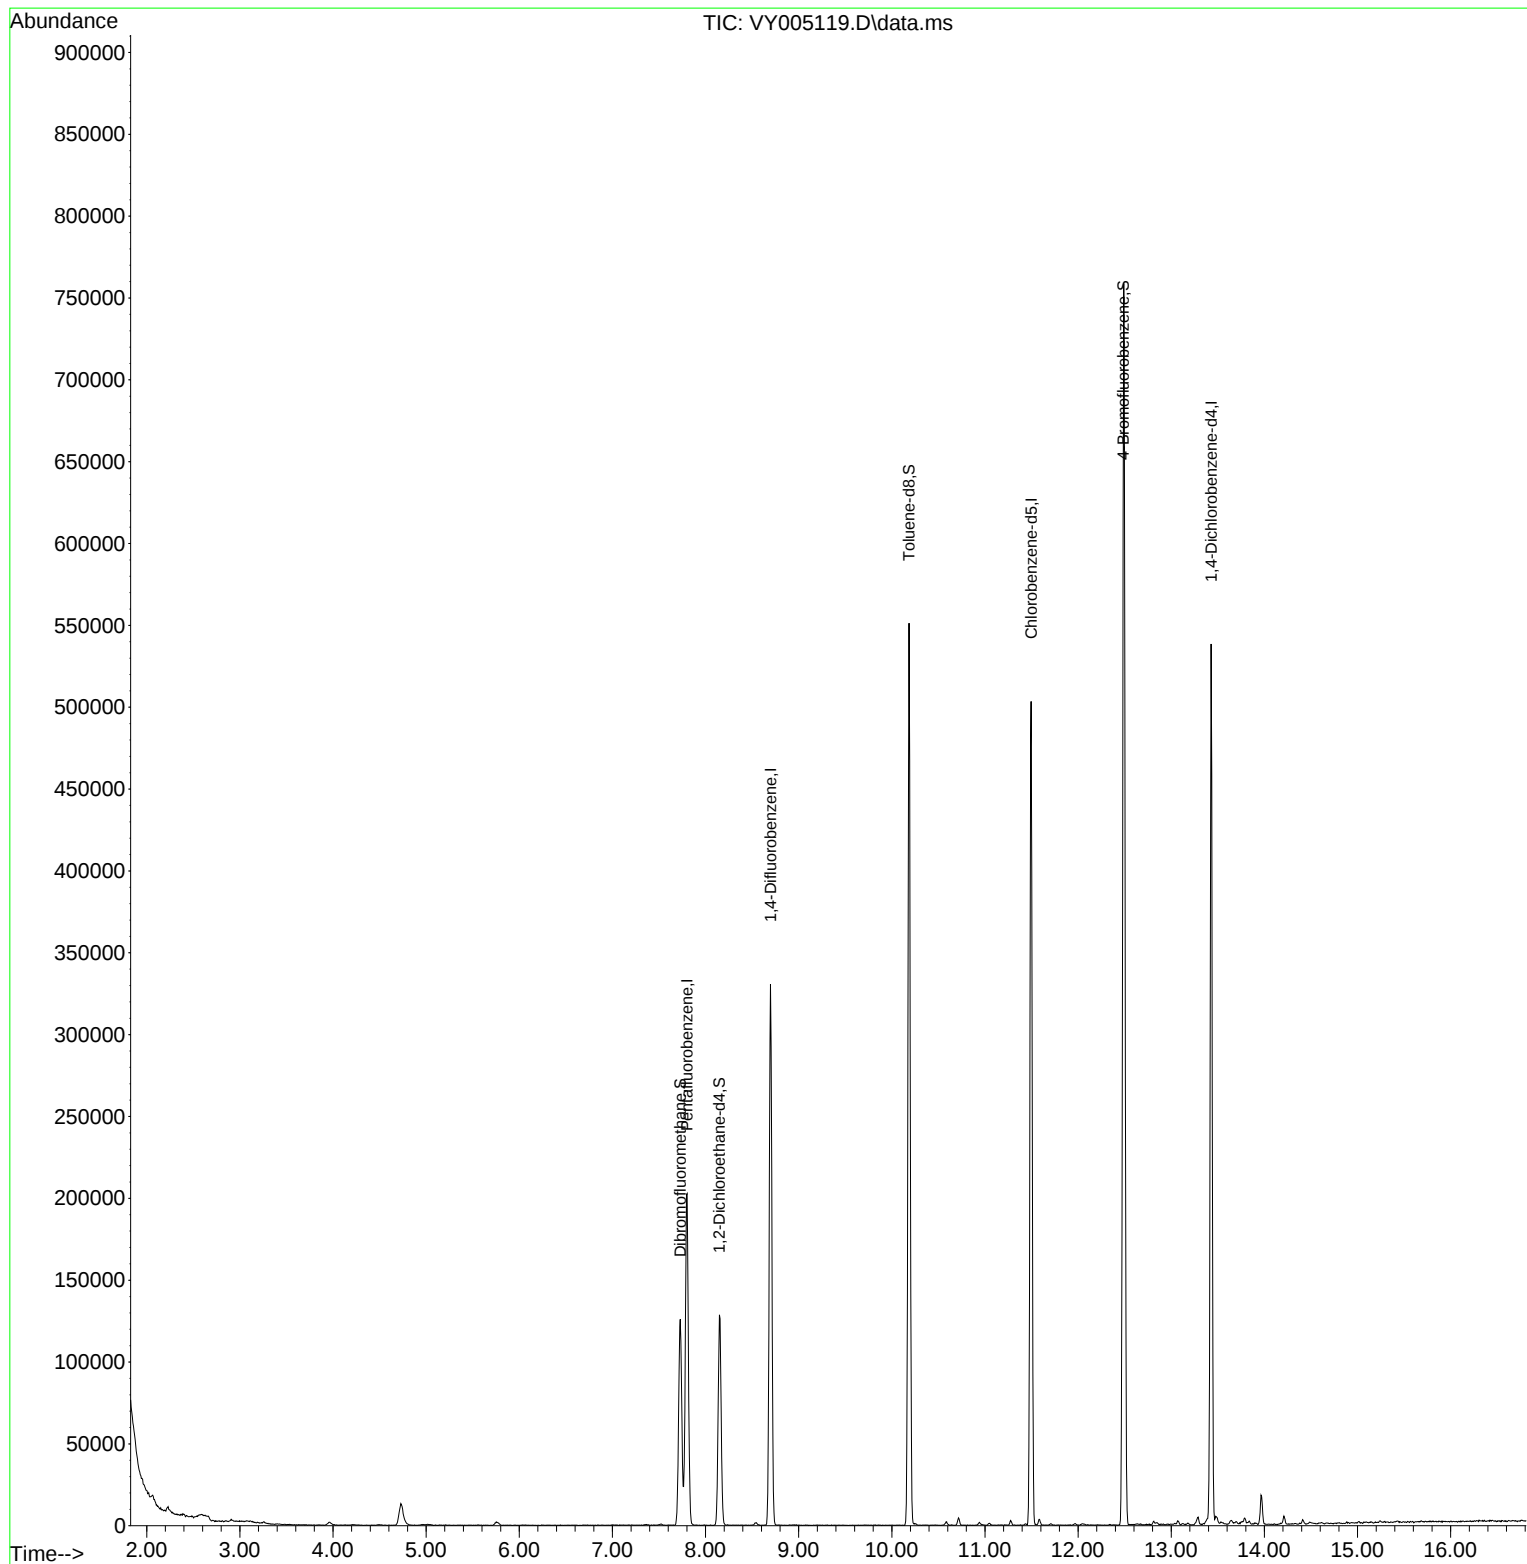



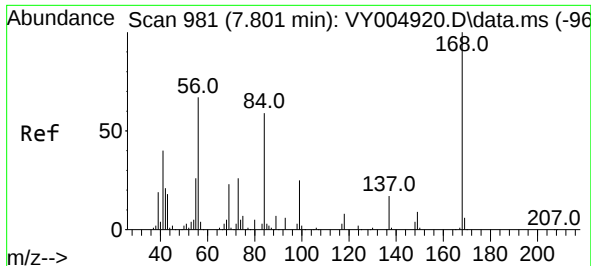


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.801 min Scan# 981
Delta R.T. 0.000 min
Lab File: VY005119.D
Acq: 11 Jun 2021 13:11

Instrument :
MSVOA_Y
ClientSampleId :
17-B6(36-40)



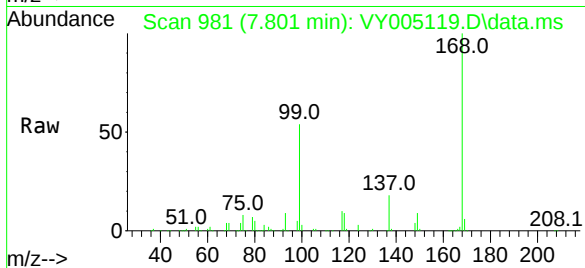



Tgt Ion:168 Resp: 157584
Ion Ratio Lower Upper
168 100
99 54.1 43.9 65.9

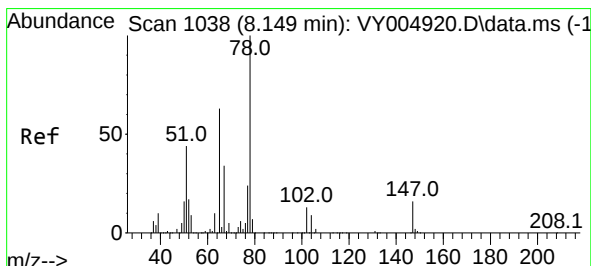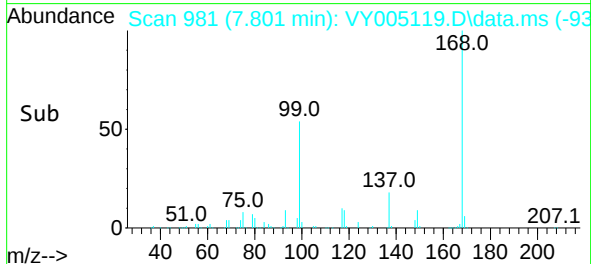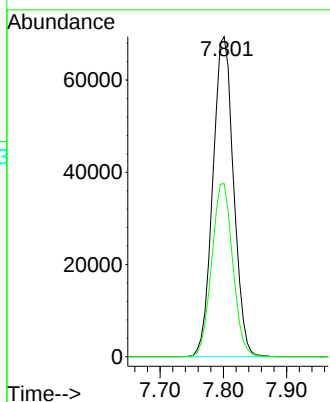

#33
1,2-Dichloroethane-d4
Concen: 60.929 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. -0.000 min
Lab File: VY005119.D
Acq: 11 Jun 2021 13:11


Tgt Ion: 65 Resp: 101504
Ion Ratio Lower Upper
65 100
67 53.3 0.0 110.6

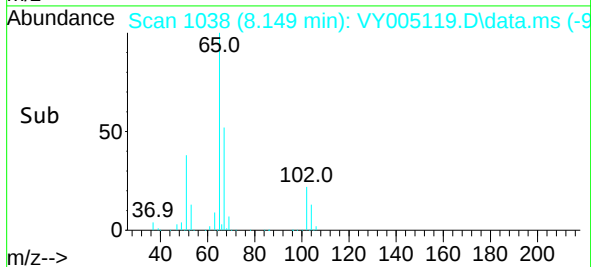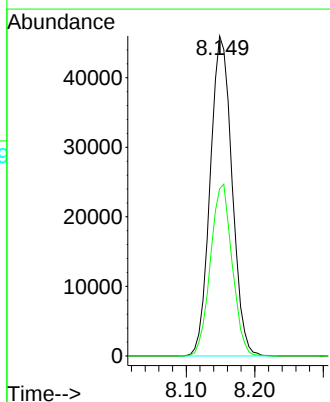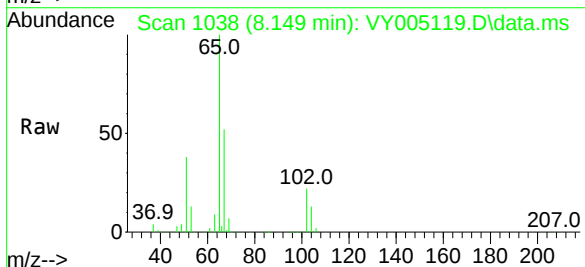



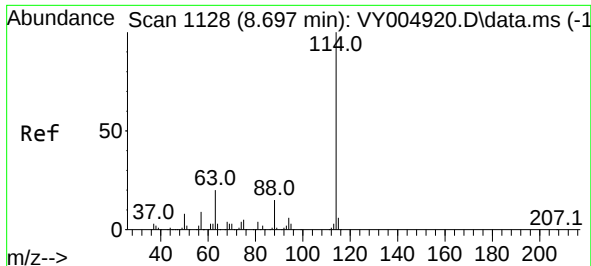


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. -0.000 min
Lab File: VY005119.D
Acq: 11 Jun 2021 13:11

Instrument :
MSVOA_Y
ClientSampleId :
17-B6(36-40)



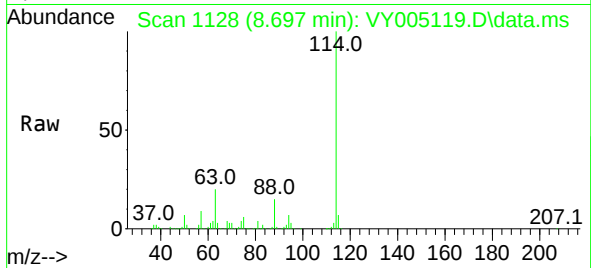



Tgt Ion:	114	Resp:	282070
Ion Ratio	Lower	Upper	
114	100		
63	19.6	0.0	41.0
88	15.3	0.0	30.6

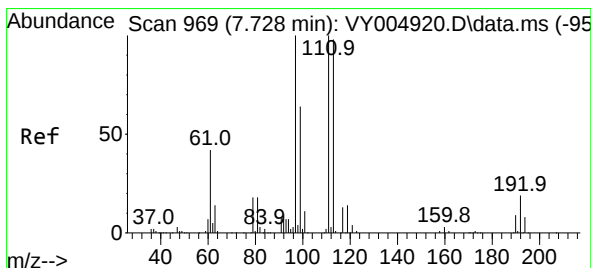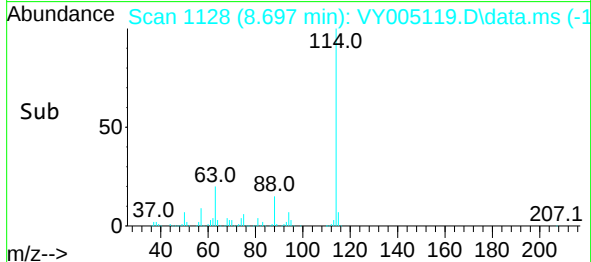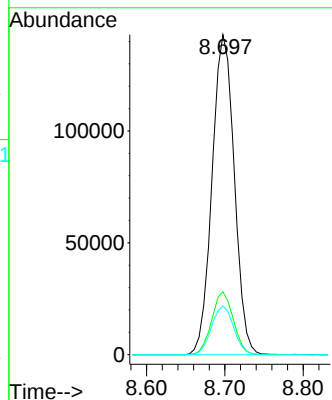

#35
Dibromofluoromethane
Concen: 57.731 ug/l
RT: 7.728 min Scan# 969
Delta R.T. -0.000 min
Lab File: VY005119.D
Acq: 11 Jun 2021 13:11

Tgt Ion:	113	Resp:	87611
Ion Ratio	Lower	Upper	
113	100		
111	104.4	81.8	122.8
192	19.6	15.3	22.9


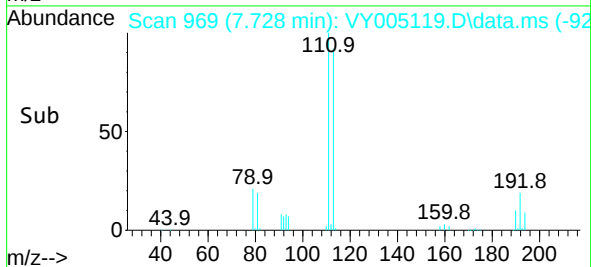
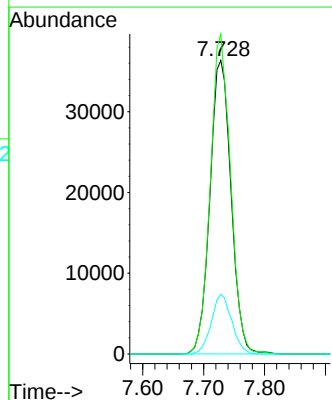
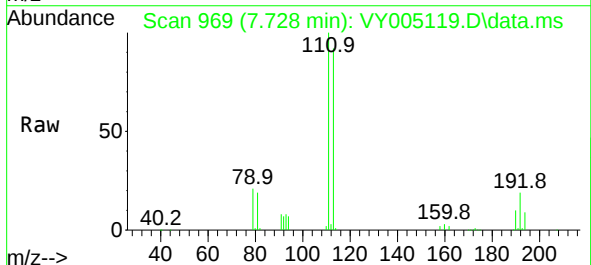


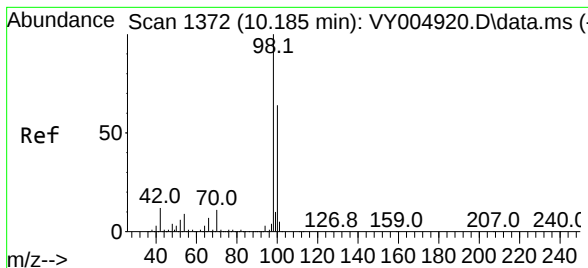

#50
Toluene-d8
Concen: 55.405 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. -0.000 min
Lab File: VY005119.D
Acq: 11 Jun 2021 13:11




Instrument :
MSVOA_Y
ClientSampleId :
17-B6(36-40)


Tgt Ion: 98 Resp: 349202
Ion Ratio Lower Upper
98 100
100 64.1 51.8 77.6

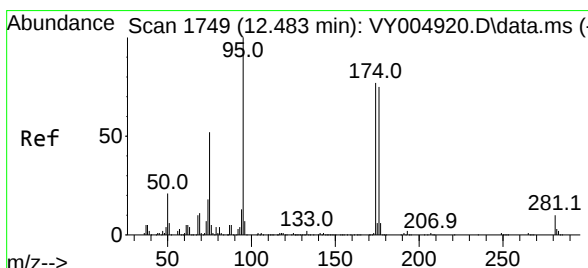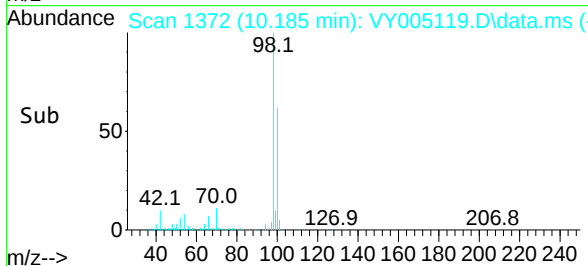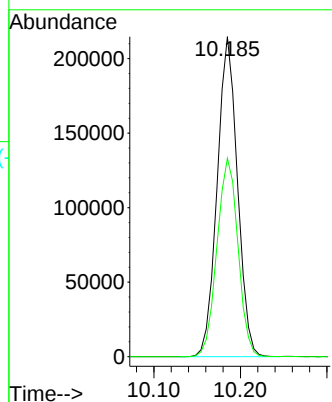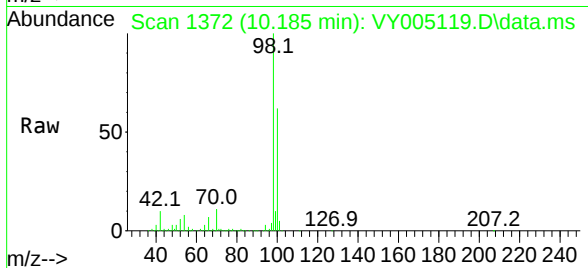

#62
4-Bromofluorobenzene
Concen: 55.298 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY005119.D
Acq: 11 Jun 2021 13:11

Tgt Ion: 95 Resp: 119864
Ion Ratio Lower Upper
95 100
174 86.5 0.0 160.8
176 84.8 0.0 155.6


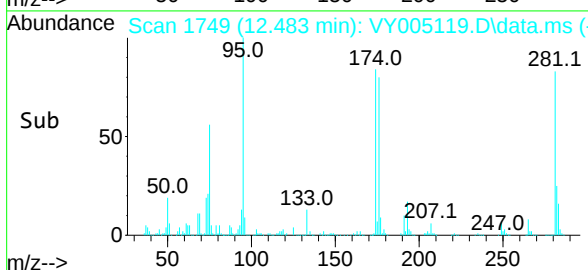
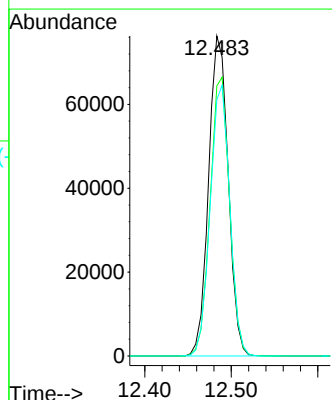
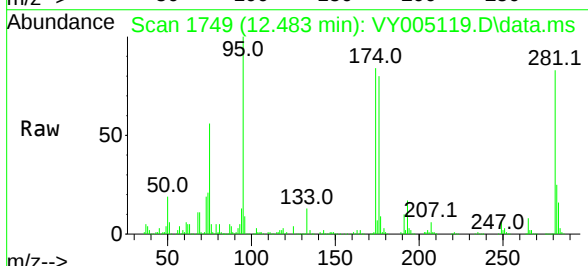


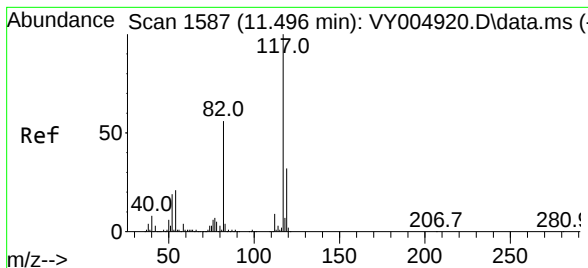

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.496 min Scan# 1587
Delta R.T. -0.000 min
Lab File: VY005119.D
Acq: 11 Jun 2021 13:11

Instrument :
MSVOA_Y
ClientSampleId :
17-B6(36-40)

Tgt Ion:117 Resp: 277473
Ion Ratio Lower Upper
117 100
82 52.7 44.8 67.2
119 31.5 25.2 37.8

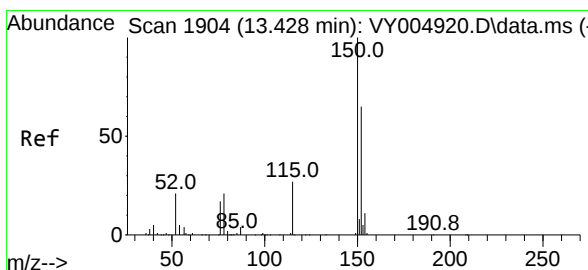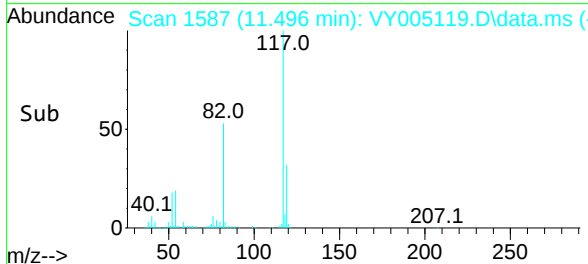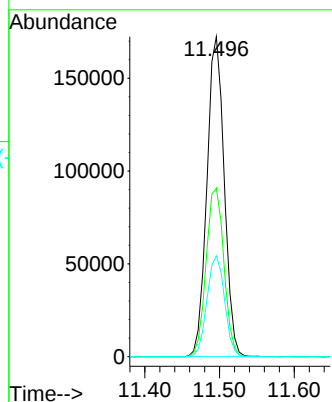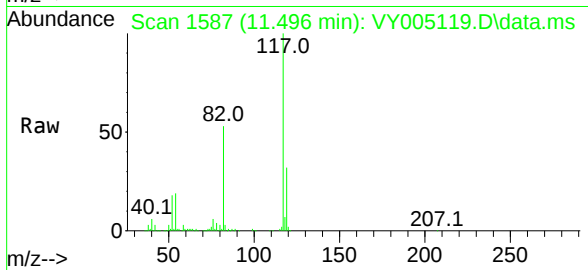

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY005119.D
Acq: 11 Jun 2021 13:11

Tgt Ion:152 Resp: 132477
Ion Ratio Lower Upper
152 100
115 57.9 29.9 89.7
150 157.4 0.0 347.8

