

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY061125\
 Data File : VY022659.D
 Acq On : 11 Jun 2025 13:11
 Operator : SY/MD
 Sample : Q2280-01
 Misc : 4.12g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VNJ-210

Quant Time: Jun 12 05:06:37 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060225S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 10 15:26:14 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.707	168	176797	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	317352	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	259001	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.347	152	94902	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	99807	50.474	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 100.940%	
35) Dibromofluoromethane	7.634	113	95147	50.230	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 100.460%	
50) Toluene-d8	10.103	98	384462	50.231	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	= 100.460%	
62) 4-Bromofluorobenzene	12.402	95	97298	42.666	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	= 85.340%	
Target Compounds						
16) Acetone	3.873	43	3361	8.370	ug/l	Qvalue # 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY061125\
Data File : VY022659.D
Acq On : 11 Jun 2025 13:11
Operator : SY/MD
Sample : Q2280-01
Misc : 4.12g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VNJ-210

Quant Time: Jun 12 05:06:37 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060225S.M
Quant Title : SW846 8260
QLast Update : Tue Jun 10 15:26:14 2025
Response via : Initial Calibration




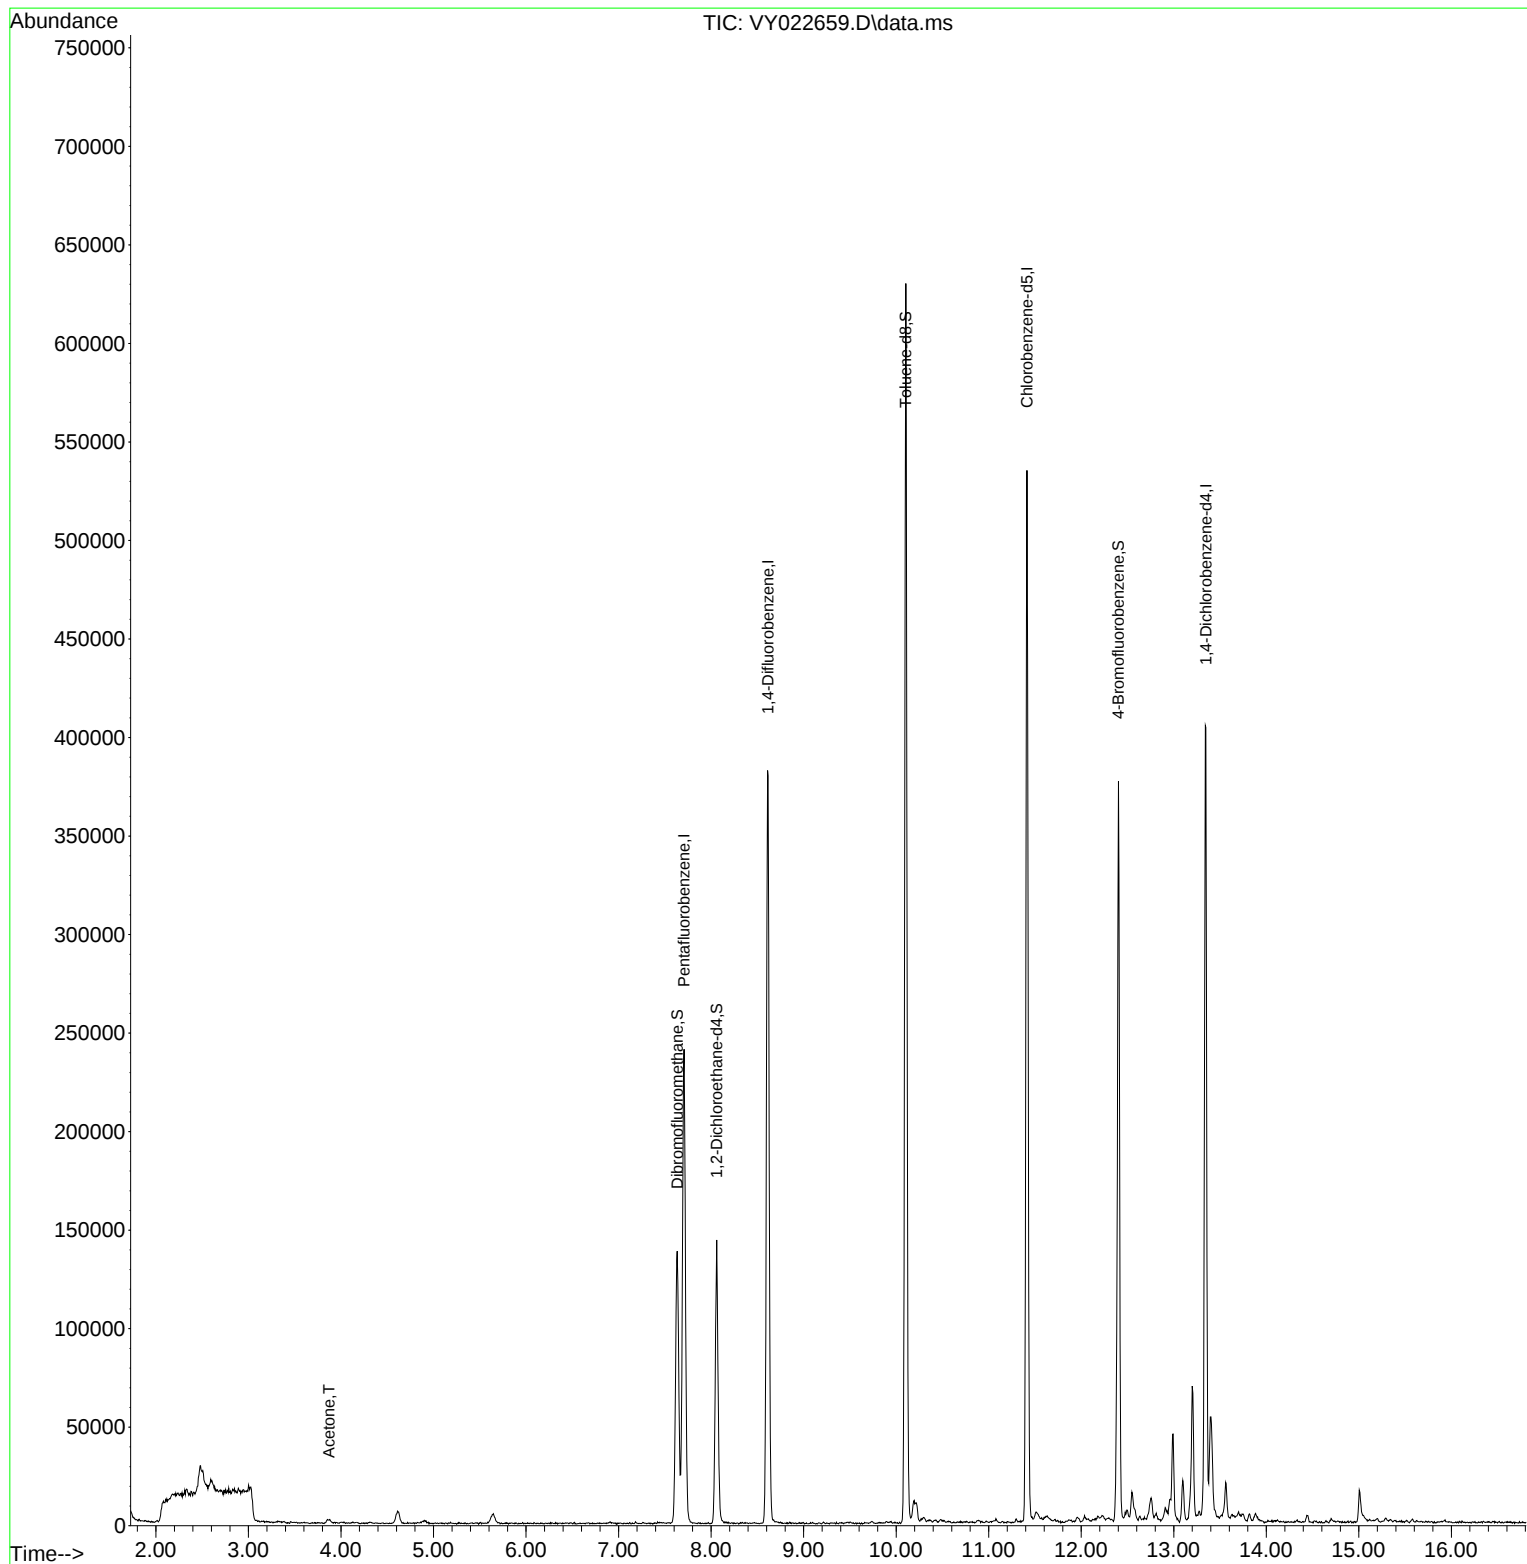


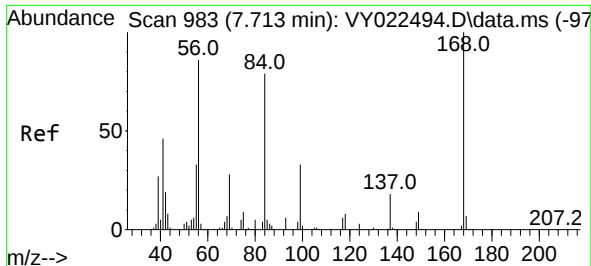

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY022659.D
Acq: 11 Jun 2025 13:11




Instrument :
MSVOA_Y
ClientSampleId :
VNJ-210


Tgt Ion:168 Resp: 176797
Ion Ratio Lower Upper
168 100
99 55.1 44.3 66.5

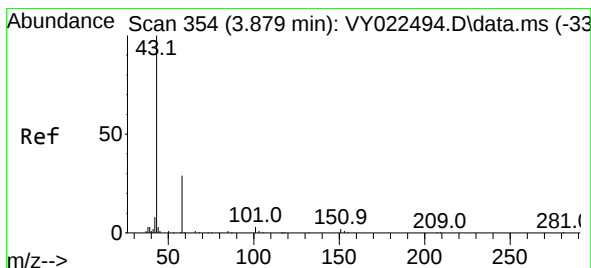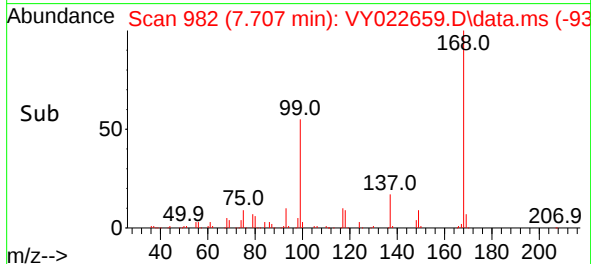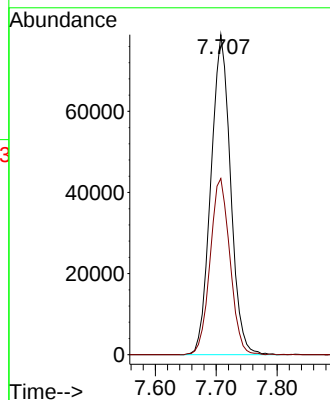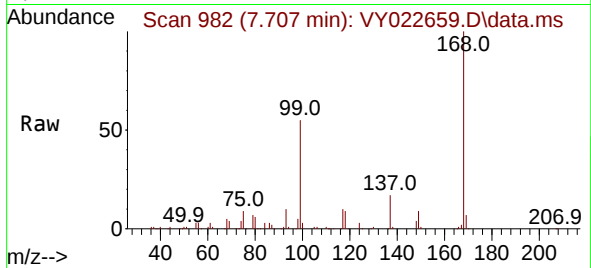

#16
Acetone
Concen: 8.370 ug/l
RT: 3.873 min Scan# 353
Delta R.T. -0.006 min
Lab File: VY022659.D
Acq: 11 Jun 2025 13:11

Tgt Ion: 43 Resp: 3361
Ion Ratio Lower Upper
43 100
58 21.1 24.0 36.0#

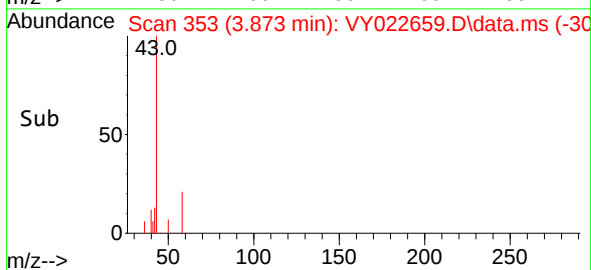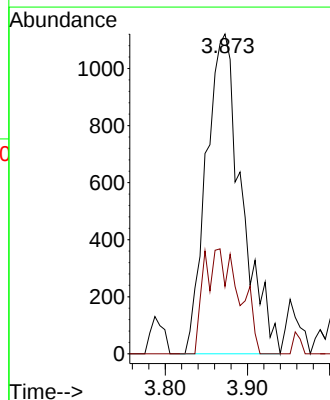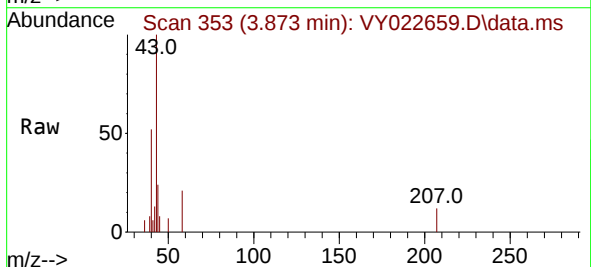

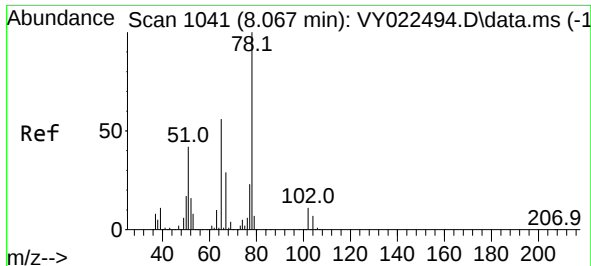

#33

1,2-Dichloroethane-d4

Concen: 50.474 ug/l

RT: 8.061 min Scan# 1

Delta R.T. -0.006 min

Lab File: VY022659.D

Acq: 11 Jun 2025 13:11

Instrument :

MSVOA_Y

ClientSampleId :





VNJ-210

Tgt Ion: 65 Resp: 99807

Ion Ratio Lower Upper

65 100

67 51.5 0.0 103.4

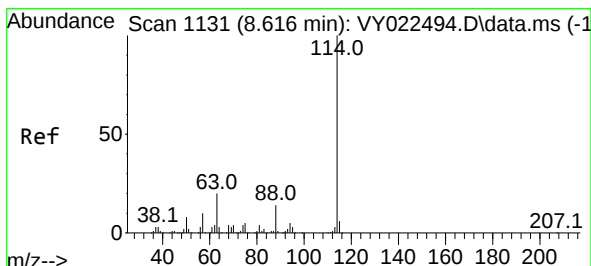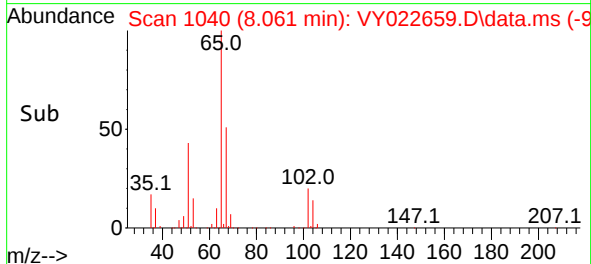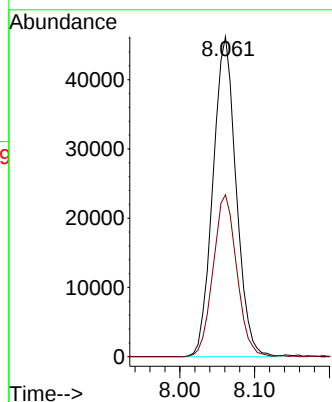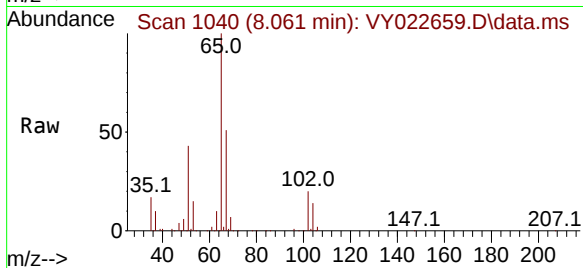

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.616 min Scan# 1131

Delta R.T. 0.000 min

Lab File: VY022659.D

Acq: 11 Jun 2025 13:11




Tgt Ion: 114 Resp: 317352

Ion Ratio Lower Upper

114 100

63 20.6 0.0 40.8

88 14.7 0.0 27.8

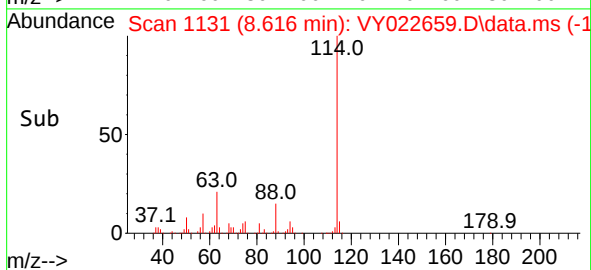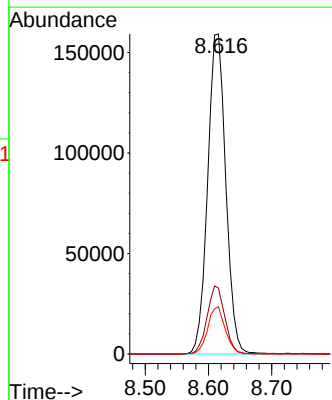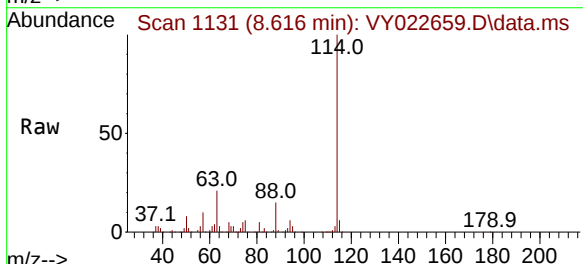



#35

Dibromofluoromethane

Concen: 50.230 ug/l

RT: 7.634 min Scan# 91

Delta R.T. -0.006 min

Lab File: VY022659.D

Acq: 11 Jun 2025 13:11

Instrument :

MSVOA_Y

ClientSampleId :

VNJ-210





Tgt Ion:113 Resp: 95147

Ion Ratio Lower Upper

113 100

111 102.4 81.1 121.7

192 17.6 14.2 21.2

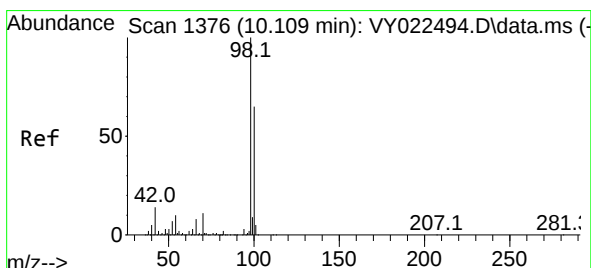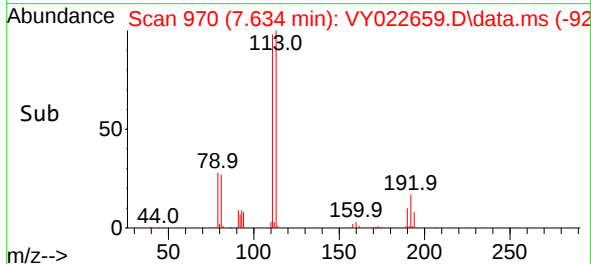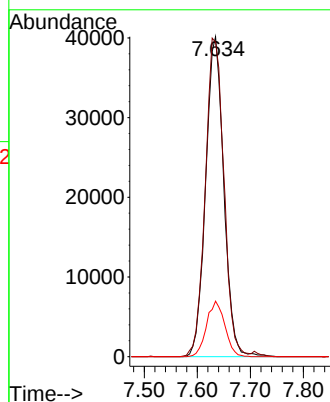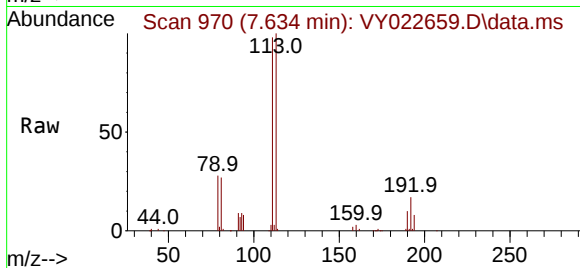

#50

Toluene-d8

Concen: 50.231 ug/l

RT: 10.103 min Scan# 1375

Delta R.T. -0.006 min

Lab File: VY022659.D




Acq: 11 Jun 2025 13:11


Tgt Ion: 98 Resp: 384462

Ion Ratio Lower Upper

98 100

100 64.0 51.4 77.0

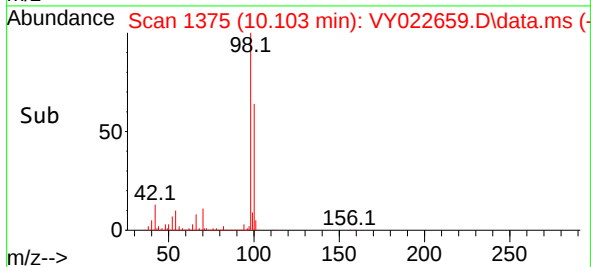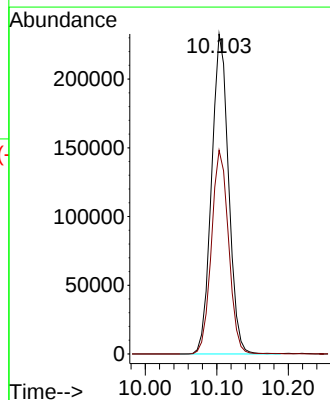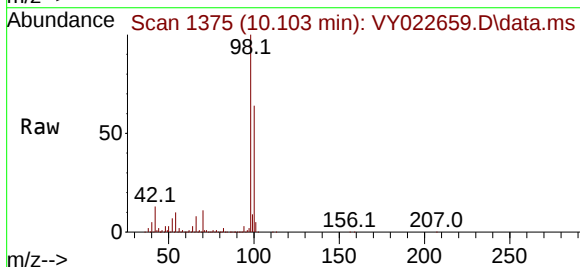

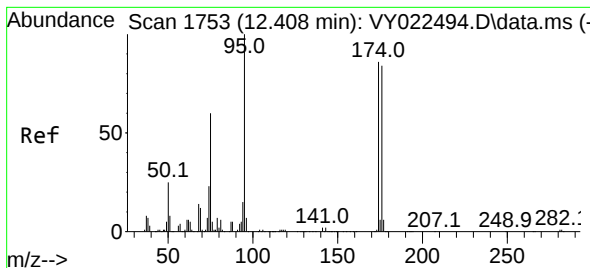

#62

4-Bromofluorobenzene

Concen: 42.666 ug/l

RT: 12.402 min Scan# 1752

Delta R.T. -0.006 min

Lab File: VY022659.D

Acq: 11 Jun 2025 13:11

Instrument :

MSVOA_Y

ClientSampleId :

VNJ-210





Tgt Ion: 95 Resp: 97298

Ion Ratio Lower Upper

95 100

174 84.7 0.0 170.0

176 81.9 0.0 166.2

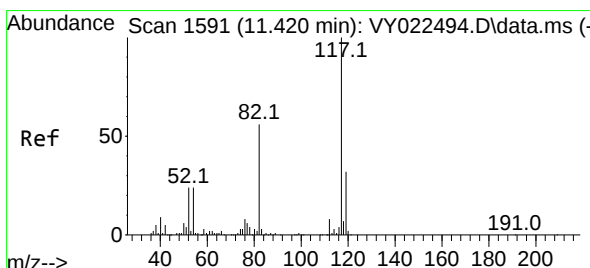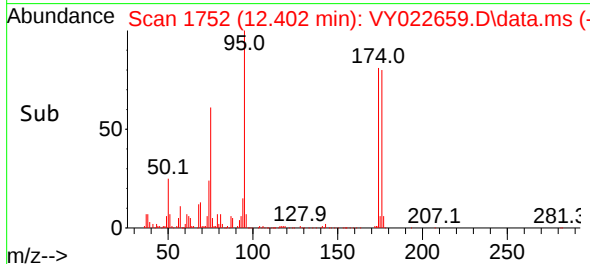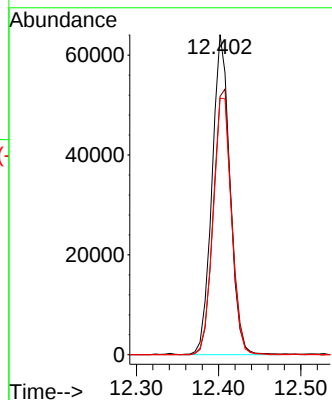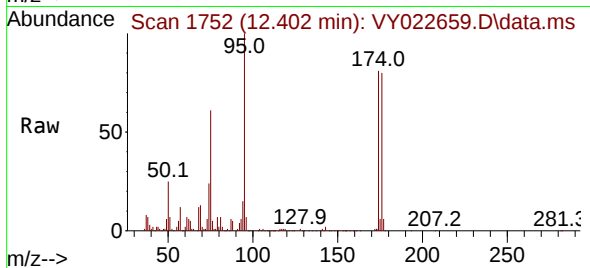

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 1590

Delta R.T. -0.006 min

Lab File: VY022659.D

Acq: 11 Jun 2025 13:11




Tgt Ion: 117 Resp: 259001


Ion Ratio Lower Upper

117 100

82 55.3 44.6 66.8

119 33.1 25.4 38.0

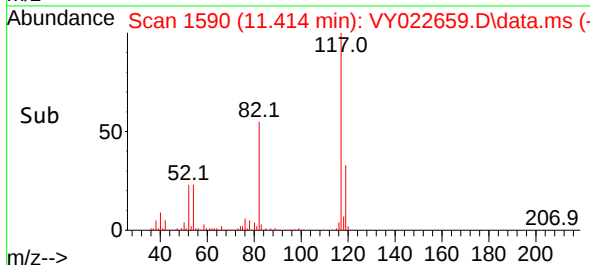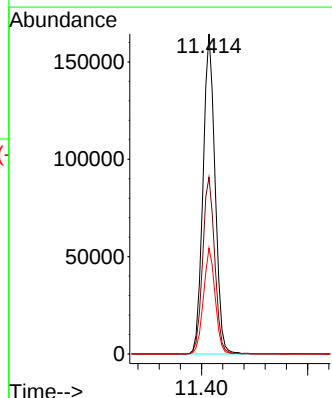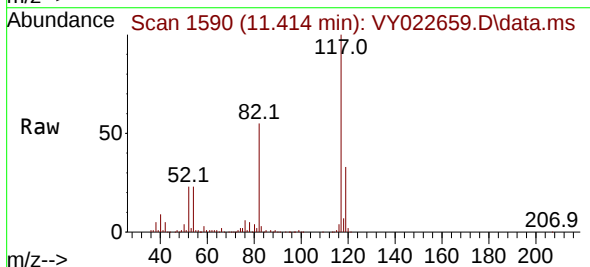

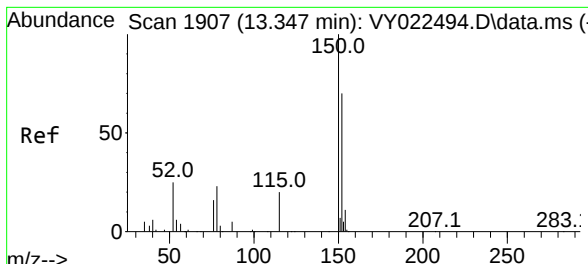

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.347 min Scan# 1907
 Delta R.T. 0.000 min
 Lab File: VY022659.D
 Acq: 11 Jun 2025 13:11

Instrument :
 MSVOA_Y
 ClientSampleId :
 VNJ-210

Tgt Ion:152	Resp:	94902
Ion Ratio	Lower	Upper
152	100	
115	58.8	28.9 86.7
150	156.7	0.0 349.6

