
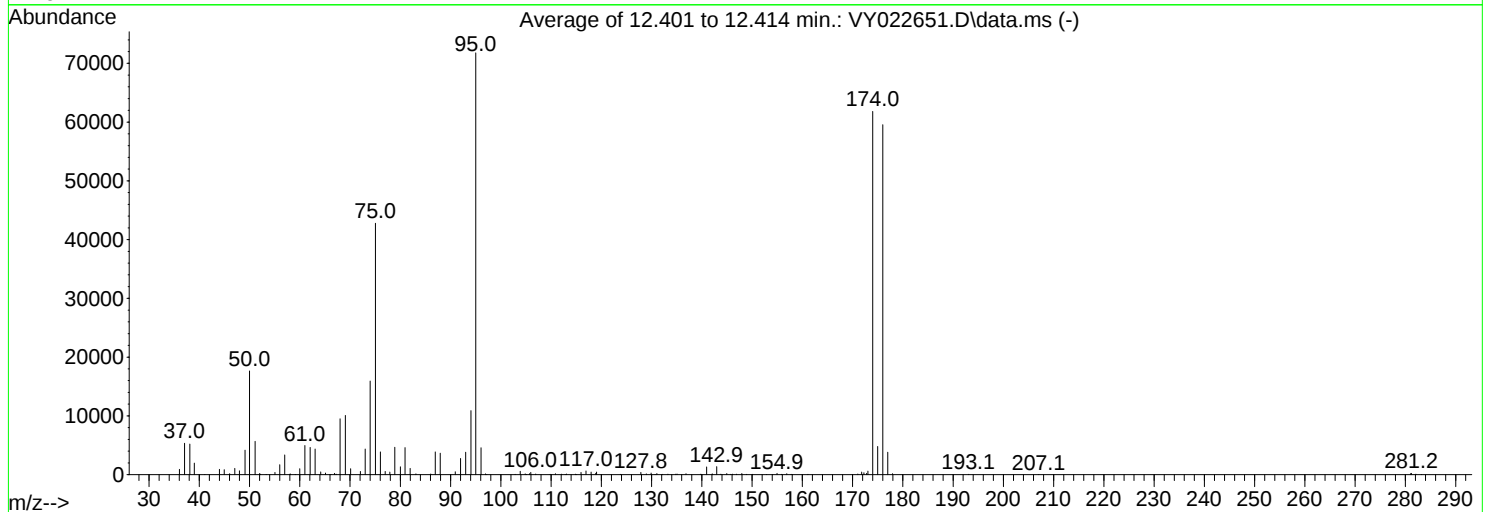


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY061125\
Data File : VY022651.D
Acq On : 11 Jun 2025 09:22
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060225S.M
Title : SW846 8260
Last Update : Tue Jun 10 15:26:14 2025

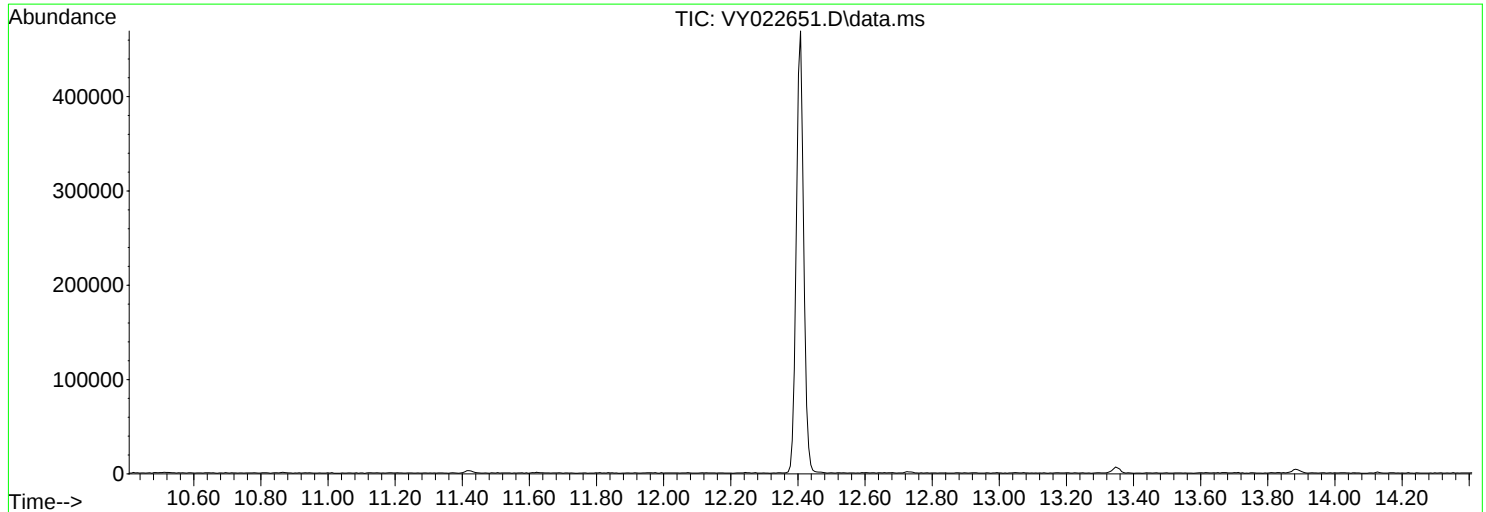

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1743

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.6	17654	PASS
75	95	30	60	59.6	42768	PASS
95	95	100	100	100.0	71789	PASS
96	95	5	9	6.4	4589	PASS
173	174	0.00	2	1.0	605	PASS
174	95	50	100	86.1	61819	PASS
175	174	5	9	7.8	4802	PASS
176	174	95	101	96.3	59552	PASS
177	176	5	9	6.4	3824	PASS