

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY061423\
 Data File : VY014158.D
 Acq On : 14 Jun 2023 17:03
 Operator : KP/MD
 Sample : 03224-18
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 TRIP-BLANK

Quant Time: Jun 15 01:43:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060923S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 09 18:07:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	148620	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	255025	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	266924	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	130608	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	107905	52.139	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	104.280%
35) Dibromofluoromethane	7.716	113	87037	48.124	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	96.240%
50) Toluene-d8	10.179	98	317437	46.947	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	93.900%
62) 4-Bromofluorobenzene	12.483	95	111613	46.469	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	92.940%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY061423\
Data File : VY014158.D
Acq On : 14 Jun 2023 17:03
Operator : KP/MD
Sample : 03224-18
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
TRIP-BLANK

Quant Time: Jun 15 01:43:39 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060923S.M
Quant Title : SW846 8260
QLast Update : Fri Jun 09 18:07:13 2023
Response via : Initial Calibration



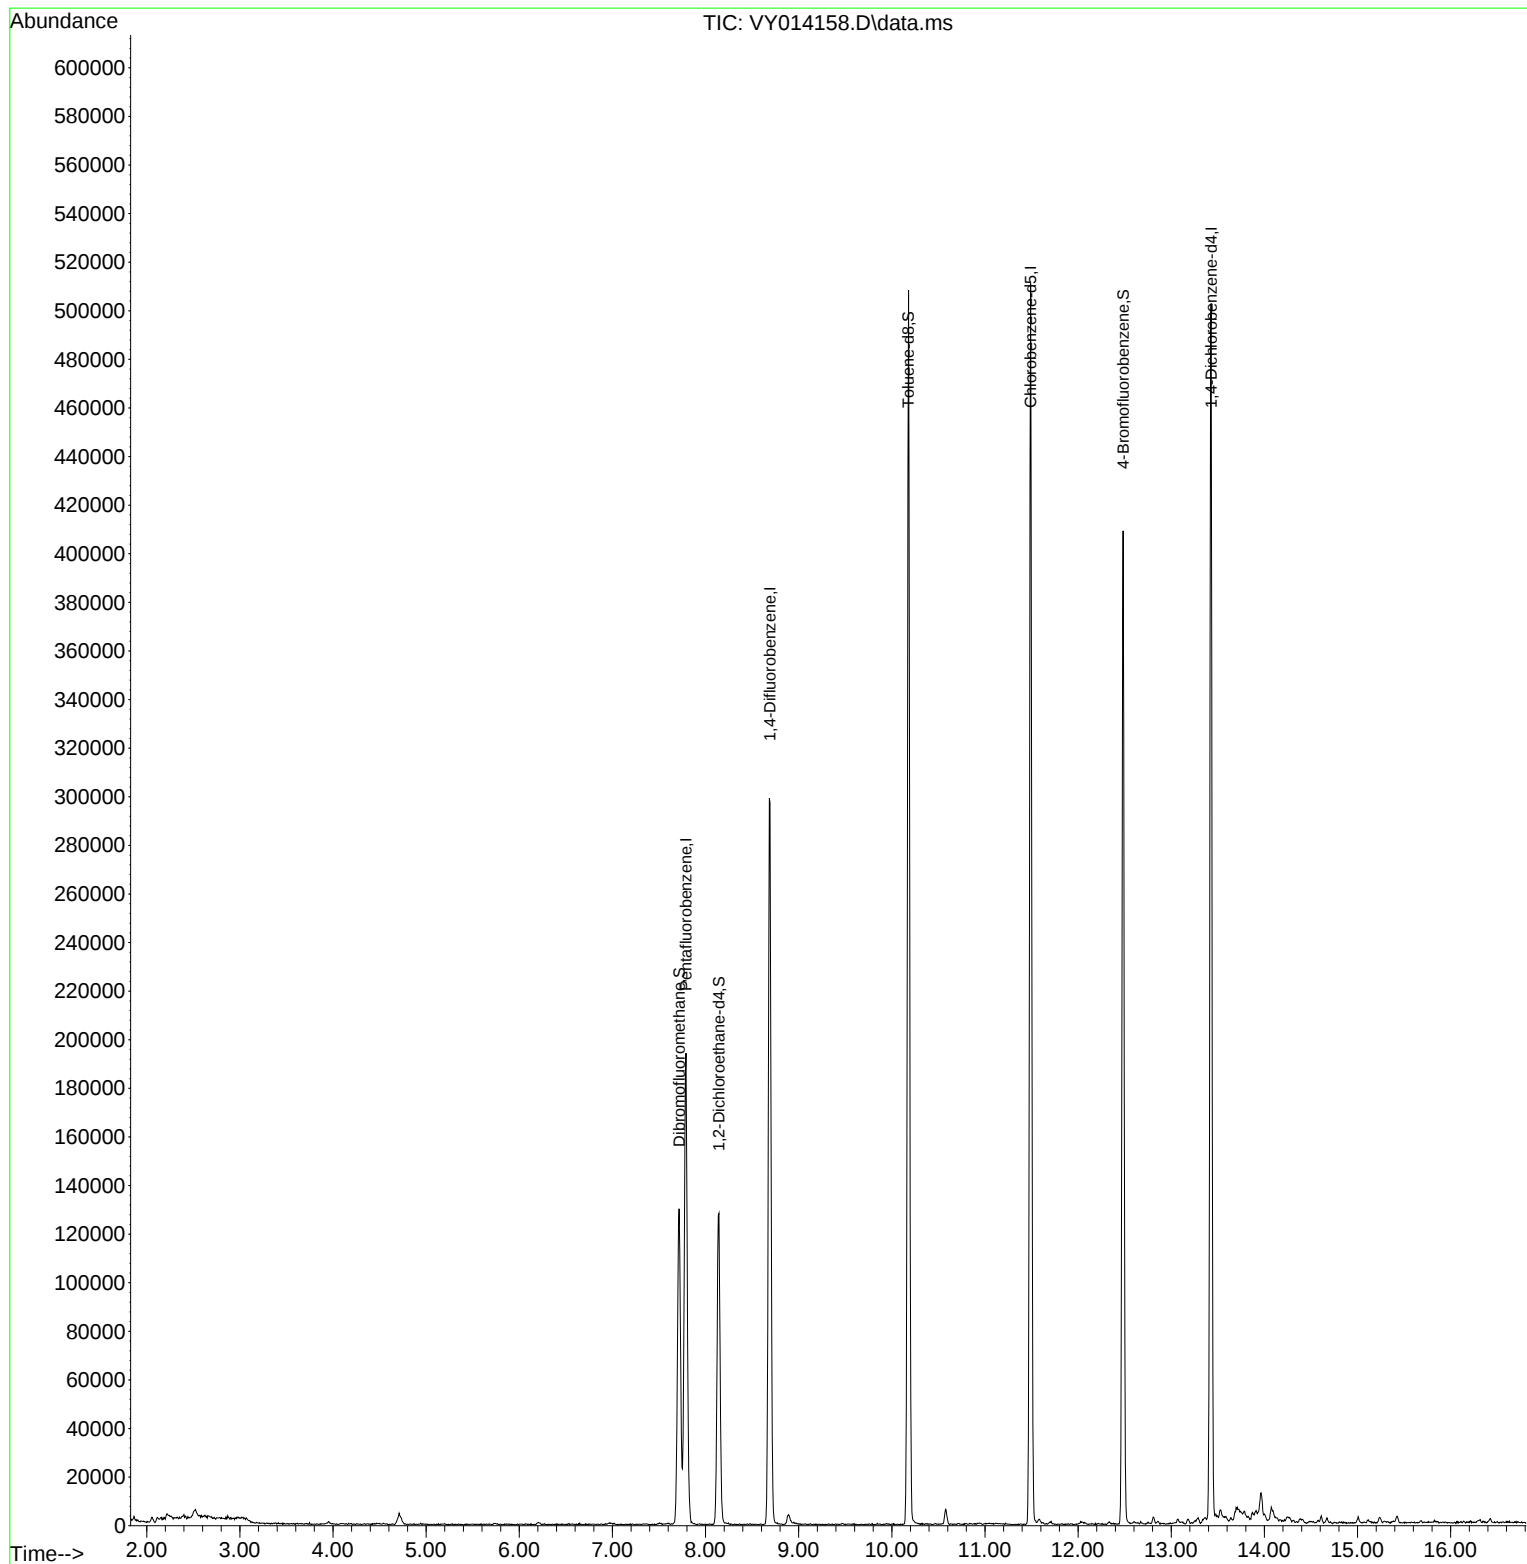




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY014158.D
Acq: 14 Jun 2023 17:03




Instrument :
MSVOA_Y
ClientSampleId :
TRIP-BLANK

Tgt Ion:168 Resp: 148620
Ion Ratio Lower Upper
168 100
99 52.7 43.4 65.0

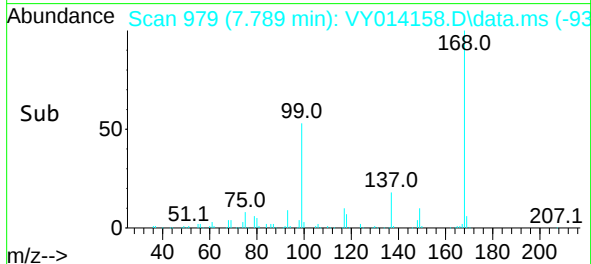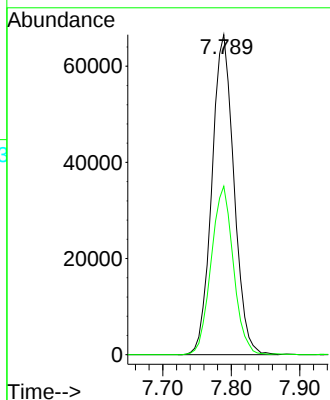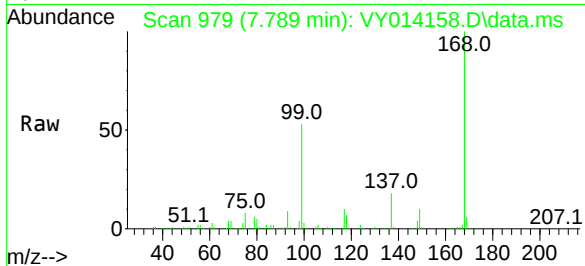

#33
1,2-Dichloroethane-d4
Concen: 52.139 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. 0.001 min
Lab File: VY014158.D
Acq: 14 Jun 2023 17:03

Tgt Ion: 65 Resp: 107905
Ion Ratio Lower Upper
65 100
67 50.5 0.0 101.8


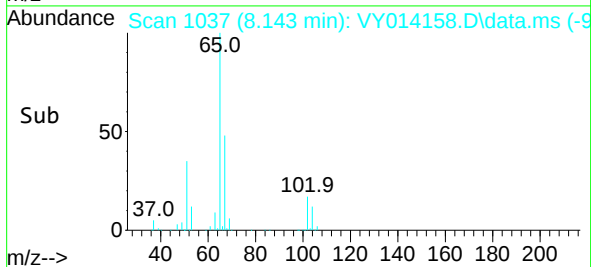
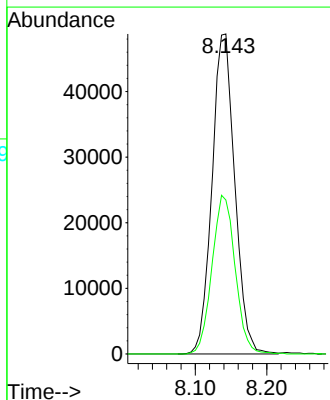
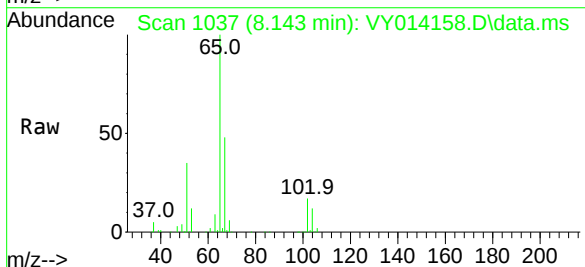




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.691 min Scan# 1127
Delta R.T. 0.000 min
Lab File: VY014158.D
Acq: 14 Jun 2023 17:03




Instrument :
MSVOA_Y
ClientSampleId :
TRIP-BLANK


Tgt Ion:114 Resp: 255025
Ion Ratio Lower Upper
114 100
63 19.8 0.0 42.4
88 14.5 0.0 30.6

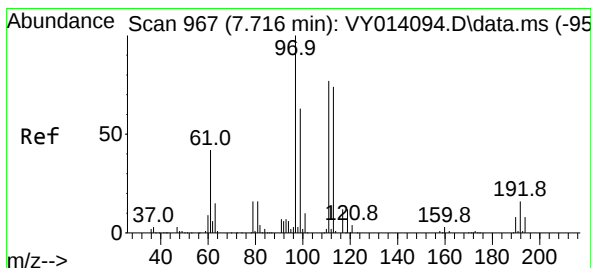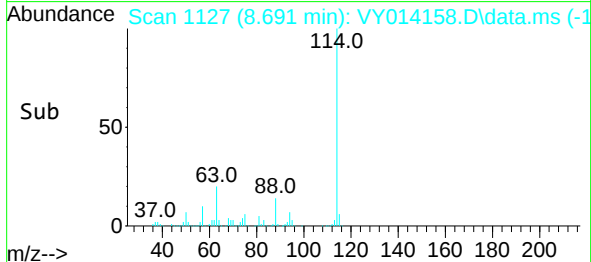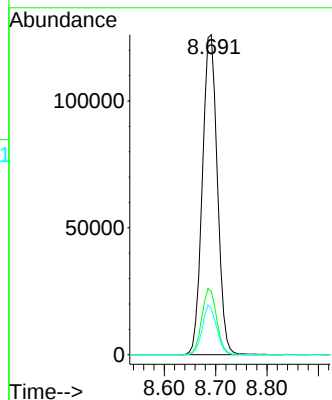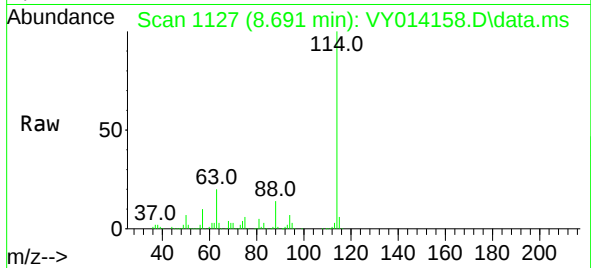

#35
Dibromofluoromethane
Concen: 48.124 ug/l
RT: 7.716 min Scan# 967
Delta R.T. -0.000 min
Lab File: VY014158.D
Acq: 14 Jun 2023 17:03

Tgt Ion:113 Resp: 87037
Ion Ratio Lower Upper
113 100
111 101.0 81.3 121.9
192 22.0 16.9 25.3

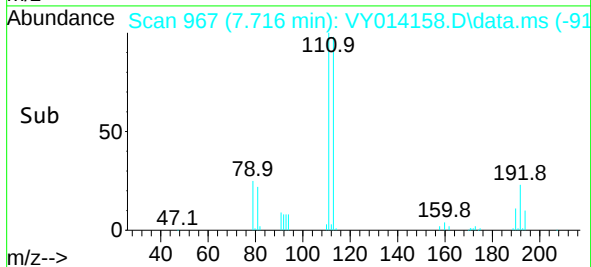
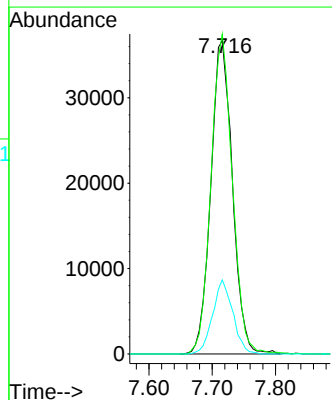
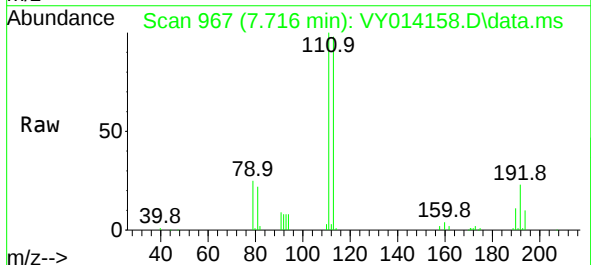


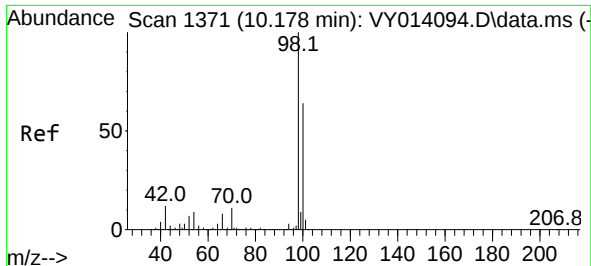

#50
Toluene-d8
Concen: 46.947 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. 0.001 min
Lab File: VY014158.D
Acq: 14 Jun 2023 17:03




Instrument :
MSVOA_Y
ClientSampleId :
TRIP-BLANK


Tgt Ion: 98 Resp: 317437
Ion Ratio Lower Upper
98 100
100 62.1 50.1 75.1

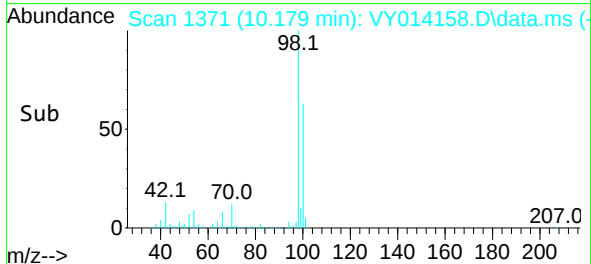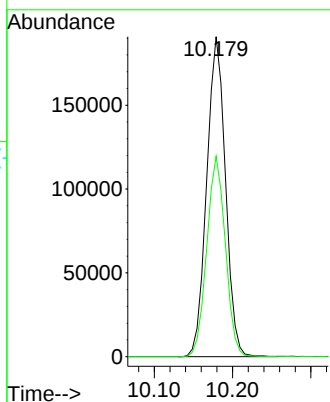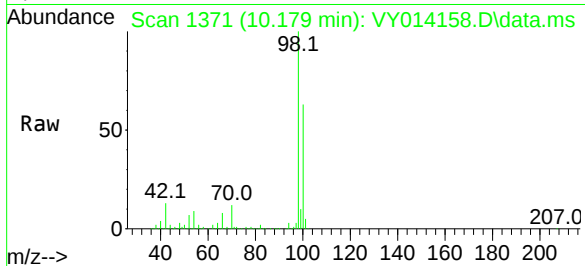

#62
4-Bromofluorobenzene
Concen: 46.469 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY014158.D
Acq: 14 Jun 2023 17:03

Tgt Ion: 95 Resp: 111613
Ion Ratio Lower Upper
95 100
174 95.6 0.0 178.2
176 91.7 0.0 173.8

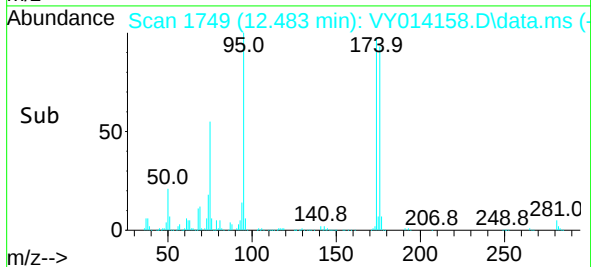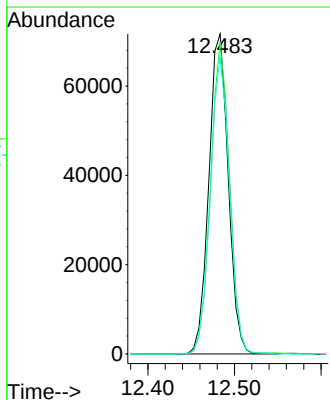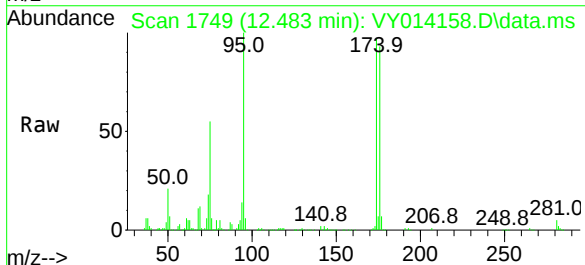

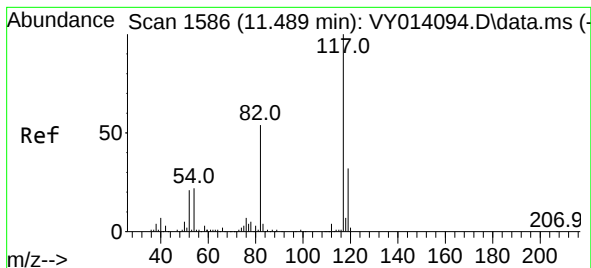

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.490 min Scan# 11

Delta R.T. 0.001 min

Lab File: VY014158.D

Acq: 14 Jun 2023 17:03

Instrument :

MSVOA_Y

ClientSampleId :

TRIP-BLANK





Tgt Ion:117 Resp: 266924

Ion Ratio Lower Upper

117 100

82 52.7 43.4 65.0

119 30.8 26.3 39.5

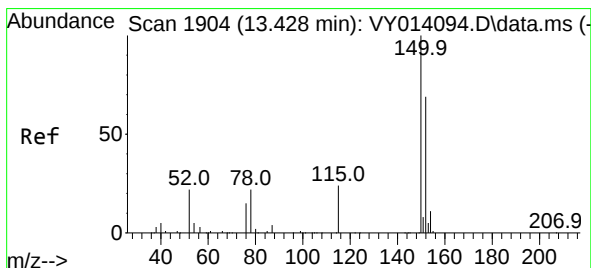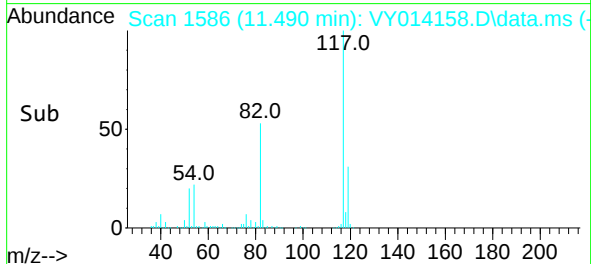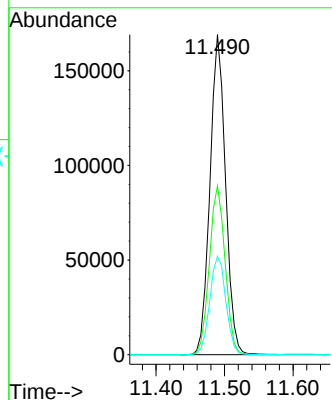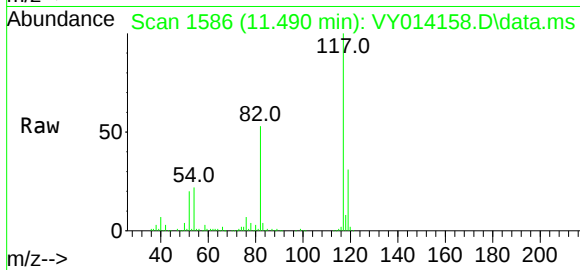

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.428 min Scan# 1904

Delta R.T. 0.000 min

Lab File: VY014158.D

Acq: 14 Jun 2023 17:03

Tgt Ion:152 Resp: 130608

Ion Ratio Lower Upper

152 100

115 56.9 28.8 86.5

150 156.5 0.0 348.8

