
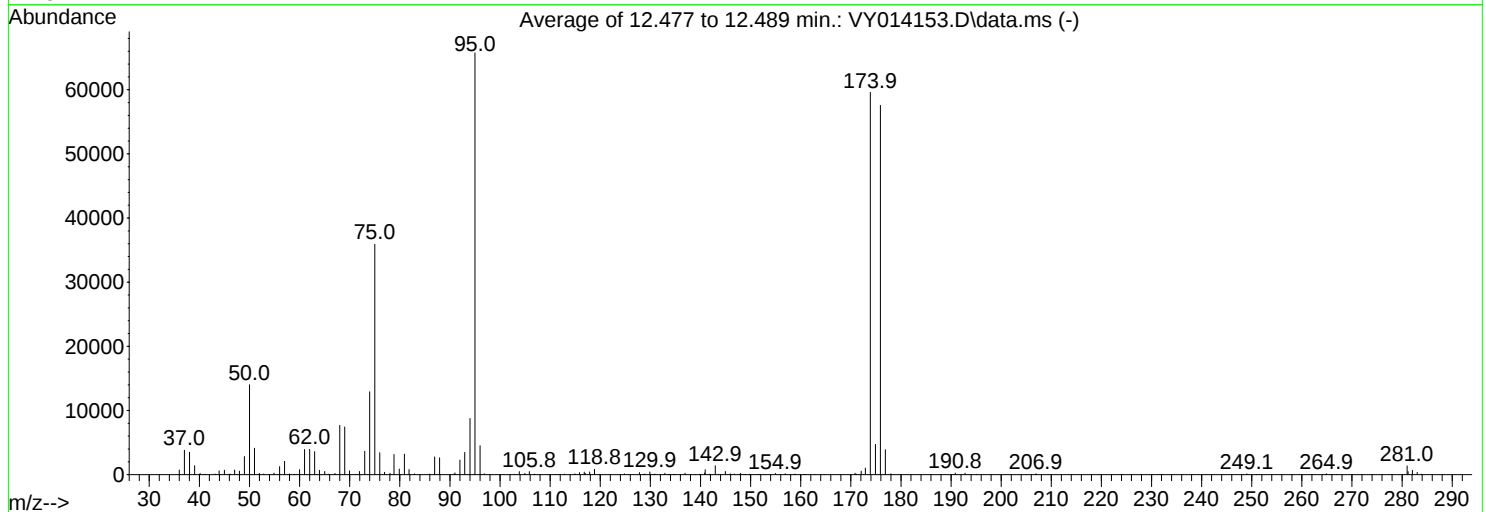


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY061423\
Data File : VY014153.D
Acq On : 14 Jun 2023 13:59
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060923S.M
Title : SW846 8260
Last Update : Fri Jun 09 18:07:13 2023

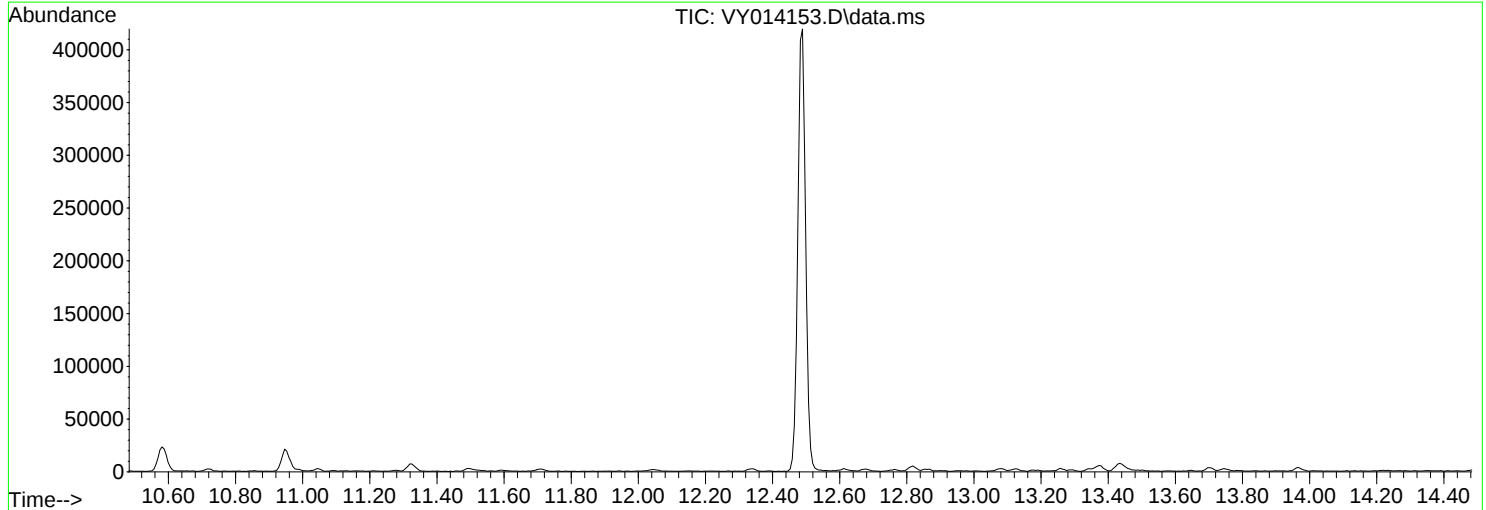

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	14008	PASS
75	95	30	60	54.6	35912	PASS
95	95	100	100	100.0	65752	PASS
96	95	5	9	6.9	4511	PASS
173	174	0.00	2	1.7	1018	PASS
174	95	50	100	90.6	59584	PASS
175	174	5	9	7.9	4705	PASS
176	174	95	101	96.6	57557	PASS
177	176	5	9	6.8	3893	PASS