
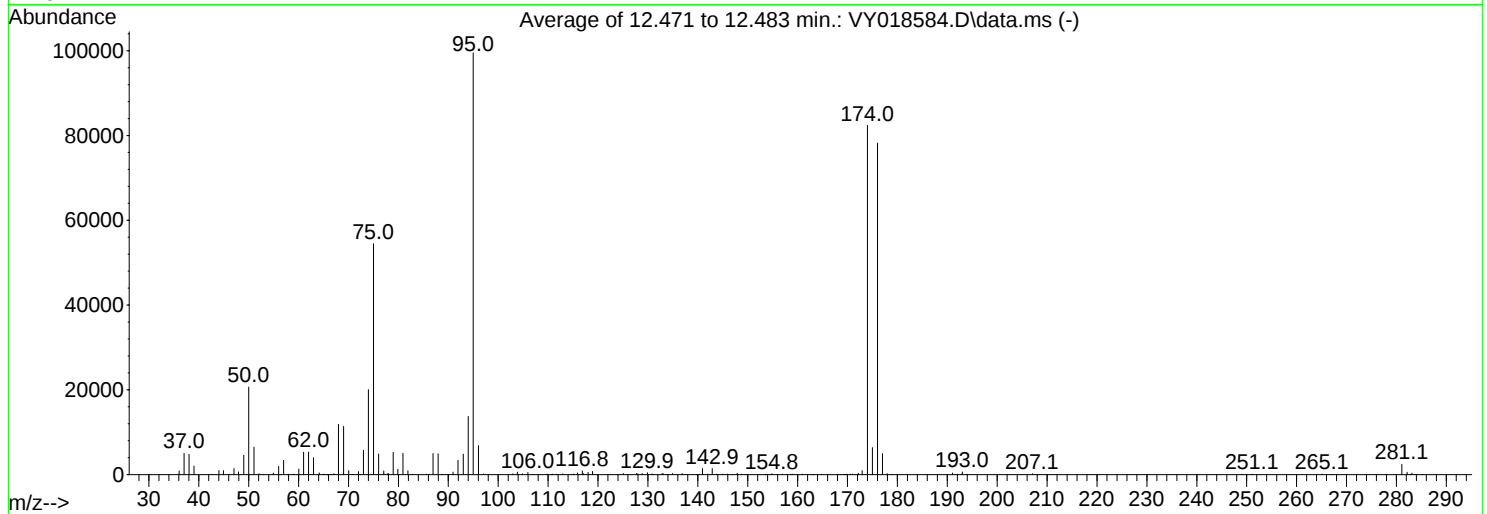


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY061424\
Data File : VY018584.D
Acq On : 14 Jun 2024 08:42
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y061324S.M
Title : SW846 8260
Last Update : Fri Jun 14 07:08:24 2024

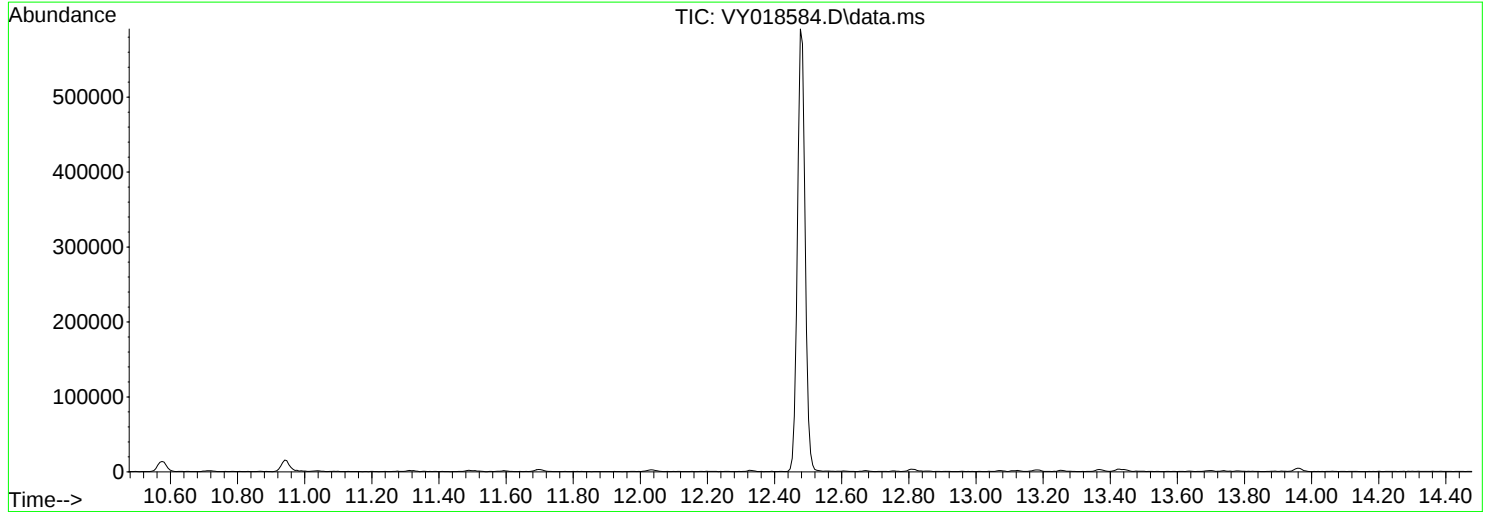

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.7	20637	PASS
75	95	30	60	54.7	54461	PASS
95	95	100	100	100.0	99501	PASS
96	95	5	9	6.9	6887	PASS
173	174	0.00	2	1.1	933	PASS
174	95	50	100	82.8	82395	PASS
175	174	5	9	7.7	6385	PASS
176	174	95	101	94.9	78208	PASS
177	176	5	9	6.4	4995	PASS