


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv061520\
Data File : VY002891.D
Acq On : 15 Jun 2020 09:23
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y052720S.M
Title : SW846 8260
Last Update : Wed May 27 13:13:33 2020

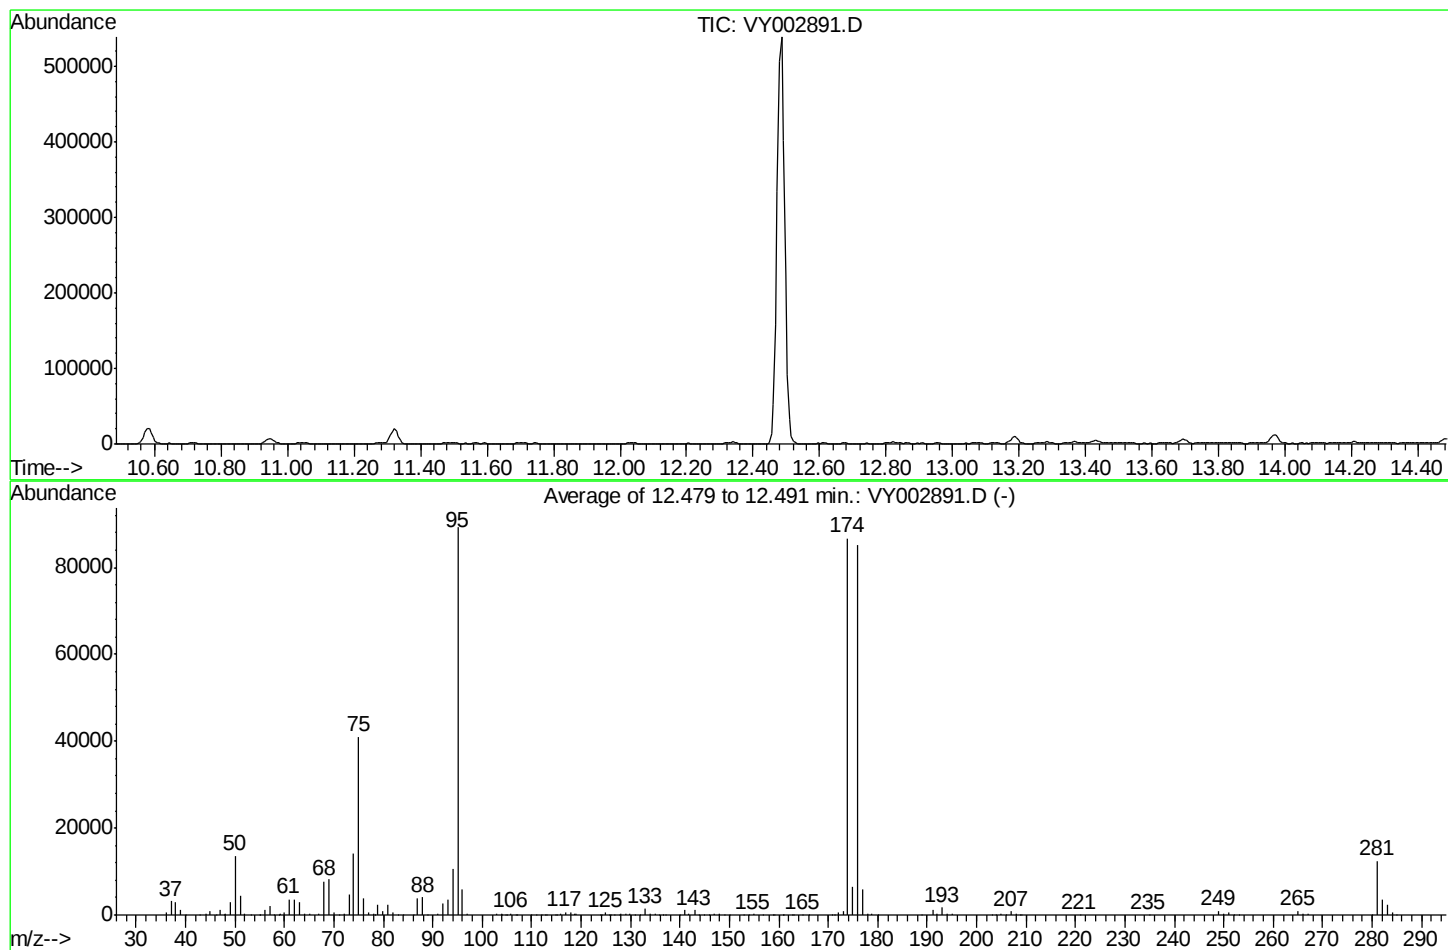

AutoFind: Scans 1762, 1763, 1764; Background Corrected with Scan 1753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	13695	PASS
75	95	30	60	45.9	40994	PASS
95	95	100	100	100.0	89237	PASS
96	95	5	9	6.5	5820	PASS
173	174	0.00	2	1.2	1025	PASS
174	95	50	100	97.1	86632	PASS
175	174	5	9	7.4	6419	PASS
176	174	95	101	98.3	85125	PASS
177	176	5	9	7.0	5941	PASS