


Tert butyl alcohol

Response Ratio

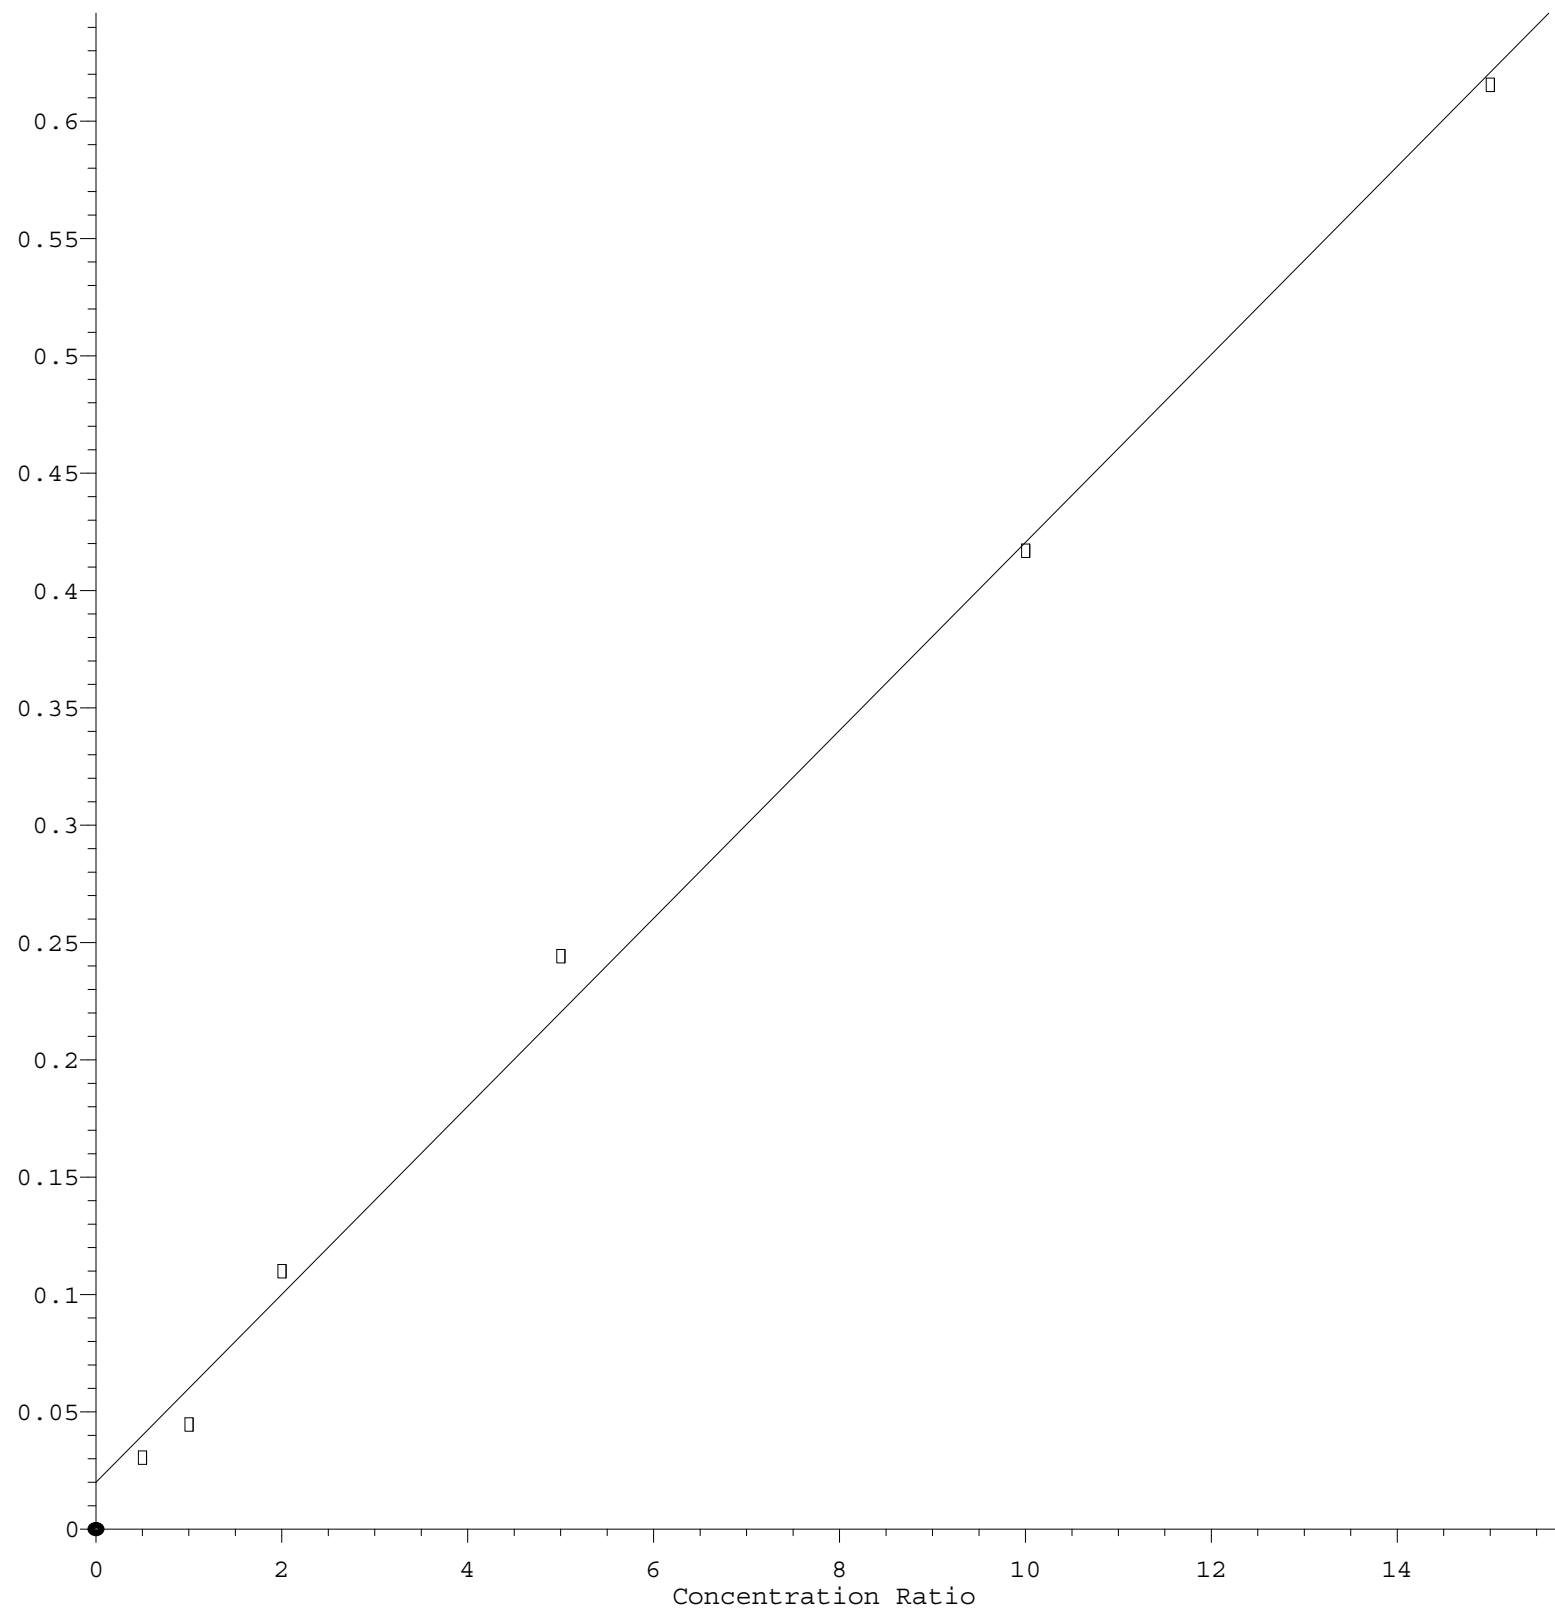

$$\text{Response} = 4.008\text{e-}002 * \text{Amt} + 1.982\text{e-}002$$


Coef of Det (r^2) = 0.996170 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y061521S.M

Calibration Table Last Updated: Wed Jun 16 04:40:35 2021

Methylene Chloride

Response Ratio

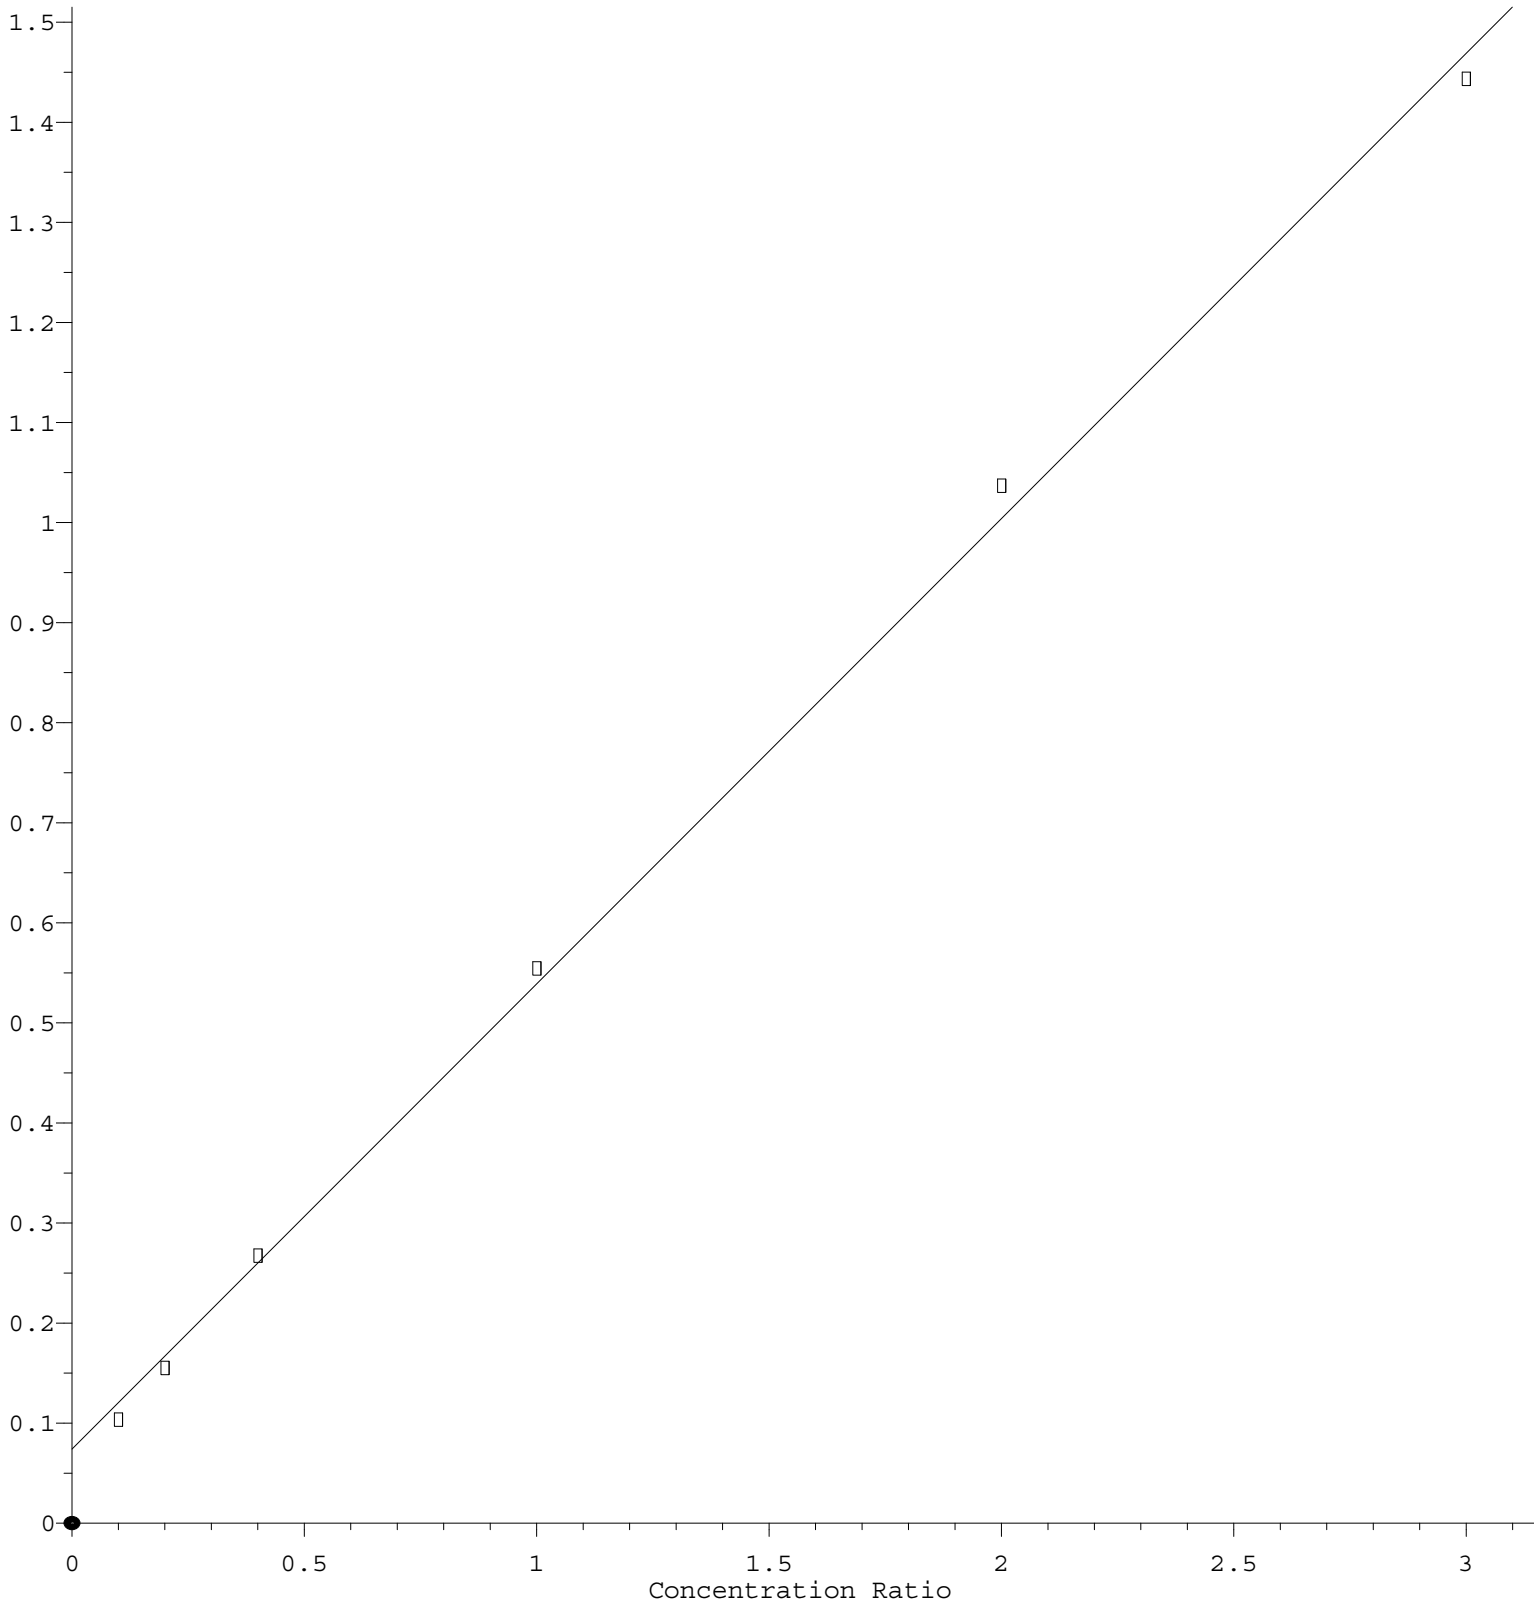


$$\text{Response} = 4.653\text{e-}001 * \text{Amt} + 7.384\text{e-}002$$

Coef of Det (r^2) = 0.998318 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y061521S.M

Calibration Table Last Updated: Wed Jun 16 04:40:35 2021

Dibromofluoromethane

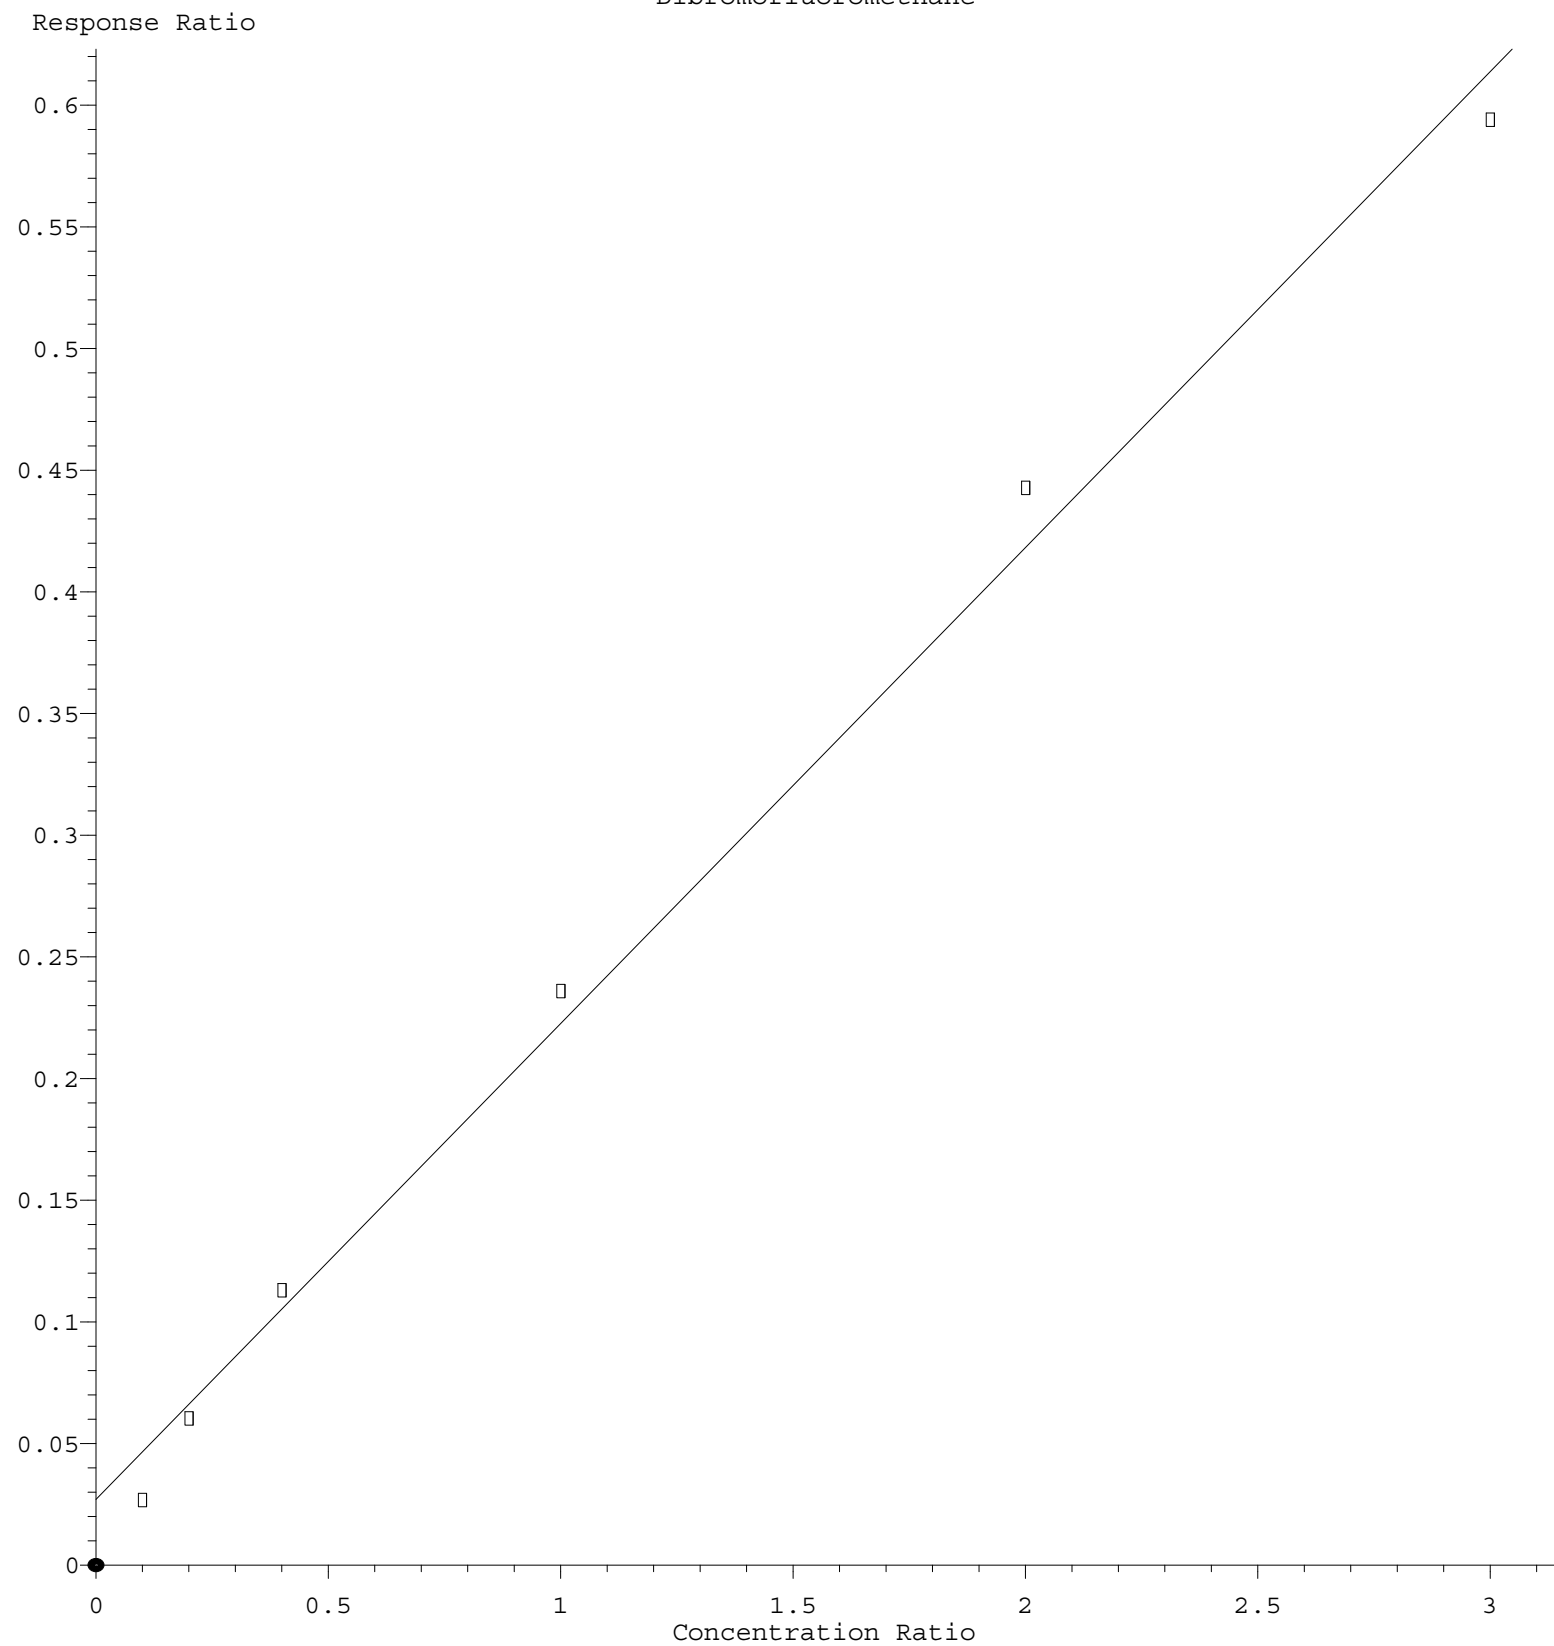

$\text{Response} = 1.960\text{e-}001 * \text{Amt} + 2.656\text{e-}002$
 Coef of Det (r^2) = 0.993638 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y061521S.M
 Calibration Table Last Updated: Wed Jun 16 04:40:35 2021