
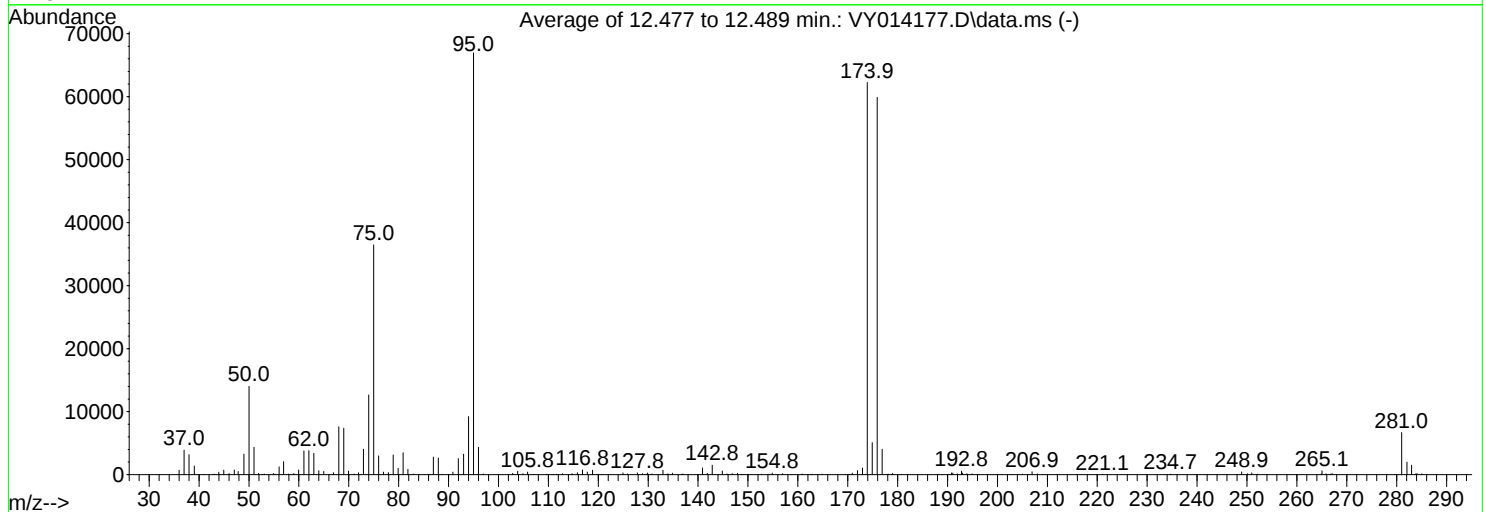


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY061523\
Data File : VY014177.D
Acq On : 15 Jun 2023 09:19
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060923S.M
Title : SW846 8260
Last Update : Fri Jun 09 18:07:13 2023

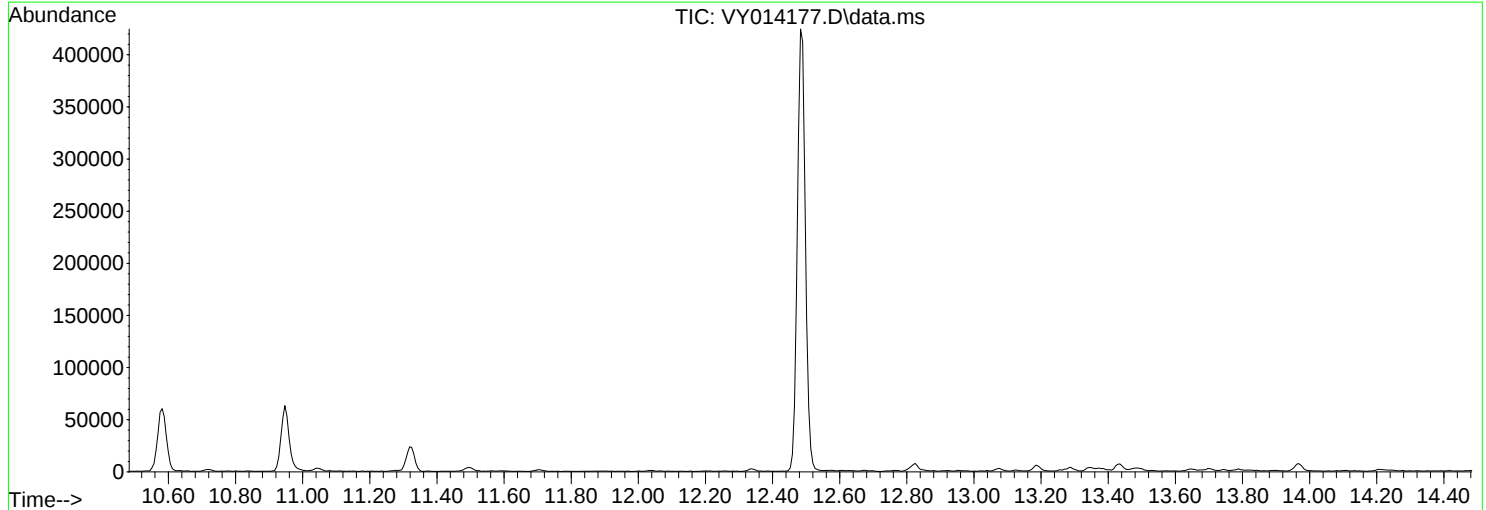

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.9	14025	PASS
75	95	30	60	54.5	36461	PASS
95	95	100	100	100.0	66955	PASS
96	95	5	9	6.5	4339	PASS
173	174	0.00	2	1.7	1039	PASS
174	95	50	100	93.0	62248	PASS
175	174	5	9	8.1	5068	PASS
176	174	95	101	96.2	59893	PASS
177	176	5	9	6.7	4041	PASS