

Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv061620\
 Data File : VY002908.D
 Acq On : 16 Jun 2020 14:34
 Operator : SY/MD
 Sample : L3020-03
 Misc : 7.30G/5ML/MSVOA Y/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 MW-24(19-21)

Quant Time: Jul 01 12:15:09 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y052720S.M
 Quant Title : SW846 8260
 QLast Update : Wed May 27 13:13:33 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.80	168	226114	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.69	114	370430	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.49	117	351926	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.42	152	179529	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.15	65	112635	57.37	ug/l	0.00
Spiked Amount 50.000			Recovery	=	114.74%	
35) Dibromofluoromethane	7.72	113	112709	51.92	ug/l	0.00
Spiked Amount 50.000			Recovery	=	103.84%	
50) Toluene-d8	10.18	98	437712	49.87	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.74%	
62) 4-Bromofluorobenzene	12.48	95	147649	49.22	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.44%	
Target Compounds						
20) Methylene Chloride	4.72	84	22283	9.904	ug/l	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv061620\
Data File : VY002908.D
Acq On : 16 Jun 2020 14:34
Operator : SY/MD
Sample : L3020-03
Misc : 7.30G/5ML/MSVOA Y/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
MW-24(19-21)

Quant Time: Jul 01 12:15:09 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y052720S.M
Quant Title : SW846 8260
QLast Update : Wed May 27 13:13:33 2020
Response via : Initial Calibration

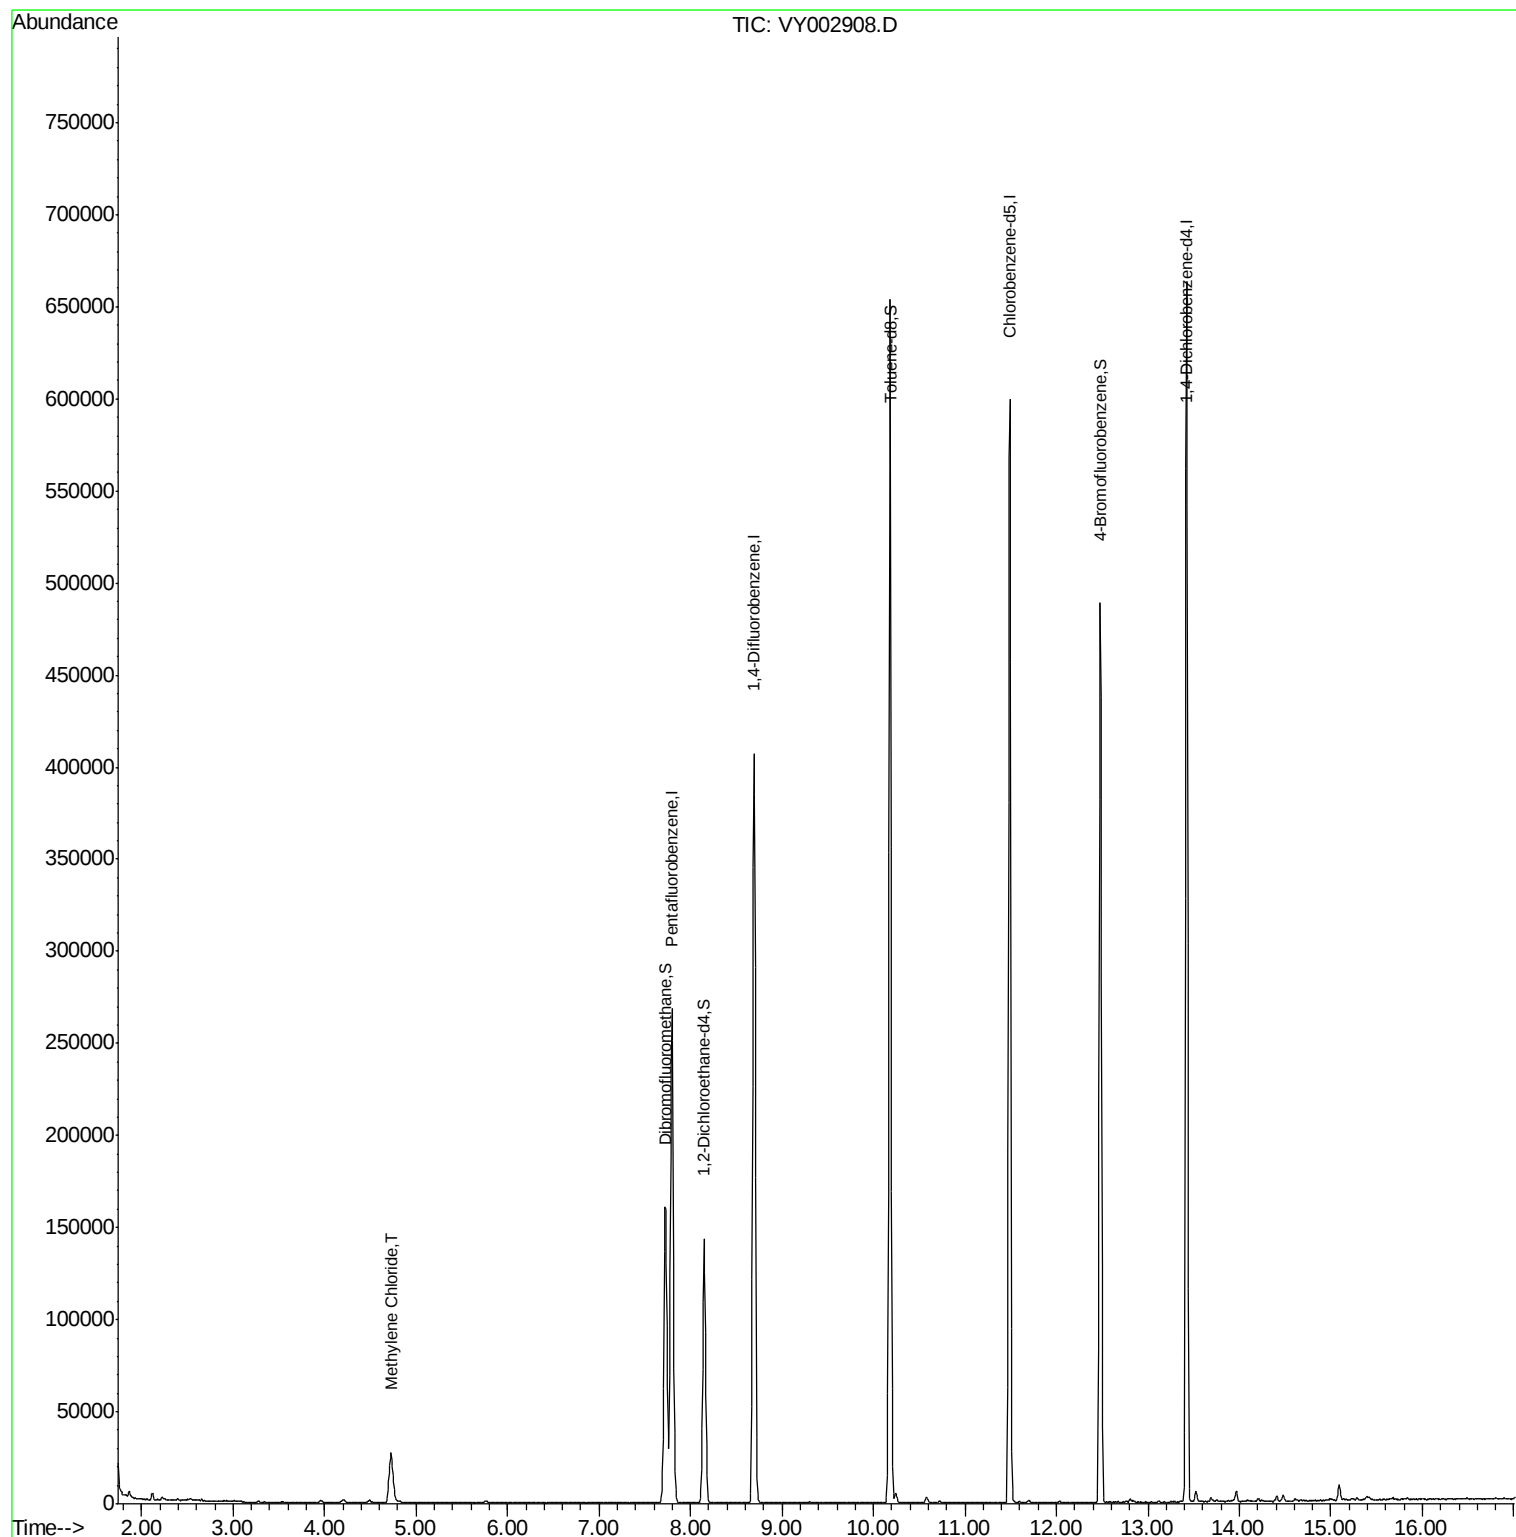



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.80 min Scan# 994

Delta R.T. 0.00 min

Lab File: VY002908.D

Acq: 16 Jun 2020 14:34

Instrument :

MSVOA_Y

ClientSampleId :


MW-24(19-21)

Tot Ion:168 Resp: 226114

Ion Ratio Lower Upper

168 100

99 51.4 39.0 58.4



Abundance Ion 167.90 (167.60 to 168.60): VY002758.D (-983) (-)

Ion 98.90 (98.60 to 99.60): VY002758.D (-983) (-)

7.80

100000

80000



60000

40000

20000

0

Time-->



#20

Methylene Chloride

Concen: 9.904 ug/l

RT: 4.72 min Scan# 490

Delta R.T. 0.00 min

Lab File: VY002908.D

Acq: 16 Jun 2020 14:34

Tgt Ion: 84 Resp: 22283


Ion Ratio Lower Upper

84 100

49 107.9 88.5 132.7

51 33.4 26.8 40.2

86 66.8 50.6 75.8



Abundance Ion 83.90 (83.60 to 84.60): VY002758.D (-476) (-)

Ion 48.90 (48.60 to 49.60): VY002758.D (-476) (-)

Ion 50.90 (50.60 to 51.60): VY002758.D (-476) (-)

Ion 85.90 (85.60 to 86.60): VY002758.D (-476) (-)

12000

10000

8000


6000


4000

2000

0

Time-->









#33
 1,2-Dichloroethane-d4
 Concen: 57.370 ug/l
 RT: 8.15 min Scan# 1052
 Delta R.T. 0.00 min
 Lab File: VY002908.D
 Acq: 16 Jun 2020 14:34




Instrument :
 MSVOA_Y
 ClientSampleId :
 MW-24(19-21)


Tot Ion: 65 Resp: 112635
 Ion Ratio Lower Upper
 65 100
 67 53.6 0.0 111.0

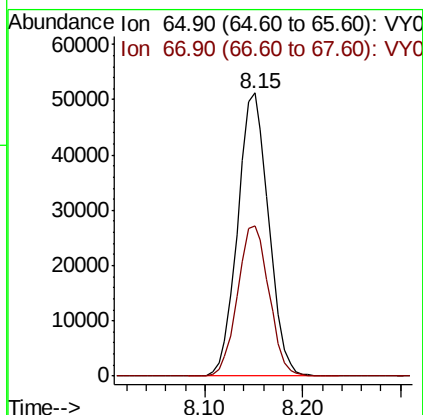

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.69 min Scan# 1141
 Delta R.T. 0.00 min
 Lab File: VY002908.D
 Acq: 16 Jun 2020 14:34

Tgt Ion: 114 Resp: 370430
 Ion Ratio Lower Upper
 114 100
 63 17.8 0.0 35.2
 88 14.8 0.0 29.2



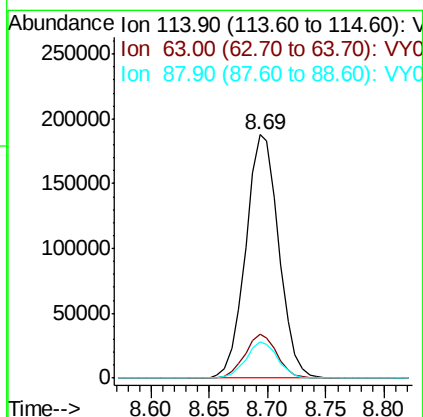





#35
 Dibromofluoromethane
 Concen: 51.918 ug/l
 RT: 7.72 min Scan# 982
 Delta R.T. -0.01 min
 Lab File: VY002908.D
 Acq: 16 Jun 2020 14:34




Instrument :
 MSVOA_Y
 ClientSampleId :
 MW-24(19-21)


Tot Ion	Ratio	Lower	Upper
113	100		
111	103.4	82.0	123.0
192	23.7	18.9	28.3

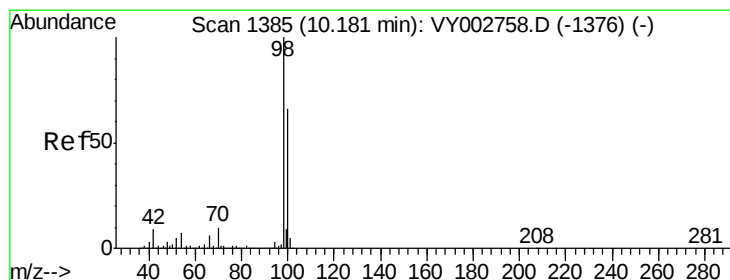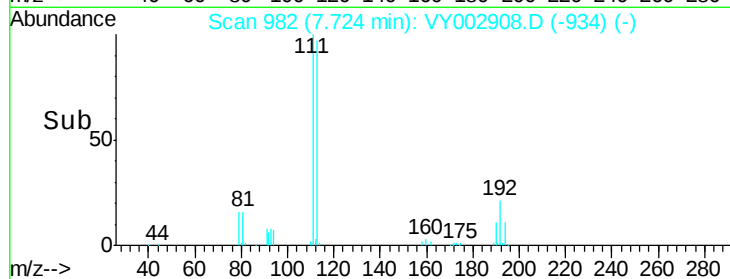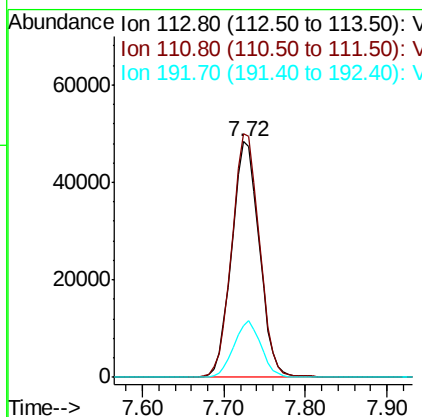

#50
 Toluene-d8
 Concen: 49.867 ug/l
 RT: 10.18 min Scan# 1385
 Delta R.T. 0.00 min
 Lab File: VY002908.D
 Acq: 16 Jun 2020 14:34

Tgt Ion	Ratio	Lower	Upper
98	100		
100	64.2	52.2	78.2

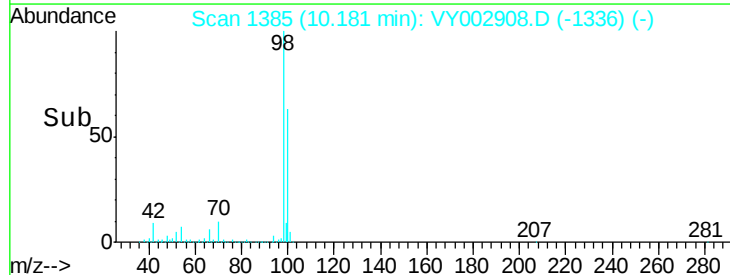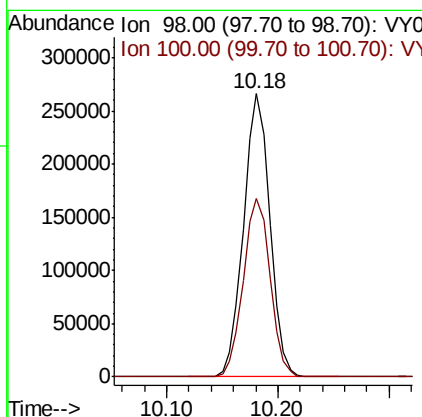



#62

4-Bromofluorobenzene

Concen: 49.221 ug/l

RT: 12.48 min Scan# 1762

Delta R.T. 0.00 min

Lab File: VY002908.D

Acq: 16 Jun 2020 14:34

Instrument :

MSVOA_Y

ClientSampleId :

MW-24(19-21)


Tot Ion: 95 Resp: 147649

Ion Ratio Lower Upper

95 100

174 97.5 0.0 191.2




176 95.0 0.0 188.8

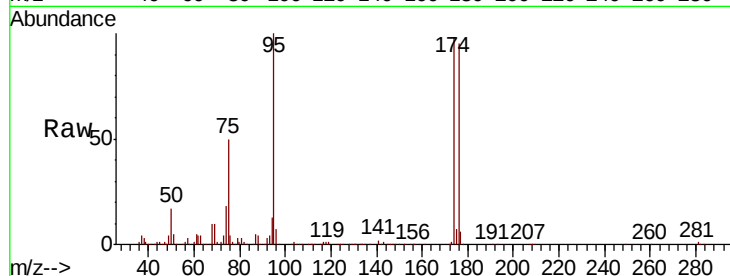

Abundance Ion 94.90 (94.60 to 95.60): VY002908.D (-1713) (-)

Ion 173.80 (173.50 to 174.50): VY002908.D (-1713) (-)

Ion 175.80 (175.50 to 176.50): VY002908.D (-1713) (-)

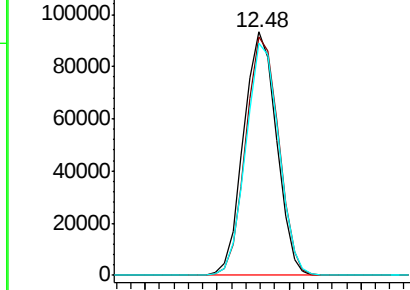

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.49 min Scan# 1600

Delta R.T. 0.00 min

Lab File: VY002908.D

Acq: 16 Jun 2020 14:34


Tgt Ion: 117 Resp: 351926

Ion Ratio Lower Upper

117 100

82 51.5 40.2 60.4



119 32.5 25.8 38.8




Abundance Ion 116.90 (116.60 to 117.60): VY002908.D (-1551) (-)

Ion 82.00 (81.70 to 82.70): VY002908.D (-1551) (-)

Ion 118.90 (118.60 to 119.60): VY002908.D (-1551) (-)

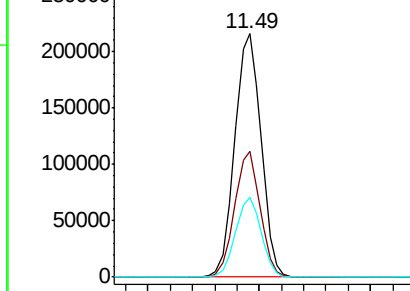

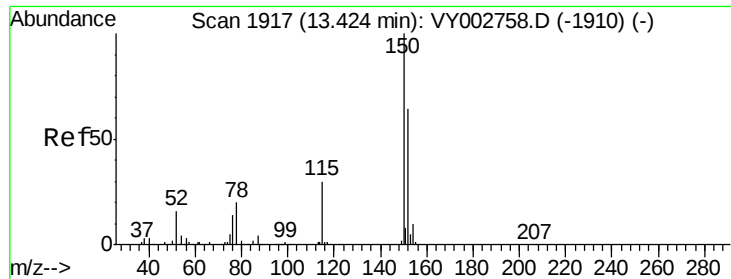

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.42 min Scan# 1917

Delta R.T. 0.00 min

Lab File: VY002908.D

Acq: 16 Jun 2020 14:34

Instrument :

MSVOA_Y

ClientSampleId :

MW-24(19-21)


Tot Ion:152 Resp: 179529

Ion Ratio Lower Upper

152 100

115 54.0 27.0 81.0

150 157.9 0.0 344.8

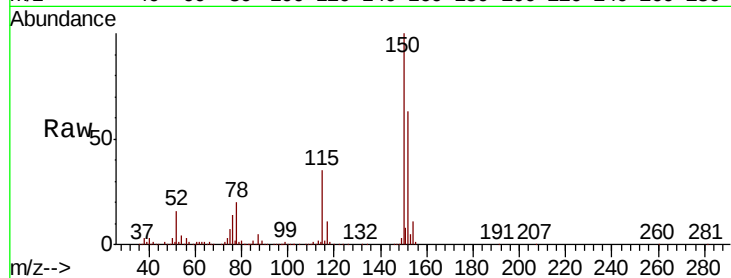

Abundance

Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

