
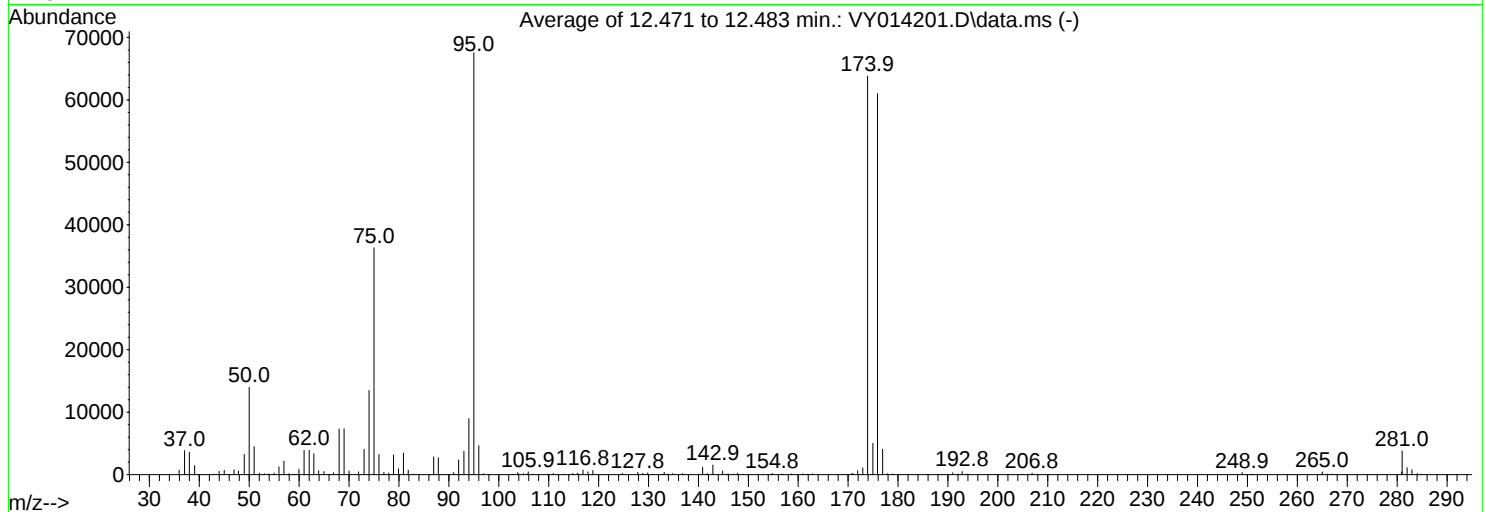


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY061623\
Data File : VY014201.D
Acq On : 16 Jun 2023 13:19
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060923S.M
Title : SW846 8260
Last Update : Fri Jun 09 18:07:13 2023

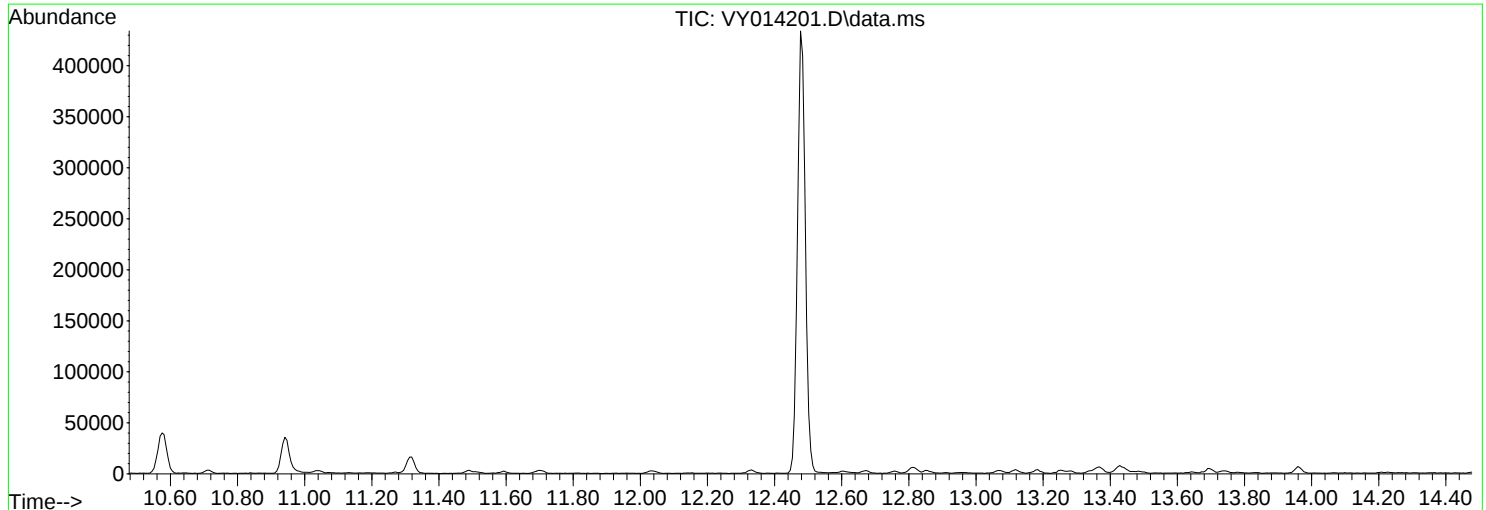

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1739

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.7	13987	PASS
75	95	30	60	53.8	36328	PASS
95	95	100	100	100.0	67533	PASS
96	95	5	9	6.9	4646	PASS
173	174	0.00	2	1.7	1077	PASS
174	95	50	100	94.5	63821	PASS
175	174	5	9	7.9	5014	PASS
176	174	95	101	95.6	61021	PASS
177	176	5	9	6.7	4064	PASS