
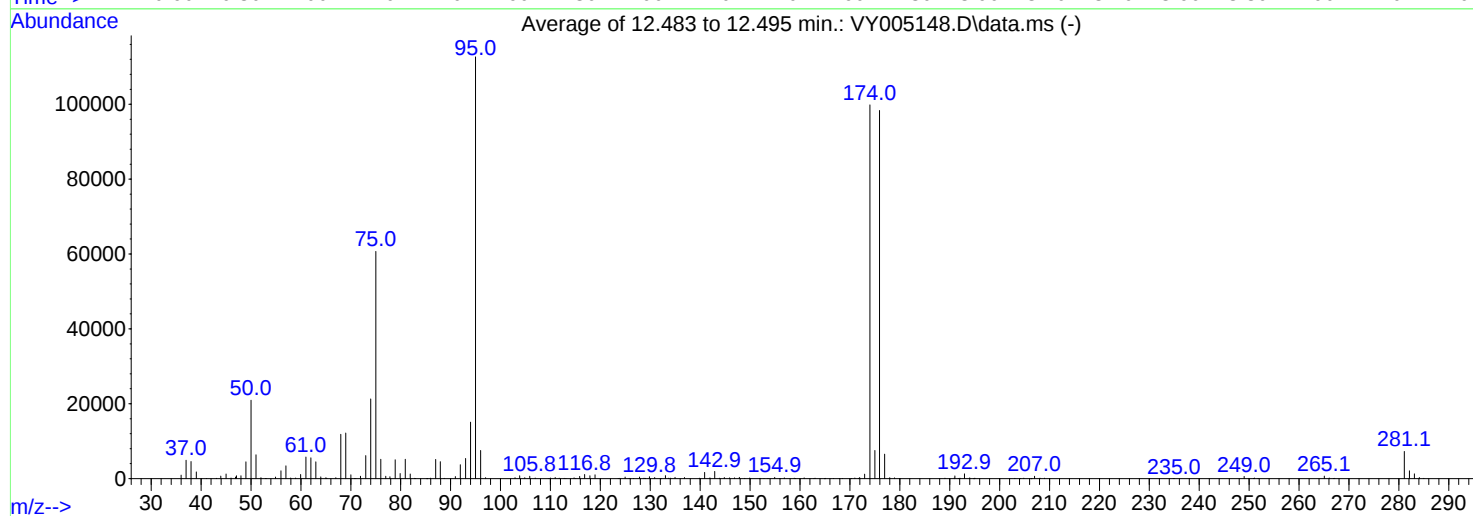


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY061721\
 Data File : VY005148.D
 Acq On : 17 Jun 2021 10:03
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y061521S.M
 Title : SW846 8260
 Last Update : Wed Jun 16 04:40:35 2021

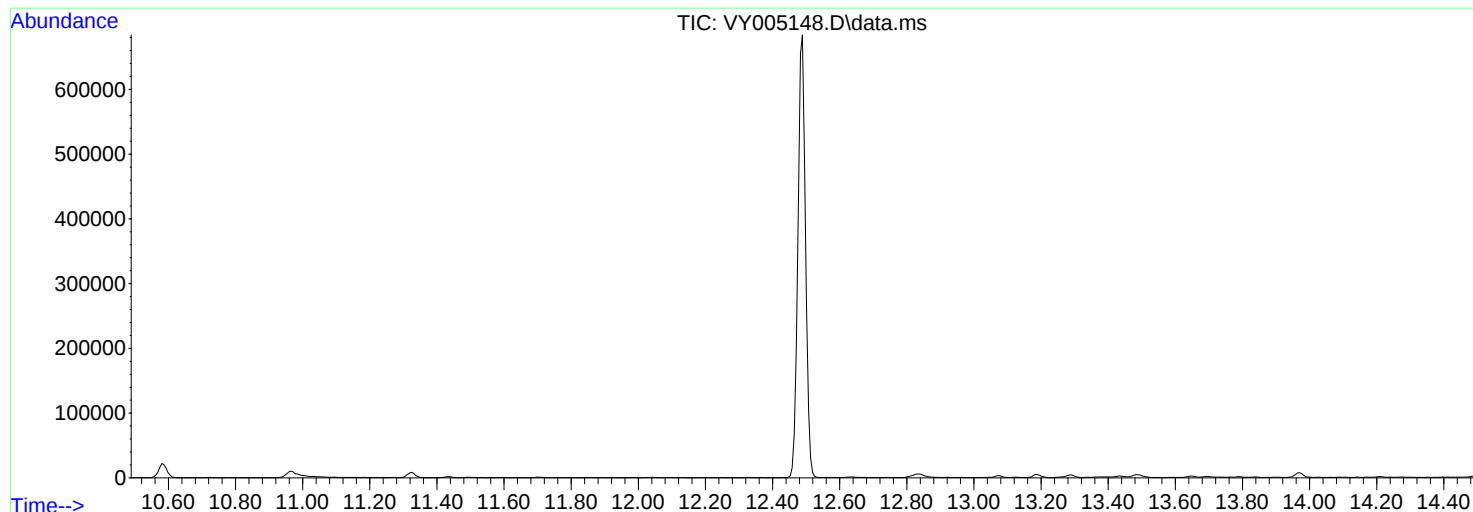

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	20925	PASS
75	95	30	60	53.9	60704	PASS
95	95	100	100	100.0	112664	PASS
96	95	5	9	6.7	7518	PASS
173	174	0.00	2	1.2	1212	PASS
174	95	50	100	88.6	99835	PASS
175	174	5	9	7.6	7543	PASS
176	174	95	101	98.5	98339	PASS
177	176	5	9	6.6	6526	PASS