

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY061920\
 Data File : VY002953.D
 Acq On : 19 Jun 2020 21:23
 Operator : SY/MD
 Sample : L3046-08
 Misc : 9.73G/5ML/MSVOA Y/SOIL
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 ISS-C-G2

Quant Time: Jun 20 05:11:15 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y061920S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 19 15:04:26 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.80	168	287362	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.69	114	468751	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.49	117	439809	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.42	152	221642	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.15	65	142315	59.96	ug/l	0.00
Spiked Amount 50.000			Recovery	=	119.92%	
35) Dibromofluoromethane	7.72	113	145331	54.79	ug/l	0.00
Spiked Amount 50.000			Recovery	=	109.58%	
50) Toluene-d8	10.18	98	550253	52.62	ug/l	0.00
Spiked Amount 50.000			Recovery	=	105.24%	
62) 4-Bromofluorobenzene	12.48	95	190870	52.62	ug/l	0.00
Spiked Amount 50.000			Recovery	=	105.24%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY061920\
Data File : VY002953.D
Acq On : 19 Jun 2020 21:23
Operator : SY/MD
Sample : L3046-08
Misc : 9.73G/5ML/MSVOA Y/SOIL
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
ISS-C-G2

Quant Time: Jun 20 05:11:15 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y061920S.M
Quant Title : SW846 8260
QLast Update : Fri Jun 19 15:04:26 2020
Response via : Initial Calibration

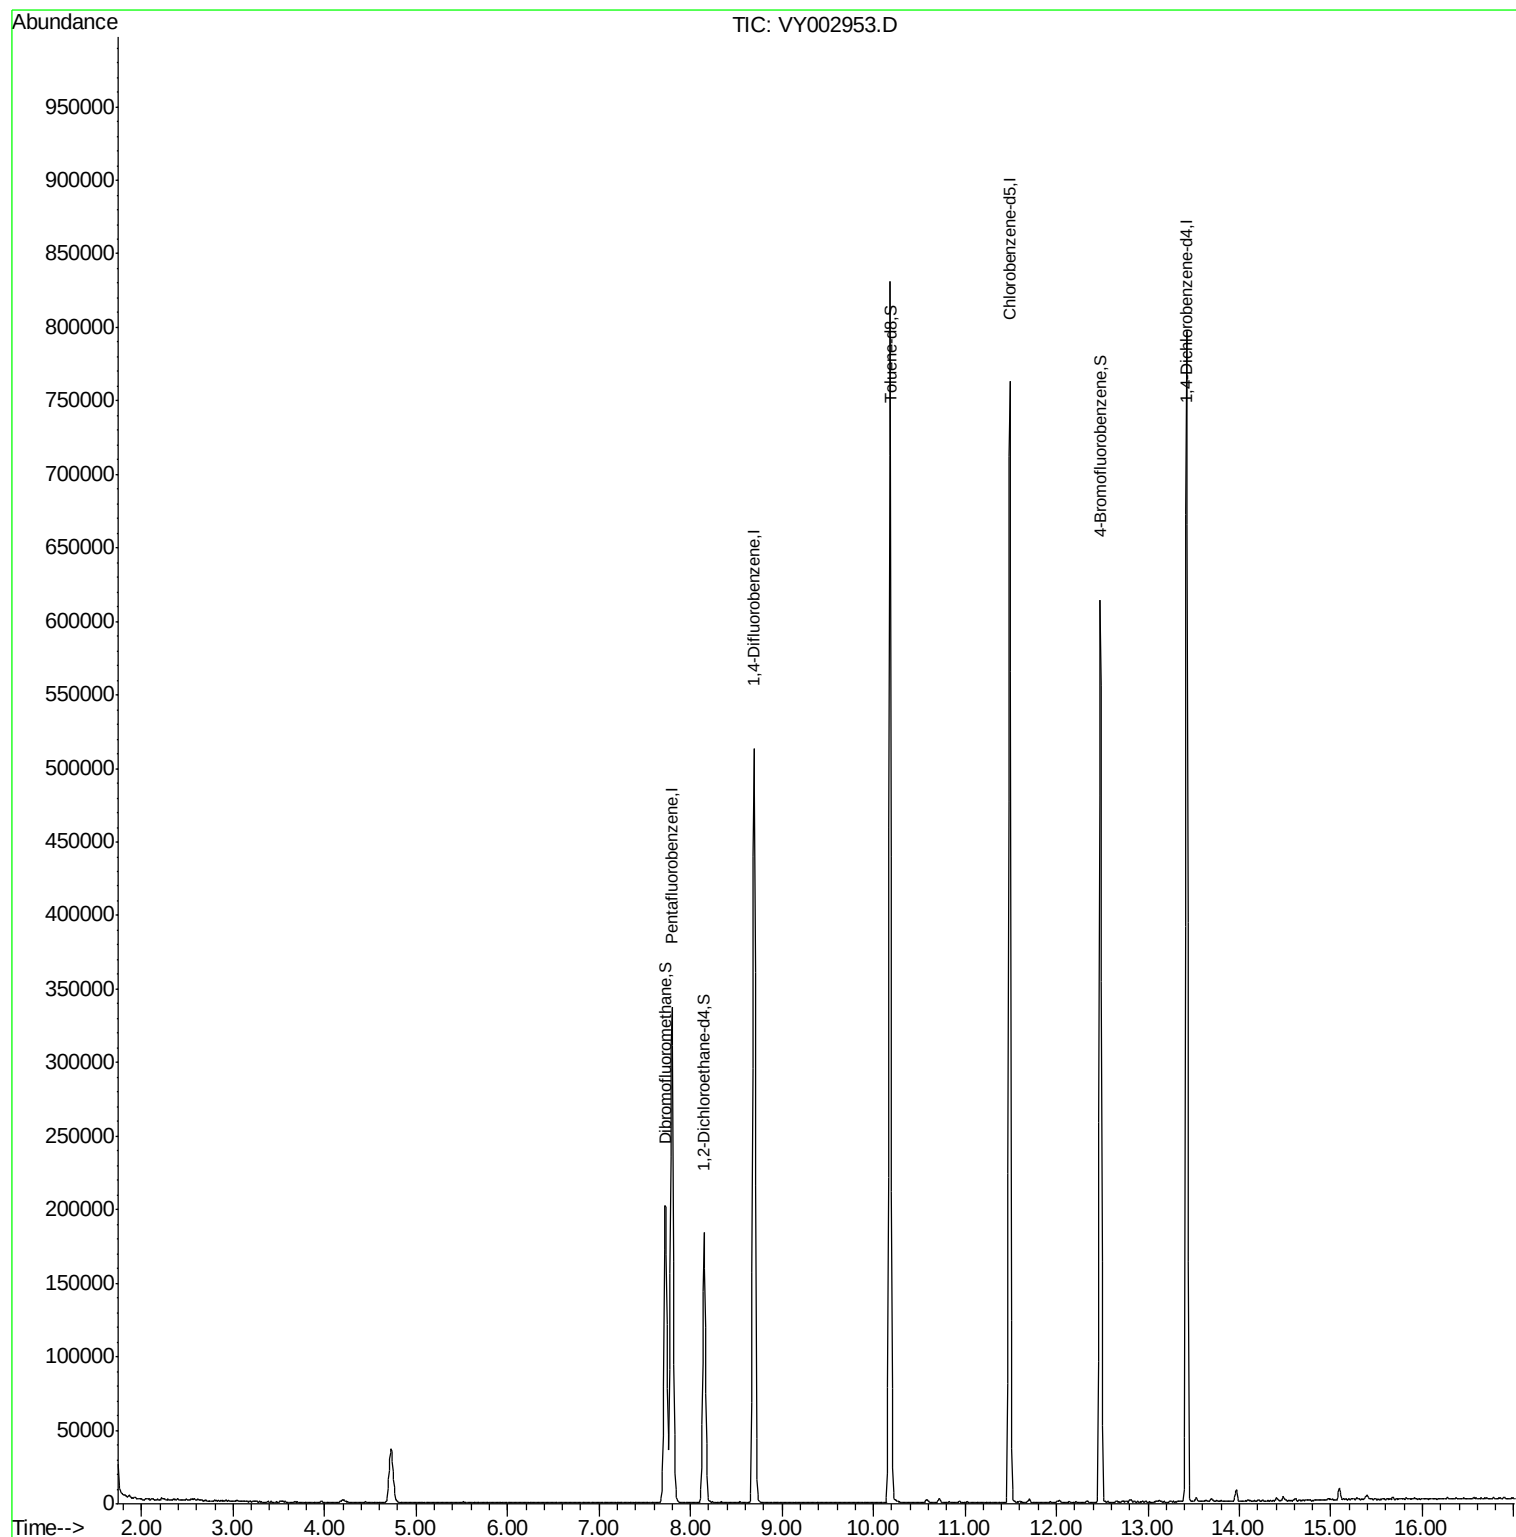

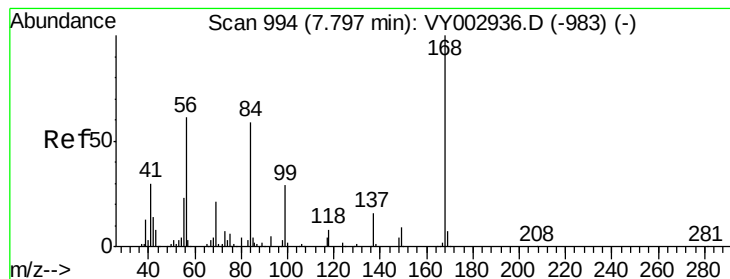

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.80 min Scan# 994

Delta R.T. 0.00 min

Lab File: VY002953.D

Acq: 19 Jun 2020 21:23

Instrument :

MSVOA_Y

ClientSampleId :


ISS-C-G2

Tot Ion:168 Resp: 287362

Ion Ratio Lower Upper

168 100

99 48.8 39.5 59.3

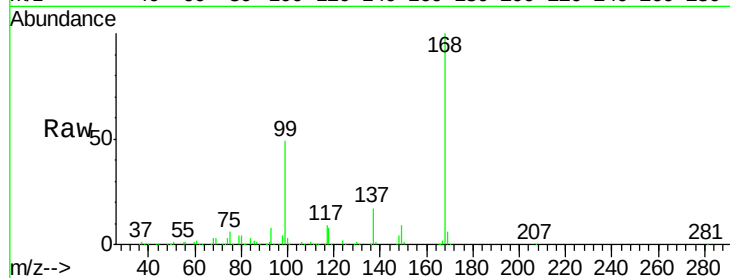

Abundance Ion 167.90 (167.60 to 168.60): VY002953.D (-945) (-)

Ion 98.90 (98.60 to 99.60): VY002953.D (-945) (-)

7.80



150000

100000

50000

0

Time-->

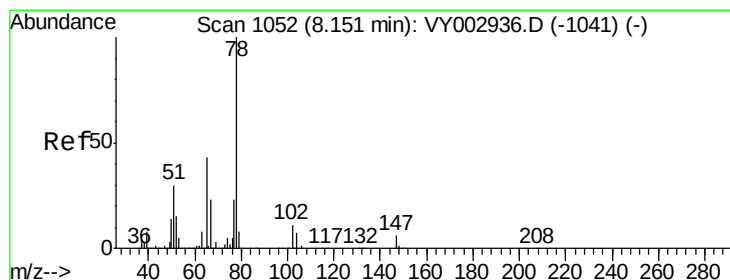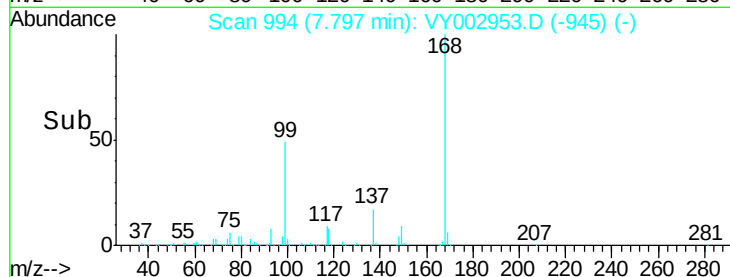

#33

1,2-Dichloroethane-d4

Concen: 59.958 ug/l

RT: 8.15 min Scan# 1052

Delta R.T. 0.00 min

Lab File: VY002953.D


Acq: 19 Jun 2020 21:23

Tgt Ion: 65 Resp: 142315

Ion Ratio Lower Upper

65 100

67 54.5 0.0 109.4

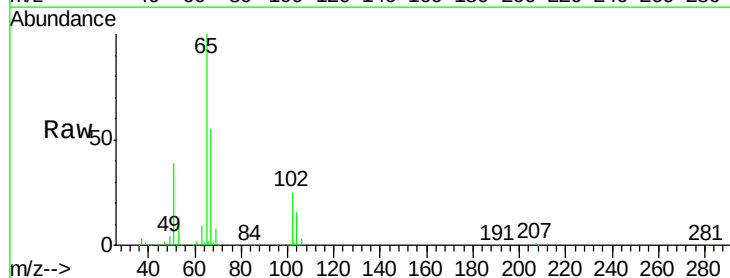

Abundance Ion 64.90 (64.60 to 65.60): VY002953.D (-1003) (-)

Ion 66.90 (66.60 to 67.60): VY002953.D (-1003) (-)

8.15


60000


40000

20000

0

Time-->

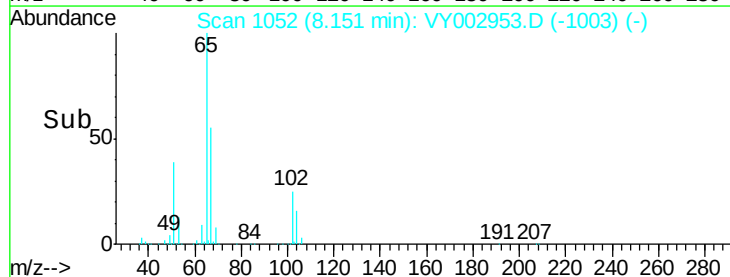

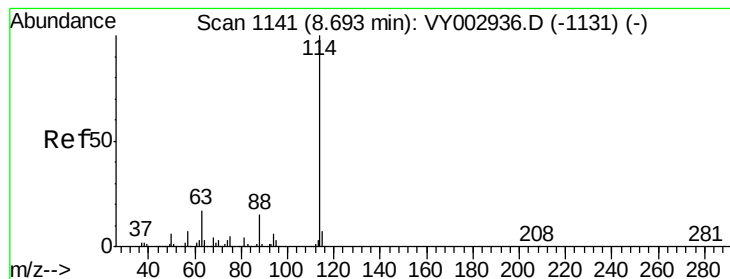

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.69 min Scan# 1141

Delta R.T. 0.00 min

Lab File: VY002953.D

Acq: 19 Jun 2020 21:23

Instrument :

MSVOA_Y

ClientSampleId :

ISS-C-G2


Tot Ion:114 Resp: 468751

Ion Ratio Lower Upper

114 100

63 17.4 0.0 34.6




88 14.7 0.0 29.2

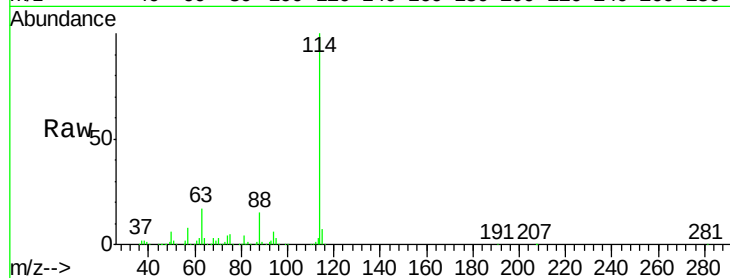

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VY0

Ion 87.90 (87.60 to 88.60): VY0

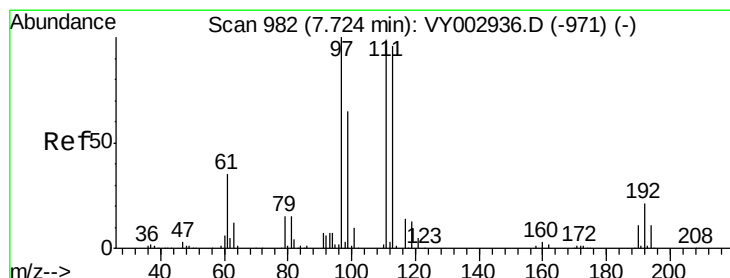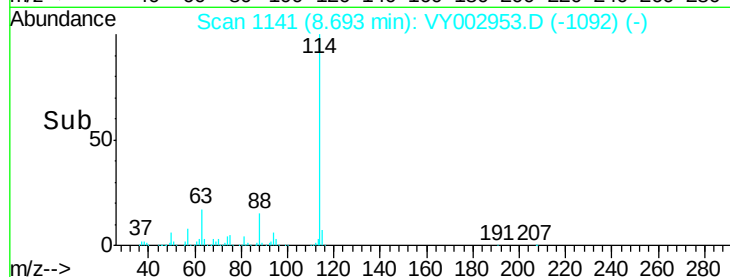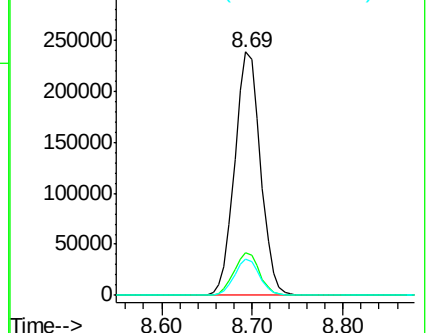

#35

Dibromofluoromethane

Concen: 54.794 ug/l

RT: 7.72 min Scan# 982

Delta R.T. 0.00 min

Lab File: VY002953.D

Acq: 19 Jun 2020 21:23


Tgt Ion:113 Resp: 145331

Ion Ratio Lower Upper

113 100

111 102.2 81.5 122.3



192 23.0 19.2 28.8

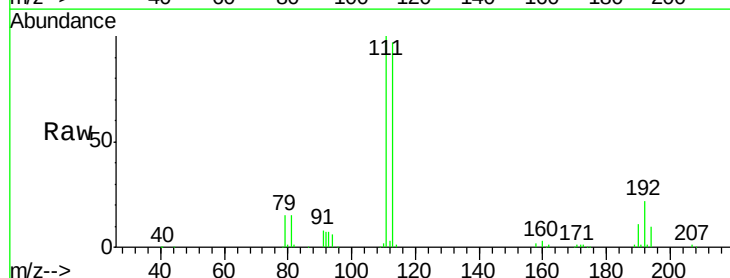


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

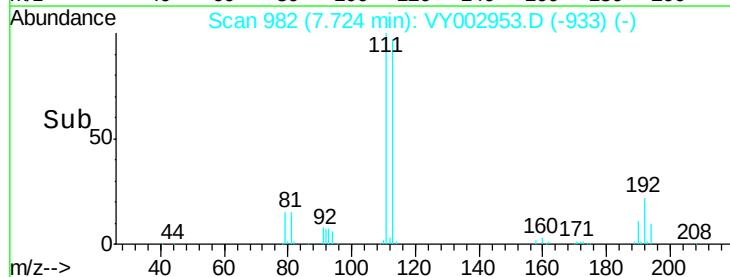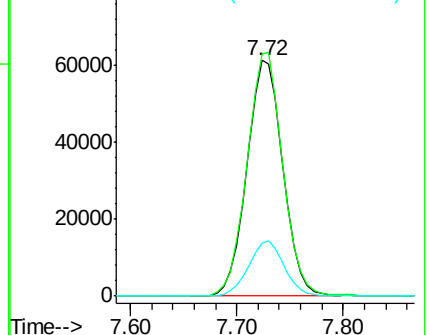

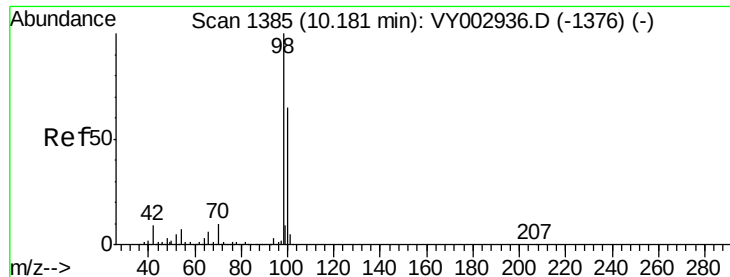

#50

Toluene-d8

Concen: 52.616 ug/l

RT: 10.18 min Scan# 1385

Delta R.T. 0.00 min

Lab File: VY002953.D

Acq: 19 Jun 2020 21:23

Instrument :

MSVOA_Y

ClientSampleId :





ISS-C-G2

Tot Ion: 98 Resp: 550253

Ion Ratio Lower Upper

98 100

100 64.7 51.9 77.9

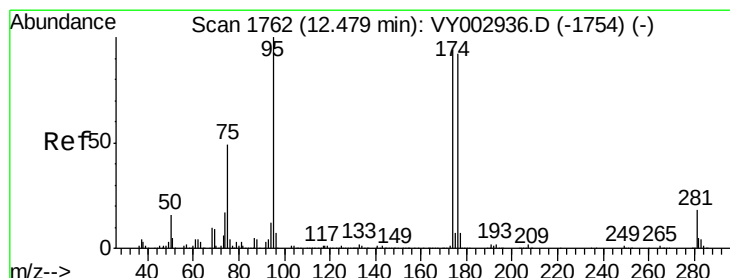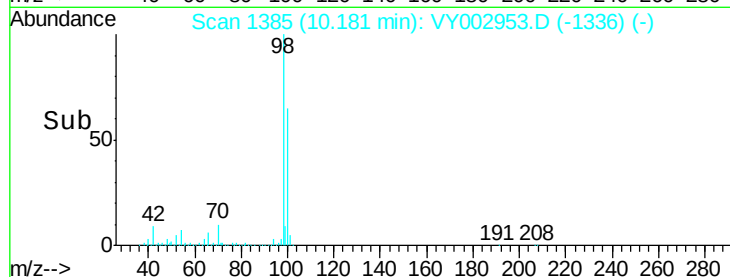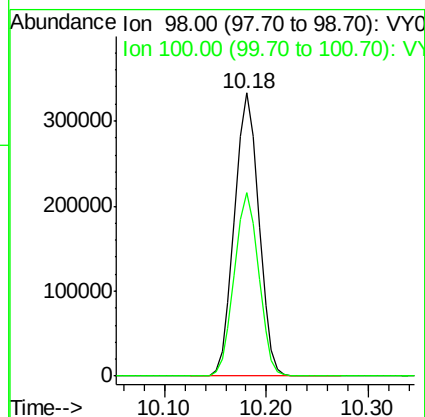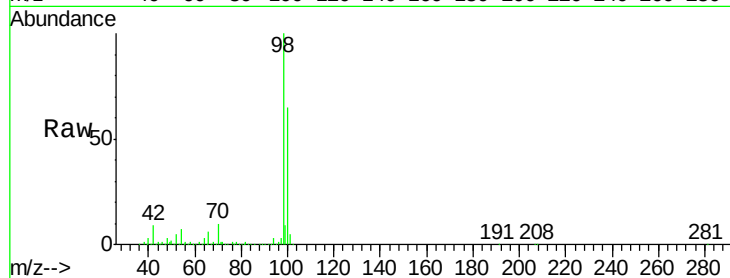

#62

4-Bromofluorobenzene

Concen: 52.616 ug/l

RT: 12.48 min Scan# 1762

Delta R.T. 0.00 min

Lab File: VY002953.D

Acq: 19 Jun 2020 21:23




Tgt Ion: 95 Resp: 190870


Ion Ratio Lower Upper

95 100

174 94.6 0.0 191.2

176 91.4 0.0 186.0

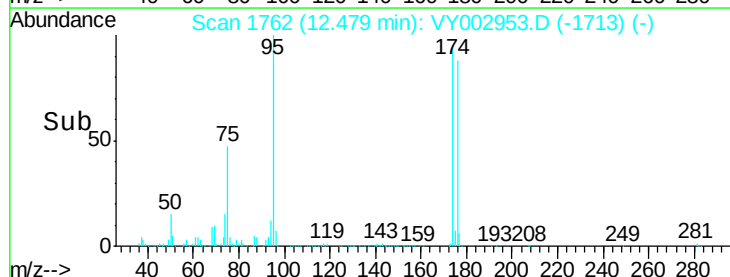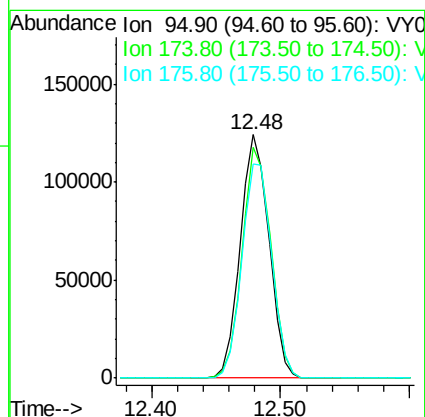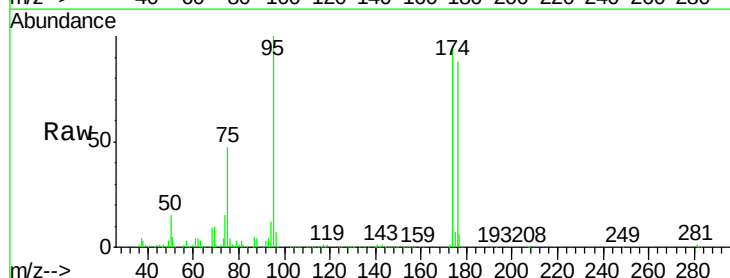


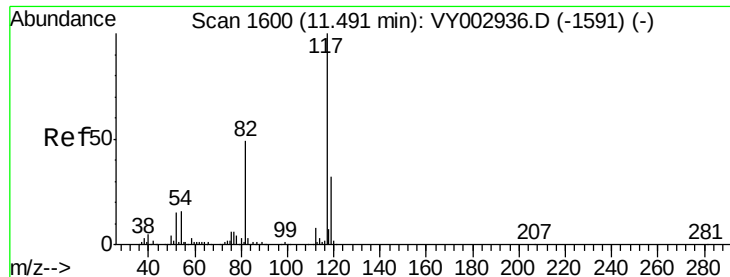


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.49 min Scan# 1600
Delta R.T. 0.00 min
Lab File: VY002953.D
Acq: 19 Jun 2020 21:23

Instrument :
MSVOA_Y
ClientSampleId :
ISS-C-G2



Tot Ion	Ratio	Lower	Upper
117	100		
82	51.2	39.4	59.0
119	32.6	25.4	38.0

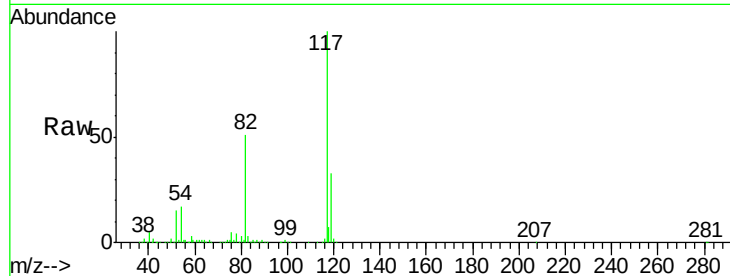

Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VY0
Ion 118.90 (118.60 to 119.60): V

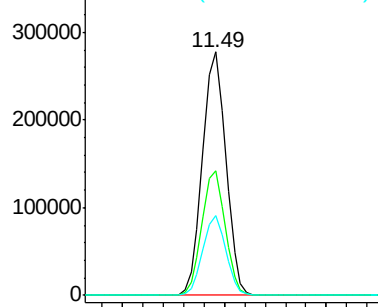


Time-->

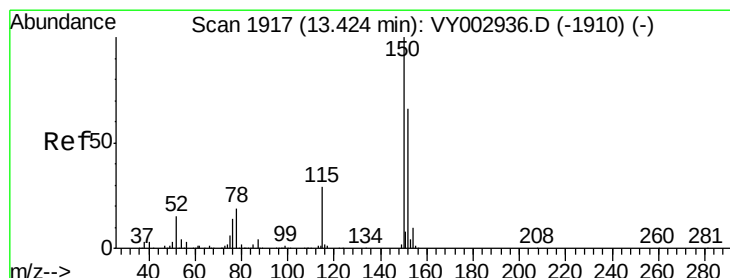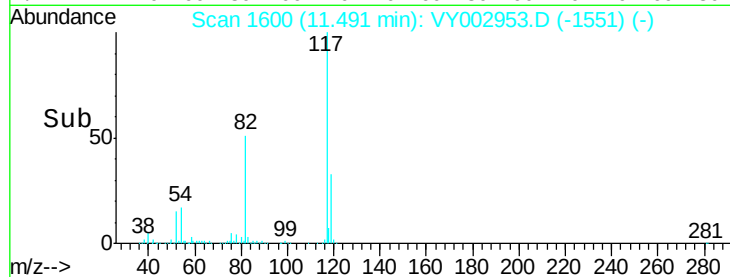


#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.42 min Scan# 1917
Delta R.T. 0.00 min
Lab File: VY002953.D
Acq: 19 Jun 2020 21:23

Tgt Ion	Ratio	Lower	Upper
152	100		
115	54.5	26.9	80.6
150	154.3	0.0	341.8

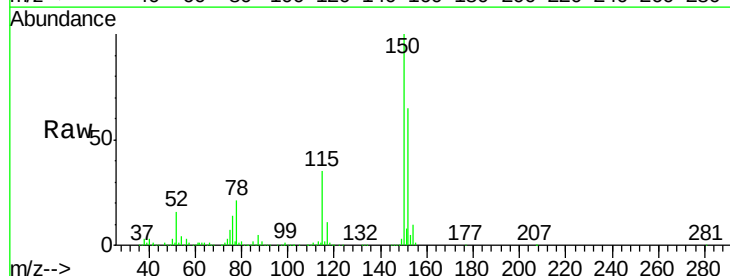

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

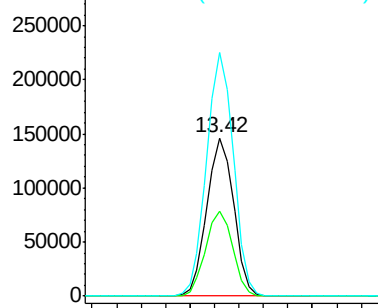

Time-->

