


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061720\
 Data File : VV016953.D
 Acq On : 17 Jun 2020 08:48
 Operator : SY/MD
 Sample : BFB39
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Jul 01 06:00:36 2020

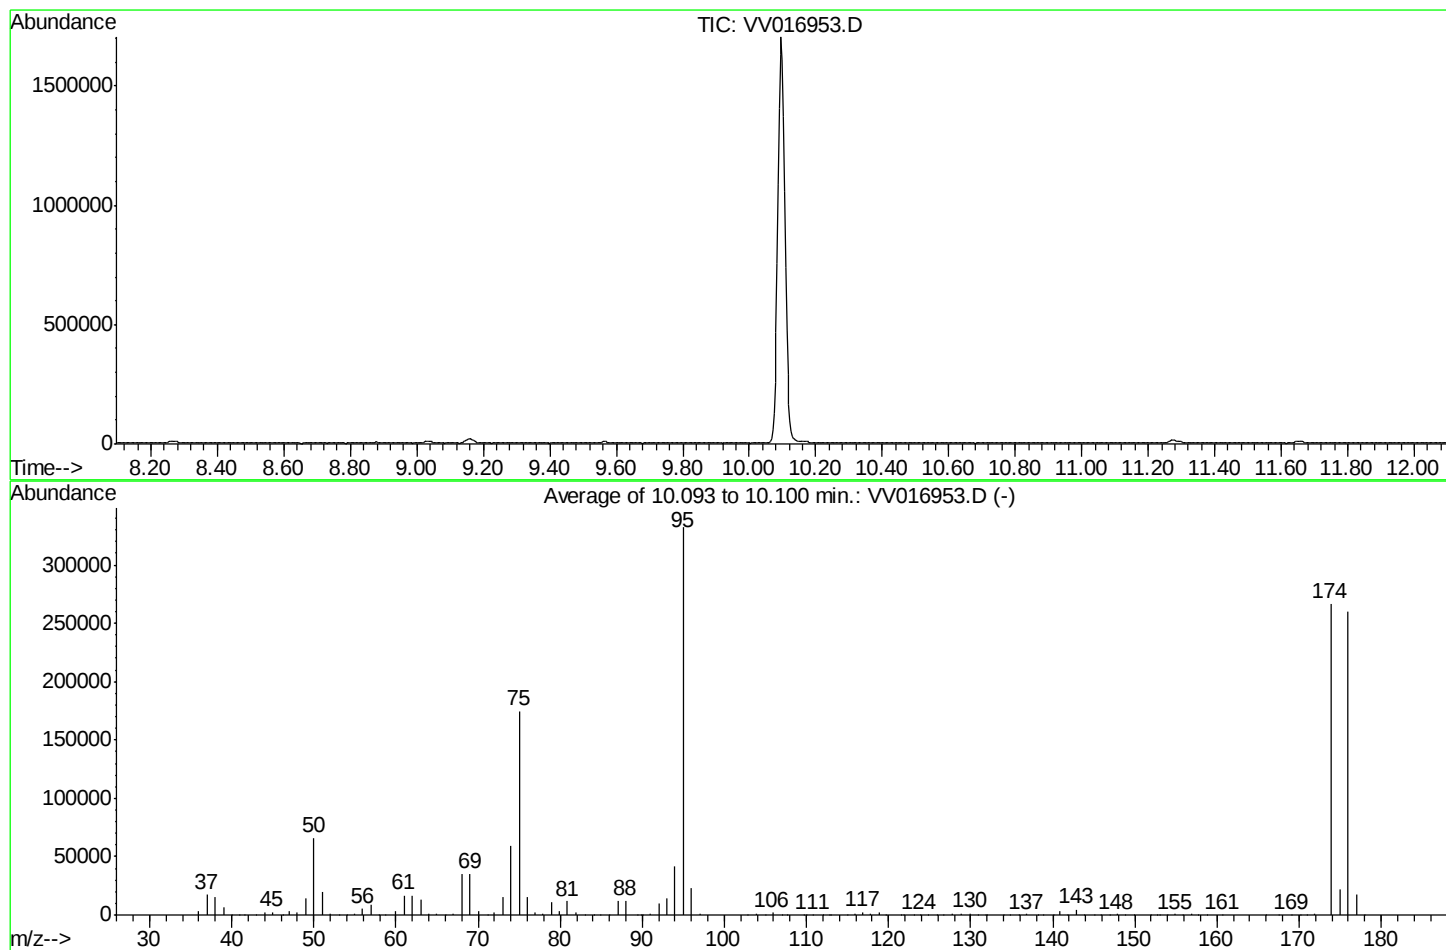

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2787

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	66069	PASS
75	95	30	80	52.6	174890	PASS
95	95	100	100	100.0	332266	PASS
96	95	5	9	6.9	22776	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	80.3	266773	PASS
175	174	5	9	8.2	21949	PASS
176	174	95	101	97.3	259584	PASS
177	176	5	9	6.6	17248	PASS