

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY061923\
 Data File : VY014269.D
 Acq On : 20 Jun 2023 08:33
 Operator : KP/MD
 Sample : 03302-04
 Misc : 10.16g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-3

Quant Time: Jun 20 11:25:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060923S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 09 18:07:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.801	168	120092	50.000	ug/l	0.01
34) 1,4-Difluorobenzene	8.697	114	181574	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.496	117	166623	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	74652	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	78010	46.648	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	93.300%
35) Dibromofluoromethane	7.728	113	60290	46.821	ug/l	0.01
Spiked Amount	50.000	Range	54 - 147	Recovery	=	93.640%
50) Toluene-d8	10.185	98	219467	45.588	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	91.180%
62) 4-Bromofluorobenzene	12.489	95	63453	37.104	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	74.200%
Target Compounds						
16) Acetone	3.954	43	6862	13.613	ug/l	95
20) Methylene Chloride	4.723	84	15487	6.505	ug/l	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY061923\
Data File : VY014269.D
Acq On : 20 Jun 2023 08:33
Operator : KP/MD
Sample : 03302-04
Misc : 10.16g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SB-3

Quant Time: Jun 20 11:25:17 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060923S.M
Quant Title : SW846 8260
QLast Update : Fri Jun 09 18:07:13 2023
Response via : Initial Calibration




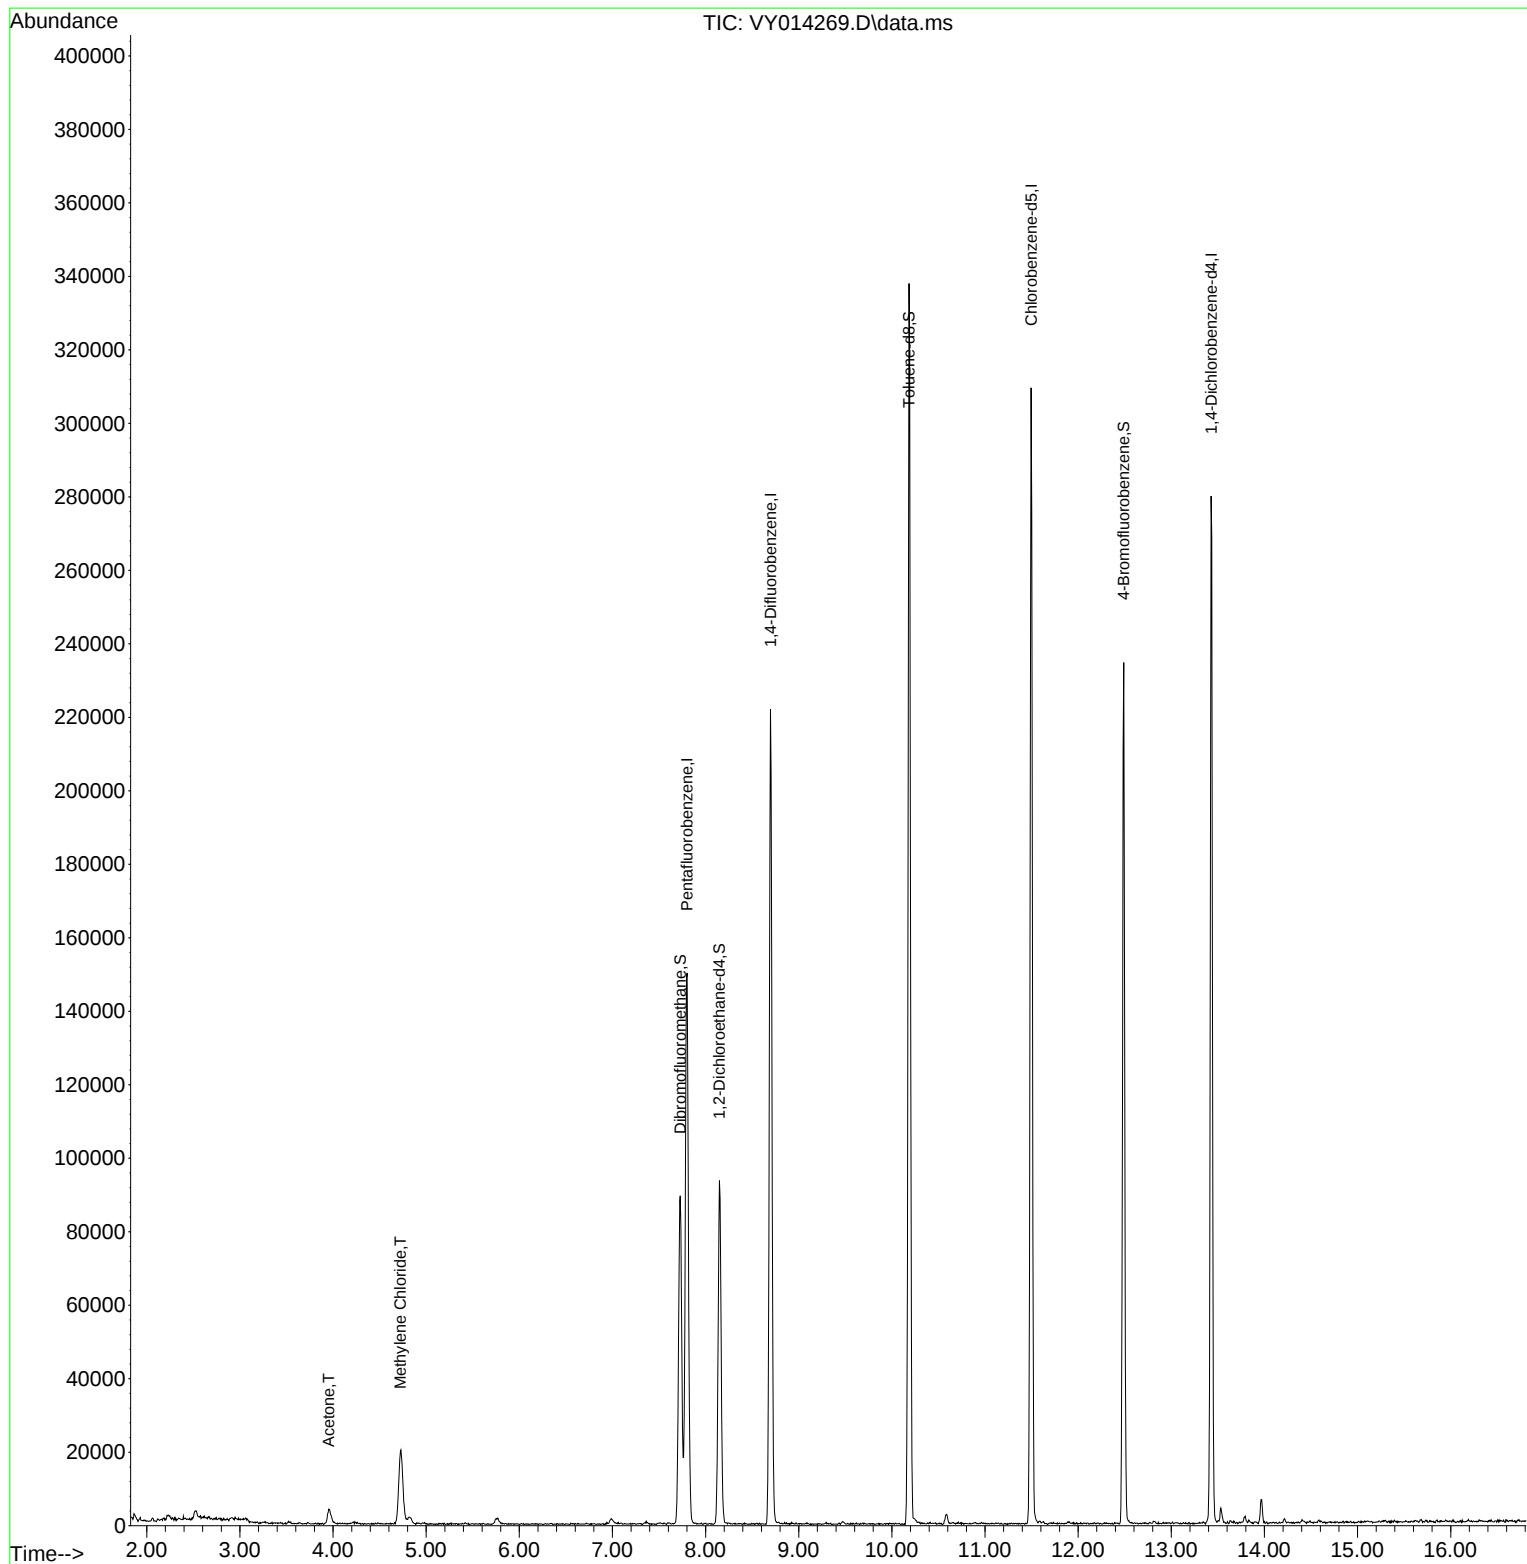


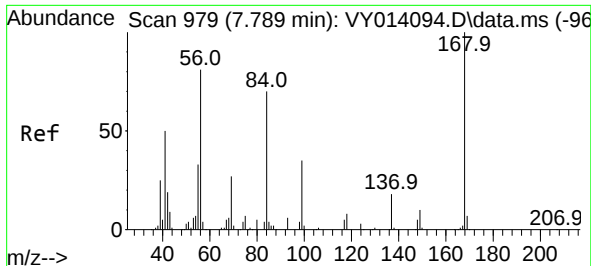

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.801 min Scan# 91
Delta R.T. 0.012 min
Lab File: VY014269.D
Acq: 20 Jun 2023 08:33




Instrument :
MSVOA_Y
ClientSampleId :
SB-3


Tgt Ion:168 Resp: 120092
Ion Ratio Lower Upper
168 100
99 52.3 43.4 65.0

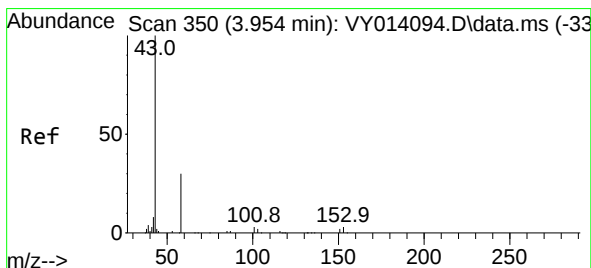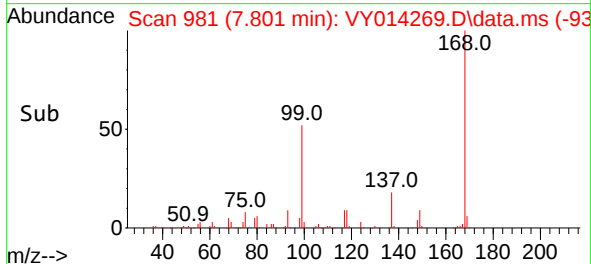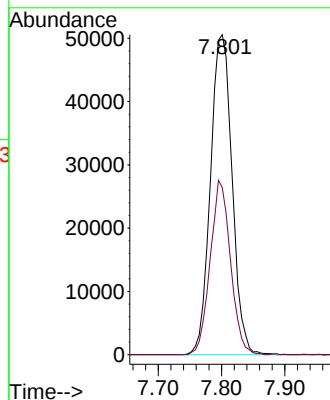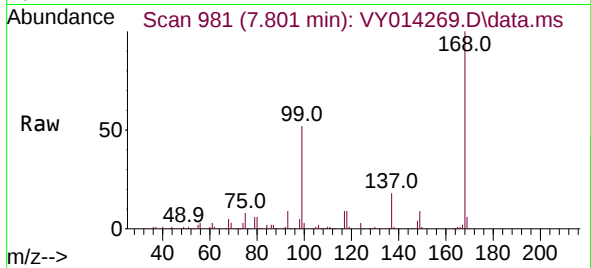

#16
Acetone
Concen: 13.613 ug/l
RT: 3.954 min Scan# 350
Delta R.T. 0.000 min
Lab File: VY014269.D
Acq: 20 Jun 2023 08:33

Tgt Ion: 43 Resp: 6862
Ion Ratio Lower Upper
43 100
58 25.9 22.7 34.1


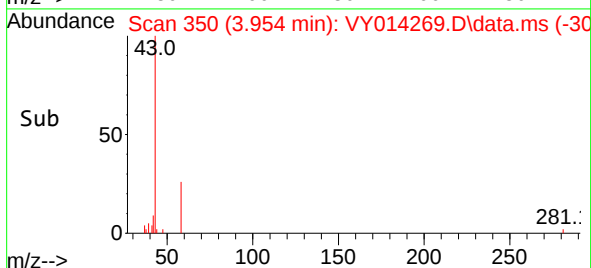
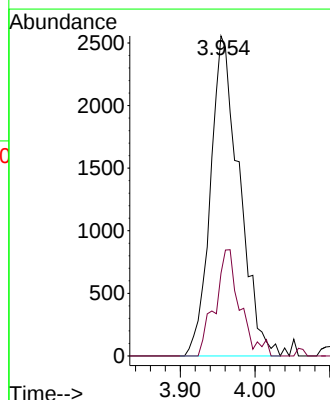
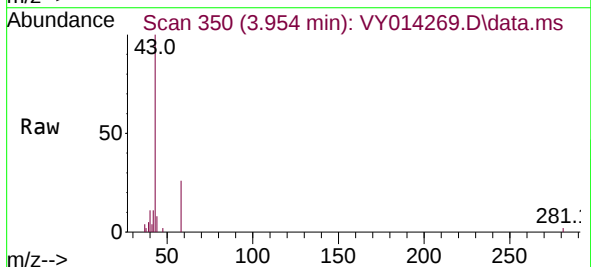


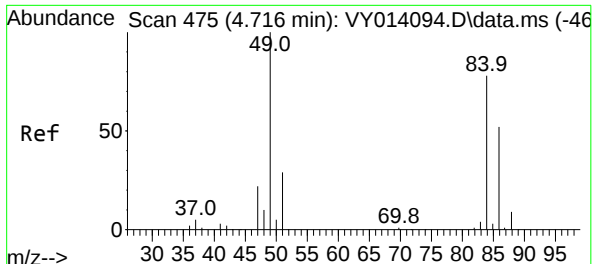

#20
Methylene Chloride
Concen: 6.505 ug/l
RT: 4.723 min Scan# 41
Delta R.T. 0.006 min
Lab File: VY014269.D
Acq: 20 Jun 2023 08:33




Instrument :
MSVOA_Y
ClientSampleId :
SB-3


Tgt Ion:	84	Resp:	15487
Ion	Ratio	Lower	Upper
84	100		
49	110.7	106.9	160.3
51	41.1	33.2	49.8
86	54.1	51.0	76.6

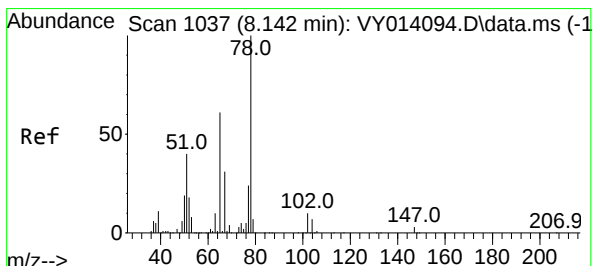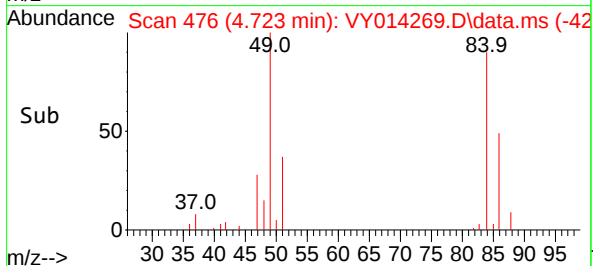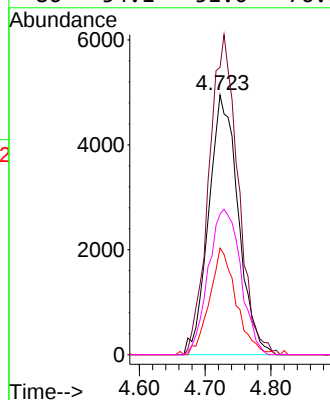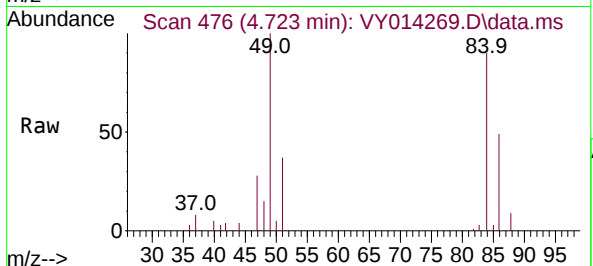

#33
1,2-Dichloroethane-d4
Concen: 46.648 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. 0.007 min
Lab File: VY014269.D
Acq: 20 Jun 2023 08:33

Tgt Ion:	65	Resp:	78010
Ion	Ratio	Lower	Upper
65	100		
67	50.3	0.0	101.8


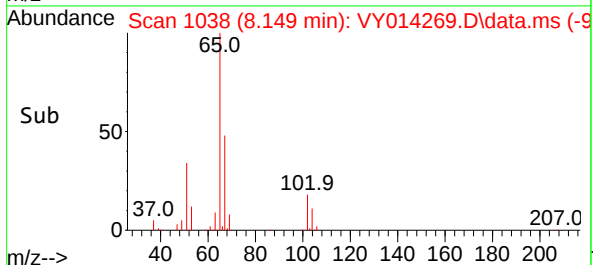
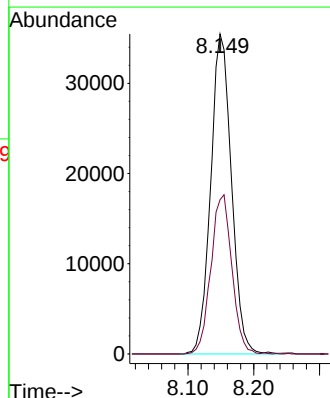
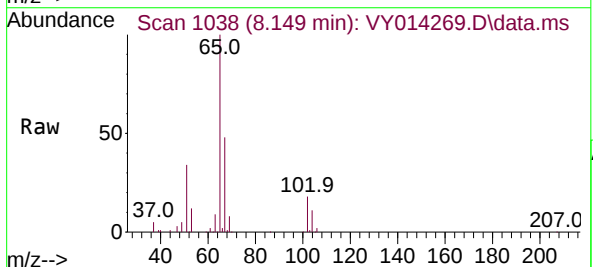


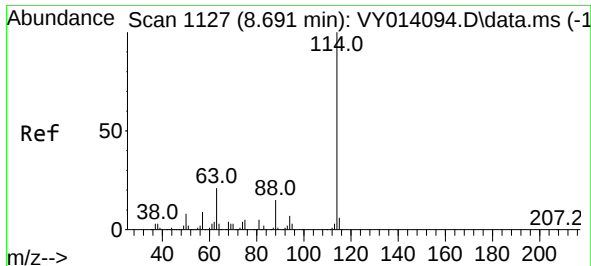

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.697 min Scan# 1127
Delta R.T. 0.006 min
Lab File: VY014269.D
Acq: 20 Jun 2023 08:33




Instrument :
MSVOA_Y
ClientSampleId :
SB-3


Tgt Ion:114 Resp: 181574
Ion Ratio Lower Upper
114 100
63 20.5 0.0 42.4
88 14.7 0.0 30.6

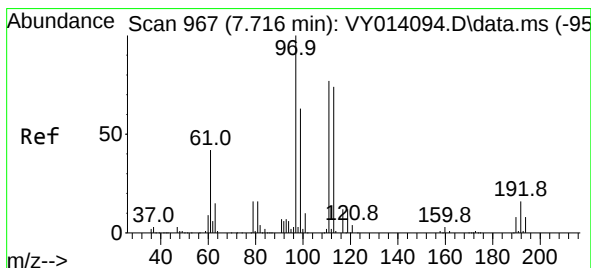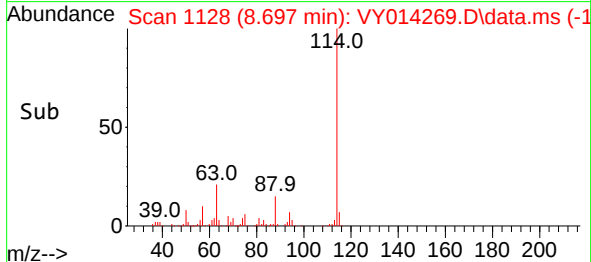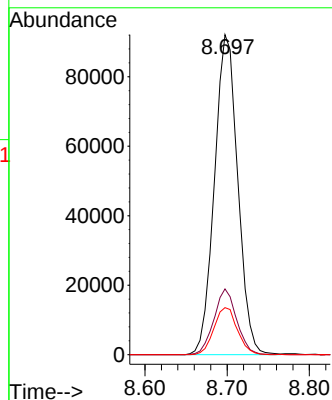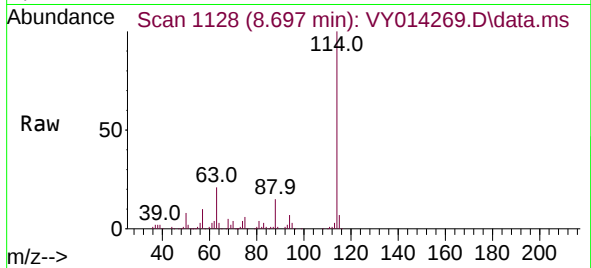

#35
Dibromofluoromethane
Concen: 46.821 ug/l
RT: 7.728 min Scan# 969
Delta R.T. 0.012 min
Lab File: VY014269.D
Acq: 20 Jun 2023 08:33

Tgt Ion:113 Resp: 60290
Ion Ratio Lower Upper
113 100
111 106.0 81.3 121.9
192 22.1 16.9 25.3


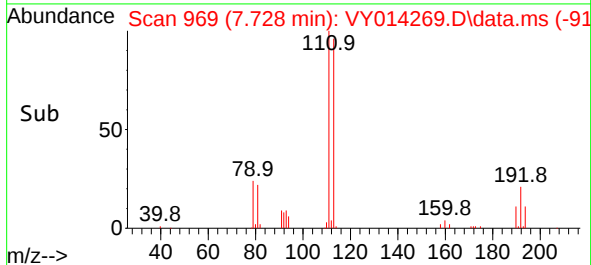
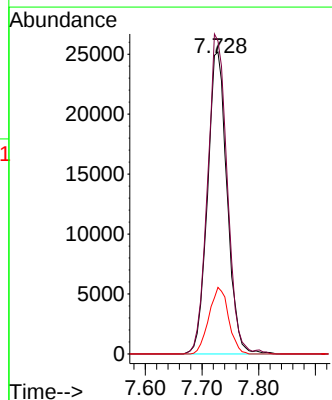
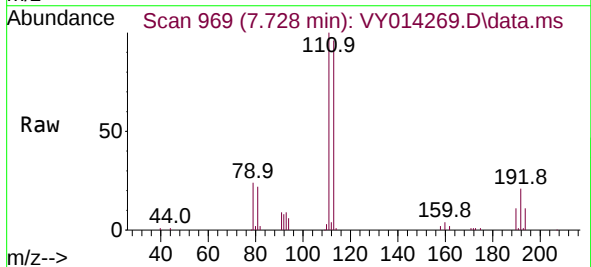


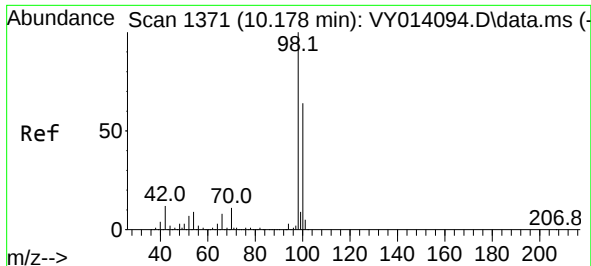

#50
Toluene-d8
Concen: 45.588 ug/l
RT: 10.185 min Scan# 11
Delta R.T. 0.007 min
Lab File: VY014269.D
Acq: 20 Jun 2023 08:33




Instrument :
MSVOA_Y
ClientSampleId :
SB-3


Tgt Ion: 98 Resp: 219467
Ion Ratio Lower Upper
98 100
100 62.9 50.1 75.1

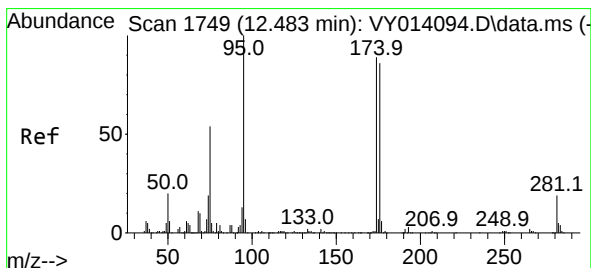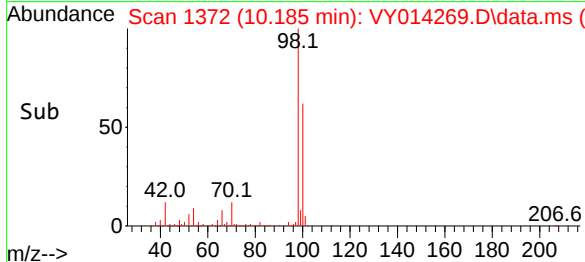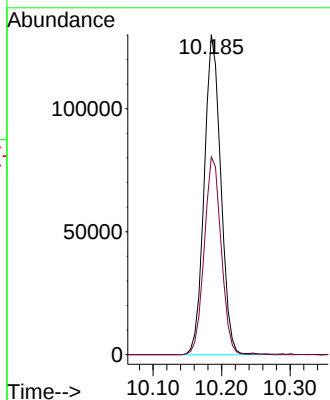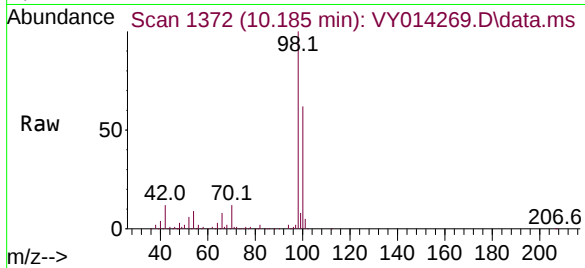

#62
4-Bromofluorobenzene
Concen: 37.104 ug/l
RT: 12.489 min Scan# 1750
Delta R.T. 0.006 min
Lab File: VY014269.D
Acq: 20 Jun 2023 08:33

Tgt Ion: 95 Resp: 63453
Ion Ratio Lower Upper
95 100
174 97.3 0.0 178.2
176 92.4 0.0 173.8

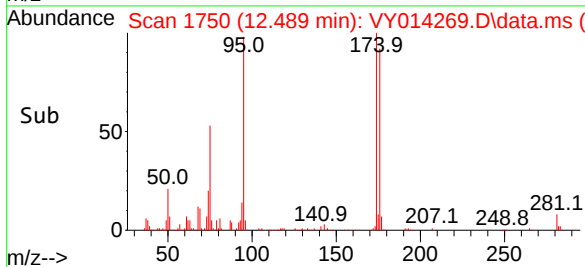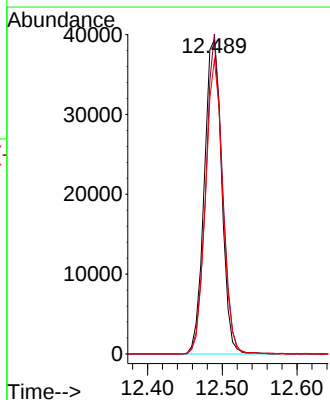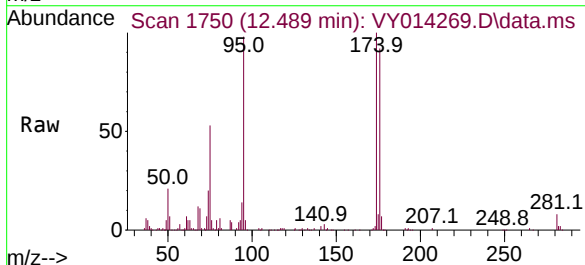

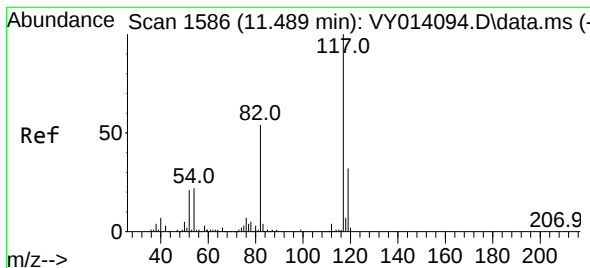

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.496 min Scan# 11

Delta R.T. 0.007 min

Lab File: VY014269.D

Acq: 20 Jun 2023 08:33

Instrument :

MSVOA_Y

ClientSampleId :

SB-3





Tgt Ion:117 Resp: 166623

Ion Ratio Lower Upper

117 100

82 53.3 43.4 65.0

119 29.2 26.3 39.5

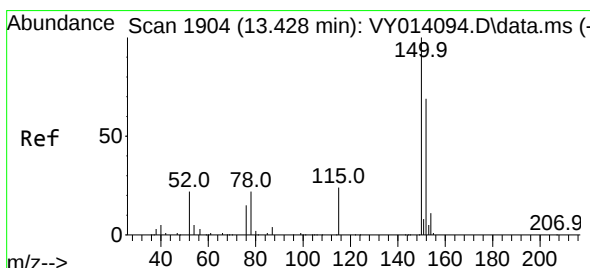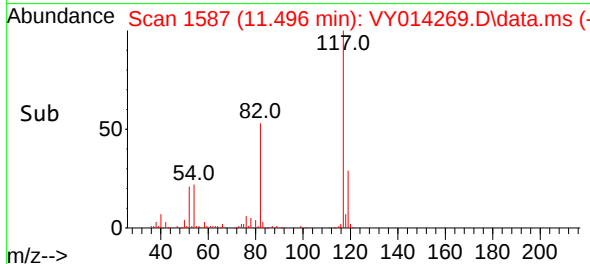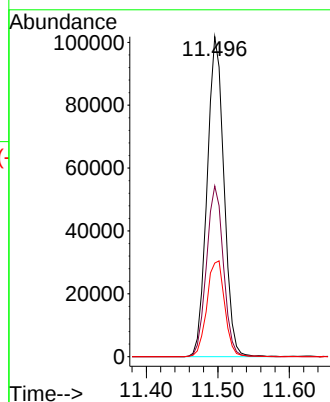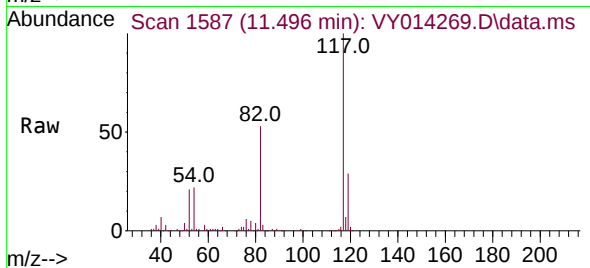

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.428 min Scan# 1904

Delta R.T. 0.000 min

Lab File: VY014269.D

Acq: 20 Jun 2023 08:33

Tgt Ion:152 Resp: 74652

Ion Ratio Lower Upper

152 100

115 55.8 28.8 86.5

150 155.5 0.0 348.8

