


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY061923\
Data File : VY014226.D
Acq On : 19 Jun 2023 12:09
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060923S.M
Title : SW846 8260
Last Update : Fri Jun 09 18:07:13 2023

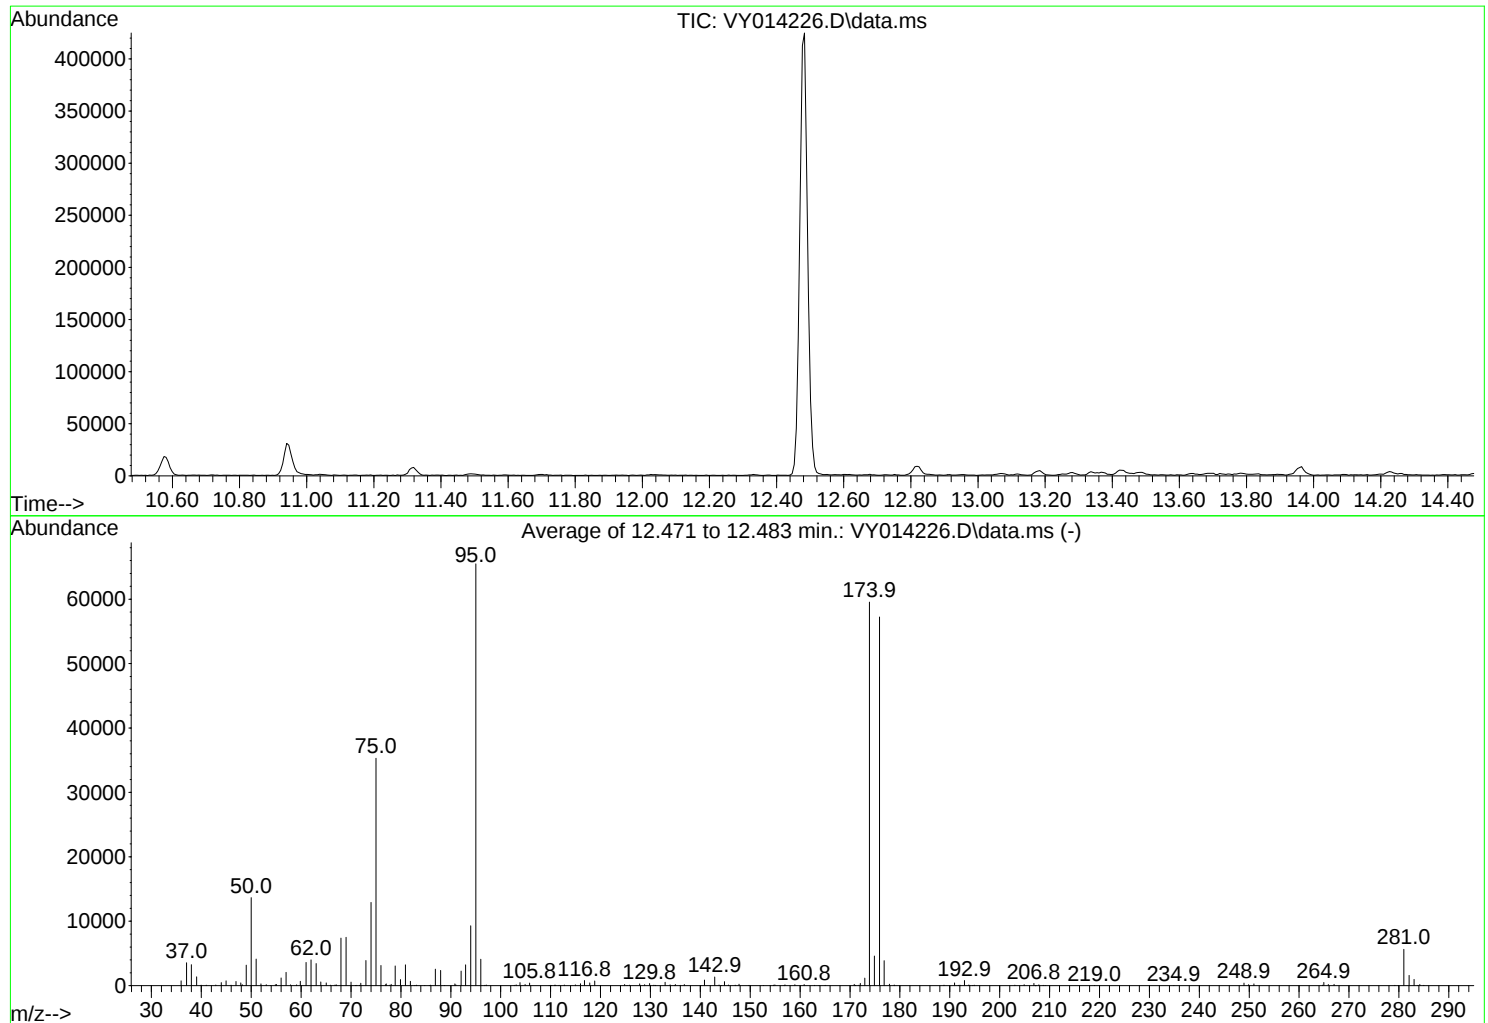

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	13671	PASS
75	95	30	60	53.9	35309	PASS
95	95	100	100	100.0	65491	PASS
96	95	5	9	6.3	4110	PASS
173	174	0.00	2	2.0	1172	PASS
174	95	50	100	90.9	59544	PASS
175	174	5	9	7.7	4600	PASS
176	174	95	101	96.1	57248	PASS
177	176	5	9	6.8	3878	PASS