
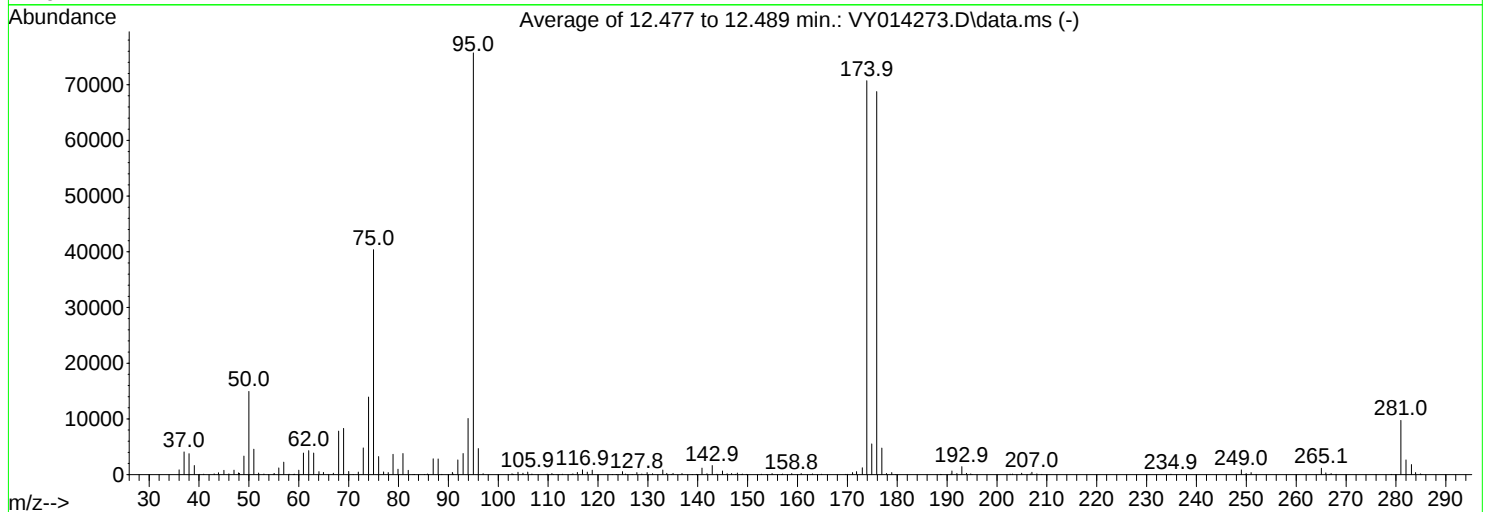


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY062023\
Data File : VY014273.D
Acq On : 20 Jun 2023 10:05
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060923S.M
Title : SW846 8260
Last Update : Fri Jun 09 18:07:13 2023

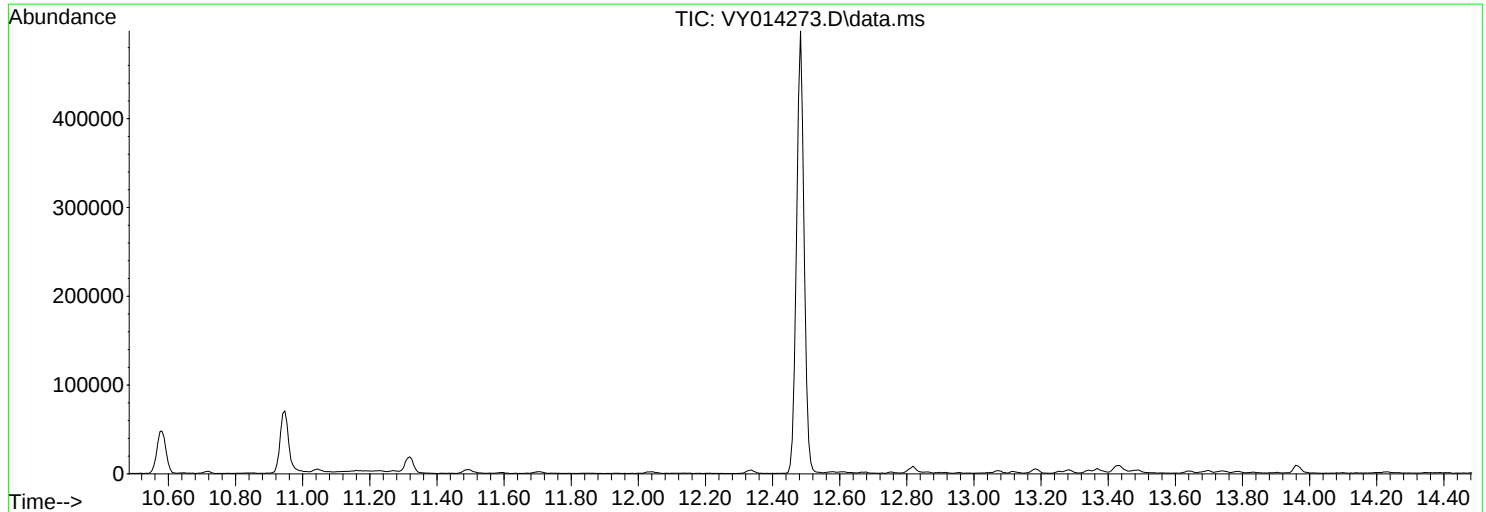

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.7	14949	PASS
75	95	30	60	53.3	40371	PASS
95	95	100	100	100.0	75712	PASS
96	95	5	9	6.2	4694	PASS
173	174	0.00	2	1.8	1242	PASS
174	95	50	100	93.4	70701	PASS
175	174	5	9	7.8	5516	PASS
176	174	95	101	97.2	68744	PASS
177	176	5	9	6.9	4771	PASS