


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY062023\
Data File : VY014300.D
Acq On : 20 Jun 2023 22:09
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Jun 22 02:42:14 2023

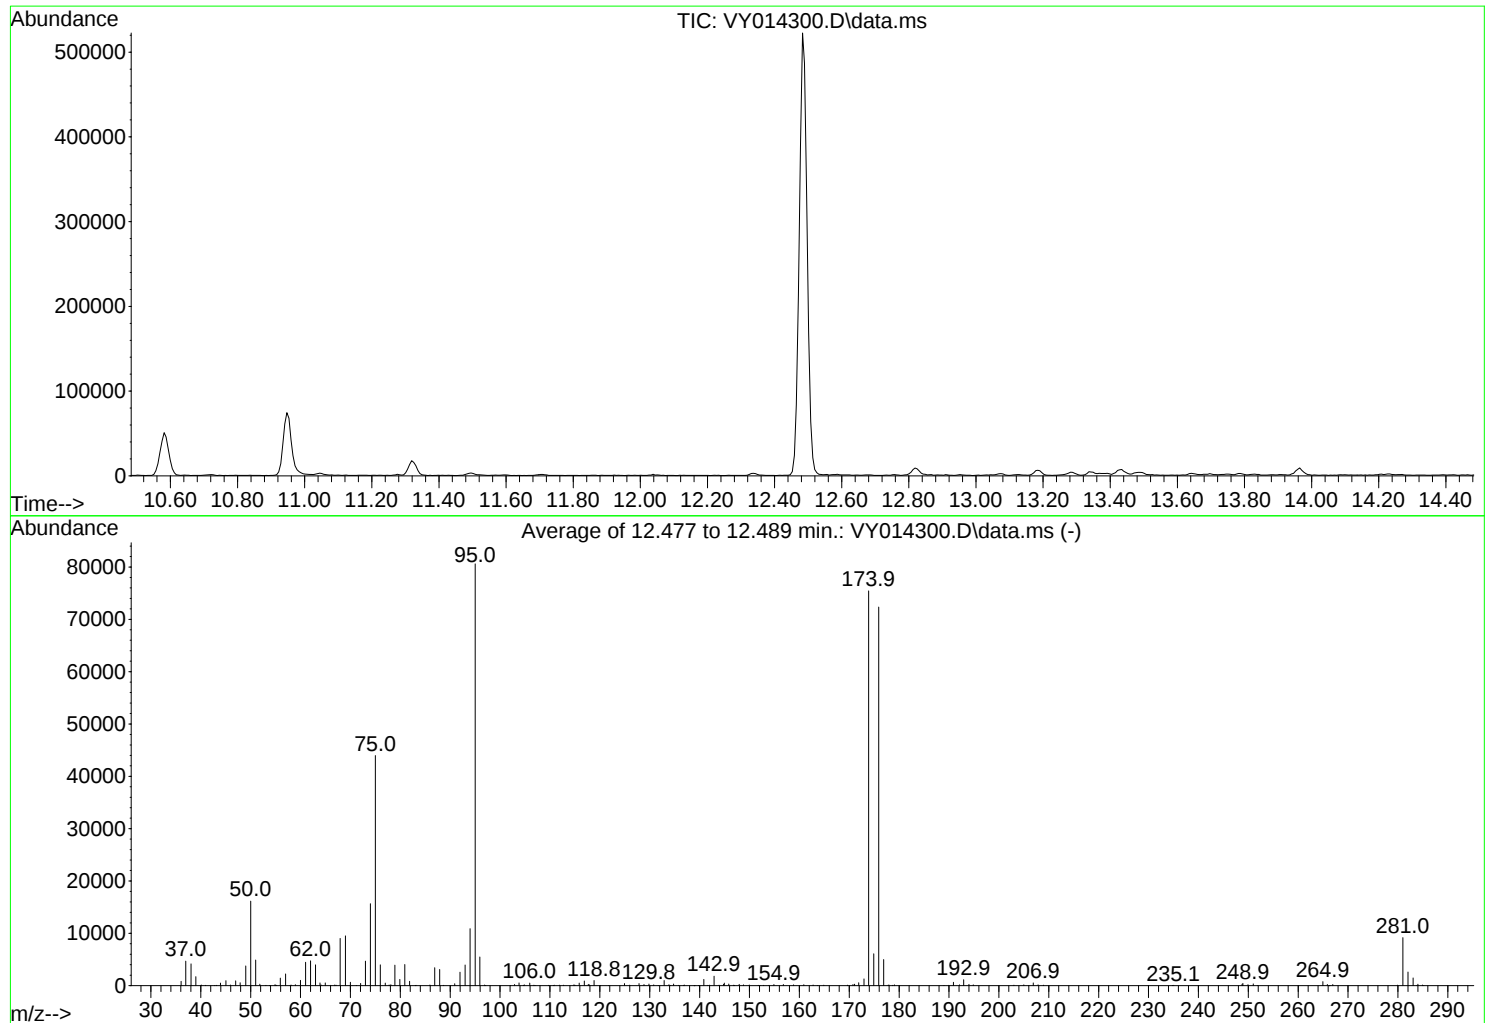

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	16132	PASS
75	95	30	80	54.6	43971	PASS
95	95	100	100	100.0	80603	PASS
96	95	5	9	6.8	5460	PASS
173	174	0.00	2	1.7	1292	PASS
174	95	50	120	93.6	75416	PASS
175	174	5	9	8.1	6096	PASS
176	174	95	101	95.9	72349	PASS
177	176	5	9	6.9	4986	PASS