


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_Y\DATA\VY062220\
 Data File : VY002962.D
 Acq On : 22 Jun 2020 09:23
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y061920S.M
 Title : SW846 8260
 Last Update : Sat Jun 20 06:39:15 2020

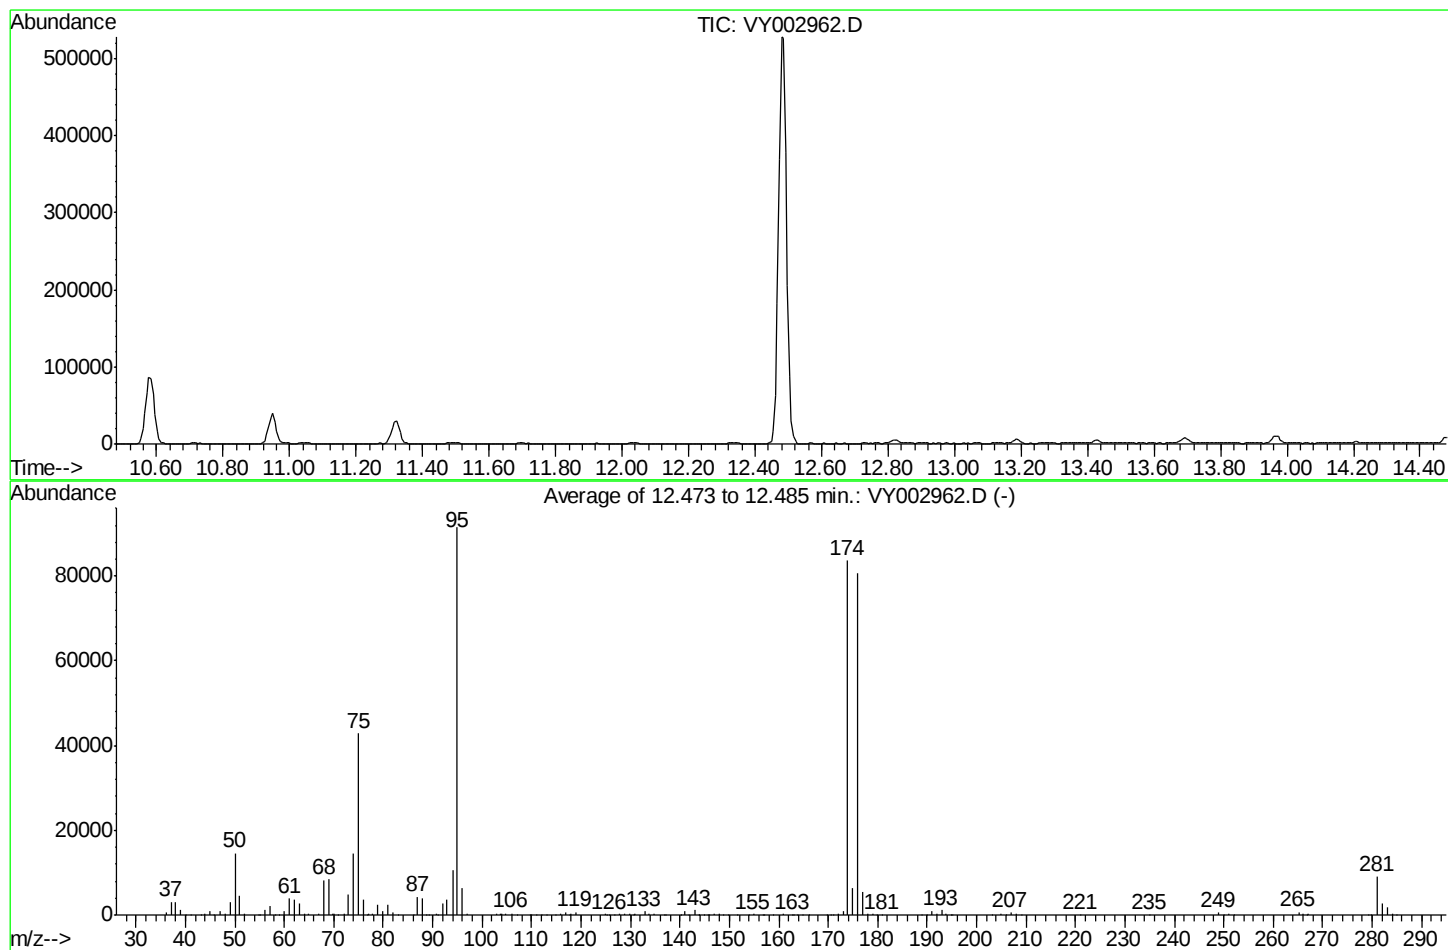

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	14657	PASS
75	95	30	60	46.8	42805	PASS
95	95	100	100	100.0	91504	PASS
96	95	5	9	7.0	6368	PASS
173	174	0.00	2	1.2	990	PASS
174	95	50	100	91.4	83594	PASS
175	174	5	9	7.7	6411	PASS
176	174	95	101	96.7	80802	PASS
177	176	5	9	6.7	5416	PASS