


Tert butyl alcohol

Response Ratio

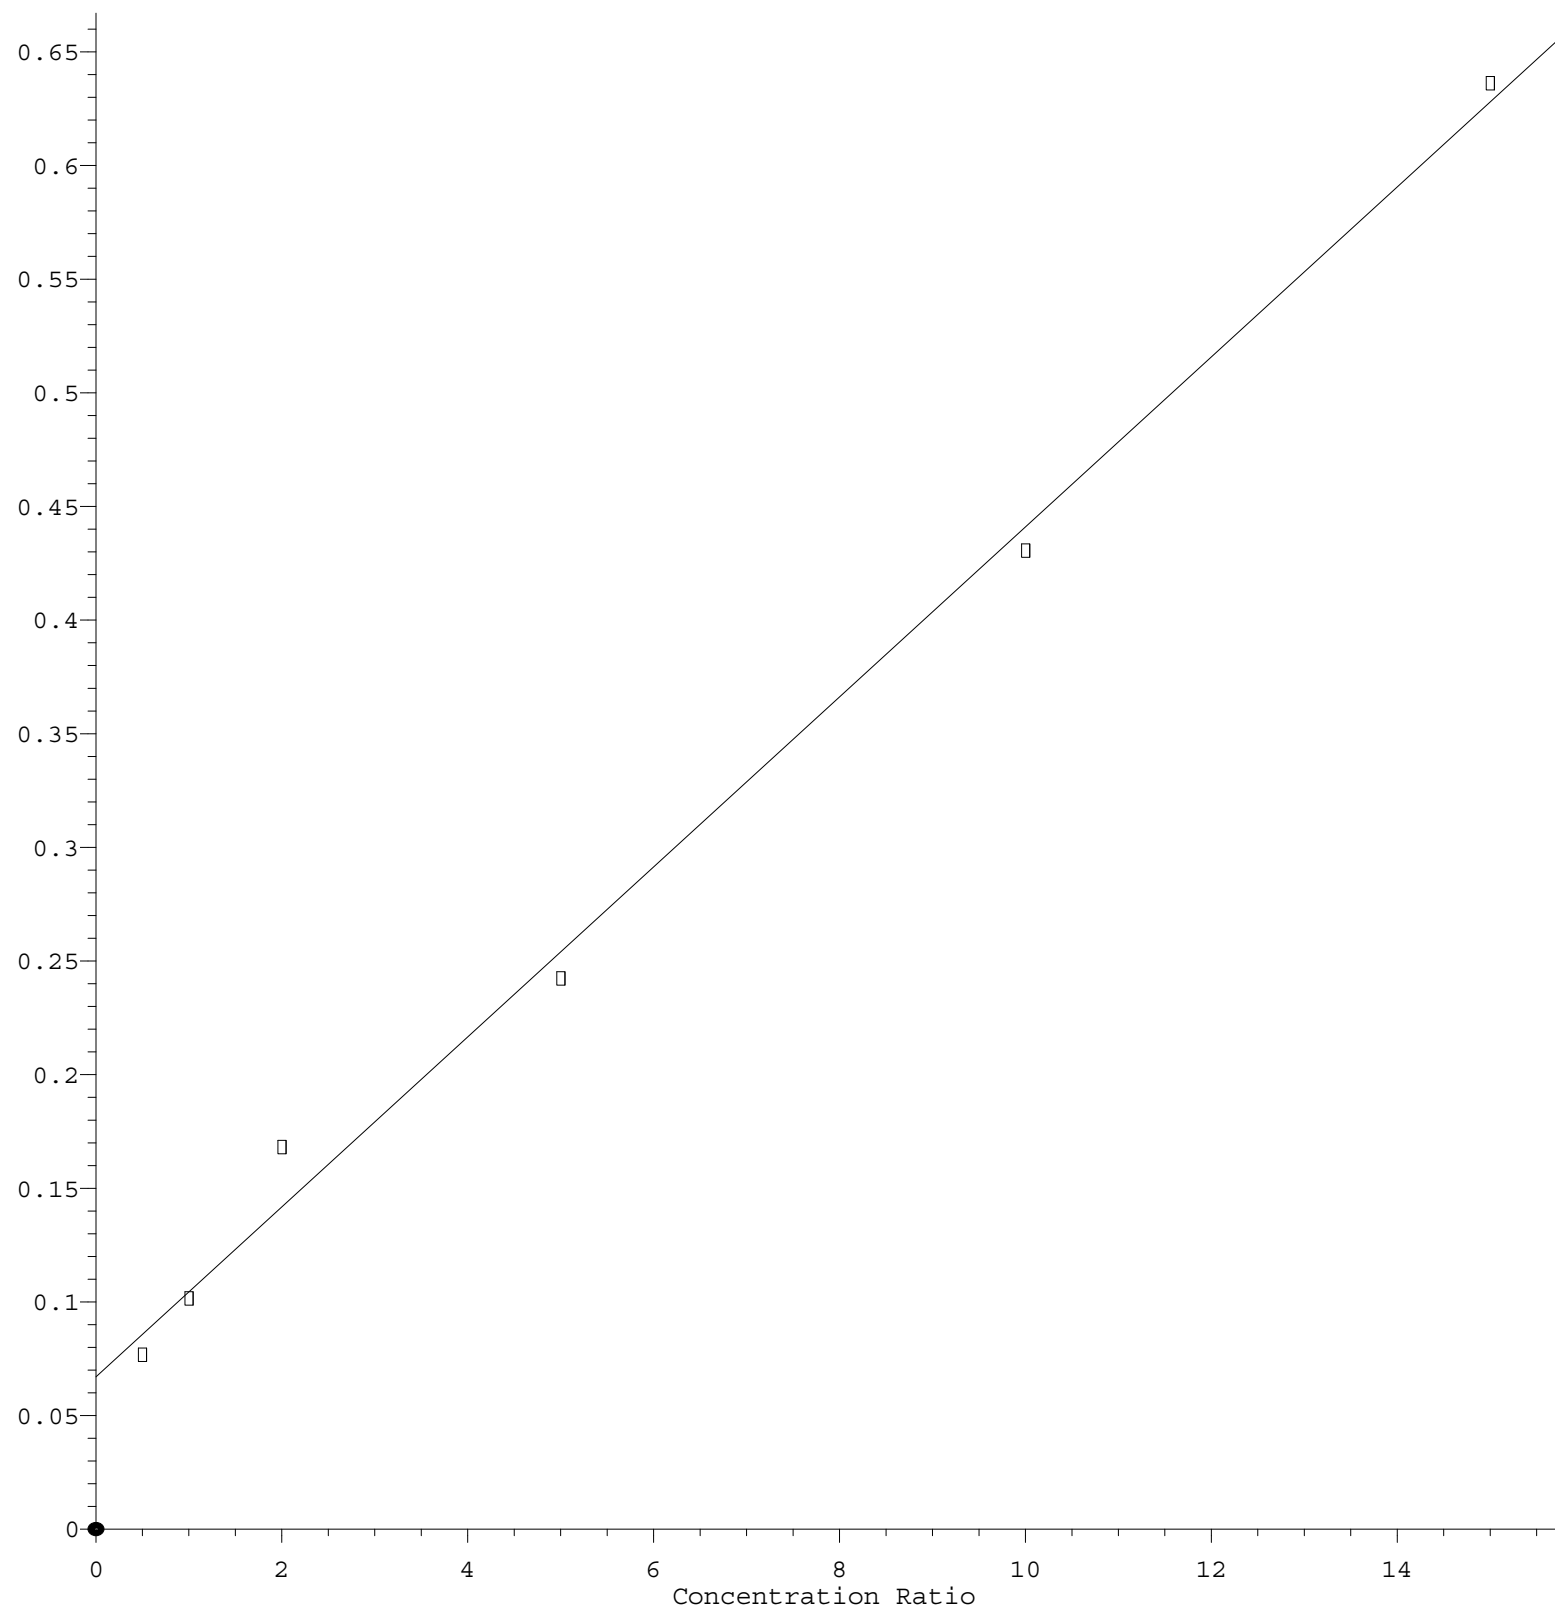

$$\text{Response} = 3.741\text{e-}002 * \text{Amt} + 6.701\text{e-}002$$


Coef of Det (r^2) = 0.995373 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y062221S.M

Calibration Table Last Updated: Wed Jun 23 07:57:52 2021

Methylene Chloride

Response Ratio

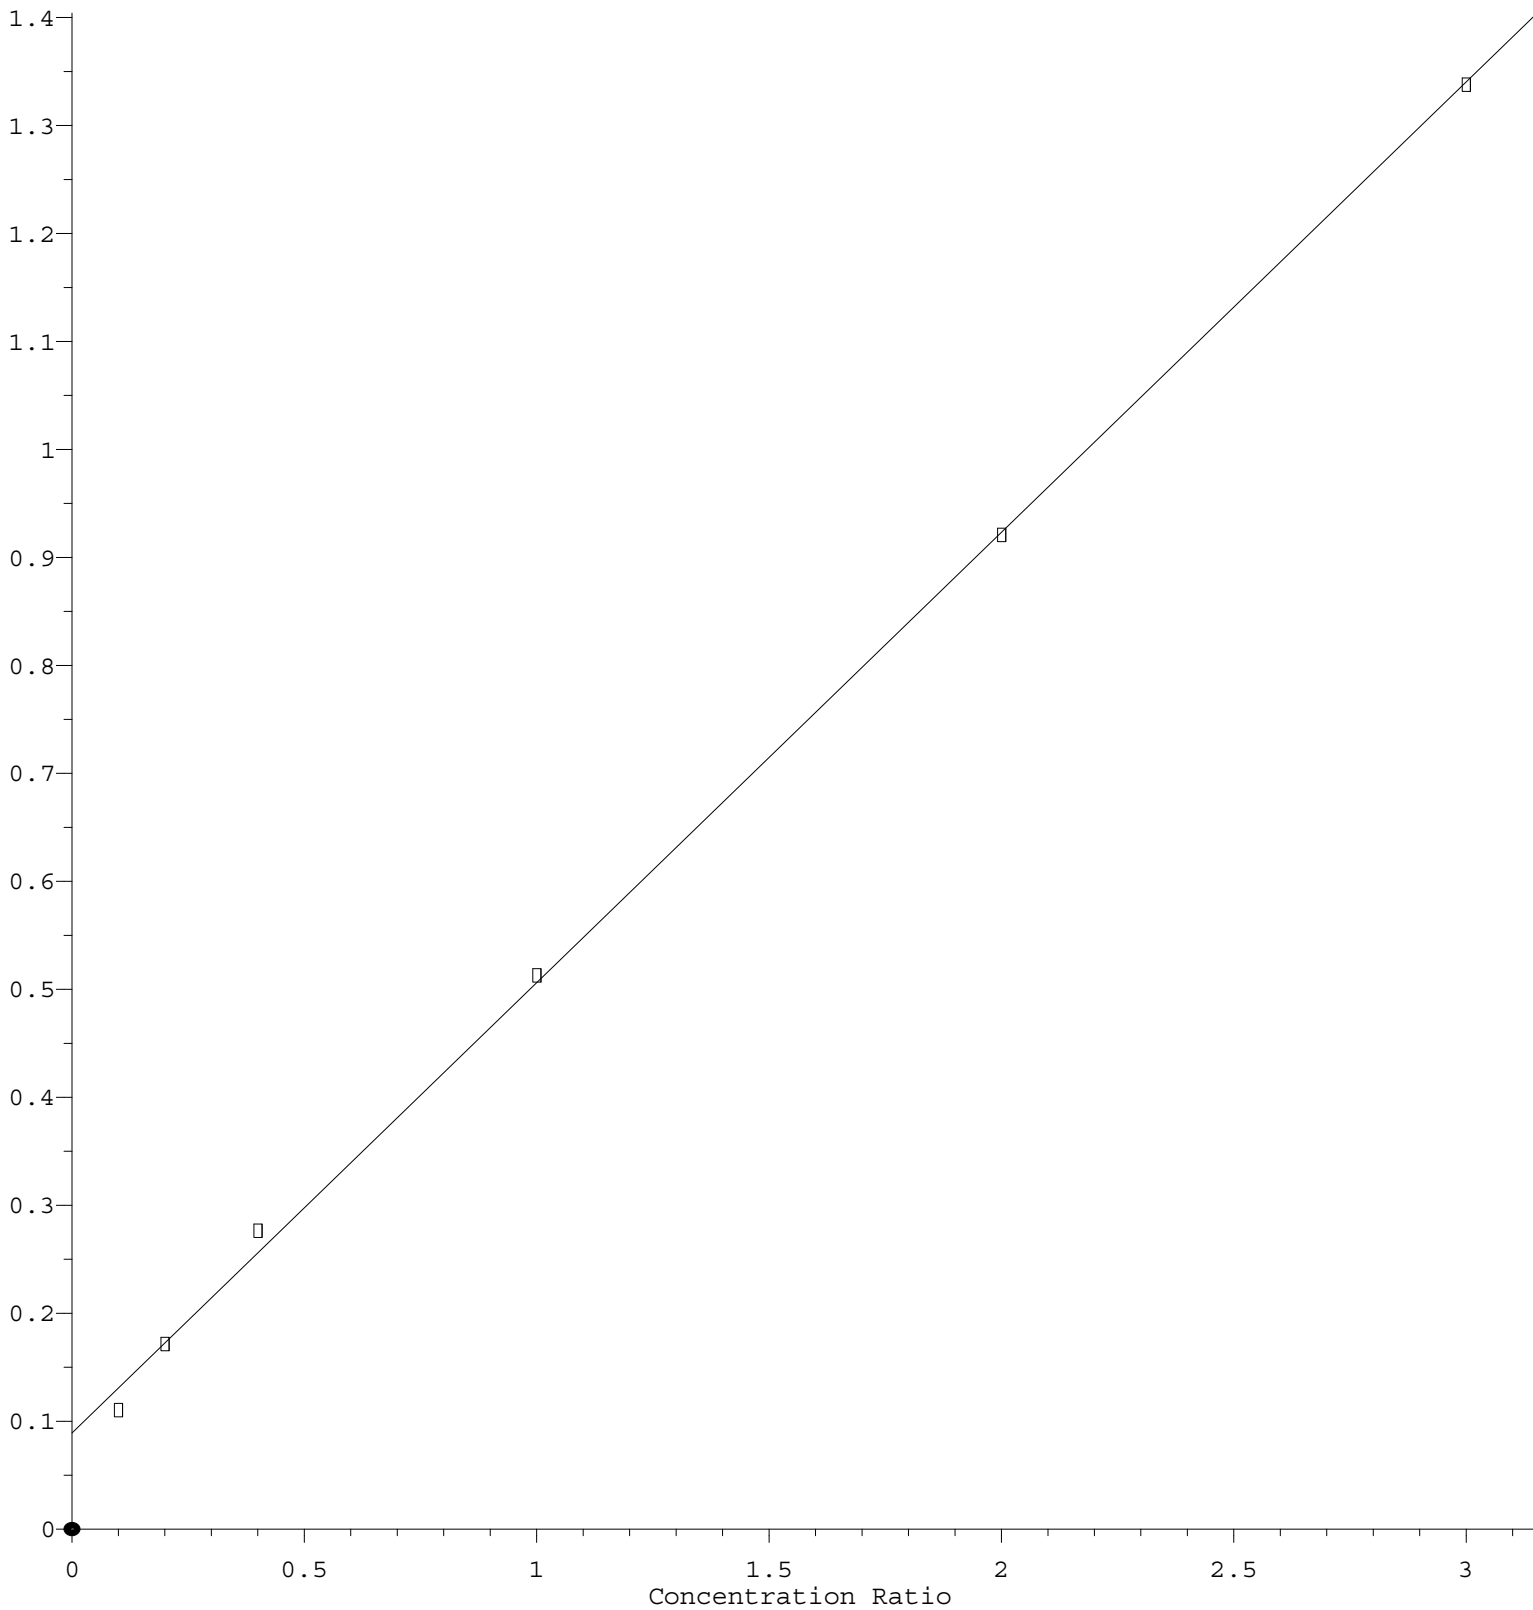

$$\text{Response} = 4.170\text{e-}001 * \text{Amt} + 8.927\text{e-}002$$

Coef of Det (r^2) = 0.999232 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y062221S.M

Calibration Table Last Updated: Wed Jun 23 07:57:52 2021